
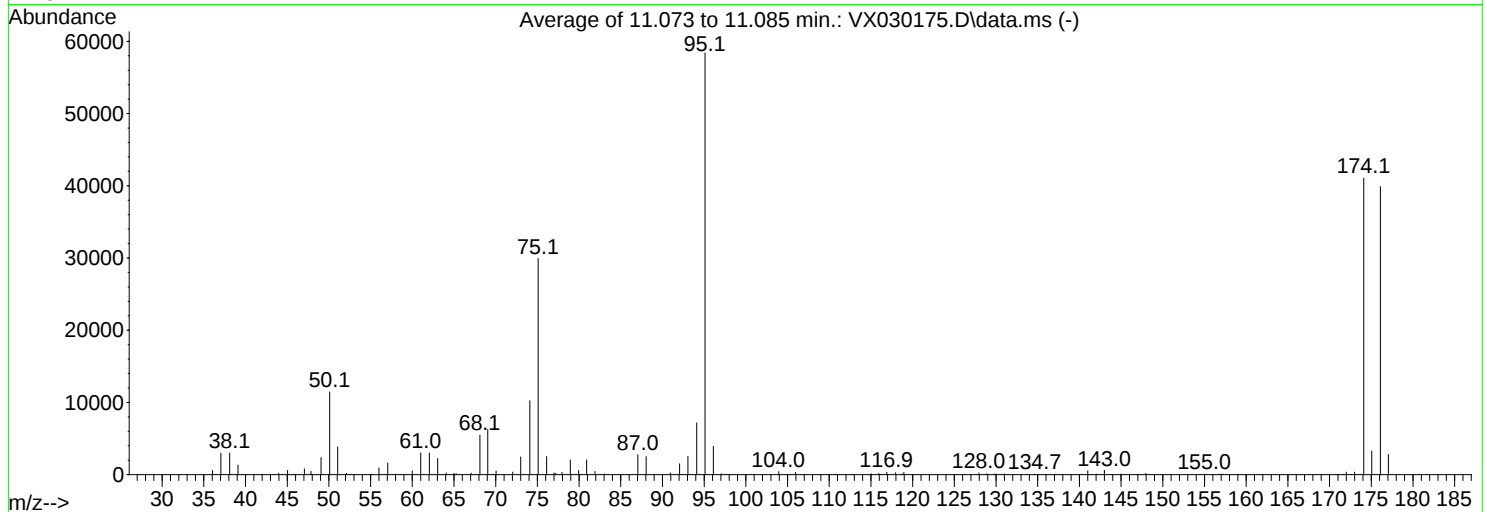


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072222\
Data File : VX030175.D
Acq On : 22 Jul 2022 09:51
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X071222W.M
Title : SW846 8260
Last Update : Wed Jul 13 09:05:23 2022

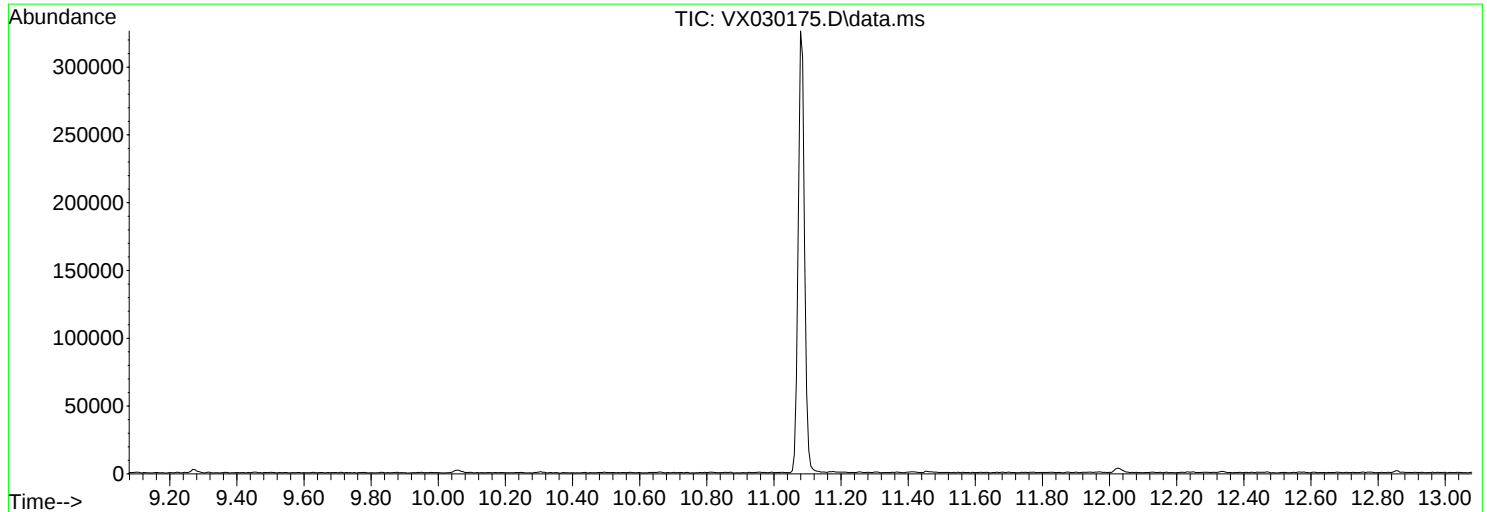

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.6	11452	PASS
75	95	30	60	51.3	29944	PASS
95	95	100	100	100.0	58408	PASS
96	95	5	9	6.7	3932	PASS
173	174	0.00	2	0.9	358	PASS
174	95	50	100	70.3	41051	PASS
175	174	5	9	8.0	3284	PASS
176	174	95	101	97.1	39880	PASS
177	176	5	9	7.0	2788	PASS