

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072224\
 Data File : VX042435.D
 Acq On : 22 Jul 2024 09:32
 Operator : JC/MD
 Sample : VX0722MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK688

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

Signal : TIC: VX042435.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.239	22	25	28	rBV	9365	11331	1.51%	0.200%
2	1.367	43	46	62	rVB	70093	90918	12.15%	1.602%
3	1.648	88	92	102	rVB	55463	72232	9.65%	1.273%
4	2.294	192	198	210	rBV	159411	251945	33.66%	4.439%
5	2.495	229	231	232	rBV	363	220	0.03%	0.004%
6	2.642	254	255	256	rBV	157	113	0.02%	0.002%
7	2.751	272	273	274	rBV	132	79	0.01%	0.001%
8	2.788	274	279	286	rVV2	999	1883	0.25%	0.033%
9	2.940	301	304	305	rBV2	319	326	0.04%	0.006%
10	3.007	311	315	317	rBV2	113	155	0.02%	0.003%
11	3.026	317	318	320	rVV	148	63	0.01%	0.001%
12	3.081	325	327	328	rVV2	147	72	0.01%	0.001%
13	3.123	332	334	336	rBV	148	141	0.02%	0.002%
14	3.196	345	346	349	rVB	126	75	0.01%	0.001%
15	3.233	349	352	355	rBV2	139	198	0.03%	0.003%
16	3.257	355	356	358	rVV2	176	96	0.01%	0.002%
17	3.276	358	359	361	rVV	114	75	0.01%	0.001%
18	3.300	361	363	364	rVV2	100	69	0.01%	0.001%
19	3.385	373	377	378	rBV	183	184	0.02%	0.003%
20	3.446	383	387	388	rBV2	107	173	0.02%	0.003%
21	3.489	392	394	396	rVB	128	113	0.02%	0.002%
22	3.513	396	398	400	rBV2	84	113	0.02%	0.002%
23	3.696	426	428	430	rBV	133	75	0.01%	0.001%
24	3.776	439	441	442	rVB	137	65	0.01%	0.001%
25	3.940	466	468	471	rBV2	92	93	0.01%	0.002%
26	4.251	517	519	520	rBV2	81	71	0.01%	0.001%
27	4.294	525	526	528	rVV	157	114	0.02%	0.002%
28	4.324	528	531	534	rVB2	96	118	0.02%	0.002%
29	4.471	546	555	571	rBV	50031	149536	19.98%	2.635%
30	5.056	639	651	671	rBV	93670	290035	38.75%	5.111%
31	5.397	701	707	708	rBV3	454	803	0.11%	0.014%
32	5.544	726	731	733	rBV3	567	945	0.13%	0.017%
33	5.623	742	744	749	rBV	105	78	0.01%	0.001%
34	5.873	782	785	787	rVB2	136	135	0.02%	0.002%
35	5.964	789	800	823	rBV2	254074	748411	100.00%	13.187%
36	6.342	860	862	863	rVB	133	65	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072224\
 Data File : VX042435.D
 Acq On : 22 Jul 2024 09:32
 Operator : JC/MD
 Sample : VX0722MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK688

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

37	6.385	867	869	871	rBV2	257	249	0.03%	0.004%
38	6.489	885	886	889	rVB	183	138	0.02%	0.002%
39	6.519	889	891	894	rVB2	132	140	0.02%	0.002%
40	6.543	894	895	898	rBV2	168	172	0.02%	0.003%
41	6.574	898	900	901	rVB	124	66	0.01%	0.001%
42	6.763	921	931	946	rBV	192876	467690	62.49%	8.241%
43	7.116	983	989	997	rVB3	1219	3232	0.43%	0.057%
44	7.214	1001	1005	1012	rBV2	268	484	0.06%	0.009%
45	7.305	1012	1020	1038	rBV	148525	330141	44.11%	5.817%
46	7.525	1054	1056	1058	rVB	174	94	0.01%	0.002%
47	7.757	1092	1094	1096	rBV	138	112	0.01%	0.002%
48	7.921	1119	1121	1123	rBV2	106	95	0.01%	0.002%
49	7.958	1125	1127	1130	rBV3	212	257	0.03%	0.005%
50	8.092	1148	1149	1152	rVB	140	101	0.01%	0.002%
51	8.122	1152	1154	1156	rBV	102	89	0.01%	0.002%
52	8.281	1178	1180	1181	rBV	86	67	0.01%	0.001%
53	8.324	1181	1187	1205	rBV	93882	159374	21.29%	2.808%
54	8.513	1217	1218	1219	rBV	344	210	0.03%	0.004%
55	8.647	1234	1240	1257	rBV	394359	627037	83.78%	11.049%
56	8.952	1285	1290	1306	rBV	67987	104311	13.94%	1.838%
57	9.128	1317	1319	1320	rVB	255	139	0.02%	0.002%
58	9.153	1320	1323	1326	rVB	189	250	0.03%	0.004%
59	9.275	1341	1343	1348	rVB2	496	467	0.06%	0.008%
60	9.384	1356	1361	1378	rBV	223164	343878	45.95%	6.059%
61	9.817	1430	1432	1435	rBV2	124	127	0.02%	0.002%
62	10.055	1465	1471	1491	rBV	391461	546596	73.03%	9.631%
63	10.268	1504	1506	1508	rVB2	193	150	0.02%	0.003%
64	10.311	1508	1513	1519	rBV3	451	780	0.10%	0.014%
65	10.390	1525	1526	1527	rBV	119	63	0.01%	0.001%
66	10.585	1555	1558	1559	rBV2	121	122	0.02%	0.002%
67	10.652	1566	1569	1570	rBV2	299	348	0.05%	0.006%
68	10.969	1616	1621	1624	rBV2	191	302	0.04%	0.005%
69	11.018	1628	1629	1630	rVV	134	71	0.01%	0.001%
70	11.110	1641	1644	1646	rBV2	304	408	0.05%	0.007%
71	11.189	1652	1657	1672	rBV	289468	381908	51.03%	6.729%
72	11.317	1675	1678	1682	rVB2	492	598	0.08%	0.011%
73	11.494	1705	1707	1708	rBV	91	64	0.01%	0.001%
74	11.707	1741	1742	1744	rBV	245	195	0.03%	0.003%
75	11.756	1748	1750	1754	rVB	264	312	0.04%	0.005%
76	11.823	1759	1761	1765	rVB	145	124	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072224\
 Data File : VX042435.D
 Acq On : 22 Jul 2024 09:32
 Operator : JC/MD
 Sample : VX0722MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK688

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

77	11.981	1784	1787	1788	rBV2	517	643	0.09%	0.011%
78	12.024	1788	1794	1806	rVV	385615	513913	68.67%	9.055%
79	12.317	1837	1842	1853	rBV	446263	560165	74.85%	9.870%
80	12.579	1883	1885	1886	rBV	158	62	0.01%	0.001%
81	12.762	1910	1915	1918	rBV2	1011	1210	0.16%	0.021%
82	12.804	1921	1922	1925	rBV2	154	124	0.02%	0.002%
83	12.908	1938	1939	1943	rVB2	121	129	0.02%	0.002%
84	12.939	1943	1944	1946	rBV	157	130	0.02%	0.002%
85	13.067	1963	1965	1966	rBV	113	79	0.01%	0.001%
86	13.115	1970	1973	1980	rVV3	480	639	0.09%	0.011%
87	13.182	1982	1984	1986	rBV2	79	95	0.01%	0.002%
88	13.530	2039	2041	2044	rBV2	101	114	0.02%	0.002%
89	13.554	2044	2045	2047	rVV2	168	140	0.02%	0.002%
90	13.597	2049	2052	2054	rVB3	458	538	0.07%	0.009%
91	13.786	2079	2083	2087	rBV2	800	1460	0.20%	0.026%
92	13.914	2102	2104	2109	rVB	105	128	0.02%	0.002%
93	13.963	2109	2112	2117	rVB3	710	977	0.13%	0.017%
94	13.999	2117	2118	2119	rBV	119	75	0.01%	0.001%
95	14.127	2135	2139	2143	rVB	1028	1475	0.20%	0.026%
96	14.243	2157	2158	2160	rBV	162	159	0.02%	0.003%
97	14.365	2177	2178	2180	rVB	238	91	0.01%	0.002%
98	14.554	2208	2209	2212	rBV3	197	235	0.03%	0.004%
99	14.707	2232	2234	2238	rVB3	250	266	0.04%	0.005%
100	14.737	2238	2239	2242	rBV2	301	254	0.03%	0.004%

Sum of corrected areas: 5675180



Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072224\
Data File : VX042435.D
Acq On : 22 Jul 2024 09:32
Operator : JC/MD
Sample : VX0722MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK688

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

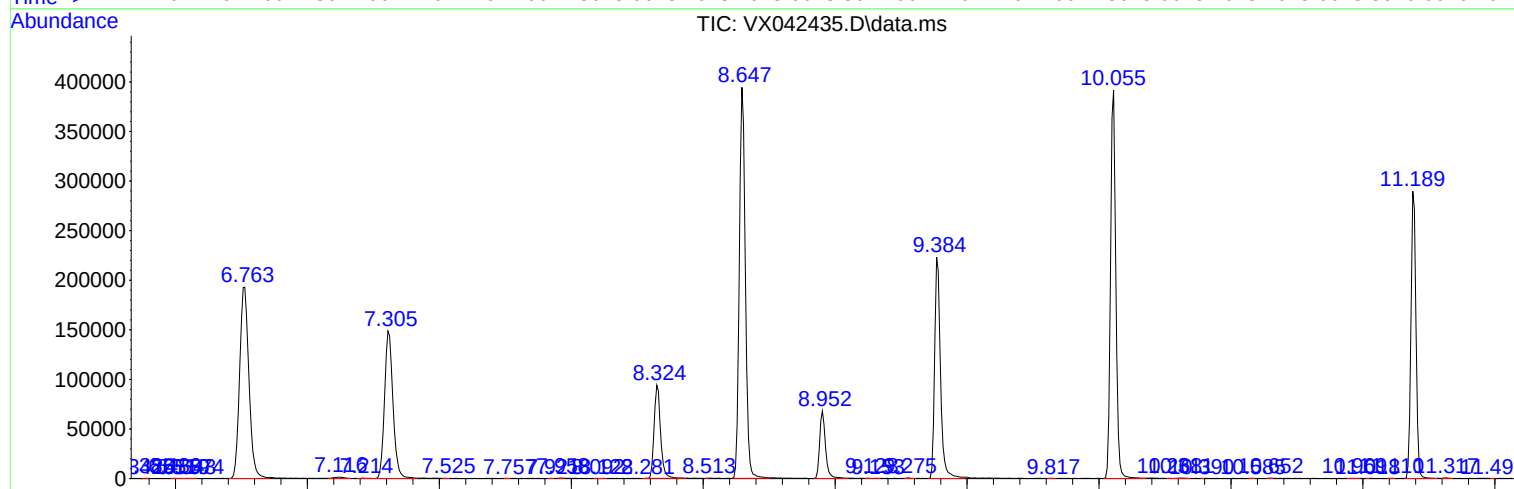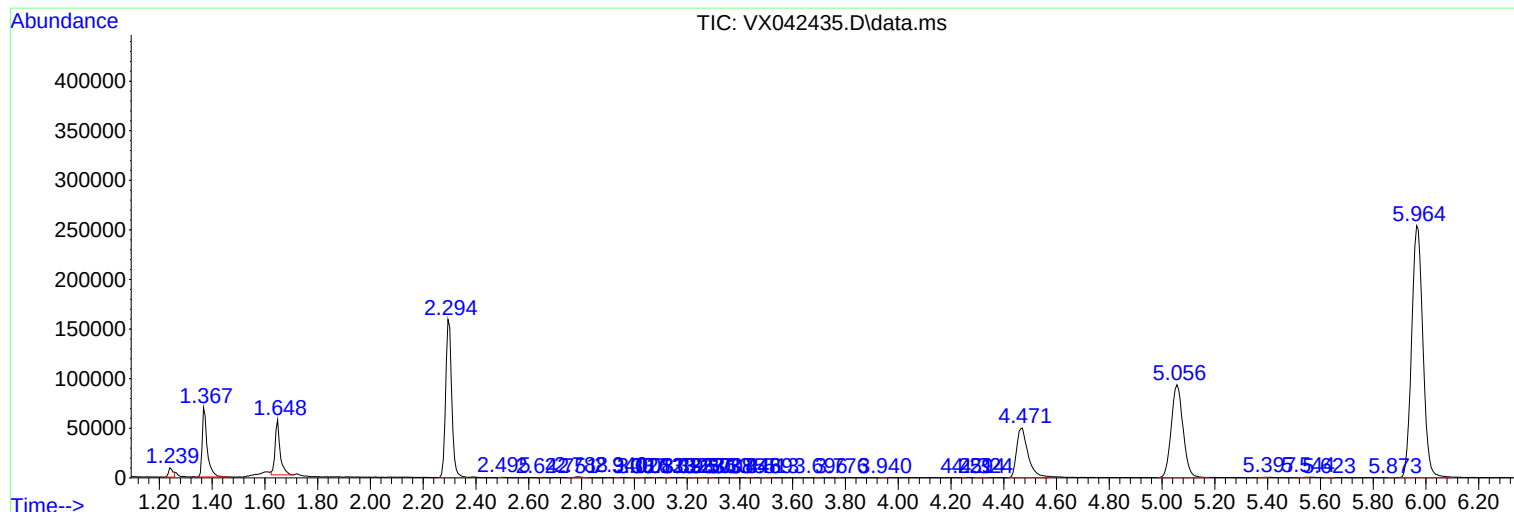

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072224\
Data File : VX042435.D
Acq On : 22 Jul 2024 09:32
Operator : JC/MD
Sample : VX0722MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK688

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072224\
Data File : VX042435.D
Acq On : 22 Jul 2024 09:32
Operator : JC/MD
Sample : VX0722MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK688

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc