

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072224\
 Data File : VX042436.D
 Acq On : 22 Jul 2024 10:01
 Operator : JC/MD
 Sample : VX0722WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK689

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

Signal : TIC: VX042436.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	33	rBV2	9497	14453	2.05%	0.271%
2	1.368	43	46	59	rVB	65188	84695	12.02%	1.589%
3	1.648	88	92	101	rVB	47922	64247	9.12%	1.205%
4	2.099	164	166	167	rBV	263	146	0.02%	0.003%
5	2.294	191	198	210	rBV	150262	230991	32.79%	4.333%
6	2.380	210	212	218	rVB3	738	1249	0.18%	0.023%
7	2.428	218	220	221	rBV	143	71	0.01%	0.001%
8	2.502	229	232	234	rBV2	361	437	0.06%	0.008%
9	2.678	258	261	262	rBV	170	114	0.02%	0.002%
10	2.703	264	265	270	rVV2	226	335	0.05%	0.006%
11	2.788	274	279	285	rVB2	1291	2313	0.33%	0.043%
12	2.843	285	288	289	rBV2	154	173	0.02%	0.003%
13	2.940	299	304	311	rVB3	893	1997	0.28%	0.037%
14	3.014	314	316	318	rBV2	136	165	0.02%	0.003%
15	3.099	329	330	333	rBV2	130	137	0.02%	0.003%
16	3.129	333	335	336	rVB2	114	75	0.01%	0.001%
17	3.233	349	352	354	rBV	109	136	0.02%	0.003%
18	3.257	354	356	358	rBV	95	101	0.01%	0.002%
19	3.331	365	368	369	rBV2	150	126	0.02%	0.002%
20	3.361	371	373	374	rVV	119	75	0.01%	0.001%
21	3.483	390	393	394	rBV	85	68	0.01%	0.001%
22	3.556	403	405	406	rBV2	97	95	0.01%	0.002%
23	3.635	416	418	420	rBV	121	116	0.02%	0.002%
24	3.678	423	425	426	rBV	114	74	0.01%	0.001%
25	3.696	426	428	431	rVB2	161	123	0.02%	0.002%
26	3.739	433	435	436	rVB	163	85	0.01%	0.002%
27	3.782	440	442	443	rBV	83	80	0.01%	0.002%
28	3.812	446	447	448	rBV	170	102	0.01%	0.002%
29	3.959	470	471	474	rBV2	90	103	0.01%	0.002%
30	3.983	474	475	477	rVB	160	95	0.01%	0.002%
31	4.013	477	480	482	rBV2	162	194	0.03%	0.004%
32	4.141	499	501	503	rBV	131	104	0.01%	0.002%
33	4.245	516	518	520	rBV2	115	88	0.01%	0.002%
34	4.465	546	554	575	rBV	49275	149670	21.25%	2.807%
35	5.056	639	651	671	rBV	88198	272863	38.74%	5.118%
36	5.306	691	692	695	rVB2	81	66	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072224\
 Data File : VX042436.D
 Acq On : 22 Jul 2024 10:01
 Operator : JC/MD
 Sample : VX0722WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK689

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

37	5.336	695	697	700	rBV2	141	139	0.02%	0.003%
38	5.385	700	705	711	rVV4	494	1150	0.16%	0.022%
39	5.550	727	732	735	rBV3	397	745	0.11%	0.014%
40	5.751	763	765	767	rBV2	102	72	0.01%	0.001%
41	5.794	769	772	773	rBV2	136	157	0.02%	0.003%
42	5.964	788	800	822	rBV2	240797	704360	100.00%	13.212%
43	6.233	842	844	845	rBV	115	82	0.01%	0.002%
44	6.440	875	878	880	rBV	127	168	0.02%	0.003%
45	6.464	880	882	883	rVV2	142	110	0.02%	0.002%
46	6.757	921	930	945	rBV	179919	431382	61.24%	8.091%
47	7.117	983	989	994	rVB2	1593	2787	0.40%	0.052%
48	7.214	1001	1005	1007	rBV3	218	314	0.04%	0.006%
49	7.306	1012	1020	1037	rBV	141720	310757	44.12%	5.829%
50	7.495	1047	1051	1056	rBV3	313	379	0.05%	0.007%
51	7.592	1064	1067	1068	rBV	164	166	0.02%	0.003%
52	7.805	1100	1102	1103	rBV	104	75	0.01%	0.001%
53	7.952	1124	1126	1127	rBV	155	105	0.01%	0.002%
54	8.055	1141	1143	1145	rBV2	78	90	0.01%	0.002%
55	8.183	1162	1164	1165	rBV	139	92	0.01%	0.002%
56	8.244	1172	1174	1176	rBV2	79	77	0.01%	0.001%
57	8.324	1181	1187	1205	rVV	90245	148245	21.05%	2.781%
58	8.647	1234	1240	1256	rBV	374223	586044	83.20%	10.992%
59	8.952	1285	1290	1305	rBV	64897	97913	13.90%	1.837%
60	9.275	1341	1343	1348	rVB2	447	535	0.08%	0.010%
61	9.384	1356	1361	1382	rBV	222932	335729	47.66%	6.297%
62	9.701	1411	1413	1416	rVV2	357	380	0.05%	0.007%
63	9.744	1418	1420	1424	rBV2	205	192	0.03%	0.004%
64	9.860	1437	1439	1442	rVB	124	125	0.02%	0.002%
65	9.890	1442	1444	1446	rBV2	114	89	0.01%	0.002%
66	10.055	1465	1471	1492	rBV	361609	506779	71.95%	9.506%
67	10.305	1510	1512	1516	rVB2	389	510	0.07%	0.010%
68	10.348	1517	1519	1521	rVB	140	82	0.01%	0.002%
69	10.415	1528	1530	1532	rBV2	104	116	0.02%	0.002%
70	10.512	1543	1546	1549	rBV2	170	261	0.04%	0.005%
71	10.640	1566	1567	1570	rBV3	268	293	0.04%	0.005%
72	10.732	1580	1582	1584	rVB2	90	68	0.01%	0.001%
73	10.835	1595	1599	1600	rVB2	158	116	0.02%	0.002%
74	10.854	1600	1602	1603	rBV	128	68	0.01%	0.001%
75	10.963	1619	1620	1623	rVB2	142	123	0.02%	0.002%
76	11.128	1645	1647	1649	rBV2	113	82	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072224\
 Data File : VX042436.D
 Acq On : 22 Jul 2024 10:01
 Operator : JC/MD
 Sample : VX0722WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK689

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

77	11.152	1649	1651	1652	rVV	100	79	0.01%	0.001%
78	11.189	1652	1657	1671	rVV	280527	368694	52.34%	6.916%
79	11.317	1673	1678	1682	rVB	629	801	0.11%	0.015%
80	11.585	1720	1722	1724	rVB2	148	116	0.02%	0.002%
81	11.616	1726	1727	1730	rBV2	103	97	0.01%	0.002%
82	11.713	1741	1743	1745	rBV2	185	105	0.01%	0.002%
83	11.762	1747	1751	1754	rVV3	187	274	0.04%	0.005%
84	11.793	1755	1756	1760	rVV2	91	110	0.02%	0.002%
85	11.829	1760	1762	1765	rVB2	130	110	0.02%	0.002%
86	11.982	1783	1787	1788	rBV3	363	502	0.07%	0.009%
87	12.024	1788	1794	1806	rVV	360264	476190	67.61%	8.932%
88	12.317	1837	1842	1856	rBV	410732	522354	74.16%	9.798%
89	12.536	1876	1878	1880	rBV	179	102	0.01%	0.002%
90	12.683	1901	1902	1904	rBV	94	66	0.01%	0.001%
91	12.762	1912	1915	1919	rBV2	901	1189	0.17%	0.022%
92	13.597	2050	2052	2056	rVB	426	405	0.06%	0.008%
93	13.786	2080	2083	2086	rBV3	314	491	0.07%	0.009%
94	13.969	2111	2113	2117	rVB2	380	350	0.05%	0.007%
95	14.030	2121	2123	2124	rBV	147	114	0.02%	0.002%
96	14.134	2136	2140	2144	rVB2	993	1383	0.20%	0.026%
97	14.280	2163	2164	2166	rBV	207	162	0.02%	0.003%
98	14.640	2222	2223	2225	rBV	285	154	0.02%	0.003%
99	14.938	2270	2272	2275	rBV3	303	375	0.05%	0.007%
100	15.237	2319	2321	2322	rBV	438	260	0.04%	0.005%




Sum of corrected areas: 5331402

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072224\
Data File : VX042436.D
Acq On : 22 Jul 2024 10:01
Operator : JC/MD
Sample : VX0722WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK689

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

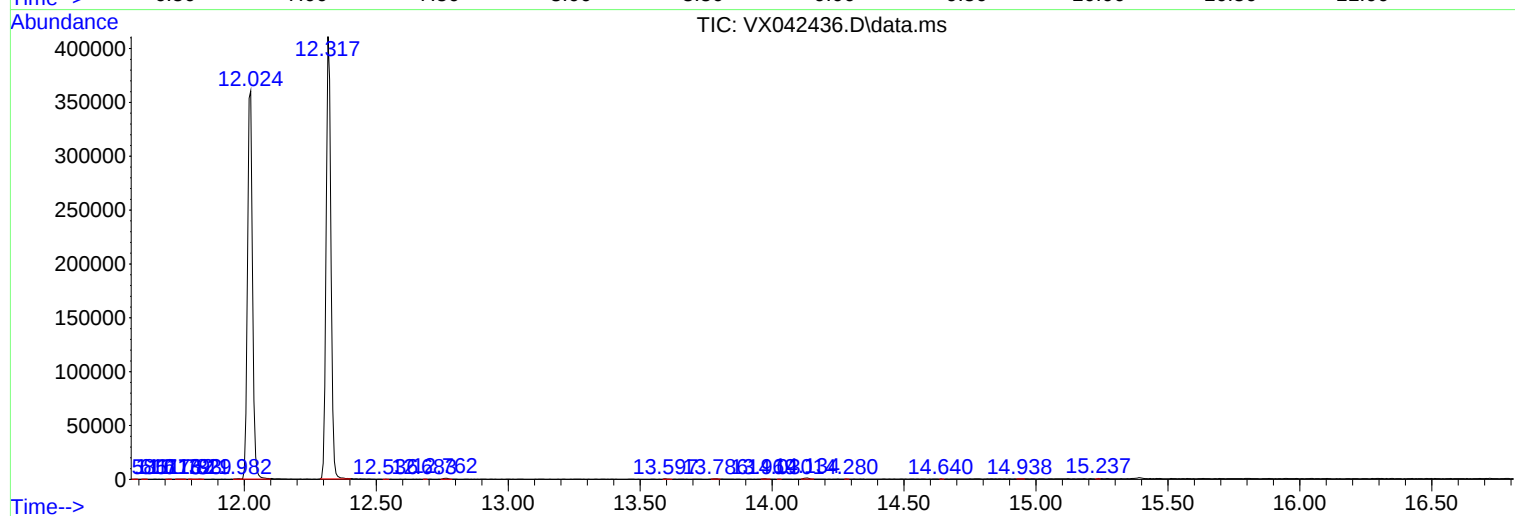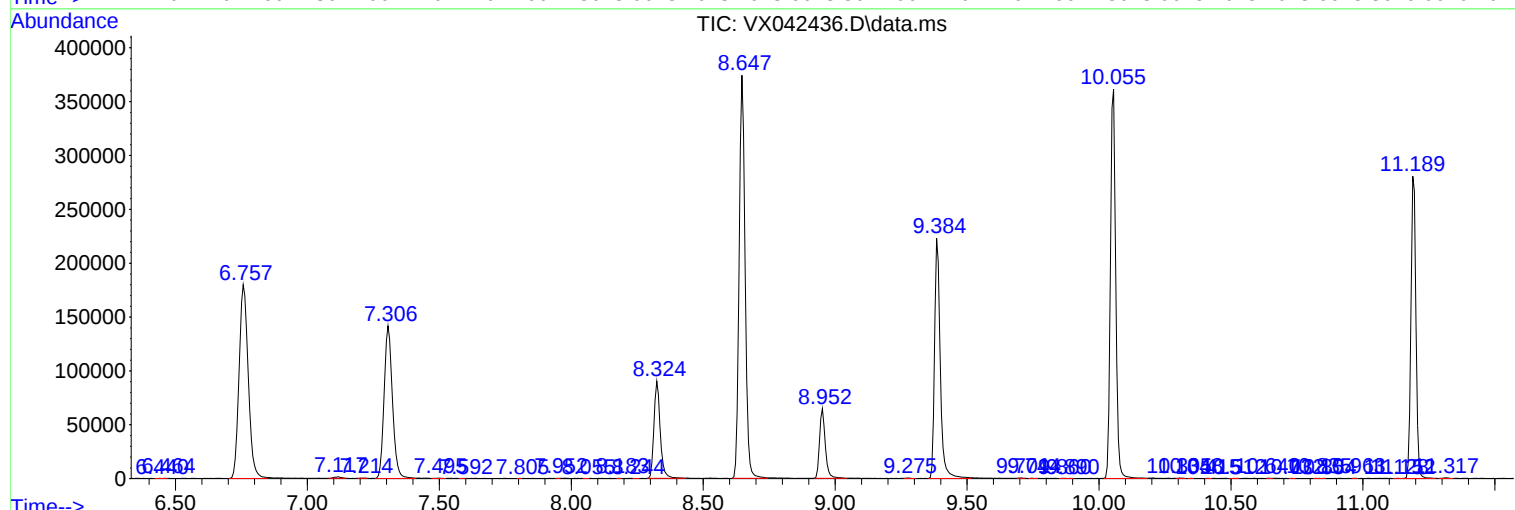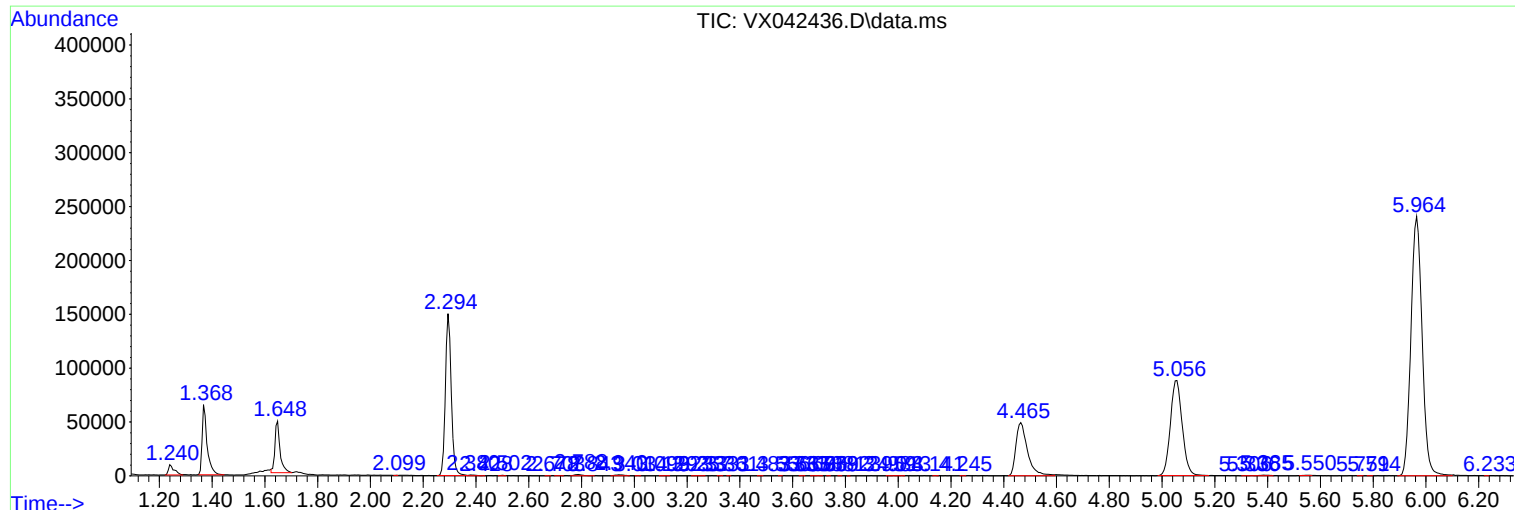

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072224\
Data File : VX042436.D
Acq On : 22 Jul 2024 10:01
Operator : JC/MD
Sample : VX0722WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK689

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072224\
Data File : VX042436.D
Acq On : 22 Jul 2024 10:01
Operator : JC/MD
Sample : VX0722WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK689

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc