

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072224\
 Data File : VX042437.D
 Acq On : 22 Jul 2024 10:24
 Operator : JC/MD
 Sample : P3277-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E1ZR6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

Signal : TIC: VX042437.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	27	rBV	7992	8761	1.34%	0.173%
2	1.368	43	46	58	rBV	57261	70583	10.81%	1.396%
3	1.648	88	92	101	rVB	48965	62404	9.56%	1.235%
4	2.203	181	183	184	rBV	182	83	0.01%	0.002%
5	2.252	190	191	192	rBV	244	135	0.02%	0.003%
6	2.294	192	198	209	rVV	131326	207193	31.74%	4.099%
7	2.392	209	214	220	rVB	3012	5100	0.78%	0.101%
8	2.502	229	232	237	rVB2	301	406	0.06%	0.008%
9	2.623	249	252	255	rBV2	124	199	0.03%	0.004%
10	2.709	263	266	272	rVB2	487	789	0.12%	0.016%
11	2.788	272	279	286	rBV3	990	2047	0.31%	0.040%
12	2.861	289	291	293	rBV	164	162	0.02%	0.003%
13	2.947	301	305	308	rVB3	362	485	0.07%	0.010%
14	3.044	319	321	322	rBV	101	45	0.01%	0.001%
15	3.160	339	340	342	rBV	109	107	0.02%	0.002%
16	3.203	345	347	349	rBV	166	169	0.03%	0.003%
17	3.306	363	364	365	rBV	87	43	0.01%	0.001%
18	3.410	379	381	382	rBV	97	77	0.01%	0.002%
19	3.471	388	391	394	rBV	110	162	0.02%	0.003%
20	3.544	400	403	404	rBV	103	68	0.01%	0.001%
21	3.581	406	409	410	rBV2	104	104	0.02%	0.002%
22	3.599	410	412	413	rVB	146	93	0.01%	0.002%
23	3.611	413	414	415	rBV	118	78	0.01%	0.002%
24	3.739	434	435	437	rBV	102	108	0.02%	0.002%
25	3.764	437	439	442	rVB	112	105	0.02%	0.002%
26	3.904	460	462	463	rBV	101	89	0.01%	0.002%
27	3.959	467	471	472	rBV	170	184	0.03%	0.004%
28	3.977	472	474	478	rVB	133	144	0.02%	0.003%
29	4.343	532	534	536	rBV	131	115	0.02%	0.002%
30	4.465	546	554	570	rBV	46887	140618	21.54%	2.782%
31	4.879	620	622	624	rBV2	87	66	0.01%	0.001%
32	5.056	639	651	668	rBV	83825	257264	39.41%	5.089%
33	5.403	701	708	710	rBV2	532	1132	0.17%	0.022%
34	5.471	717	719	720	rVB2	128	79	0.01%	0.002%
35	5.501	720	724	726	rBV2	125	188	0.03%	0.004%
36	5.556	727	733	734	rBV	505	696	0.11%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072224\
 Data File : VX042437.D
 Acq On : 22 Jul 2024 10:24
 Operator : JC/MD
 Sample : P3277-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E1ZR6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

37	5.727	759	761	764	rBV2	97	111	0.02%	0.002%
38	5.818	774	776	777	rBV	132	80	0.01%	0.002%
39	5.855	780	782	784	rBV2	112	108	0.02%	0.002%
40	5.964	789	800	818	rBV2	219924	652789	100.00%	12.914%
41	6.300	853	855	856	rVB	164	80	0.01%	0.002%
42	6.318	856	858	859	rVV	84	57	0.01%	0.001%
43	6.367	863	866	869	rVB2	199	211	0.03%	0.004%
44	6.470	882	883	886	rVB	225	169	0.03%	0.003%
45	6.757	922	930	950	rBV	183073	440536	67.49%	8.715%
46	7.080	981	983	984	rBV	145	76	0.01%	0.002%
47	7.123	985	990	994	rVB4	608	1249	0.19%	0.025%
48	7.202	1002	1003	1006	rBV2	285	294	0.05%	0.006%
49	7.306	1012	1020	1041	rBV	128827	288955	44.26%	5.716%
50	7.488	1047	1050	1051	rBV	285	304	0.05%	0.006%
51	7.635	1071	1074	1075	rBV2	155	154	0.02%	0.003%
52	7.897	1116	1117	1122	rBV2	106	116	0.02%	0.002%
53	7.952	1122	1126	1131	rBV3	558	1168	0.18%	0.023%
54	8.092	1147	1149	1150	rVB2	101	46	0.01%	0.001%
55	8.263	1175	1177	1178	rVB	162	92	0.01%	0.002%
56	8.324	1181	1187	1203	rBV	78792	133780	20.49%	2.647%
57	8.513	1211	1218	1221	rBV3	490	1066	0.16%	0.021%
58	8.586	1228	1230	1234	rVB	312	218	0.03%	0.004%
59	8.647	1234	1240	1252	rBV	343342	535859	82.09%	10.601%
60	8.885	1277	1279	1282	rVB	251	215	0.03%	0.004%
61	8.952	1285	1290	1302	rBV	57334	85684	13.13%	1.695%
62	9.275	1339	1343	1346	rVB2	845	1246	0.19%	0.025%
63	9.384	1356	1361	1380	rBV	208258	312742	47.91%	6.187%
64	9.531	1382	1385	1394	rVB4	2985	6109	0.94%	0.121%
65	9.720	1415	1416	1421	rVB2	186	207	0.03%	0.004%
66	9.775	1421	1425	1426	rBV2	160	172	0.03%	0.003%
67	9.927	1449	1450	1451	rVB	172	63	0.01%	0.001%
68	9.945	1451	1453	1454	rBV	114	78	0.01%	0.002%
69	10.055	1465	1471	1487	rBV	363757	512971	78.58%	10.148%
70	10.195	1492	1494	1500	rVV3	586	886	0.14%	0.018%
71	10.244	1500	1502	1505	rVV2	189	196	0.03%	0.004%
72	10.311	1509	1513	1518	rVB3	711	1155	0.18%	0.023%
73	10.653	1565	1569	1570	rBV2	543	622	0.10%	0.012%
74	10.732	1579	1582	1583	rBV	136	122	0.02%	0.002%
75	10.793	1589	1592	1596	rBV2	179	257	0.04%	0.005%
76	10.963	1618	1620	1625	rVB2	291	370	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072224\
 Data File : VX042437.D
 Acq On : 22 Jul 2024 10:24
 Operator : JC/MD
 Sample : P3277-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E1ZR6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

77	11.012	1625	1628	1629	rBV2	64	62	0.01%	0.001%
78	11.098	1639	1642	1644	rBB2	164	174	0.03%	0.003%
79	11.189	1652	1657	1665	rBV	259451	341767	52.35%	6.761%
80	11.311	1674	1677	1681	rVB2	900	1258	0.19%	0.025%
81	11.732	1744	1746	1747	rBV2	118	65	0.01%	0.001%
82	11.939	1778	1780	1781	rBV	121	64	0.01%	0.001%
83	11.975	1783	1786	1788	rBV2	368	356	0.05%	0.007%
84	12.018	1788	1793	1801	rBV	360059	470231	72.03%	9.303%
85	12.219	1821	1826	1835	rBV	12411	16702	2.56%	0.330%
86	12.317	1837	1842	1855	rVV	368994	475637	72.86%	9.410%
87	12.500	1870	1872	1874	rVB2	274	172	0.03%	0.003%
88	12.634	1893	1894	1896	rBV	202	103	0.02%	0.002%
89	12.731	1906	1910	1912	rBV2	139	180	0.03%	0.004%
90	12.859	1928	1931	1934	rBV3	859	947	0.15%	0.019%
91	13.036	1958	1960	1964	rBV	151	182	0.03%	0.004%
92	13.116	1969	1973	1977	rVV2	263	382	0.06%	0.008%
93	13.628	2054	2057	2058	rBV	154	122	0.02%	0.002%
94	13.786	2078	2083	2087	rVB	574	794	0.12%	0.016%
95	13.957	2110	2111	2114	rBV2	321	283	0.04%	0.006%
96	14.018	2118	2121	2123	rBV2	193	187	0.03%	0.004%
97	14.128	2134	2139	2143	rVB	1179	1669	0.26%	0.033%
98	14.262	2159	2161	2162	rVB	171	90	0.01%	0.002%
99	15.383	2343	2345	2352	rVB3	1371	2342	0.36%	0.046%
100	16.292	2493	2494	2496	rBV2	491	389	0.06%	0.008%




Sum of corrected areas: 5054852

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072224\
Data File : VX042437.D
Acq On : 22 Jul 2024 10:24
Operator : JC/MD
Sample : P3277-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E1ZR6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

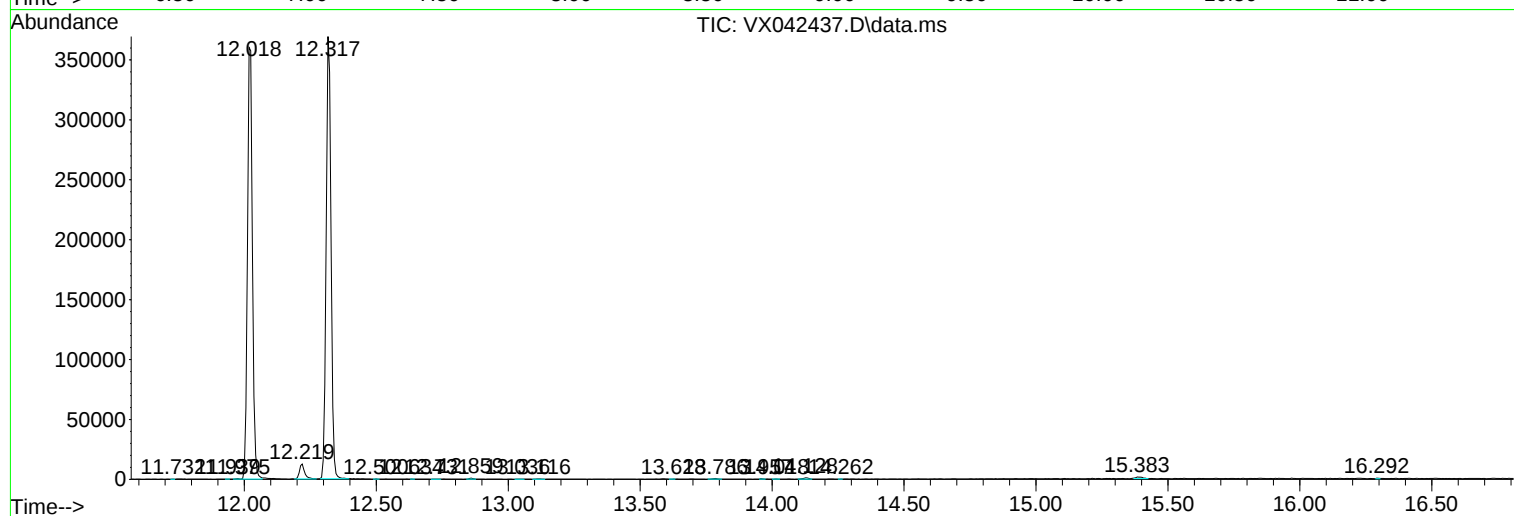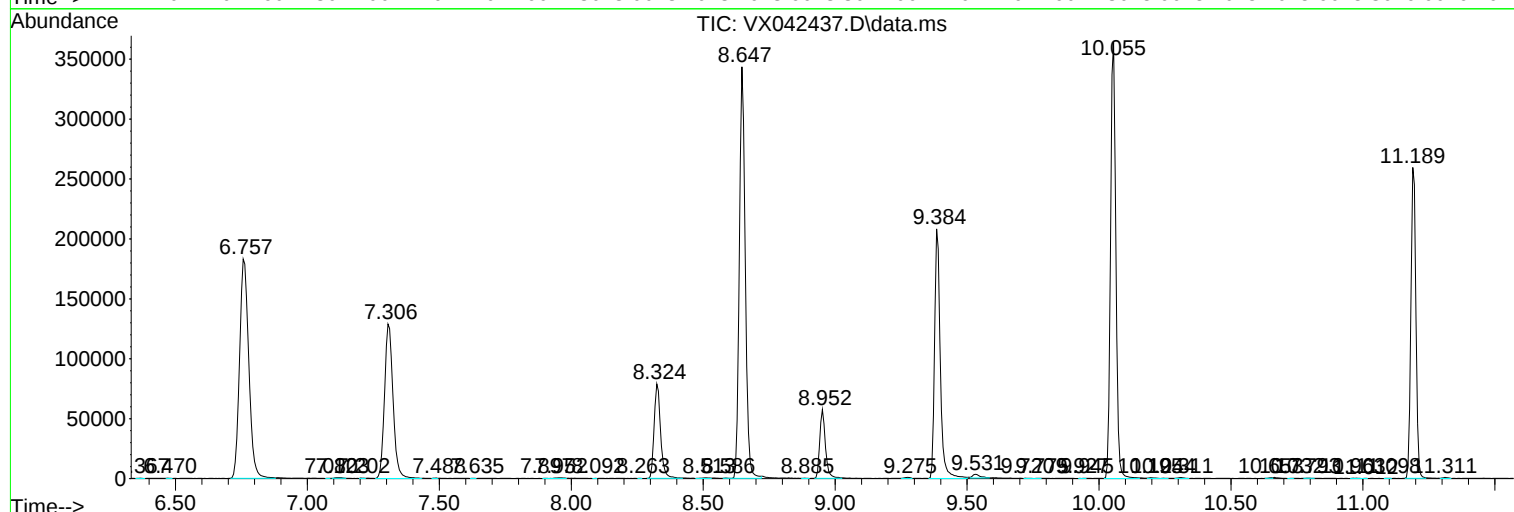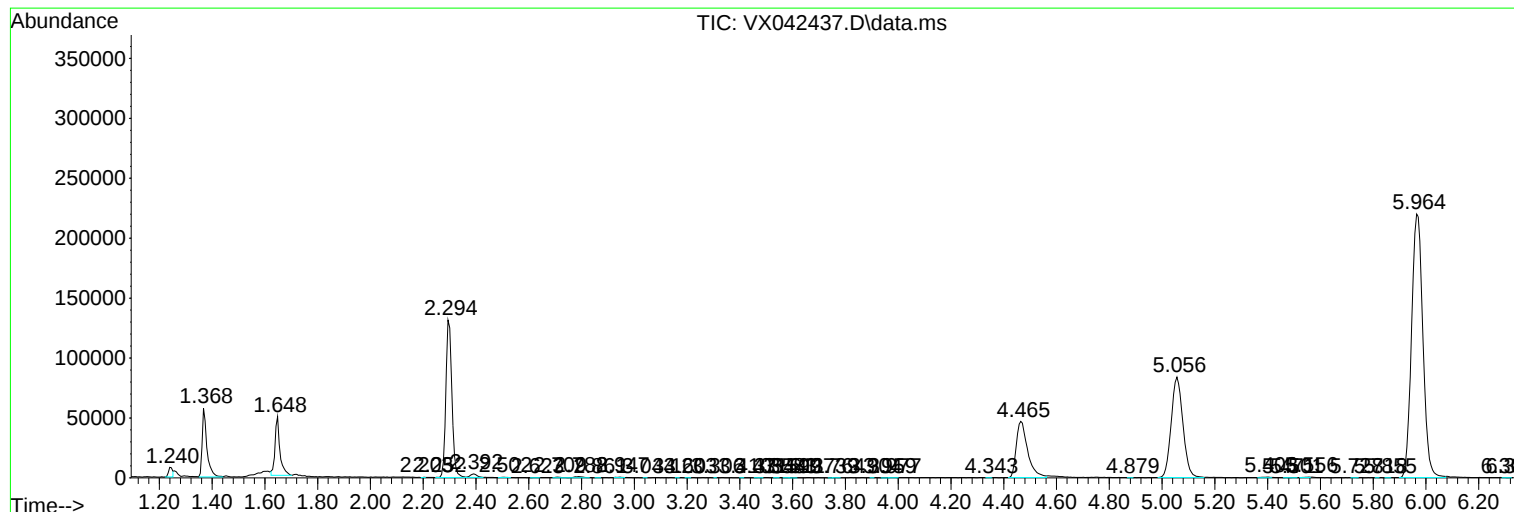

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072224\
Data File : VX042437.D
Acq On : 22 Jul 2024 10:24
Operator : JC/MD
Sample : P3277-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E1ZR6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072224\
Data File : VX042437.D
Acq On : 22 Jul 2024 10:24
Operator : JC/MD
Sample : P3277-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E1ZR6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc