

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072224\
 Data File : VX042438.D
 Acq On : 22 Jul 2024 10:47
 Operator : JC/MD
 Sample : P3277-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E1ZS8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M

Title : VOC Analysis

Signal : TIC: VX042438.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	33	rBV2	8814	14821	2.15%	0.277%
2	1.368	43	46	58	rBV	55554	70774	10.28%	1.324%
3	1.569	71	79	80	rBV4	2942	5747	0.83%	0.107%
4	1.648	88	92	102	rVB	47381	64968	9.43%	1.215%
5	2.294	192	198	208	rBV	133574	206455	29.98%	3.861%
6	2.398	210	215	220	rVB	3153	5661	0.82%	0.106%
7	2.611	249	250	255	rVB2	153	203	0.03%	0.004%
8	2.648	255	256	258	rBV	168	115	0.02%	0.002%
9	2.788	274	279	286	rVB3	970	1910	0.28%	0.036%
10	2.849	286	289	290	rBV2	129	99	0.01%	0.002%
11	2.947	298	305	313	rBV	2960	6593	0.96%	0.123%
12	3.190	343	345	347	rBV2	154	166	0.02%	0.003%
13	3.245	352	354	355	rVV	113	91	0.01%	0.002%
14	3.276	357	359	362	rVB	117	108	0.02%	0.002%
15	3.404	379	380	382	rBV	145	136	0.02%	0.003%
16	3.459	387	389	393	rVV	122	160	0.02%	0.003%
17	3.538	395	402	404	rBV	153	266	0.04%	0.005%
18	3.587	409	410	412	rVV	139	90	0.01%	0.002%
19	3.666	421	423	426	rBV2	111	119	0.02%	0.002%
20	3.696	426	428	431	rVB2	99	88	0.01%	0.002%
21	3.885	456	459	461	rBV2	126	127	0.02%	0.002%
22	3.952	467	470	472	rBV	96	143	0.02%	0.003%
23	4.056	485	487	488	rVB2	200	97	0.01%	0.002%
24	4.111	495	496	499	rVB2	103	81	0.01%	0.002%
25	4.154	501	503	505	rBV	101	94	0.01%	0.002%
26	4.391	540	542	543	rBV	125	86	0.01%	0.002%
27	4.465	546	554	570	rBV	49057	148932	21.63%	2.785%
28	4.879	620	622	626	rVB	136	170	0.02%	0.003%
29	5.056	639	651	668	rBV	87035	268927	39.05%	5.029%
30	5.397	700	707	715	rBV3	804	2074	0.30%	0.039%
31	5.556	727	733	740	rVB3	804	2016	0.29%	0.038%
32	5.611	740	742	745	rVB3	207	273	0.04%	0.005%
33	5.635	745	746	748	rBV	156	138	0.02%	0.003%
34	5.970	789	801	819	rBV2	233345	688683	100.00%	12.879%
35	6.312	855	857	858	rBV	201	111	0.02%	0.002%
36	6.373	865	867	872	rVV2	220	272	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072224\
 Data File : VX042438.D
 Acq On : 22 Jul 2024 10:47
 Operator : JC/MD
 Sample : P3277-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E1ZS8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

37	6.550	895	896	900	rBV2	133	179	0.03%	0.003%
38	6.763	921	931	952	rBV	196838	482102	70.00%	9.016%
39	7.117	984	989	992	rBV4	687	1248	0.18%	0.023%
40	7.306	1012	1020	1037	rBV	136389	304639	44.24%	5.697%
41	7.488	1047	1050	1054	rVB2	271	441	0.06%	0.008%
42	7.952	1122	1126	1127	rBV2	596	795	0.12%	0.015%
43	8.110	1149	1152	1154	rVB2	140	170	0.02%	0.003%
44	8.171	1159	1162	1163	rBV2	105	117	0.02%	0.002%
45	8.324	1181	1187	1200	rBV	83184	139000	20.18%	2.600%
46	8.415	1200	1202	1208	rVB2	500	609	0.09%	0.011%
47	8.647	1234	1240	1257	rBV	353391	562739	81.71%	10.524%
48	8.952	1285	1290	1305	rBV	59587	90123	13.09%	1.685%
49	9.232	1334	1336	1337	rBV2	106	82	0.01%	0.002%
50	9.275	1338	1343	1348	rVB2	1757	2471	0.36%	0.046%
51	9.384	1356	1361	1378	rBV	215019	328794	47.74%	6.149%
52	9.537	1381	1386	1394	rVV5	3062	6545	0.95%	0.122%
53	9.842	1434	1436	1438	rBV2	141	115	0.02%	0.002%
54	10.055	1465	1471	1483	rBV	406951	553648	80.39%	10.354%
55	10.311	1508	1513	1517	rBV3	536	923	0.13%	0.017%
56	10.561	1552	1554	1557	rBV	85	92	0.01%	0.002%
57	10.622	1562	1564	1565	rBV	166	93	0.01%	0.002%
58	10.646	1565	1568	1569	rBV2	441	411	0.06%	0.008%
59	10.781	1586	1590	1591	rBV	209	196	0.03%	0.004%
60	10.866	1602	1604	1607	rVB2	199	214	0.03%	0.004%
61	10.933	1613	1615	1617	rBV2	105	116	0.02%	0.002%
62	11.189	1652	1657	1668	rBV	272589	358562	52.06%	6.706%
63	11.317	1674	1678	1682	rVB	1374	1768	0.26%	0.033%
64	11.421	1693	1695	1699	rVV2	121	153	0.02%	0.003%
65	11.451	1699	1700	1702	rVV2	138	112	0.02%	0.002%
66	11.488	1704	1706	1710	rVB2	179	147	0.02%	0.003%
67	11.677	1734	1737	1739	rBV	111	144	0.02%	0.003%
68	11.707	1739	1742	1743	rVV2	208	142	0.02%	0.003%
69	11.762	1747	1751	1753	rBV3	216	303	0.04%	0.006%
70	11.854	1763	1766	1768	rVB	231	195	0.03%	0.004%
71	11.872	1768	1769	1771	rBV	145	98	0.01%	0.002%
72	11.933	1777	1779	1781	rBV	160	110	0.02%	0.002%
73	11.969	1783	1785	1788	rBV2	202	186	0.03%	0.003%
74	12.024	1788	1794	1803	rBV	381133	505631	73.42%	9.456%
75	12.219	1822	1826	1833	rBV2	5843	7874	1.14%	0.147%
76	12.317	1837	1842	1856	rBV	383342	494078	71.74%	9.240%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072224\
 Data File : VX042438.D
 Acq On : 22 Jul 2024 10:47
 Operator : JC/MD
 Sample : P3277-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E1ZS8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

77	12.609	1888	1890	1892	rBV2	189	131	0.02%	0.002%
78	12.762	1913	1915	1920	rVB2	409	419	0.06%	0.008%
79	12.859	1927	1931	1936	rBV2	933	1414	0.21%	0.026%
80	12.902	1936	1938	1940	rVB2	145	97	0.01%	0.002%
81	12.987	1950	1952	1956	rVV2	122	140	0.02%	0.003%
82	13.304	2001	2004	2005	rVB2	100	85	0.01%	0.002%
83	13.378	2014	2016	2019	rVB	180	140	0.02%	0.003%
84	13.408	2019	2021	2024	rBV	170	161	0.02%	0.003%
85	13.451	2024	2028	2031	rBV2	97	155	0.02%	0.003%
86	13.591	2047	2051	2056	rVB4	440	530	0.08%	0.010%
87	13.646	2058	2060	2062	rBV2	183	158	0.02%	0.003%
88	13.689	2065	2067	2071	rVV3	381	459	0.07%	0.009%
89	13.725	2071	2073	2076	rVB2	129	118	0.02%	0.002%
90	13.756	2076	2078	2079	rVB2	162	100	0.01%	0.002%
91	13.786	2079	2083	2089	rBV2	318	681	0.10%	0.013%
92	13.829	2089	2090	2093	rBV2	192	151	0.02%	0.003%
93	13.951	2108	2110	2111	rBV	154	102	0.01%	0.002%
94	14.006	2117	2119	2122	rBV2	141	138	0.02%	0.003%
95	14.048	2125	2126	2128	rBV2	113	95	0.01%	0.002%
96	14.127	2135	2139	2144	rVB2	1130	1464	0.21%	0.027%
97	14.225	2153	2155	2156	rBV2	210	143	0.02%	0.003%
98	14.493	2197	2199	2200	rBV	164	84	0.01%	0.002%
99	14.634	2221	2222	2223	rBV	173	95	0.01%	0.002%
100	15.389	2340	2346	2352	rBV4	2328	3943	0.57%	0.074%

Sum of corrected areas: 5347162




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072224\
Data File : VX042438.D
Acq On : 22 Jul 2024 10:47
Operator : JC/MD
Sample : P3277-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E1ZS8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

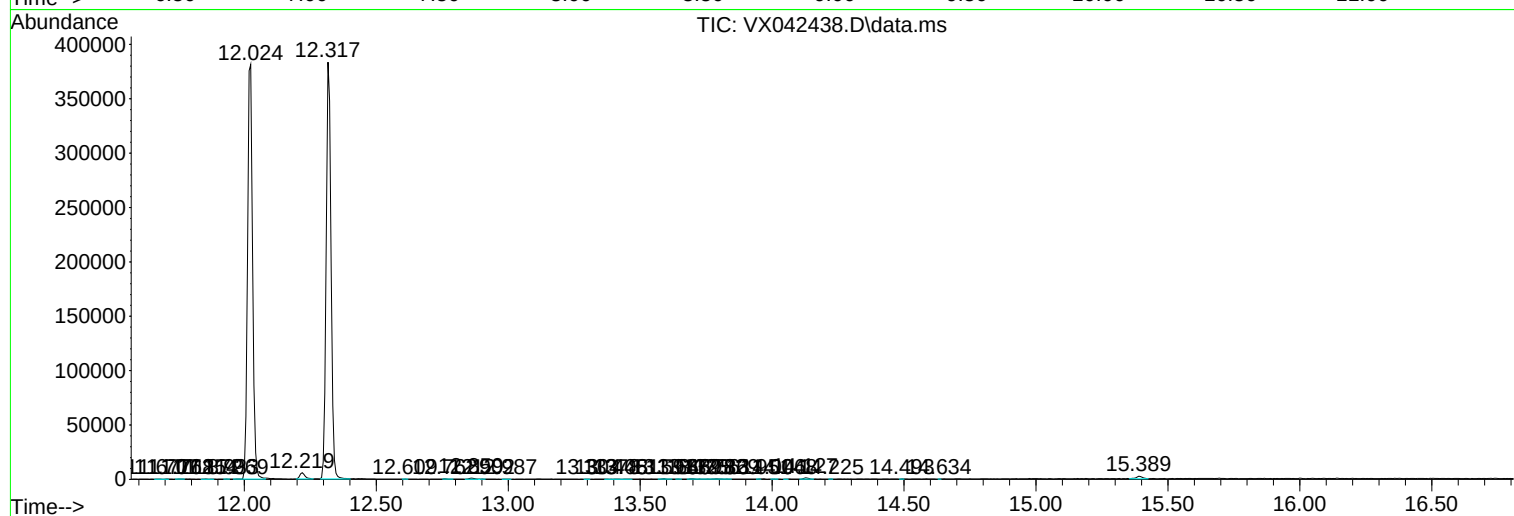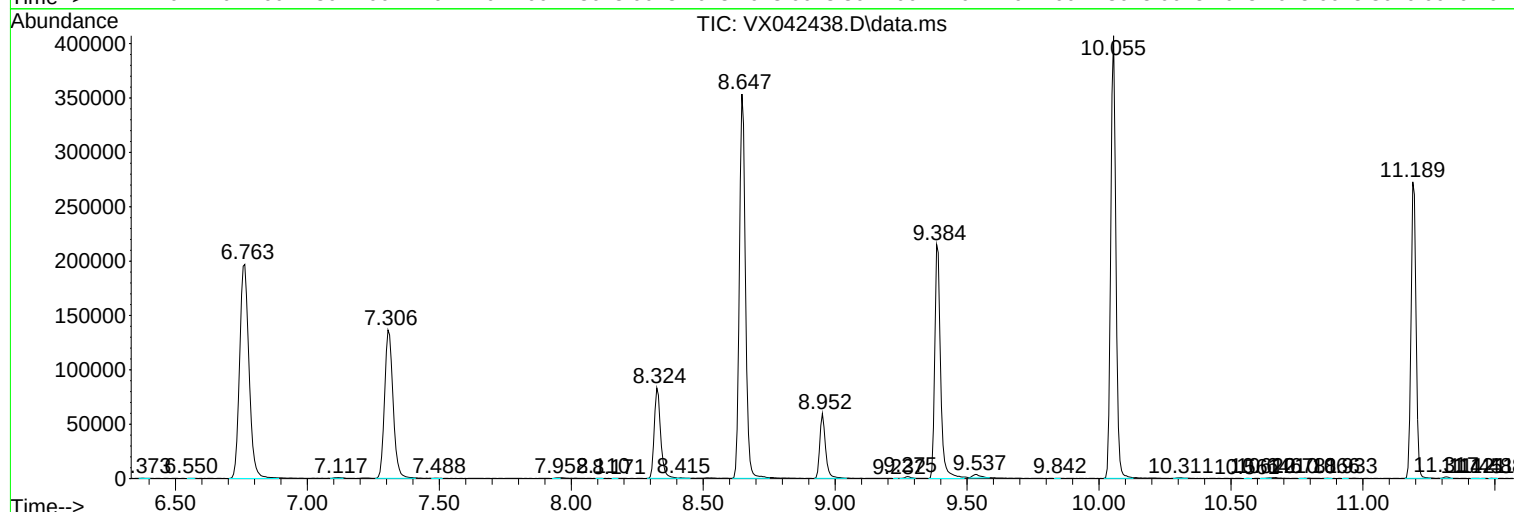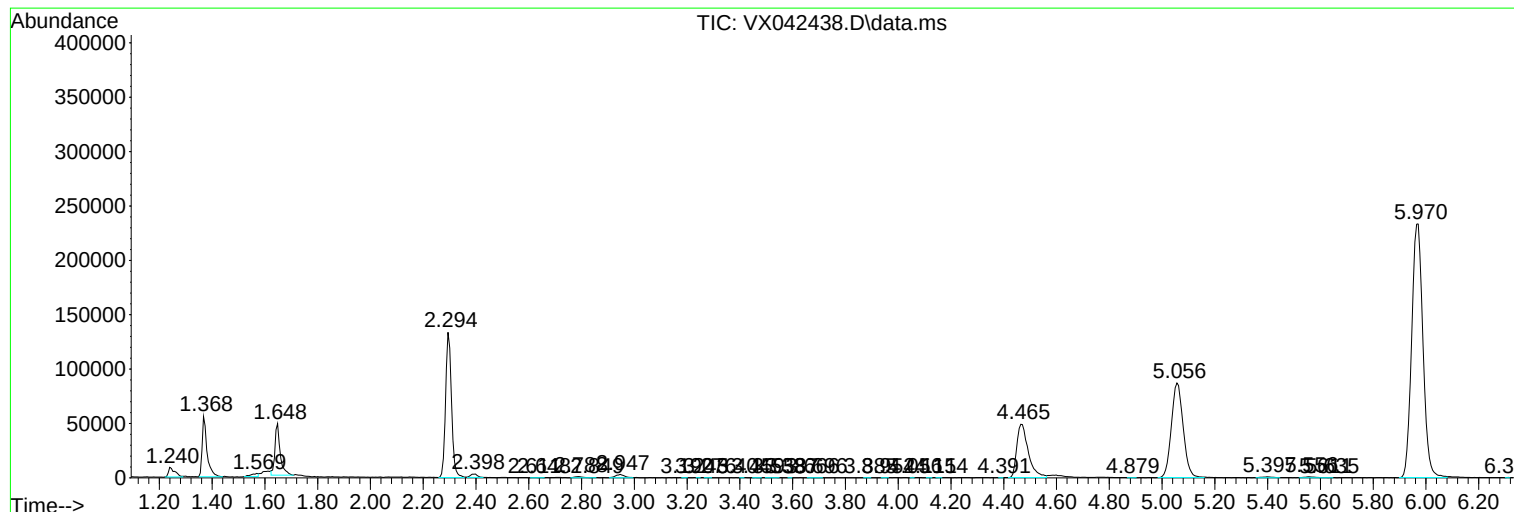

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072224\
Data File : VX042438.D
Acq On : 22 Jul 2024 10:47
Operator : JC/MD
Sample : P3277-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E1ZS8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072224\
Data File : VX042438.D
Acq On : 22 Jul 2024 10:47
Operator : JC/MD
Sample : P3277-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E1ZS8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------