

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072224\
 Data File : VX042446.D
 Acq On : 22 Jul 2024 13:54
 Operator : JC/MD
 Sample : VIBLK663
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK663

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

Signal : TIC: VX042446.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	34	rBV2	9003	15486	1.88%	0.240%
2	1.368	43	46	57	rBV	70126	89143	10.82%	1.382%
3	1.648	88	92	100	rVB	50701	69438	8.43%	1.077%
4	2.300	192	199	210	rBV	156694	253759	30.80%	3.935%
5	2.556	240	241	243	rBV	188	157	0.02%	0.002%
6	2.788	274	279	286	rVB3	1776	3445	0.42%	0.053%
7	2.947	298	305	311	rBV	1052	2427	0.29%	0.038%
8	3.002	311	314	315	rVV	130	104	0.01%	0.002%
9	3.105	330	331	332	rBV	234	142	0.02%	0.002%
10	3.282	359	360	361	rBV	174	109	0.01%	0.002%
11	3.349	369	371	372	rBV	249	147	0.02%	0.002%
12	3.379	374	376	377	rBV2	137	132	0.02%	0.002%
13	3.440	385	386	389	rBV2	169	102	0.01%	0.002%
14	3.483	391	393	394	rVB	179	106	0.01%	0.002%
15	3.666	420	423	425	rVV2	94	121	0.01%	0.002%
16	3.739	433	435	436	rBV2	171	118	0.01%	0.002%
17	3.794	441	444	447	rVV	137	164	0.02%	0.003%
18	4.300	525	527	529	rBV2	102	123	0.01%	0.002%
19	4.465	546	554	572	rBV	65577	195173	23.69%	3.027%
20	4.769	603	604	607	rBV	225	187	0.02%	0.003%
21	5.056	639	651	668	rBV	104147	319877	38.83%	4.960%
22	5.404	707	708	710	rVB	225	130	0.02%	0.002%
23	5.647	746	748	751	rBV2	214	158	0.02%	0.002%
24	5.721	756	760	761	rVB	120	118	0.01%	0.002%
25	5.861	780	783	784	rBV	198	155	0.02%	0.002%
26	5.964	789	800	819	rBV2	277525	823771	100.00%	12.774%
27	6.196	836	838	839	rVB2	197	103	0.01%	0.002%
28	6.330	859	860	865	rVB	119	112	0.01%	0.002%
29	6.373	865	867	868	rBV	153	126	0.02%	0.002%
30	6.641	909	911	913	rBV	186	107	0.01%	0.002%
31	6.690	917	919	922	rVB2	99	104	0.01%	0.002%
32	6.763	922	931	949	rBV	208630	510638	61.99%	7.918%
33	7.068	980	981	984	rBV2	155	132	0.02%	0.002%
34	7.123	984	990	1001	rVB5	3156	8393	1.02%	0.130%
35	7.196	1001	1002	1003	rBV	252	132	0.02%	0.002%
36	7.214	1003	1005	1006	rBV2	271	203	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072224\
 Data File : VX042446.D
 Acq On : 22 Jul 2024 13:54
 Operator : JC/MD
 Sample : VIBLK663
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK663

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

37	7.306	1012	1020	1042	rBV	163238	370078	44.92%	5.739%
38	7.495	1046	1051	1052	rBV2	475	598	0.07%	0.009%
39	7.543	1057	1059	1061	rVV	223	138	0.02%	0.002%
40	7.580	1061	1065	1068	rVB2	130	193	0.02%	0.003%
41	7.610	1068	1070	1071	rBV2	149	109	0.01%	0.002%
42	7.714	1084	1087	1089	rVV2	196	170	0.02%	0.003%
43	7.818	1102	1104	1106	rBV2	141	163	0.02%	0.003%
44	7.964	1122	1128	1133	rBV4	679	1611	0.20%	0.025%
45	8.257	1174	1176	1179	rBV2	132	100	0.01%	0.002%
46	8.324	1181	1187	1200	rBV	90483	160338	19.46%	2.486%
47	8.647	1234	1240	1259	rBV	412278	660845	80.22%	10.248%
48	8.952	1285	1290	1305	rBV	69674	106673	12.95%	1.654%
49	9.171	1325	1326	1330	rBV	224	215	0.03%	0.003%
50	9.275	1337	1343	1356	rVV	165586	249757	30.32%	3.873%
51	9.385	1356	1361	1383	rBV	278888	422729	51.32%	6.555%
52	9.702	1411	1413	1416	rVV	384	289	0.04%	0.004%
53	9.738	1418	1419	1423	rBV2	202	215	0.03%	0.003%
54	9.915	1446	1448	1450	rVB2	175	134	0.02%	0.002%
55	9.982	1458	1459	1461	rBV2	156	154	0.02%	0.002%
56	10.055	1465	1471	1488	rBV	458004	621246	75.41%	9.634%
57	10.189	1492	1493	1494	rVB	350	132	0.02%	0.002%
58	10.293	1507	1510	1511	rBV2	284	272	0.03%	0.004%
59	10.354	1519	1520	1524	rVB3	208	197	0.02%	0.003%
60	10.561	1553	1554	1560	rBV	137	137	0.02%	0.002%
61	10.610	1560	1562	1564	rBV2	136	142	0.02%	0.002%
62	10.793	1591	1592	1596	rBV3	154	154	0.02%	0.002%
63	10.903	1609	1610	1611	rBV	193	115	0.01%	0.002%
64	10.945	1615	1617	1618	rVV	175	114	0.01%	0.002%
65	10.976	1618	1622	1624	rVV	352	379	0.05%	0.006%
66	11.092	1640	1641	1644	rVB2	150	112	0.01%	0.002%
67	11.189	1652	1657	1671	rBV	307312	409405	49.70%	6.349%
68	11.281	1671	1672	1674	rVB	285	124	0.02%	0.002%
69	11.366	1685	1686	1690	rBV	185	149	0.02%	0.002%
70	11.512	1708	1710	1712	rVB	183	151	0.02%	0.002%
71	11.555	1714	1717	1718	rVV2	108	112	0.01%	0.002%
72	11.604	1723	1725	1727	rVB2	128	97	0.01%	0.002%
73	11.652	1731	1733	1734	rBV	186	151	0.02%	0.002%
74	11.713	1742	1743	1746	rBV	222	213	0.03%	0.003%
75	11.744	1746	1748	1751	rBV	217	216	0.03%	0.003%
76	11.927	1776	1778	1781	rVB2	123	147	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072224\
 Data File : VX042446.D
 Acq On : 22 Jul 2024 13:54
 Operator : JC/MD
 Sample : VIBLK663
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK663

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

77	11.957	1781	1783	1784	rBV	189	141	0.02%	0.002%
78	12.024	1788	1794	1806	rBV	436737	562463	68.28%	8.722%
79	12.317	1837	1842	1857	rBV	444733	578035	70.17%	8.963%
80	12.488	1869	1870	1872	rBV	172	126	0.02%	0.002%
81	12.536	1877	1878	1880	rBV	148	131	0.02%	0.002%
82	12.603	1887	1889	1892	rVB	216	166	0.02%	0.003%
83	12.628	1892	1893	1897	rBV	177	215	0.03%	0.003%
84	12.756	1912	1914	1915	rBV	311	208	0.03%	0.003%
85	12.805	1921	1922	1924	rBV	139	102	0.01%	0.002%
86	12.829	1924	1926	1929	rVV2	144	153	0.02%	0.002%
87	12.878	1932	1934	1936	rVV	157	98	0.01%	0.002%
88	12.902	1936	1938	1939	rVV	195	101	0.01%	0.002%
89	12.920	1939	1941	1944	rVB3	168	157	0.02%	0.002%
90	13.237	1991	1993	1996	rVV2	194	146	0.02%	0.002%
91	13.274	1996	1999	2000	rBV2	170	148	0.02%	0.002%
92	13.451	2024	2028	2029	rBV2	217	265	0.03%	0.004%
93	13.628	2055	2057	2060	rBV2	182	219	0.03%	0.003%
94	13.689	2064	2067	2068	rBV2	294	266	0.03%	0.004%
95	13.798	2082	2085	2089	rBV3	199	232	0.03%	0.004%
96	13.859	2094	2095	2098	rBV	156	195	0.02%	0.003%
97	13.957	2109	2111	2112	rBV	136	114	0.01%	0.002%
98	14.128	2134	2139	2145	rBV	952	1598	0.19%	0.025%
99	14.237	2156	2157	2160	rBV	233	223	0.03%	0.003%
100	14.390	2180	2182	2184	rVB	225	151	0.02%	0.002%

Sum of corrected areas: 6448769




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072224\
Data File : VX042446.D
Acq On : 22 Jul 2024 13:54
Operator : JC/MD
Sample : VIBLK663
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK663

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

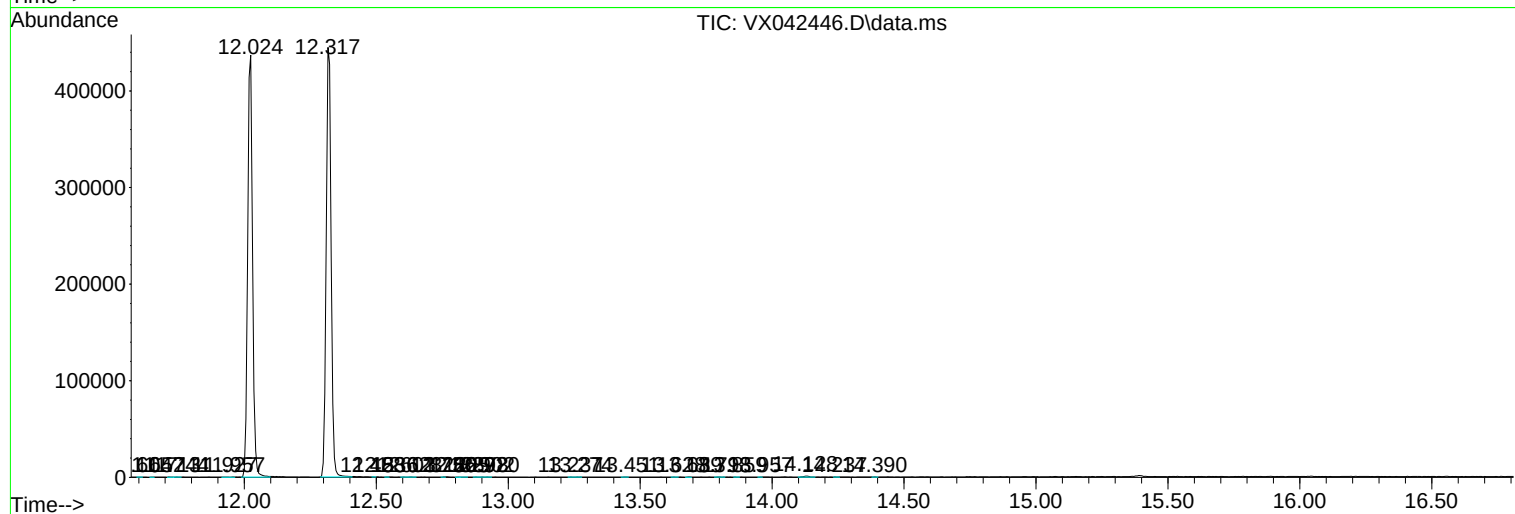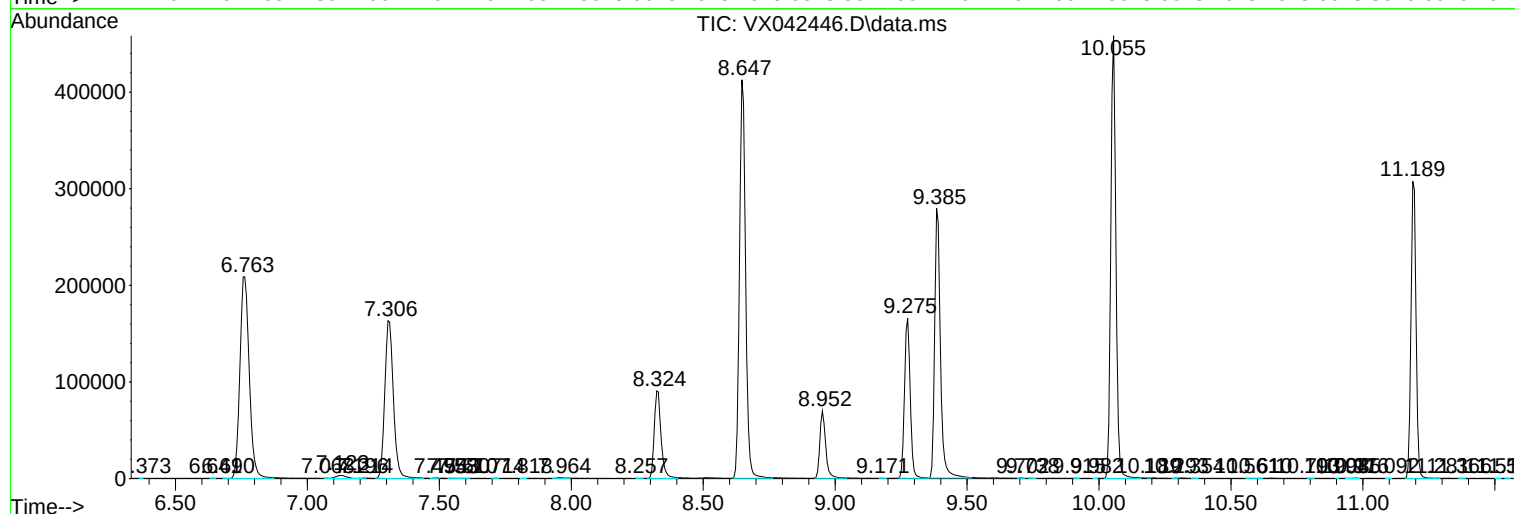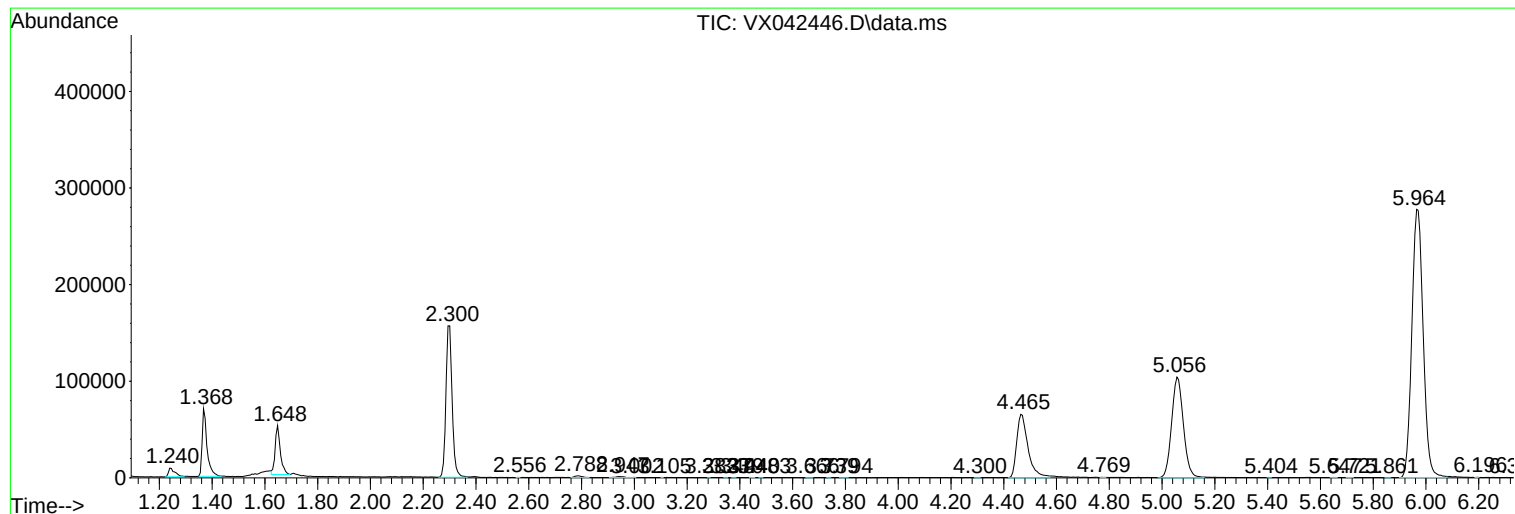

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072224\
Data File : VX042446.D
Acq On : 22 Jul 2024 13:54
Operator : JC/MD
Sample : VIBLK663
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK663

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072224\
Data File : VX042446.D
Acq On : 22 Jul 2024 13:54
Operator : JC/MD
Sample : VIBLK663
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK663

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------