
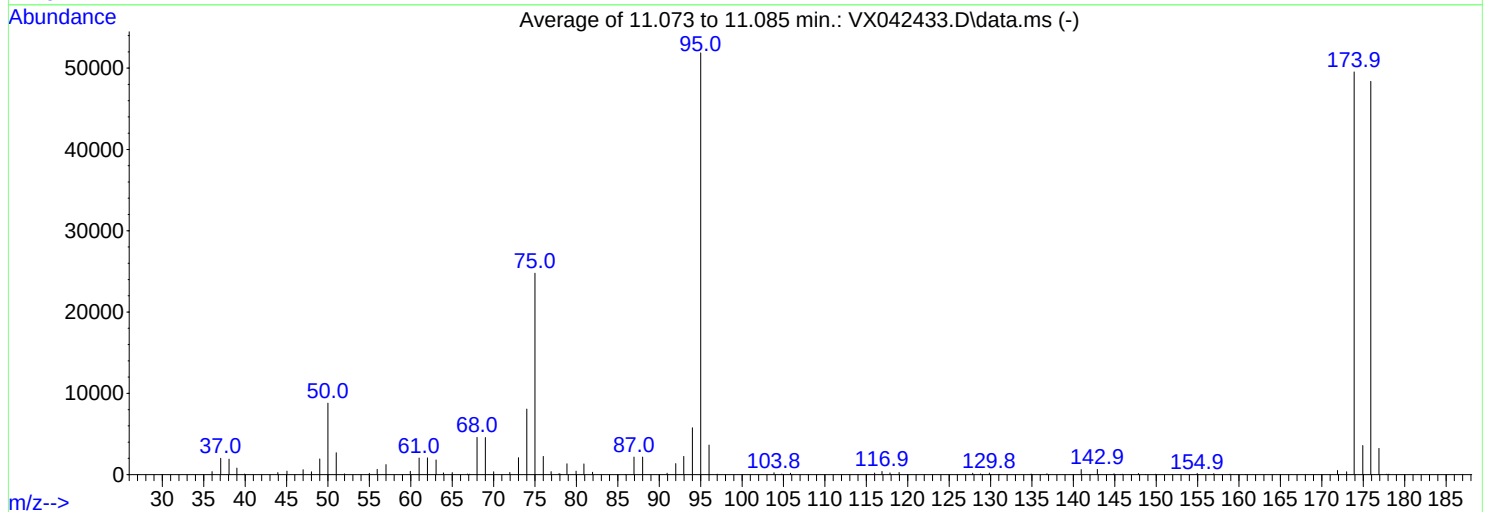


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072224\
Data File : VX042433.D
Acq On : 22 Jul 2024 07:37
Operator : JC/MD
Sample : BFB682
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB682

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM070324WMA.M
Title : VOC Analysis
Last Update : Sat Jul 20 01:45:50 2024

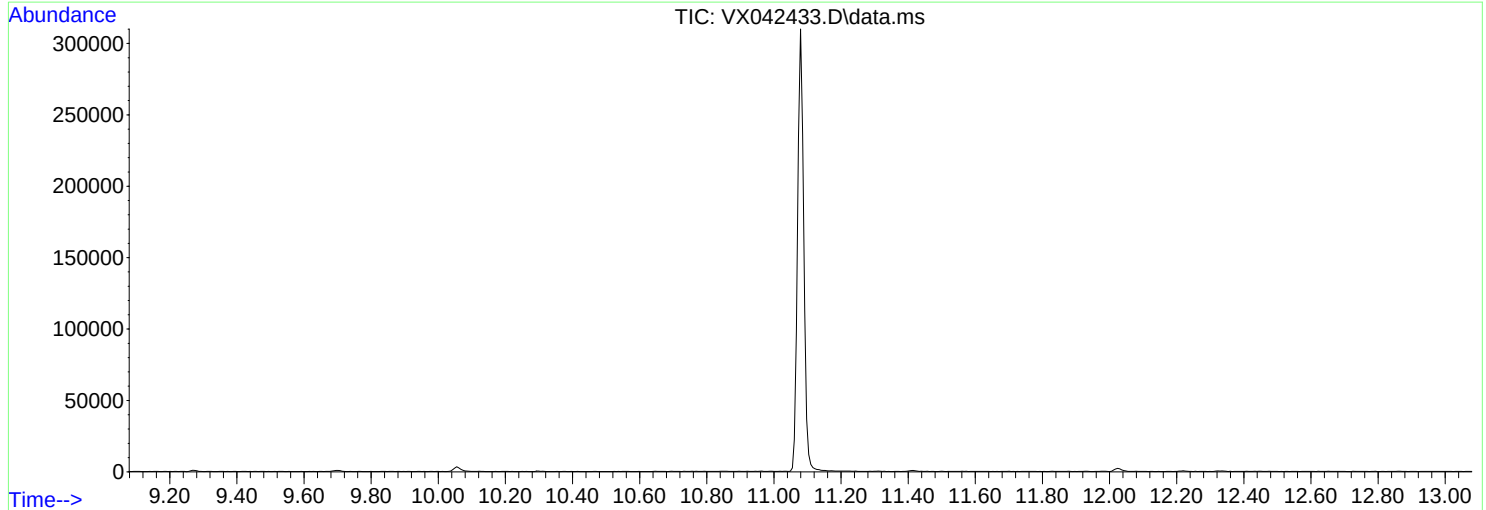

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.9	8788	PASS
75	95	30	80	47.7	24768	PASS
95	95	100	100	100.0	51880	PASS
96	95	5	9	7.0	3642	PASS
173	174	0.00	2	0.7	346	PASS
174	95	50	120	95.5	49531	PASS
175	174	5	9	7.3	3592	PASS
176	174	95	101	97.7	48376	PASS
177	176	5	9	6.7	3234	PASS

m/z	Abundance
36.00	111.0
40.00	122.0
44.10	87.0

Instrument :
MSVOA_X
ClientSampleId :
BFB682

m/z	Abundance
36.00	482.0
37.00	2149.0
38.00	2001.0
39.00	926.0
39.90	181.0
44.00	346.0
45.00	449.0
47.00	605.0
48.00	247.0
49.00	2016.0
50.00	8866.0
51.00	2945.0
52.00	106.0
55.00	228.0
56.00	633.0
57.00	1260.0
59.90	342.0
61.00	2050.0
62.00	2077.0
63.00	1736.0
64.00	217.0
65.00	335.0
66.80	110.0
68.00	4742.0
69.00	4356.0
70.00	316.0
71.90	198.0
73.00	2049.0
74.00	7849.0
75.00	24248.0
76.00	2266.0
76.90	315.0
78.00	201.0
78.90	1250.0
80.00	406.0
80.90	1238.0
82.00	302.0
86.90	2281.0
88.00	1966.0
91.00	180.0
92.00	1350.0
92.90	2026.0
94.00	5719.0
95.00	48928.0
96.00	3623.0
97.00	91.0
103.90	239.0
104.80	81.0
105.80	134.0
115.10	66.0
115.90	208.0
116.90	333.0
117.90	167.0
119.00	182.0
127.80	160.0
128.80	94.0
129.90	160.0
136.70	91.0
140.90	492.0
143.00	603.0
144.80	103.0
145.70	64.0
147.90	131.0
154.90	147.0
156.90	81.0
160.80	55.0
171.90	319.0
173.00	468.0
173.90	39664.0
175.00	3010.0
175.90	38312.0
176.90	2518.0
177.80	89.0

Instrument :
MSVOA_X
ClientSampleId :
BFB682

m/z	Abundance
36.00	550.0
37.10	2290.0
38.10	2277.0
39.00	932.0
40.00	210.0
44.00	398.0
45.10	485.0
46.00	61.0
47.00	659.0
48.10	484.0
49.00	2197.0
50.00	10600.0
51.00	3201.0
52.00	117.0
55.00	137.0
55.90	756.0
57.00	1382.0
60.00	528.0
61.00	2554.0
62.00	2625.0
63.00	2242.0
64.00	244.0
65.00	269.0
67.10	169.0
68.00	5282.0
69.00	5903.0
70.00	429.0
72.00	382.0
73.00	2433.0
74.00	9713.0
75.00	29256.0
76.00	2877.0
76.90	451.0
77.80	208.0
78.90	1612.0
79.90	570.0
80.90	1525.0
81.90	361.0
85.90	51.0
86.90	2317.0
88.00	2585.0
90.90	217.0
92.00	1567.0
93.00	2749.0
94.00	6671.0
95.00	61800.0
96.00	4213.0
97.00	106.0
103.90	220.0
104.80	104.0
105.90	231.0
115.00	74.0
116.00	229.0
116.90	480.0
117.90	284.0
118.90	368.0
127.90	230.0
128.80	187.0
129.80	194.0
131.10	58.0
134.90	133.0
136.80	131.0
141.00	755.0
142.00	91.0
142.90	730.0
144.90	115.0
145.90	110.0
147.80	187.0
149.90	62.0
153.00	50.0
155.00	191.0
157.00	185.0
158.90	65.0
171.90	644.0
173.90	59000.0
174.90	4228.0
175.90	58128.0
176.90	3847.0
178.10	151.0

Instrument :
MSVOA_X
ClientSampleId :
BFB682

m/z	Abundance
36.00	400.0
37.00	1592.0
38.10	1453.0
38.90	591.0
40.00	195.0
43.90	315.0
45.00	383.0
47.00	582.0
47.90	322.0
49.00	1591.0
50.00	6897.0
51.10	1955.0
52.10	56.0
55.10	90.0
55.90	539.0
57.00	1064.0
60.00	347.0
61.00	1555.0
62.10	1514.0
63.10	1458.0
63.90	165.0
65.00	178.0
66.90	136.0
68.00	3736.0
69.00	3427.0
70.00	351.0
72.00	261.0
73.00	1809.0
74.00	6662.0
75.00	20800.0
76.00	1574.0
77.00	342.0
78.10	151.0
78.80	1186.0
79.90	321.0
80.90	1197.0
81.90	224.0
87.00	1893.0
88.00	1923.0
90.90	129.0
92.00	1167.0
93.00	1951.0
94.00	4912.0
95.00	44912.0
96.00	3089.0
103.80	227.0
104.80	69.0
105.90	171.0
116.10	142.0
116.90	391.0
117.80	199.0
119.00	264.0
127.90	139.0
129.80	242.0
131.10	50.0
134.90	80.0
136.90	140.0
140.90	625.0
142.80	634.0
145.00	113.0
145.90	60.0
147.80	112.0
148.70	55.0
150.00	107.0
154.90	113.0
157.00	126.0
158.90	88.0
171.90	558.0
173.00	570.0
173.90	49928.0
174.90	3537.0
175.90	48688.0
176.90	3337.0
177.90	117.0

Instrument :
MSVOA_X
ClientSampleId :
BFB682