


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX072318\
Data File : VX003616.D
Acq On : 23 Jul 2018 20:56
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X071918W.M
Title : SW846 8260
Last Update : Thu Jul 19 17:09:44 2018

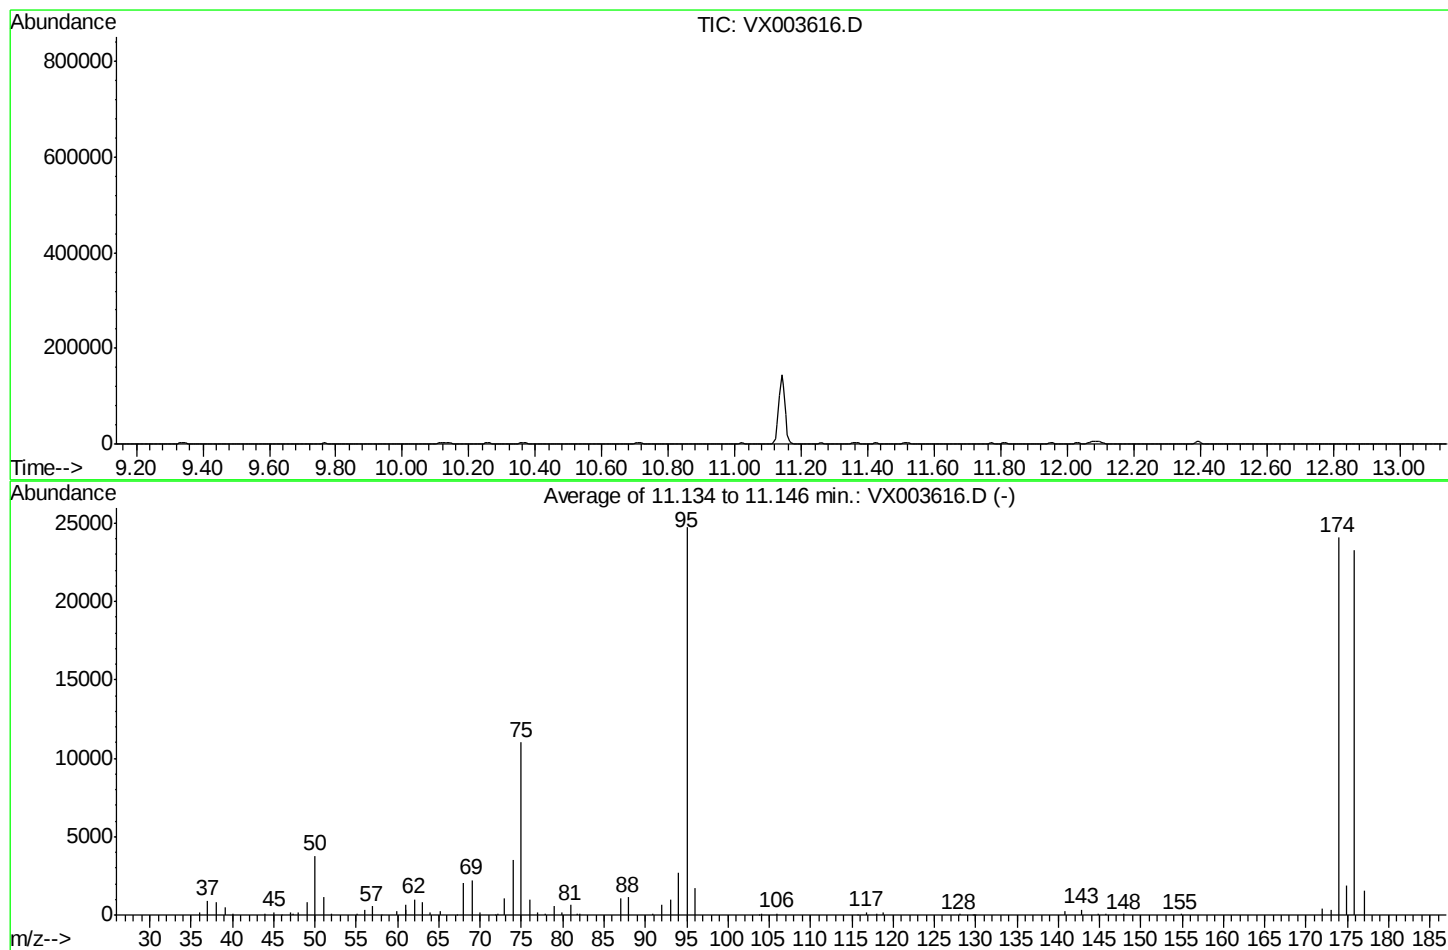

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1724

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.3	3773	PASS
75	95	30	60	44.5	11013	PASS
95	95	100	100	100.0	24730	PASS
96	95	5	9	6.9	1697	PASS
173	174	0.00	2	1.3	304	PASS
174	95	50	100	97.3	24074	PASS
175	174	5	9	7.7	1858	PASS
176	174	95	101	96.7	23290	PASS
177	176	5	9	6.6	1536	PASS