

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX072320\
 Data File : VX017521.D
 Acq On : 24 Jul 2020 03:23
 Operator : JC/SP
 Sample : PB130403ZHE#11
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 PB130403ZHE#11


Quant Time: Jul 24 06:07:20 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X072320W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jul 24 05:48:09 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.63	168	473185	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.84	114	809963	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.10	117	902266	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.06	152	452961	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.04	65	338920	55.76	ug/l	0.00
Spiked Amount			Recovery	=	111.52%	
35) Dibromofluoromethane	5.46	113	275822	50.92	ug/l	0.00
Spiked Amount			Recovery	=	101.84%	
50) Toluene-d8	8.70	98	1060237	54.25	ug/l	0.00
Spiked Amount			Recovery	=	108.50%	
62) 4-Bromofluorobenzene	11.12	95	456752	58.40	ug/l	0.00
Spiked Amount			Recovery	=	116.80%	

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) Dichlorodifluoromethane	1.18	85	183	Below Cal	#	42
3) Chloromethane	1.32	50	1163	0.564	ug/l #	42
5) Bromomethane	1.63	94	187	Below Cal	#	3
6) Chloroethane	1.72	64	364	Below Cal	#	69
8) Diethyl Ether	2.18	74	1835	Below Cal		97
11) Tert butyl alcohol	3.01	59	3244	2.532	ug/l #	81
13) Acrolein	2.28	56	626	4.778	ug/l #	6
16) Acetone	2.42	43	76226	28.493	ug/l	98
18) Methyl Acetate	2.75	43	6757	1.072	ug/l #	70
20) Methylene Chloride	2.84	84	45804	8.012	ug/l	97
25) 2-Butanone	4.64	43	14031	3.692	ug/l #	85
29) Tetrahydrofuran	5.06	42	568	0.241	ug/l #	17
36) 1,1-Dichloropropene	5.63	75	34761	4.475	ug/l #	54
38) Carbon Tetrachloride	5.63	117	47482	5.033	ug/l #	16
43) Isopropyl Acetate	6.42	43	170212	12.137	ug/l	100
48) Methyl methacrylate	7.65	41	10242	1.473	ug/l #	18
49) 1,4-Dioxane	7.72	88	137	1.028	ug/l #	22
51) 4-Methyl-2-Pentanone	8.59	43	174330	20.834	ug/l #	47
54) cis-1,3-Dichloropropene	8.59	75	70057	6.989	ug/l #	59
57) 1,3-Dichloropropane	9.52	76	12504	1.276	ug/l #	44
59) 2-Hexanone	9.52	43	190276	30.203	ug/l #	51
74) N-amyl acetate	10.80	43	9117	0.660	ug/l #	53
76) 1,2,3-Trichloropropane	11.12	75	232364	24.938	ug/l #	35
80) 1,3,5-Trimethylbenzene	11.49	105	17483	0.659	ug/l	99
81) trans-1,4-Dichloro-2-buten	11.12	75	232364	62.839	ug/l #	11
92) 1,2-Dibromo-3-Chloropropan	12.96	75	472	2.740	ug/l #	18

(#) = qualifier out of range (m) = manual integration (+) = signals summed

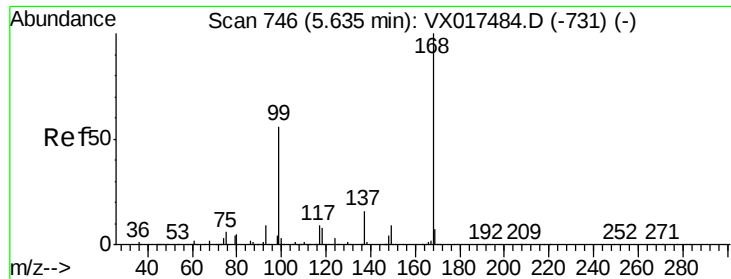

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.63 min Scan# 745

Delta R.T. -0.01 min

Lab File: VX017521.D

Acq: 24 Jul 2020 03:23

Instrument :

MSVOA_X

ClientSampleId :


PB130403ZHE#11

Tot Ion:168 Resp: 473185

Ion Ratio Lower Upper

168 100

99 58.9 43.4 65.2



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.63

150000



100000

50000

0

Time-->

5.50 5.60 5.70

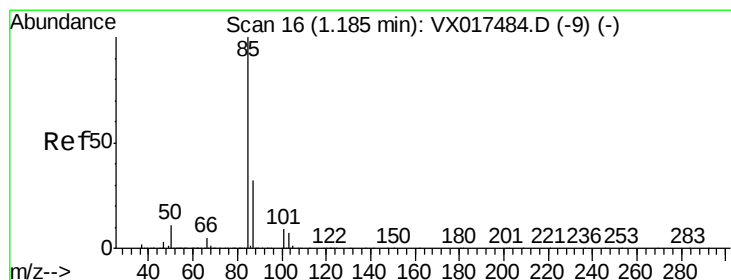

#2

Dichlorodifluoromethane

Concen: Below Cal

RT: 1.18 min Scan# 15

Delta R.T. -0.01 min

Lab File: VX017521.D


Acq: 24 Jul 2020 03:23

Tgt Ion: 85 Resp: 183

Ion Ratio Lower Upper

85 100

87 0.0 16.1 48.3#

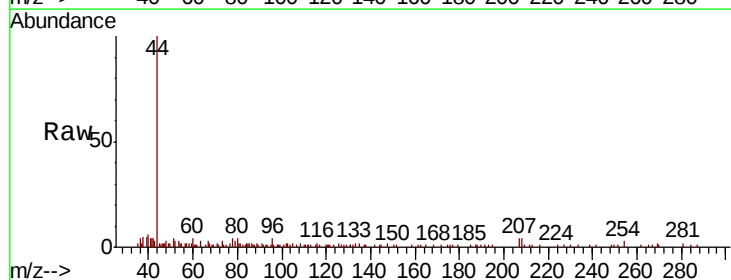

Abundance Ion 84.90 (84.60 to 85.60): VX0

Ion 86.90 (86.60 to 87.60): VX0

1.18

300


200


100

0

Time-->

1.16 1.17 1.18 1.19

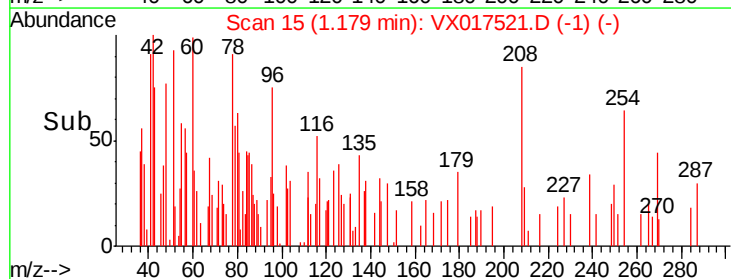

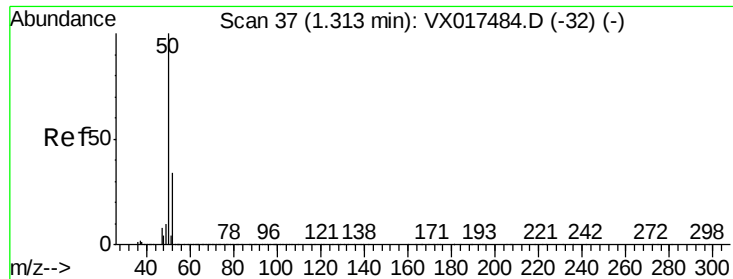

#3

Chloromethane

Concen: 0.564 ug/l

RT: 1.32 min Scan# 39

Delta R.T. 0.01 min

Lab File: VX017521.D

Acq: 24 Jul 2020 03:23

Instrument :

MSVOA_X

ClientSampleId :


PB130403ZHE#11

Tot Ion: 50 Resp: 1163

Ion Ratio Lower Upper




50 100

52 0.0 25.9 38.9#

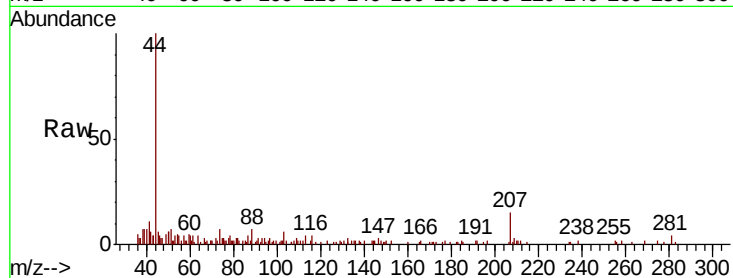

Abundance Ion 49.90 (49.60 to 50.60): VX0

Ion 51.90 (51.60 to 52.60): VX0

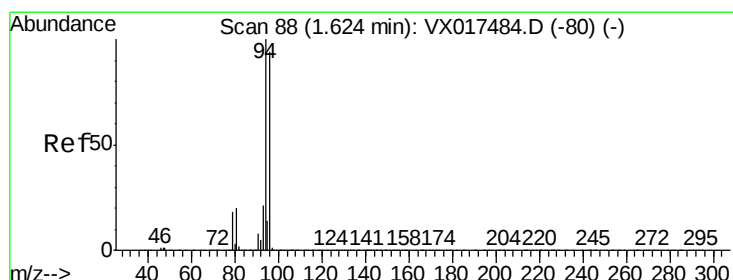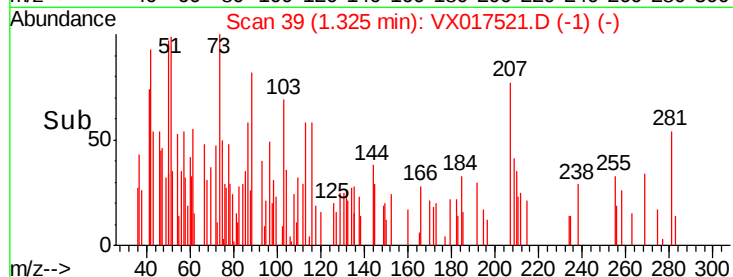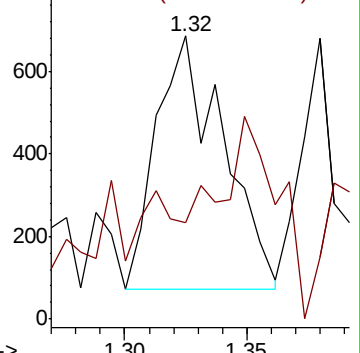

#5

Bromomethane

Concen: Below Cal

RT: 1.63 min Scan# 89

Delta R.T. 0.01 min

Lab File: VX017521.D


Acq: 24 Jul 2020 03:23

Tgt Ion: 94 Resp: 187

Ion Ratio Lower Upper



94 100


96 0.0 74.1 111.1#

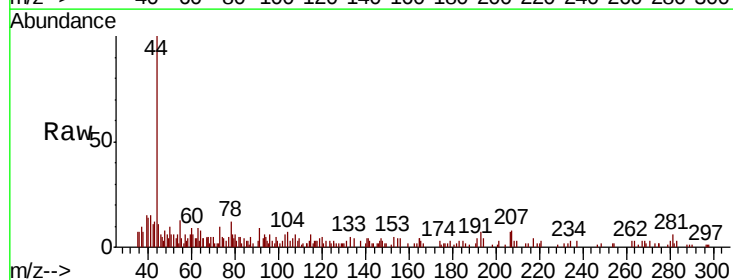

Abundance Ion 93.90 (93.60 to 94.60): VX0

Ion 95.90 (95.60 to 96.60): VX0

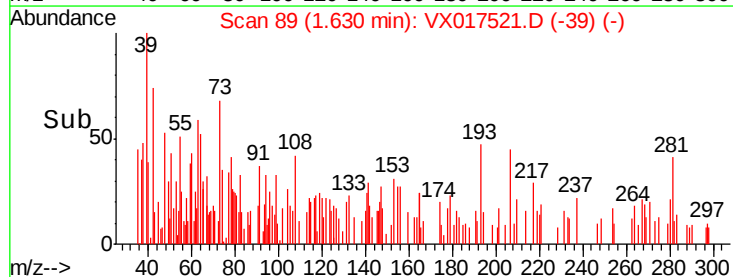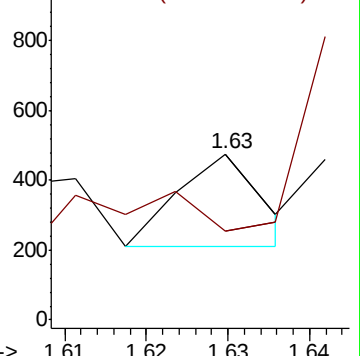



#6

Chloroethane

Concen: Below Cal

RT: 1.72 min Scan# 103

Delta R.T. 0.01 min

Lab File: VX017521.D

Acq: 24 Jul 2020 03:23

Instrument :

MSVOA_X

ClientSampleId :





PB130403ZHE#11

Tot Ion: 64 Resp: 364

Ion Ratio Lower Upper

64 100

66 48.2 24.9 37.3#

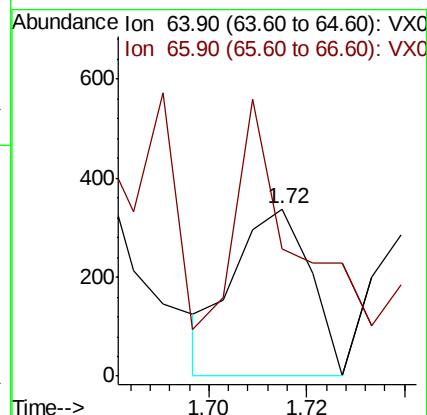

#8

Diethyl Ether

Concen: Below Cal

RT: 2.18 min Scan# 179

Delta R.T. 0.01 min

Lab File: VX017521.D




Acq: 24 Jul 2020 03:23


Tgt Ion: 74 Resp: 1835

Ion Ratio Lower Upper

74 100

45 98.6 50.8 152.5


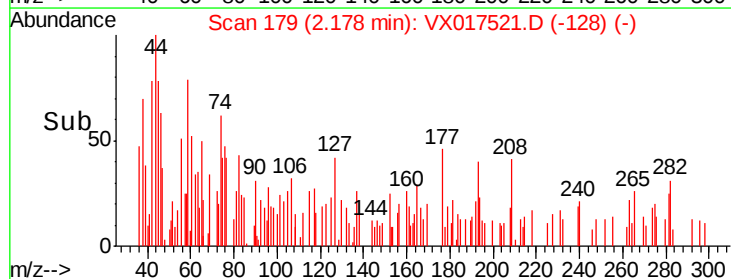
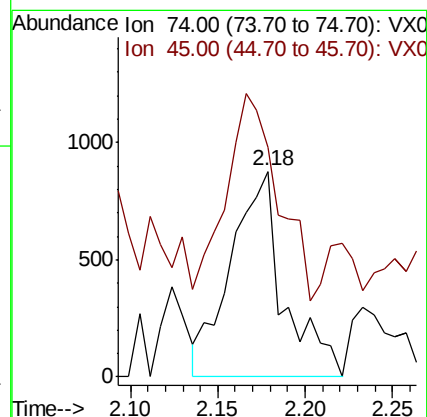





#11
Tert butyl alcohol
Concen: 2.532 ug/l
RT: 3.01 min Scan# 316
Delta R.T. -0.01 min
Lab File: VX017521.D
Acq: 24 Jul 2020 03:23




Instrument :
MSVOA_X
ClientSampleId :
PB130403ZHE#11


Tot Ion: 59 Resp: 3244
Ion Ratio Lower Upper
59 100
57 17.8 8.6 12.8#

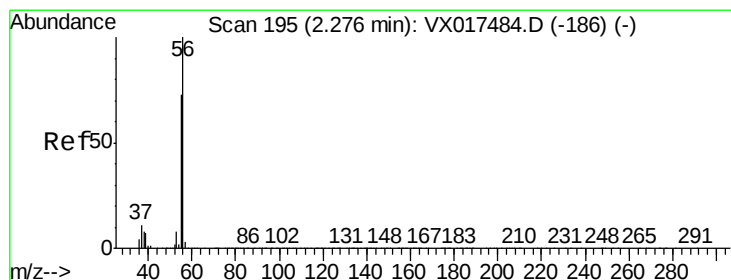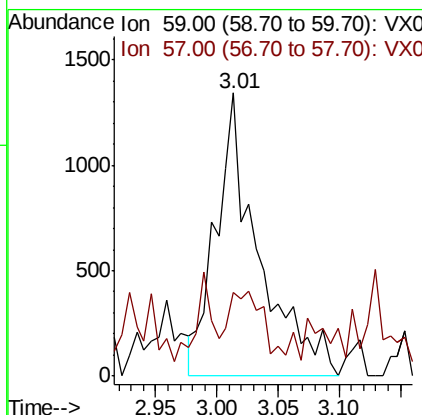

#13
Acrolein
Concen: 4.778 ug/l
RT: 2.28 min Scan# 195
Delta R.T. -0.00 min
Lab File: VX017521.D
Acq: 24 Jul 2020 03:23

Tgt Ion: 56 Resp: 626
Ion Ratio Lower Upper
56 100
55 150.3 57.4 86.2#



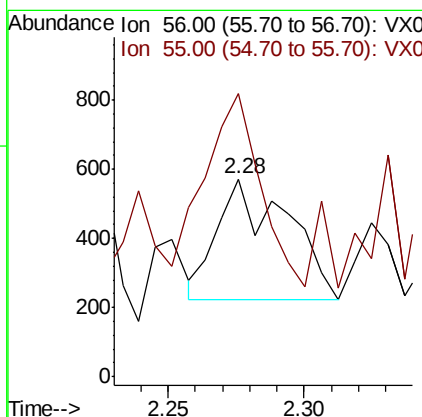



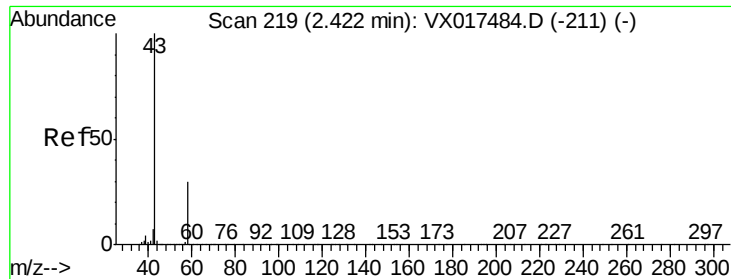

#16
Acetone
Concen: 28.493 ug/l
RT: 2.42 min Scan# 219
Delta R.T. -0.00 min
Lab File: VX017521.D
Acq: 24 Jul 2020 03:23




Instrument :
MSVOA_X
ClientSampleId :
PB130403ZHE#11


Tot Ion: 43 Resp: 76226
Ion Ratio Lower Upper
43 100
58 29.2 24.2 36.4

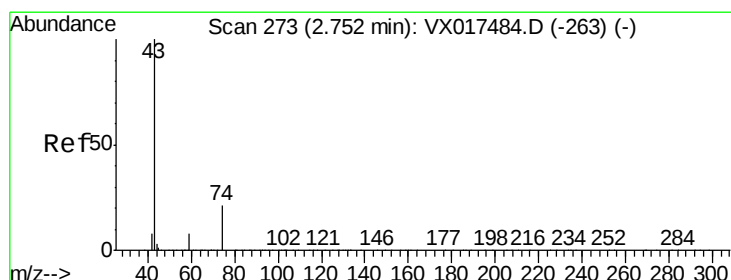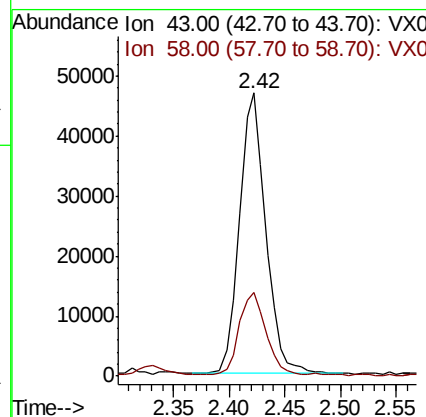

#18
Methyl Acetate
Concen: 1.072 ug/l
RT: 2.75 min Scan# 273
Delta R.T. -0.00 min
Lab File: VX017521.D
Acq: 24 Jul 2020 03:23

Tgt Ion: 43 Resp: 6757
Ion Ratio Lower Upper
43 100
74 36.3 17.5 26.3#


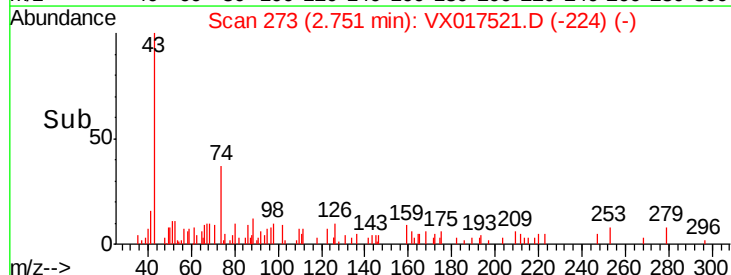
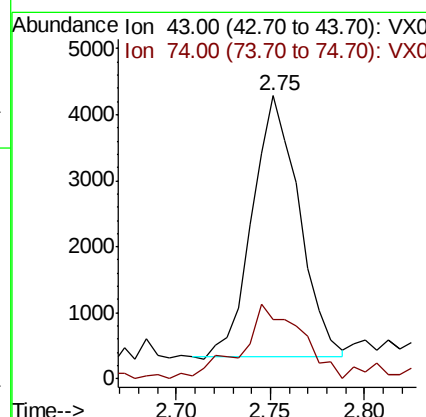





#20
Methvlene Chloride
Concen: 8.012 ug/l
RT: 2.84 min Scan# 287
Delta R.T. 0.00 min
Lab File: VX017521.D
Acq: 24 Jul 2020 03:23




Instrument :
MSVOA_X
ClientSampleId :
PB130403ZHE#11


Tot Ion: 84 Resp: 45804
Ion Ratio Lower Upper
84 100
49 128.6 100.3 150.5
51 35.0 30.5 45.7
86 63.4 51.1 76.7

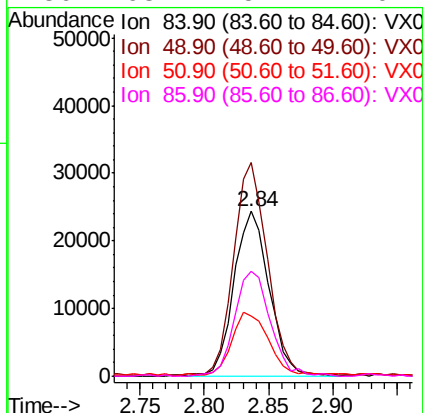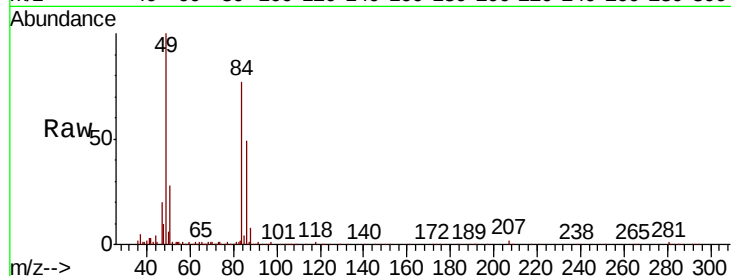

#25
2-Butanone
Concen: 3.692 ug/l
RT: 4.64 min Scan# 583
Delta R.T. -0.00 min
Lab File: VX017521.D
Acq: 24 Jul 2020 03:23

Tgt Ion: 43 Resp: 14031
Ion Ratio Lower Upper
43 100
72 31.3 19.0 28.4#

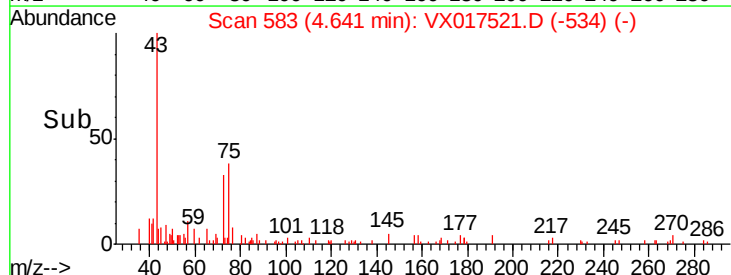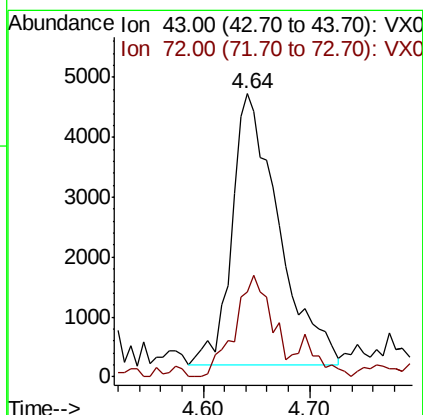

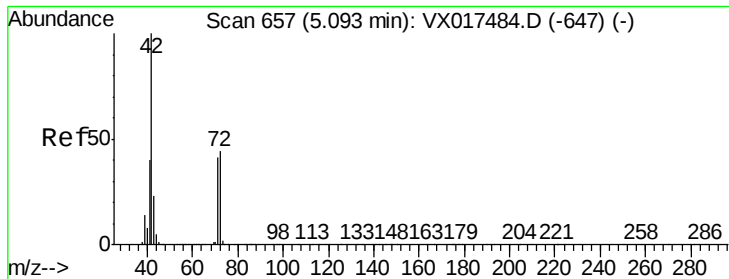

#29

Tetrahydrofuran

Concen: 0.241 ug/l

RT: 5.06 min Scan# 651

Delta R.T. -0.04 min

Lab File: VX017521.D

Acq: 24 Jul 2020 03:23

Instrument :

MSVOA_X

ClientSampleId :

PB130403ZHE#11





Tot Ion: 42 Resp: 568

Ion Ratio Lower Upper

42 100

72 108.5 35.5 53.3#

71 0.0 33.0 49.4#

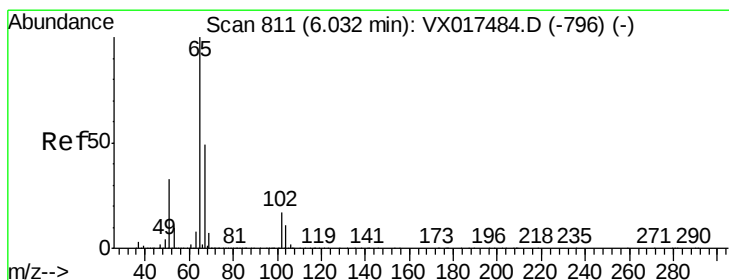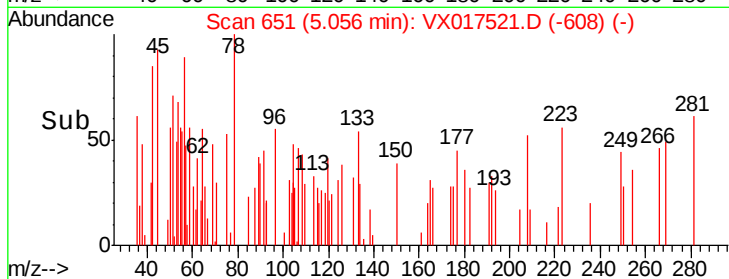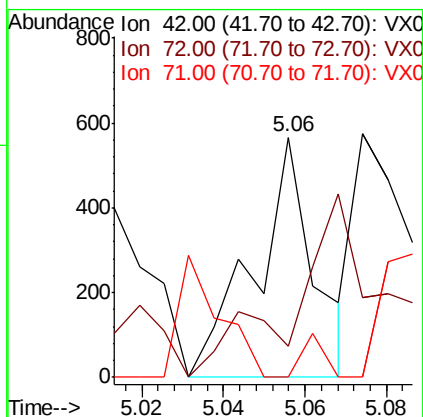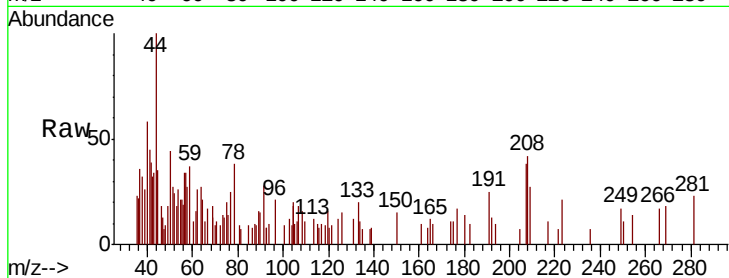

#33

1,2-Dichloroethane-d4

Concen: 55.759 ug/l

RT: 6.04 min Scan# 812

Delta R.T. 0.01 min

Lab File: VX017521.D




Acq: 24 Jul 2020 03:23


Tgt Ion: 65 Resp: 338920

Ion Ratio Lower Upper

65 100

67 50.5 0.0 102.8

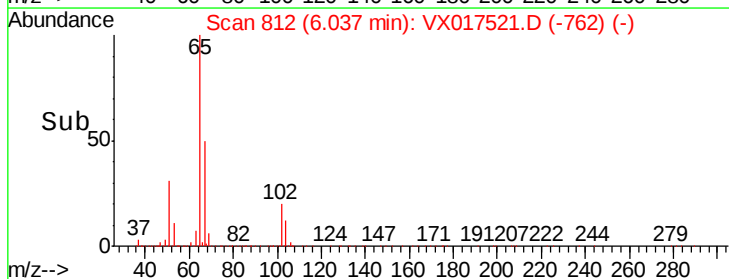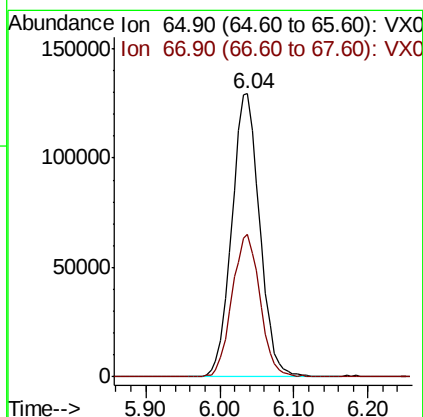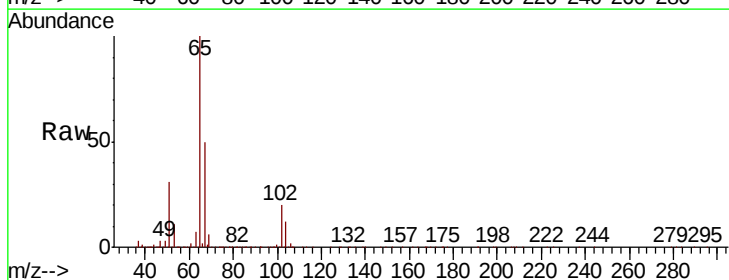



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.84 min Scan# 943

Delta R.T. 0.01 min

Lab File: VX017521.D

Acq: 24 Jul 2020 03:23

Instrument :

MSVOA_X

ClientSampleId :

PB130403ZHE#11


Tot Ion:114 Resp: 809963

Ion Ratio Lower Upper

114 100

63 19.8 0.0 40.6




88 15.3 0.0 33.4

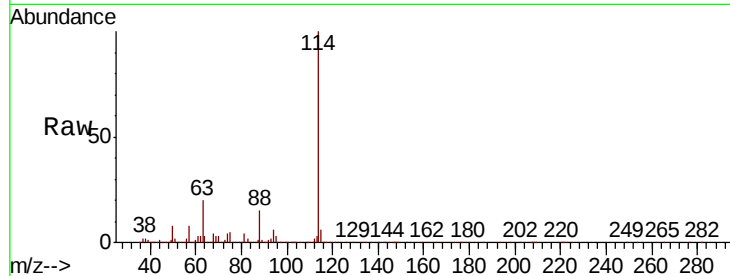

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

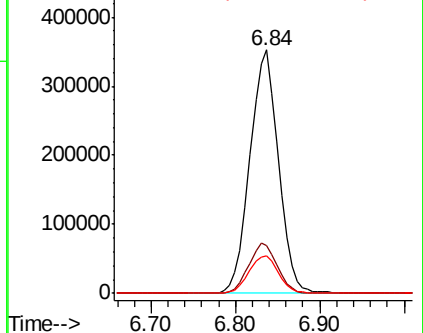

#35

Dibromofluoromethane

Concen: 50.917 ug/l

RT: 5.46 min Scan# 718

Delta R.T. -0.01 min

Lab File: VX017521.D

Acq: 24 Jul 2020 03:23


Tgt Ion:113 Resp: 275822

Ion Ratio Lower Upper

113 100

111 102.7 80.7 121.1



192 20.8 16.9 25.3




Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

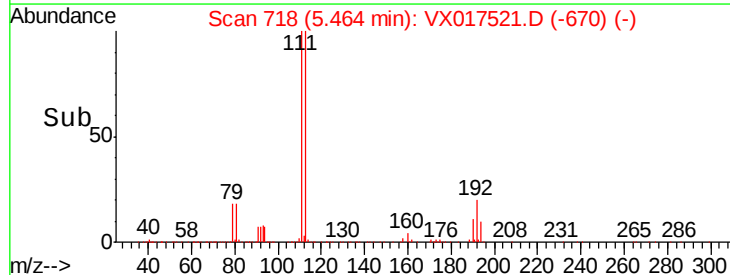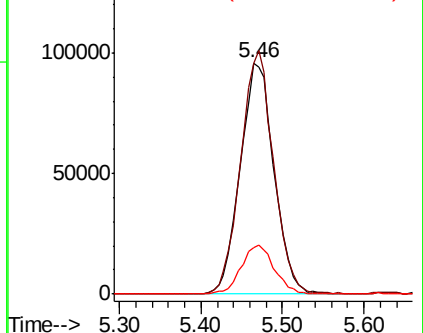

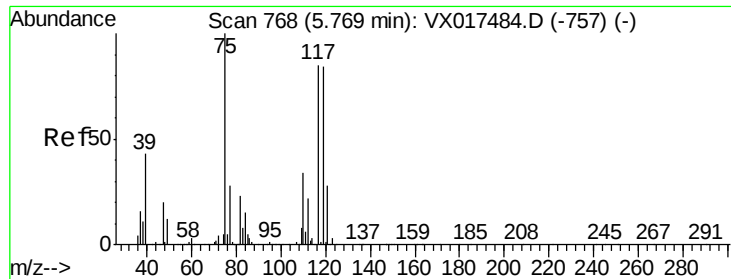

#36

1,1-Dichloropropene

Concen: 4.475 ug/l

RT: 5.63 min Scan# 745

Delta R.T. -0.14 min

Lab File: VX017521.D

Acq: 24 Jul 2020 03:23

Instrument :

MSVOA_X

ClientSampleId :

PB130403ZHE#11


Tot Ion: 75 Resp: 34761

Ion Ratio Lower Upper

75 100

110 12.9 18.1 54.3#




77 1.4 24.6 37.0#

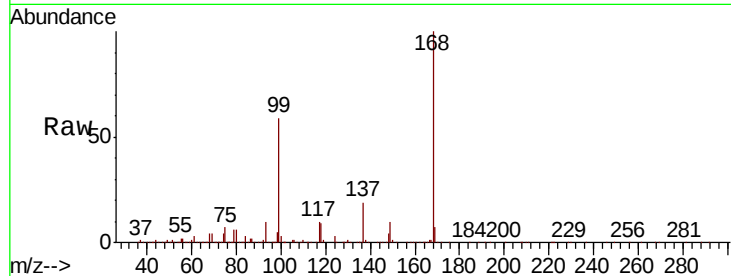

Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 109.90 (109.60 to 110.60): V

Ion 76.90 (76.60 to 77.60): VX0

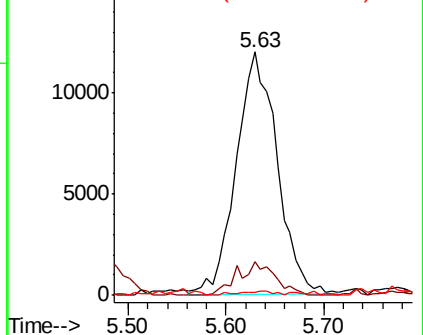

#38

Carbon Tetrachloride

Concen: 5.033 ug/l

RT: 5.63 min Scan# 745

Delta R.T. -0.13 min

Lab File: VX017521.D

Acq: 24 Jul 2020 03:23


Tgt Ion: 117 Resp: 47482

Ion Ratio Lower Upper

117 100

119 4.7 75.4 113.0#



121 0.0 24.3 36.5#




Abundance Ion 116.80 (116.50 to 117.50): V

Ion 118.80 (118.50 to 119.50): V

Ion 120.80 (120.50 to 121.50): V

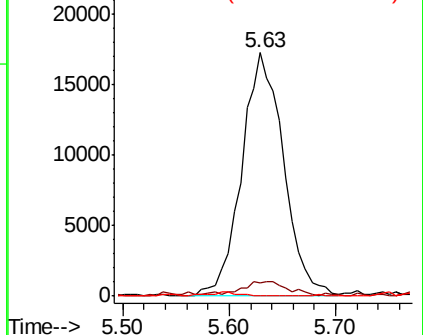







#43

Isopropyl Acetate
 Concen: 12.137 ug/l
 RT: 6.42 min Scan# 874
 Delta R.T. -0.00 min
 Lab File: VX017521.D
 Acq: 24 Jul 2020 03:23

Instrument :
 MSVOA_X
 ClientSampleId :
 PB130403ZHE#11




Tot Ion	43	Resp	170212
Ion Ratio	Lower	Upper	
43	100		
61	19.6	15.5	23.3
87	13.0	10.5	15.7

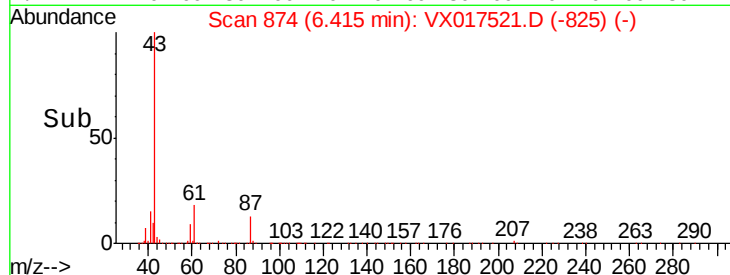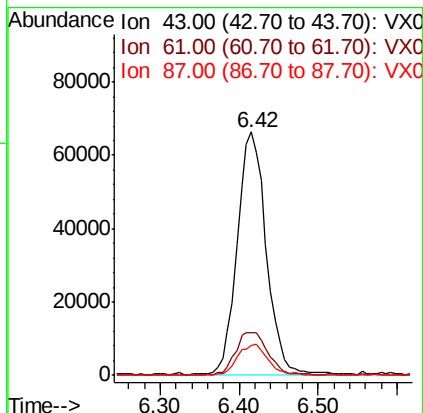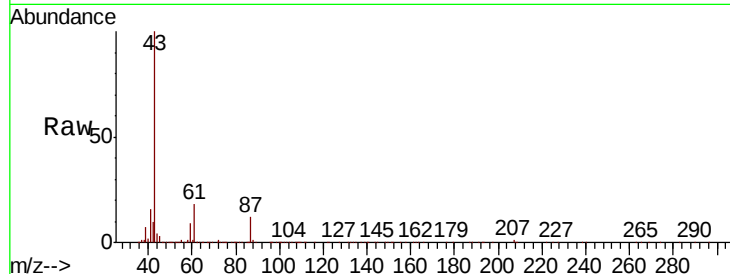


#48

Methyl methacrylate
 Concen: 1.473 ug/l
 RT: 7.65 min Scan# 1077
 Delta R.T. -0.10 min
 Lab File: VX017521.D
 Acq: 24 Jul 2020 03:23

Tgt Ion	41	Resp	10242
Ion Ratio	Lower	Upper	
41	100		
69	3.7	63.1	94.7#
39	0.0	45.1	67.7#

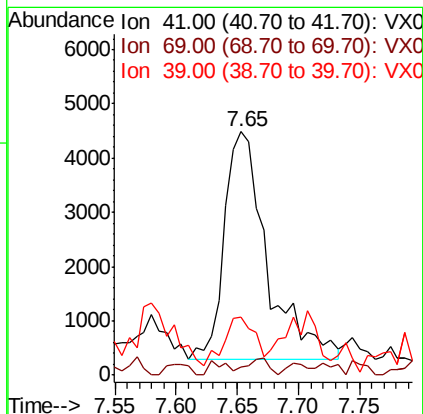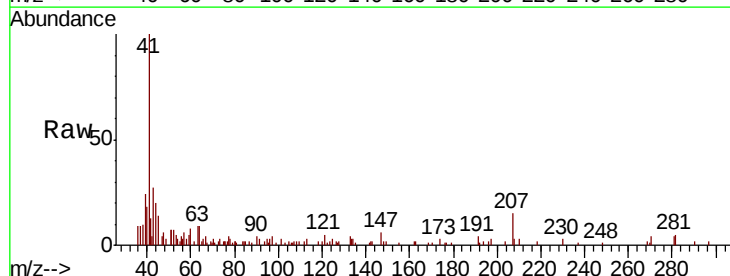

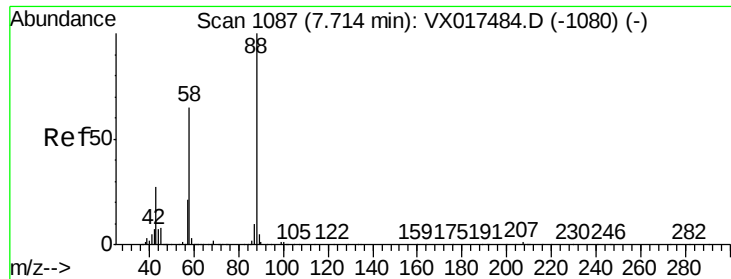

#49

1,4-Dioxane

Concen: 1.028 ug/l

RT: 7.72 min Scan# 1088

Delta R.T. 0.01 min

Lab File: VX017521.D

Acq: 24 Jul 2020 03:23

Instrument :

MSVOA_X

ClientSampleId :

PB130403ZHE#11


Tot Ion: 88 Resp: 137

Ion Ratio Lower Upper

88 100

43 0.0 27.8 41.6#




58 0.0 58.3 87.5#

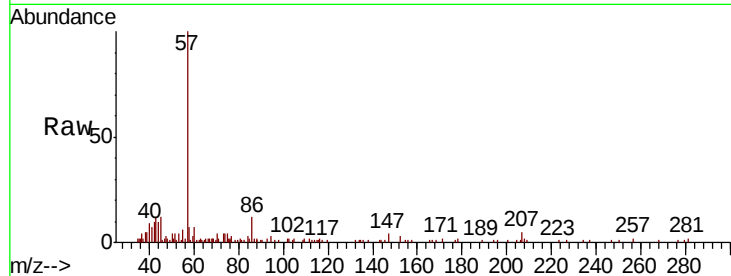

Abundance Ion 88.00 (87.70 to 88.70): VX0

Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

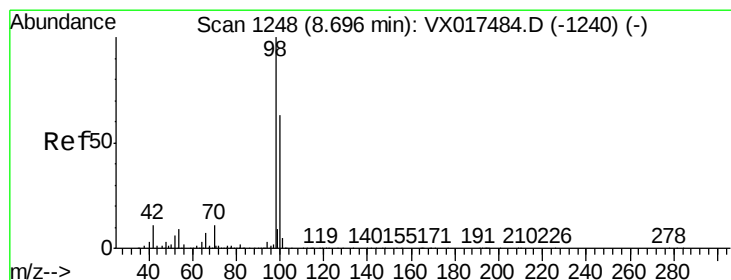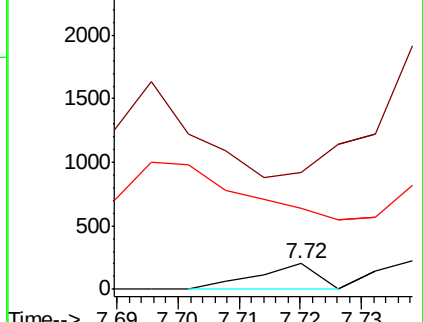

#50

Toluene-d8

Concen: 54.254 ug/l

RT: 8.70 min Scan# 1248

Delta R.T. -0.00 min

Lab File: VX017521.D


Acq: 24 Jul 2020 03:23

Tgt Ion: 98 Resp: 1060237

Ion Ratio Lower Upper



98 100


100 63.3 52.3 78.5



Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): V

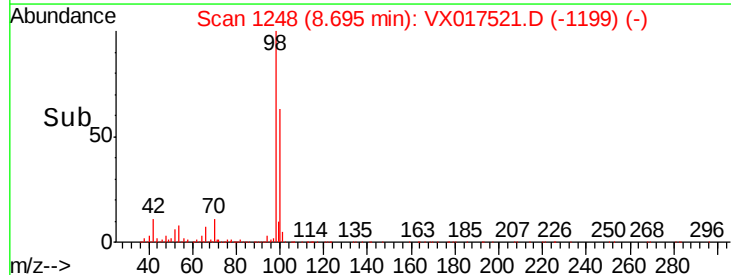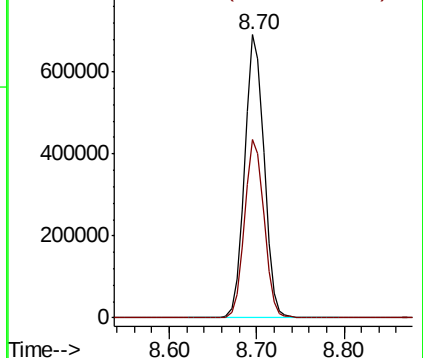



#51

4-Methyl-2-Pentanone

Concen: 20.834 ug/l

RT: 8.59 min Scan# 1231

Delta R.T. -0.03 min

Lab File: VX017521.D

Acq: 24 Jul 2020 03:23

Instrument :

MSVOA_X

ClientSampleId :





PB130403ZHE#11

Tot Ion: 43 Resp: 174330

Ion Ratio Lower Upper

43 100

58 6.3 31.0 46.4#

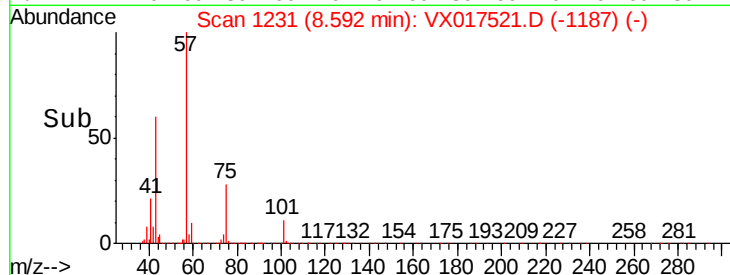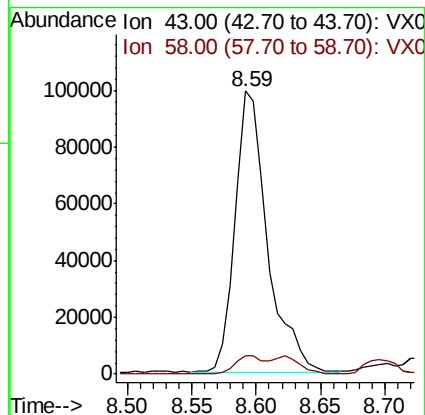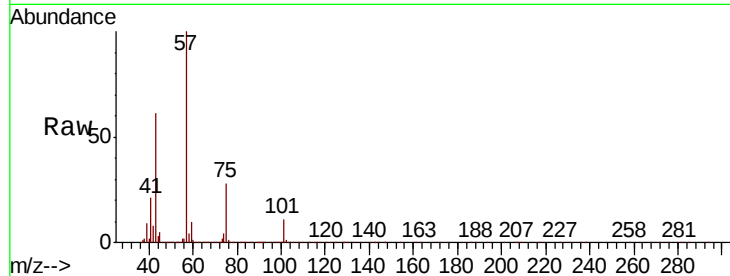

#54

cis-1,3-Dichloropropene

Concen: 6.989 ug/l

RT: 8.59 min Scan# 1231

Delta R.T. 0.18 min

Lab File: VX017521.D

Acq: 24 Jul 2020 03:23




Tgt Ion: 75 Resp: 70057


Ion Ratio Lower Upper

75 100

77 0.3 25.5 38.3#

39 30.5 41.8 62.8#

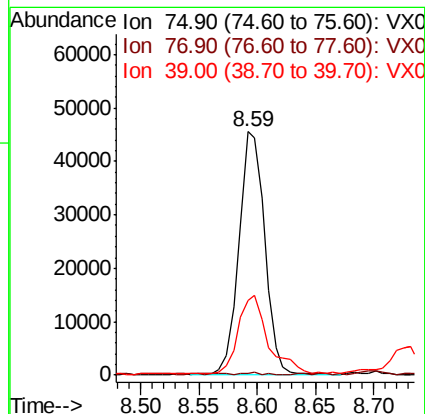

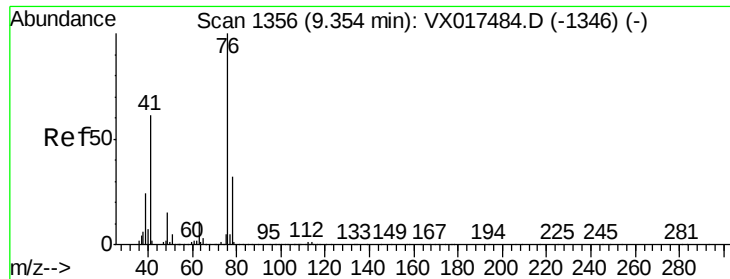

#57

1,3-Dichloropropane

Concen: 1.276 ug/l

RT: 9.52 min Scan# 1384

Delta R.T. 0.17 min

Lab File: VX017521.D

Acq: 24 Jul 2020 03:23

Instrument :

MSVOA_X

ClientSampleId :


PB130403ZHE#11

Tot Ion: 76 Resp: 12504

Ion Ratio Lower Upper




76 100

78 1.2 25.8 38.8#

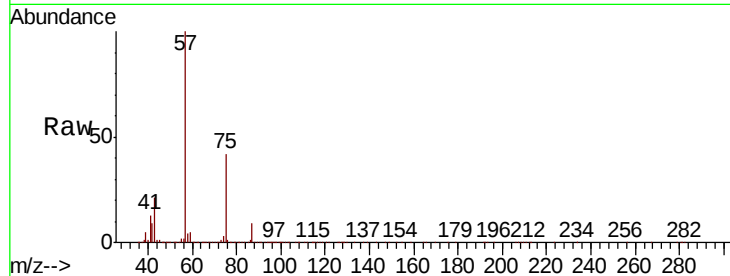

Abundance Ion 75.90 (75.60 to 76.60): VX0

Ion 77.90 (77.60 to 78.60): VX0

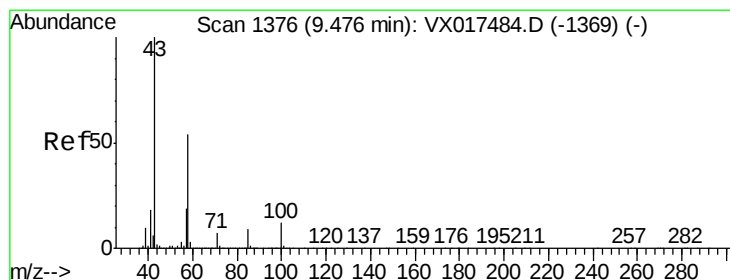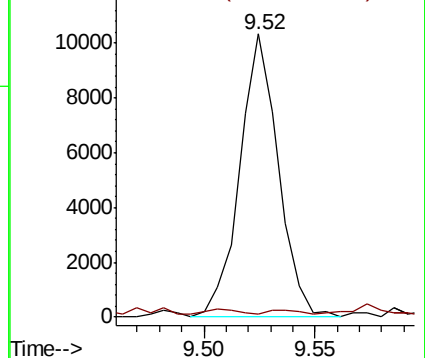

#59

2-Hexanone

Concen: 30.203 ug/l

RT: 9.52 min Scan# 1384

Delta R.T. 0.05 min

Lab File: VX017521.D


Acq: 24 Jul 2020 03:23

Tgt Ion: 43 Resp: 190276

Ion Ratio Lower Upper



43 100


58 18.2 26.6 79.8#



Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0




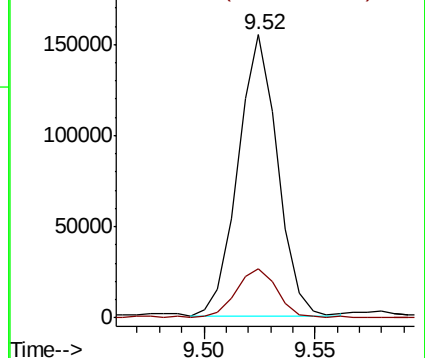




#62
4-Bromofluorobenzene
Concen: 58.403 ug/l
RT: 11.12 min Scan# 1646
Delta R.T. -0.00 min
Lab File: VX017521.D
Acq: 24 Jul 2020 03:23




Instrument :
MSVOA_X
ClientSampleId :
PB130403ZHE#11


Tot Ion	Ratio	Lower	Upper
95	100		
174	82.1	0.0	169.0
176	79.5	0.0	161.0

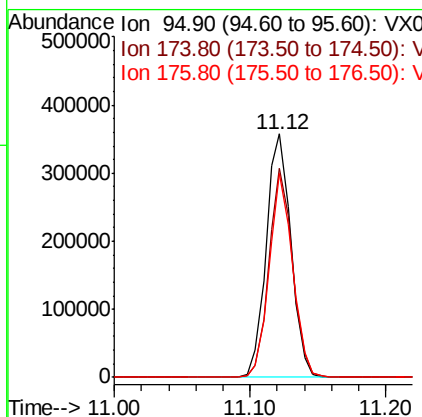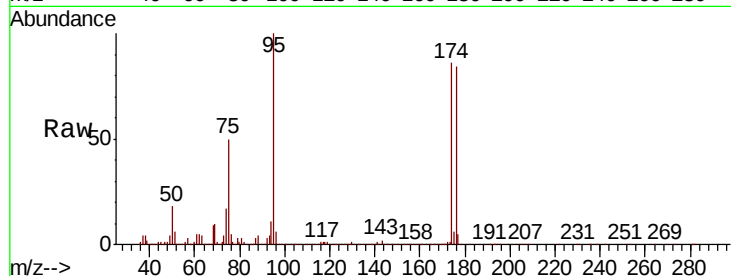

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.10 min Scan# 1478
Delta R.T. -0.00 min
Lab File: VX017521.D
Acq: 24 Jul 2020 03:23

Tgt Ion	Ratio	Lower	Upper
117	100		
82	53.6	44.0	66.0
119	31.9	25.4	38.0

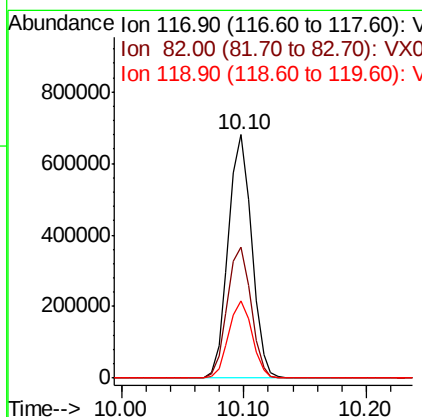



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.06 min Scan# 1800

Delta R.T. -0.00 min

Lab File: VX017521.D

Acq: 24 Jul 2020 03:23

Instrument :

MSVOA_X

ClientSampleId :

PB130403ZHE#11


Tot Ion:152 Resp: 452961

Ion Ratio Lower Upper

152 100

115 59.7 65.5 196.6#




150 158.4 0.0 412.6

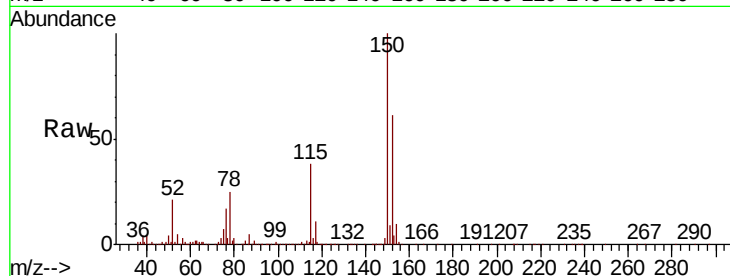

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

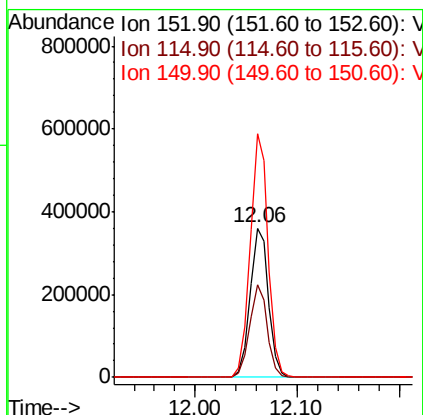

#74

N-ethyl acetate

Concen: 0.660 ug/l

RT: 10.80 min Scan# 1594

Delta R.T. -0.07 min

Lab File: VX017521.D

Acq: 24 Jul 2020 03:23

Tgt Ion: 43 Resp: 9117


Ion Ratio Lower Upper

43 100

70 1.9 32.3 48.5#

55 13.0 18.4 27.6#

61 0.0 18.6 28.0#






Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 70.00 (69.70 to 70.70): VX0

Ion 55.00 (54.70 to 55.70): VX0

Ion 61.00 (60.70 to 61.70): VX0

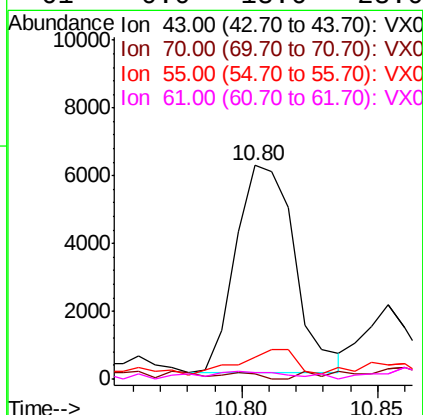

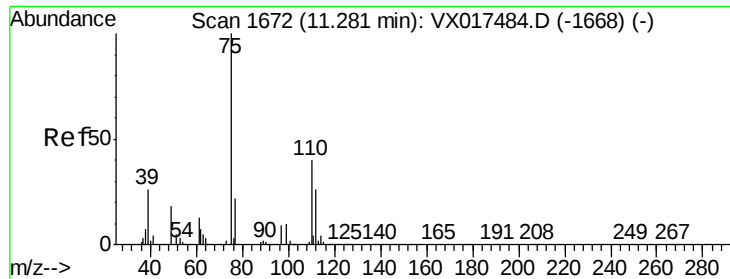

#76

1,2,3-Trichloropropane

Concen: 24.938 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. -0.16 min

Lab File: VX017521.D

Acq: 24 Jul 2020 03:23

Instrument :

MSVOA_X

ClientSampleId :


PB130403ZHE#11

Tot Ion: 75 Resp: 232364

Ion Ratio Lower Upper

75 100

77 1.4 21.8 65.3#



Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 77.00 (76.70 to 77.70): VX0

11.12

200000



150000

100000

50000

0

Time-->



#80

1,3,5-Trimethylbenzene

Concen: 0.659 ug/l

RT: 11.49 min Scan# 1707

Delta R.T. -0.00 min

Lab File: VX017521.D


Acq: 24 Jul 2020 03:23

Tgt Ion: 105 Resp: 17483

Ion Ratio Lower Upper

105 100

120 47.8 24.1 72.3



Abundance Ion 105.00 (104.70 to 105.70): V

Ion 120.00 (119.70 to 120.70): V

11.49


15000


10000

5000

0

Time-->



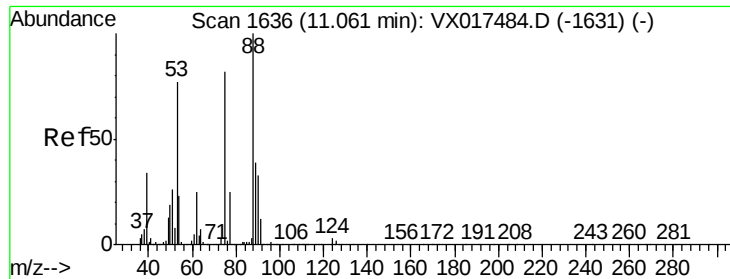

#81

trans-1,4-Dichloro-2-butene

Concen: 62.839 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. 0.06 min

Lab File: VX017521.D

Acq: 24 Jul 2020 03:23

Instrument :

MSVOA_X

ClientSampleId :

PB130403ZHE#11


Tot Ion: 75 Resp: 232364

Ion Ratio Lower Upper

75 100

53 0.2 75.9 113.9#




89 0.2 37.8 56.6#

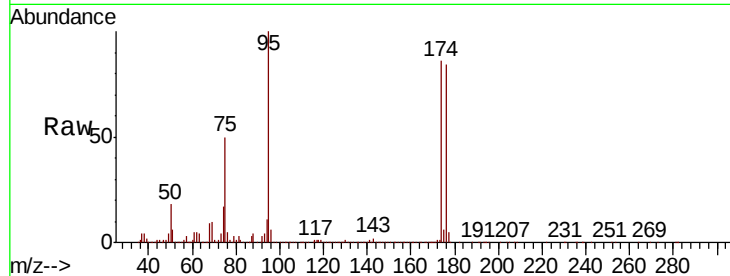

Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 53.00 (52.70 to 53.70): VX0

Ion 88.90 (88.60 to 89.60): VX0

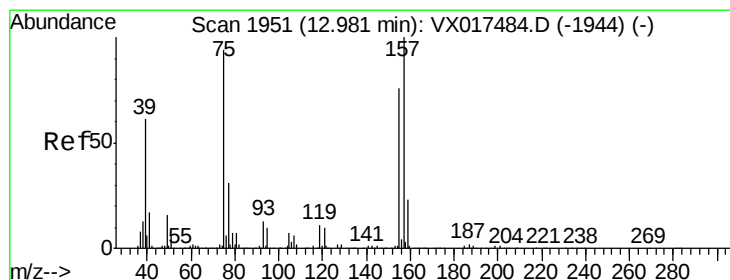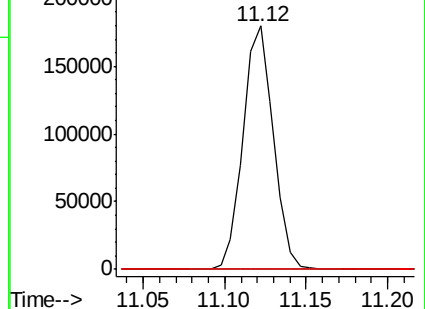

#92

1,2-Dibromo-3-Chloropropane

Concen: 2.740 ug/l

RT: 12.96 min Scan# 1948

Delta R.T. -0.02 min

Lab File: VX017521.D

Acq: 24 Jul 2020 03:23


Tgt Ion: 75 Resp: 472

Ion Ratio Lower Upper

75 100

155 8.1 42.3 126.8#

157 23.5 54.3 162.9#



Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 154.80 (154.50 to 155.50): V

Ion 156.80 (156.50 to 157.50): V

