

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\WX072320\
 Data File : VX017528.D
 Acq On : 24 Jul 2020 06:02
 Operator : JC/SP
 Sample : L3381-03
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 357-GRID-A4-A6


Quant Time: Jul 24 07:39:49 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X072320W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jul 24 05:48:09 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.64	168	476269	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.83	114	815708	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.10	117	902219	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.06	152	484611	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.03	65	334894	54.74	ug/l	0.00
Spiked Amount			Recovery	=	109.48%	
35) Dibromofluoromethane	5.46	113	280460	51.41	ug/l	0.00
Spiked Amount			Recovery	=	102.82%	
50) Toluene-d8	8.70	98	1052698	53.49	ug/l	0.00
Spiked Amount			Recovery	=	106.98%	
62) 4-Bromofluorobenzene	11.12	95	464072	58.92	ug/l	0.00
Spiked Amount			Recovery	=	117.84%	

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) Dichlorodifluoromethane	1.18	85	463	Below Cal		86
3) Chloromethane	1.31	50	606	0.469 ug/l #		87
5) Bromomethane	1.62	94	154	Below Cal #		71
6) Chloroethane	1.73	64	594	Below Cal #		73
8) Diethyl Ether	2.18	74	1369	Below Cal		70
11) Tert butyl alcohol	3.00	59	1454	1.128 ug/l		99
13) Acrolein	2.26	56	353	4.501 ug/l #		74
16) Acetone	2.42	43	44798	16.637 ug/l		93
17) Carbon Disulfide	2.55	76	3138	0.210 ug/l #		49
18) Methyl Acetate	2.75	43	6903	1.089 ug/l		91
20) Methylene Chloride	2.84	84	35099	5.785 ug/l		89
25) 2-Butanone	4.65	43	8659	2.264 ug/l #		76
29) Tetrahydrofuran	5.09	42	1498	0.632 ug/l #		82
31) Cyclohexane	5.63	56	10411	1.380 ug/l #		27
36) 1,1-Dichloropropene	5.64	75	36949	4.723 ug/l #		52
38) Carbon Tetrachloride	5.63	117	49013	5.159 ug/l #		16
43) Isopropyl Acetate	6.42	43	148845	10.539 ug/l		98
48) Methyl methacrylate	7.65	41	8869	1.267 ug/l #		18
49) 1,4-Dioxane	7.68	88	305	2.272 ug/l #		1
51) 4-Methyl-2-Pentanone	8.59	43	142086	16.861 ug/l #		47
54) cis-1,3-Dichloropropene	8.59	75	58192	5.764 ug/l #		59
57) 1,3-Dichloropropane	9.52	76	10345	1.048 ug/l #		46
59) 2-Hexanone	9.52	43	144109	22.714 ug/l #		51
74) N-amyl acetate	10.80	43	6059	0.410 ug/l #		58
76) 1,2,3-Trichloropropane	11.12	75	235578	23.632 ug/l #		35
81) trans-1,4-Dichloro-2-buten	11.12	75	235578	59.547 ug/l #		11
92) 1,2-Dibromo-3-Chloropropan	13.00	75	170	2.632 ug/l #		57

(#) = qualifier out of range (m) = manual integration (+) = signals summed

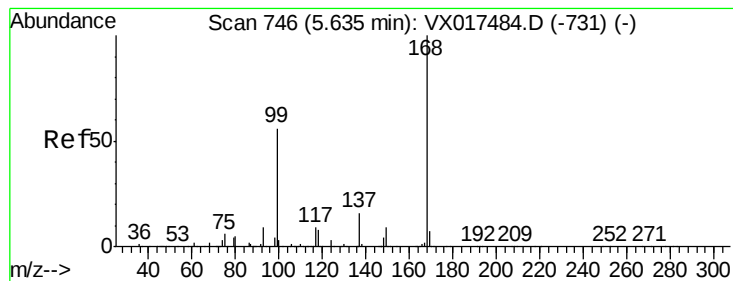

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.64 min Scan# 746

Delta R.T. -0.00 min

Lab File: VX017528.D

Acq: 24 Jul 2020 06:02

Instrument :

MSVOA_X

ClientSampleId :


357-GRID-A4-A6

Tot Ion:168 Resp: 476269

Ion Ratio Lower Upper

168 100

99 57.8 43.4 65.2

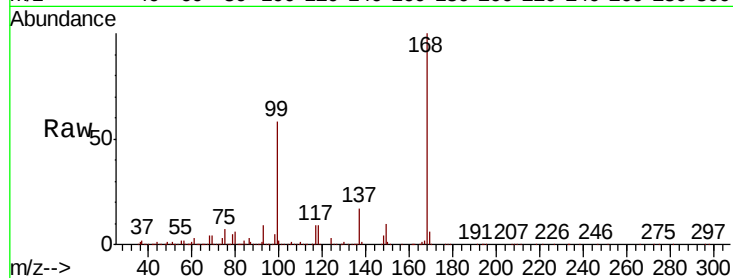

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.64

150000



100000

50000

0

Time-->

5.50 5.60 5.70

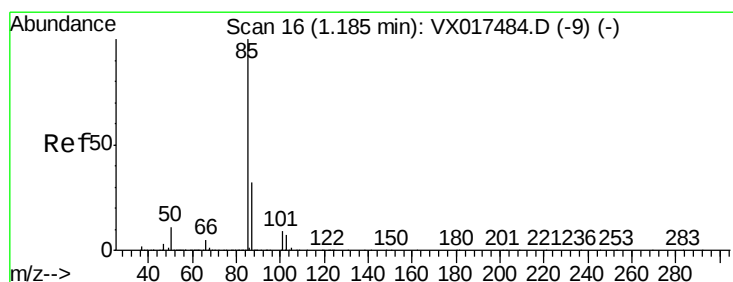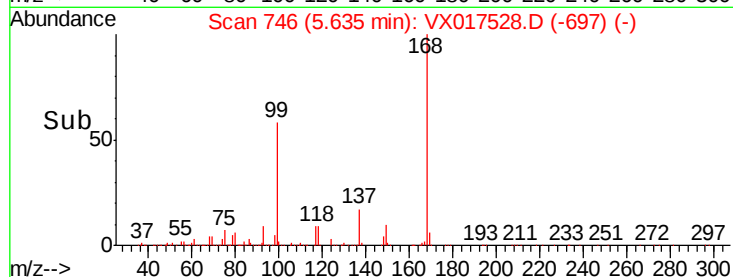

#2

Dichlorodifluoromethane

Concen: Below Cal

RT: 1.18 min Scan# 16

Delta R.T. 0.00 min

Lab File: VX017528.D


Acq: 24 Jul 2020 06:02

Tgt Ion: 85 Resp: 463

Ion Ratio Lower Upper

85 100

87 40.3 16.1 48.3

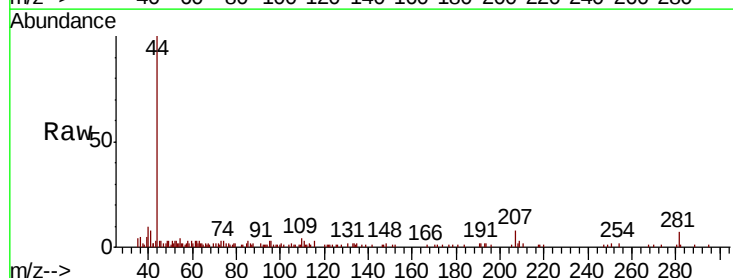

Abundance Ion 84.90 (84.60 to 85.60): VX0

Ion 86.90 (86.60 to 87.60): VX0

1.18

500

400

300


200


100

0

Time-->

1.14 1.16 1.18 1.20 1.22

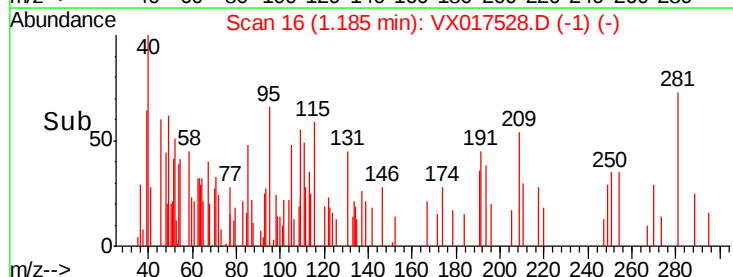



#3

Chloromethane

Concen: 0.469 ug/l

RT: 1.31 min Scan# 37

Delta R.T. 0.00 min

Lab File: VX017528.D

Acq: 24 Jul 2020 06:02

Instrument :

MSVOA_X

ClientSampleId :





357-GRID-A4-A6

Tot Ion: 50 Resp: 606

Ion Ratio Lower Upper

50 100

52 39.7 25.9 38.9#

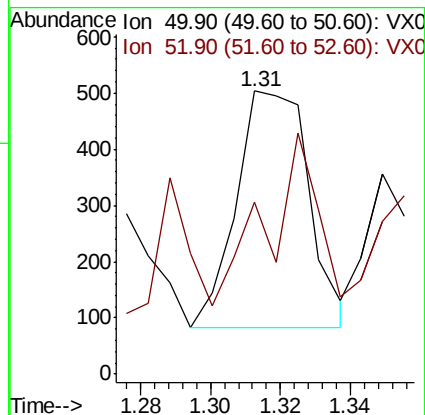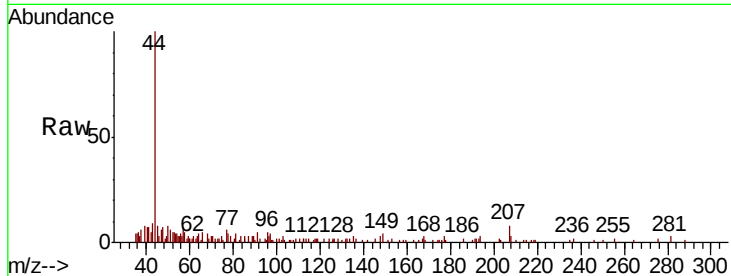

#5

Bromomethane

Concen: Below Cal

RT: 1.62 min Scan# 88

Delta R.T. 0.00 min

Lab File: VX017528.D




Acq: 24 Jul 2020 06:02


Tgt Ion: 94 Resp: 154

Ion Ratio Lower Upper

94 100

96 120.1 74.1 111.1#

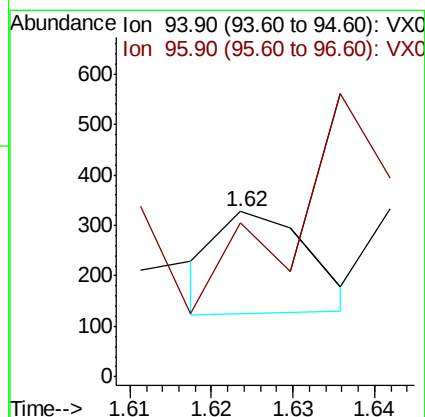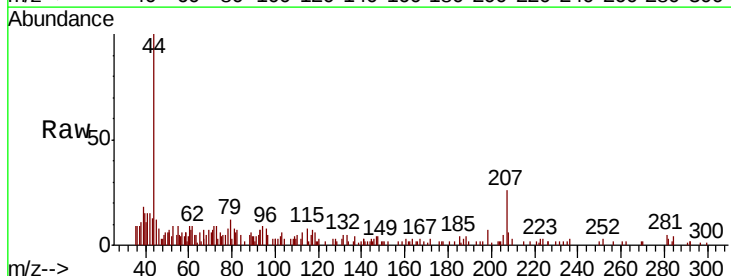



#6

Chloroethane

Concen: Below Cal

RT: 1.73 min Scan# 106

Delta R.T. 0.02 min

Lab File: VX017528.D

Acq: 24 Jul 2020 06:02

Instrument :

MSVOA_X

ClientSampled :





357-GRID-A4-A6

Tot Ion: 64 Resp: 594

Ion Ratio Lower Upper

64 100

66 46.0 24.9 37.3#

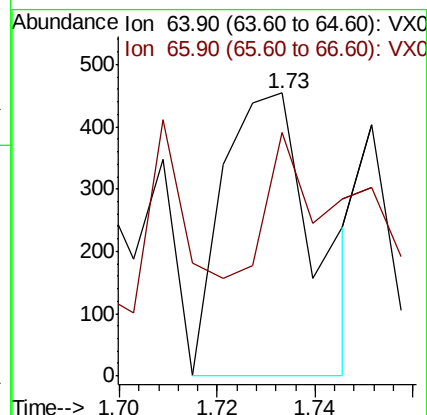

#8

Diethyl Ether

Concen: Below Cal

RT: 2.18 min Scan# 179

Delta R.T. 0.01 min

Lab File: VX017528.D




Acq: 24 Jul 2020 06:02


Tgt Ion: 74 Resp: 1369

Ion Ratio Lower Upper

74 100

45 131.6 50.8 152.5



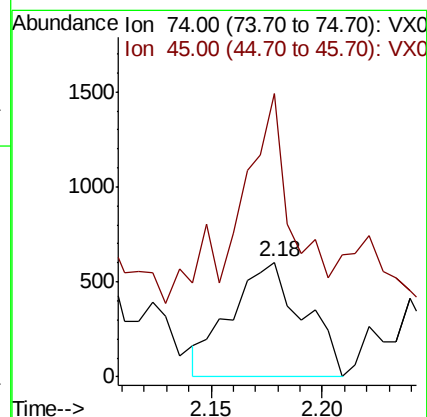





#11
Tert butyl alcohol
Concen: 1.128 ug/l
RT: 3.00 min Scan# 314
Delta R.T. -0.02 min
Lab File: VX017528.D
Acq: 24 Jul 2020 06:02




Instrument :
MSVOA_X
ClientSampleId :
357-GRID-A4-A6


Tot Ion: 59 Resp: 1454
Ion Ratio Lower Upper
59 100
57 11.1 8.6 12.8

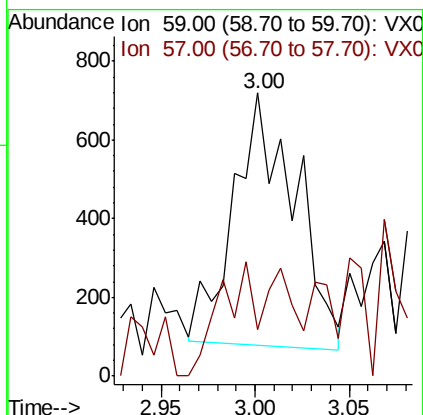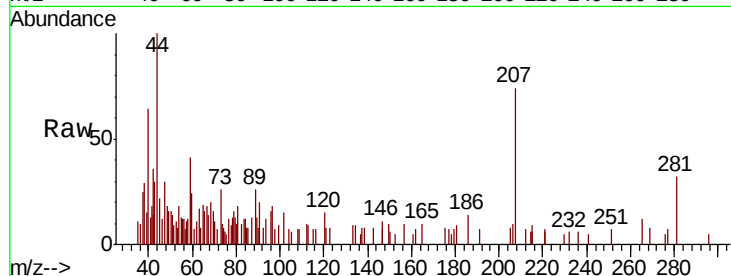

#13
Acrolein
Concen: 4.501 ug/l
RT: 2.26 min Scan# 193
Delta R.T. -0.01 min
Lab File: VX017528.D
Acq: 24 Jul 2020 06:02

Tgt Ion: 56 Resp: 353
Ion Ratio Lower Upper
56 100
55 93.2 57.4 86.2#

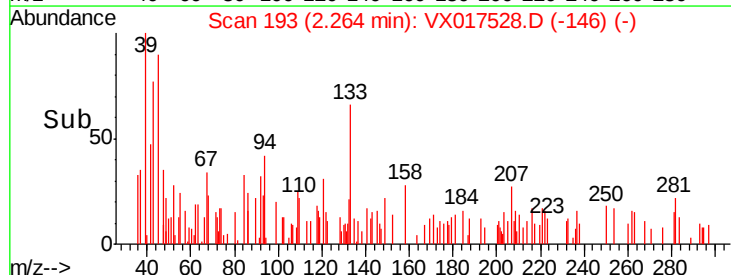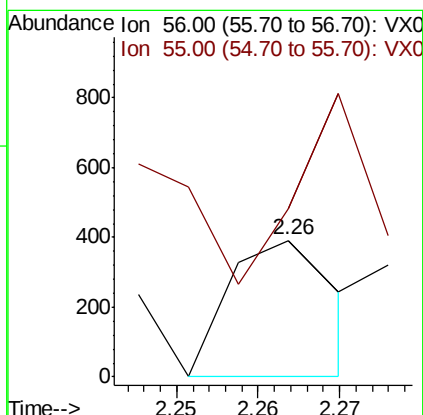

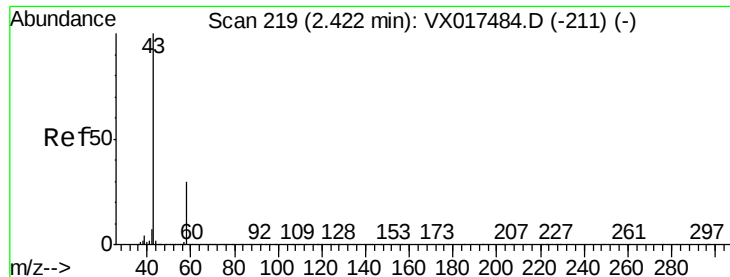

#16

Acetone

Concen: 16.637 ug/l

RT: 2.42 min Scan# 219

Delta R.T. -0.00 min

Lab File: VX017528.D

Acq: 24 Jul 2020 06:02

Instrument :

MSVOA_X

ClientSampleId :





357-GRID-A4-A6

Tot Ion: 43 Resp: 44798

Ion Ratio Lower Upper

43 100

58 26.4 24.2 36.4

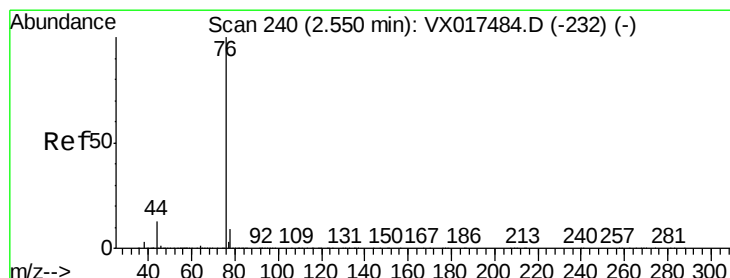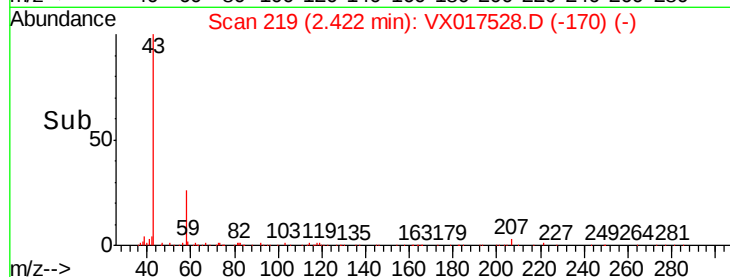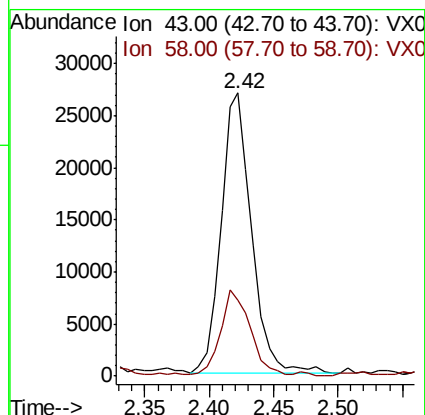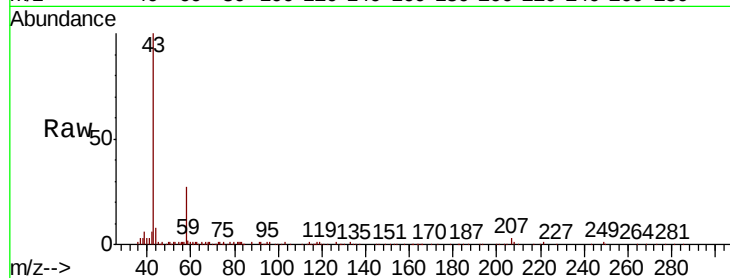

#17

Carbon Disulfide

Concen: 0.210 ug/l

RT: 2.55 min Scan# 240

Delta R.T. -0.00 min

Lab File: VX017528.D




Acq: 24 Jul 2020 06:02


Tgt Ion: 76 Resp: 3138

Ion Ratio Lower Upper

76 100

78 28.1 7.5 11.3#


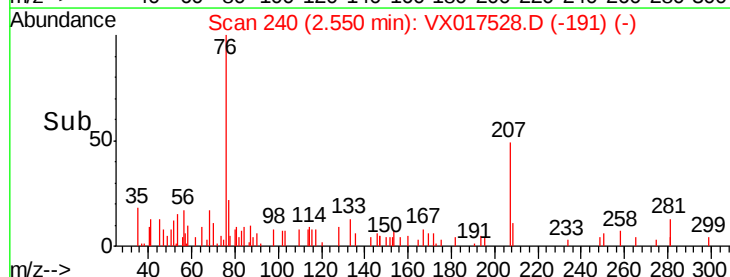
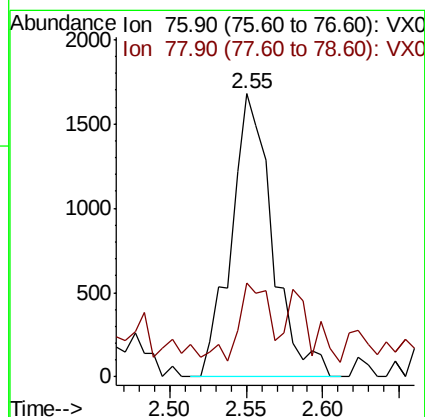
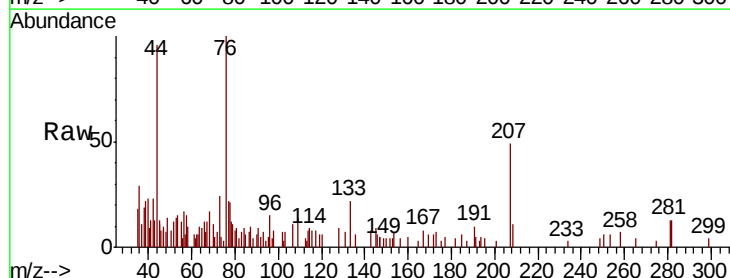




#18
Methyl Acetate
Concen: 1.089 ug/l
RT: 2.75 min Scan# 273
Delta R.T. -0.00 min
Lab File: VX017528.D
Acq: 24 Jul 2020 06:02




Instrument :
MSVOA_X
ClientSampleId :
357-GRID-A4-A6


Tot Ion: 43 Resp: 6903
Ion Ratio Lower Upper
43 100
74 26.1 17.5 26.3

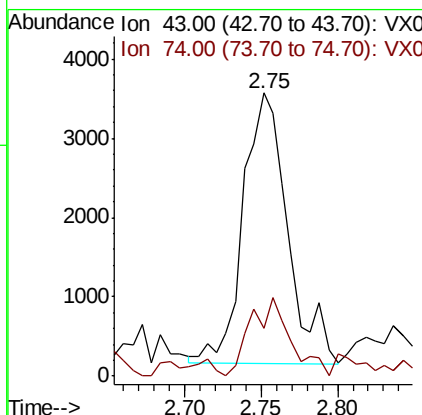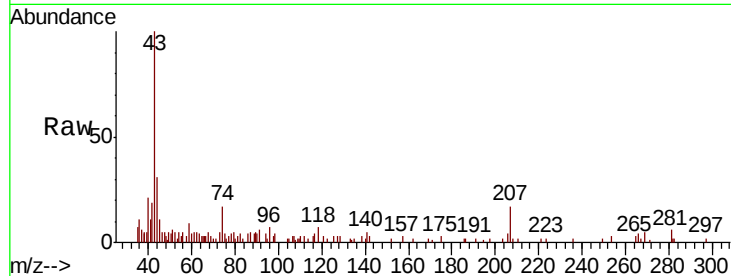

#20
Methylene Chloride
Concen: 5.785 ug/l
RT: 2.84 min Scan# 287
Delta R.T. 0.00 min
Lab File: VX017528.D
Acq: 24 Jul 2020 06:02

Tgt Ion: 84 Resp: 35099
Ion Ratio Lower Upper
84 100
49 135.3 100.3 150.5
51 43.3 30.5 45.7
86 76.2 51.1 76.7

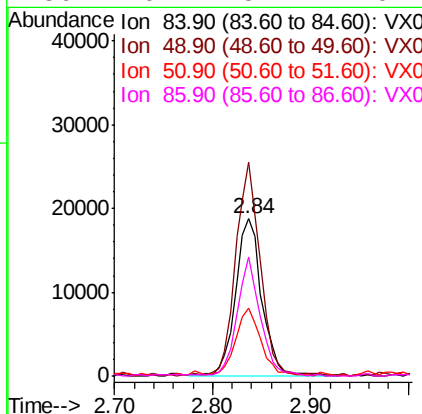



#25

2-Butanone

Concen: 2.264 ug/l

RT: 4.65 min Scan# 584

Delta R.T. 0.01 min

Lab File: VX017528.D

Acq: 24 Jul 2020 06:02

Instrument :

MSVOA_X

ClientSampleId :





357-GRID-A4-A6

Tot Ion: 43 Resp: 8659

Ion Ratio Lower Upper

43 100

72 12.1 19.0 28.4#

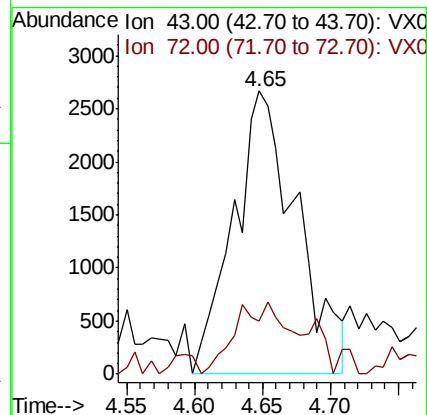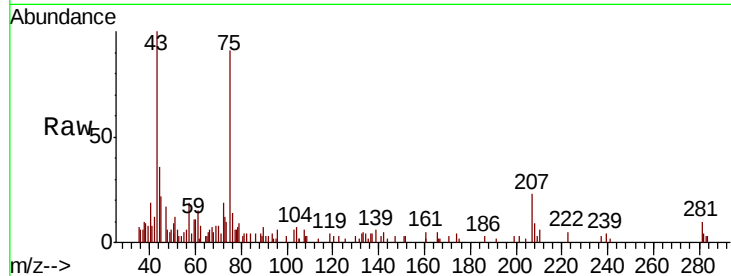

#29

Tetrahydrofuran

Concen: 0.632 ug/l

RT: 5.09 min Scan# 657

Delta R.T. -0.00 min

Lab File: VX017528.D

Acq: 24 Jul 2020 06:02




Tgt Ion: 42 Resp: 1498


Ion Ratio Lower Upper

42 100

72 41.1 35.5 53.3

71 21.8 33.0 49.4#

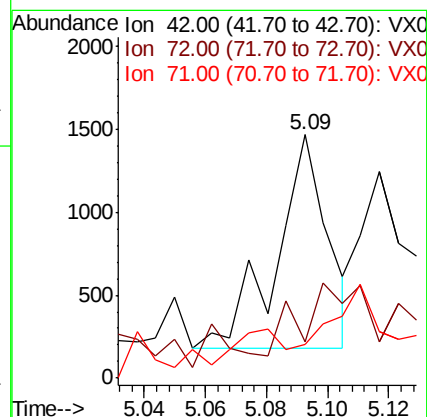


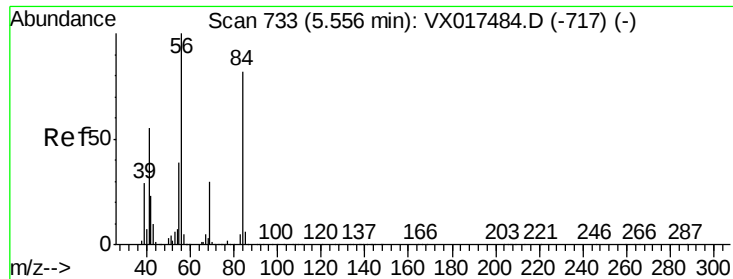




#31
Cyclohexane
Concen: 1.380 ug/l
RT: 5.63 min Scan# 745
Delta R.T. 0.07 min
Lab File: VX017528.D
Acq: 24 Jul 2020 06:02

Instrument :
MSVOA_X
ClientSampleId :
357-GRID-A4-A6

Tot Ion: 56 Resp: 10411
Ion Ratio Lower Upper
56 100
69 131.0 24.2 36.4#
84 117.3 69.0 103.6#

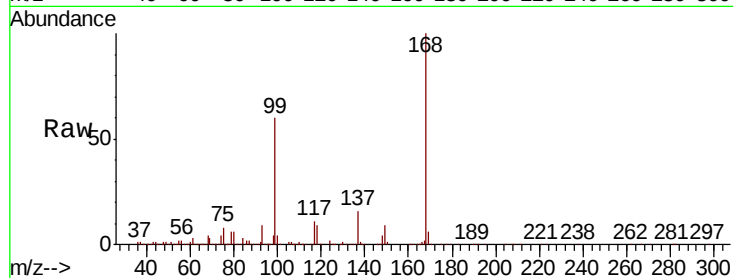


Abundance Ion 56.00 (55.70 to 56.70): VX0
Ion 69.00 (68.70 to 69.70): VX0
Ion 84.00 (83.70 to 84.70): VX0

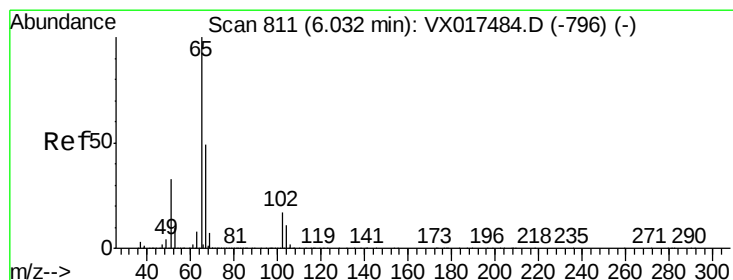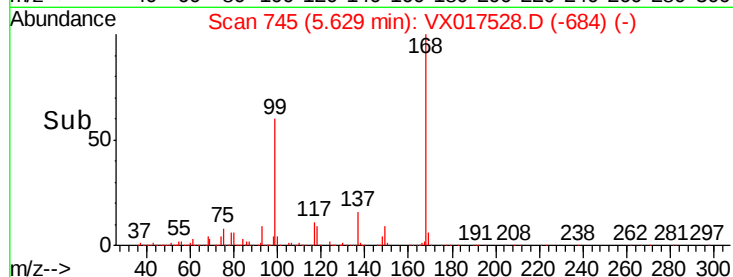
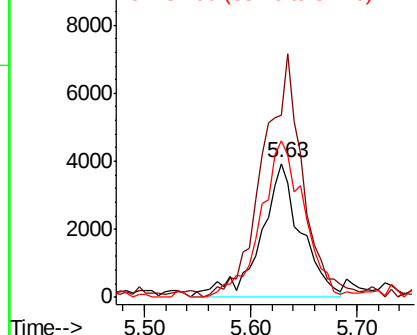



#33
1,2-Dichloroethane-d4
Concen: 54.740 ug/l
RT: 6.03 min Scan# 811
Delta R.T. -0.00 min
Lab File: VX017528.D
Acq: 24 Jul 2020 06:02

Tgt Ion: 65 Resp: 334894
Ion Ratio Lower Upper
65 100
67 50.9 0.0 102.8

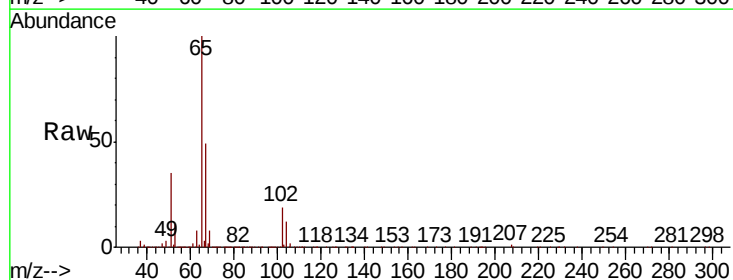

Abundance Ion 64.90 (64.60 to 65.60): VX0
Ion 66.90 (66.60 to 67.60): VX0

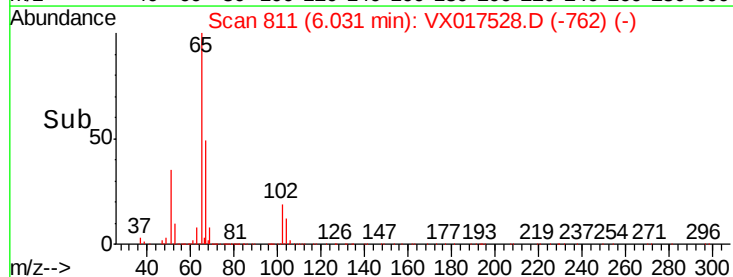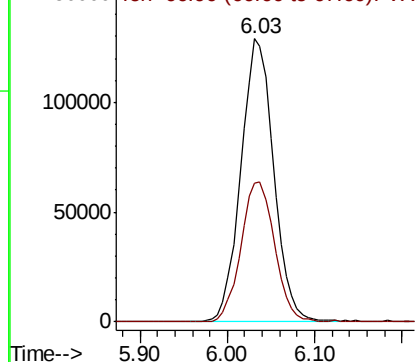

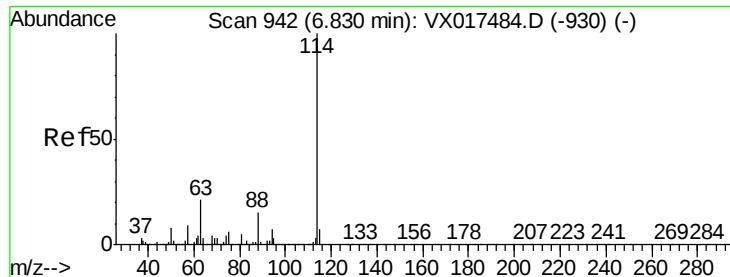

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.83 min Scan# 942

Delta R.T. -0.00 min

Lab File: VX017528.D

Acq: 24 Jul 2020 06:02

Instrument :

MSVOA_X

ClientSampleId :

357-GRID-A4-A6


Tot Ion:114 Resp: 815708

Ion Ratio Lower Upper

114 100

63 20.4 0.0 40.6




88 15.3 0.0 33.4

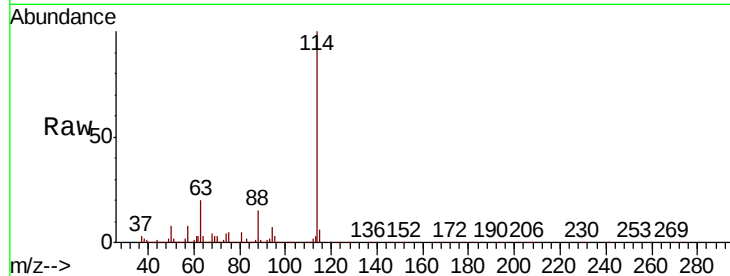

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

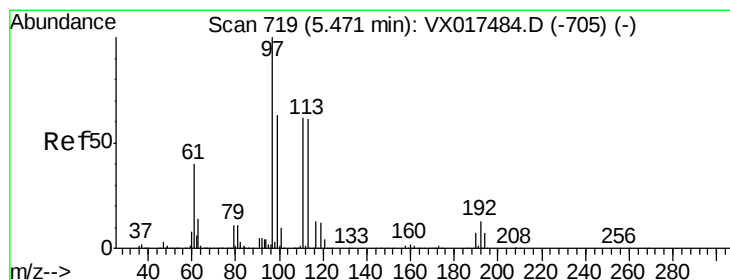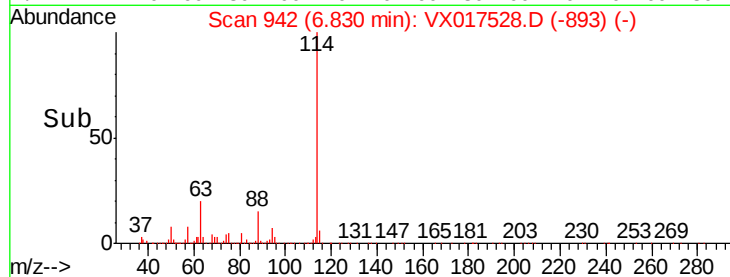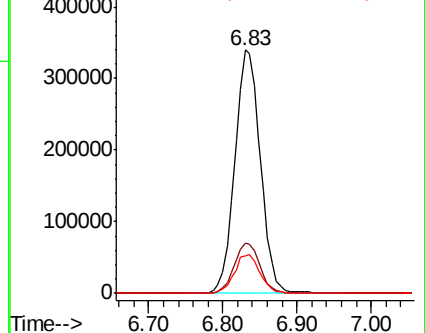

#35

Dibromofluoromethane

Concen: 51.409 ug/l

RT: 5.46 min Scan# 718

Delta R.T. -0.01 min

Lab File: VX017528.D

Acq: 24 Jul 2020 06:02


Tgt Ion:113 Resp: 280460

Ion Ratio Lower Upper

113 100

111 101.3 80.7 121.1



192 20.5 16.9 25.3

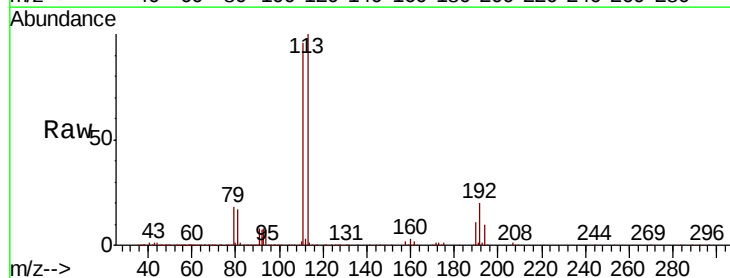


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V



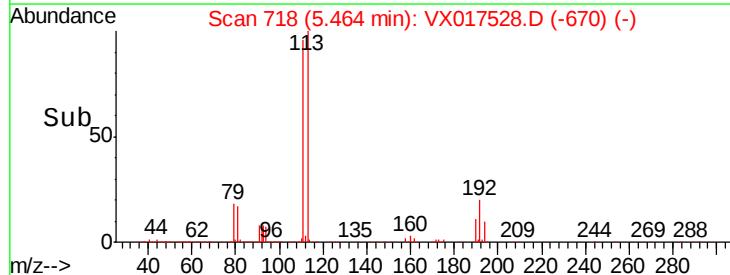
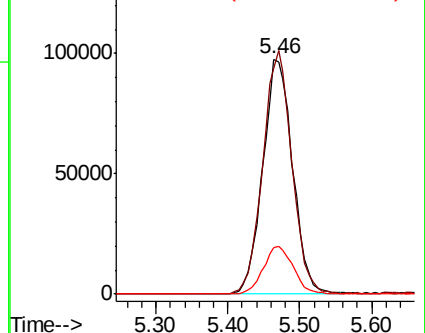


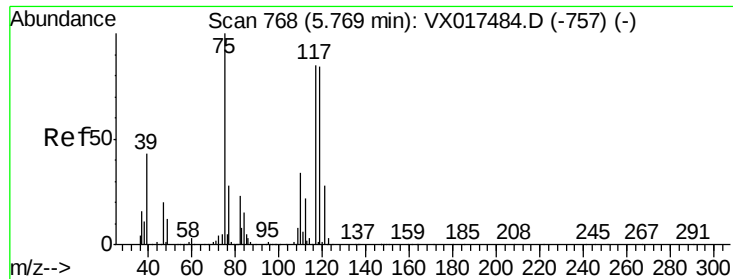

#36
 1,1-Dichloropropene
 Concen: 4.723 ug/l
 RT: 5.64 min Scan# 746
 Delta R.T. -0.13 min
 Lab File: VX017528.D
 Acq: 24 Jul 2020 06:02




Instrument :
 MSVOA_X
 ClientSampleId :
 357-GRID-A4-A6


Tot Ion: 75 Resp: 36949
 Ion Ratio Lower Upper
 75 100
 110 11.2 18.1 54.3#
 77 1.0 24.6 37.0#

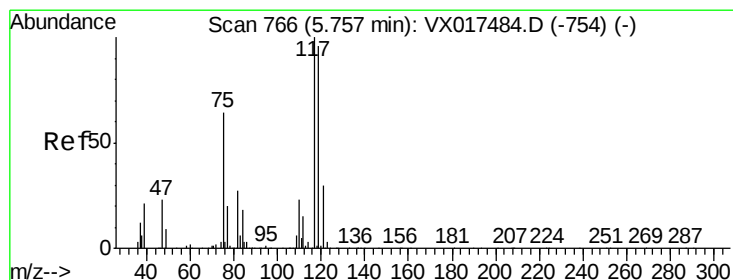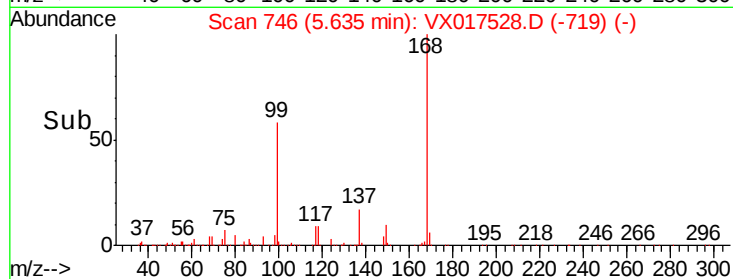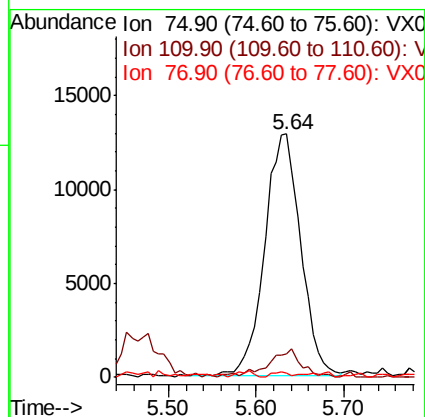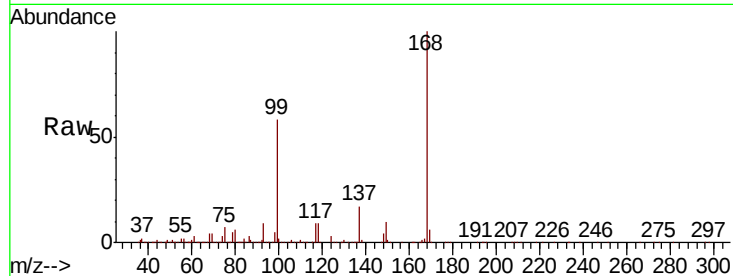

#38
 Carbon Tetrachloride
 Concen: 5.159 ug/l
 RT: 5.63 min Scan# 745
 Delta R.T. -0.13 min
 Lab File: VX017528.D
 Acq: 24 Jul 2020 06:02

Tgt Ion: 117 Resp: 49013
 Ion Ratio Lower Upper
 117 100
 119 3.8 75.4 113.0#
 121 0.0 24.3 36.5#

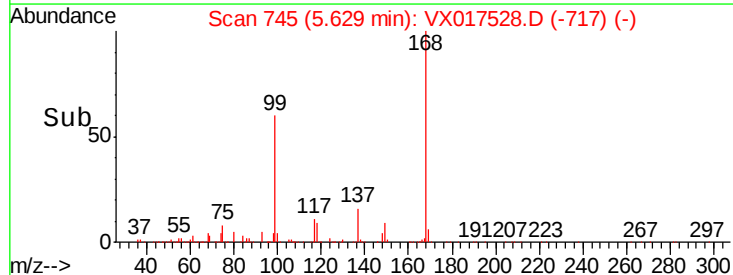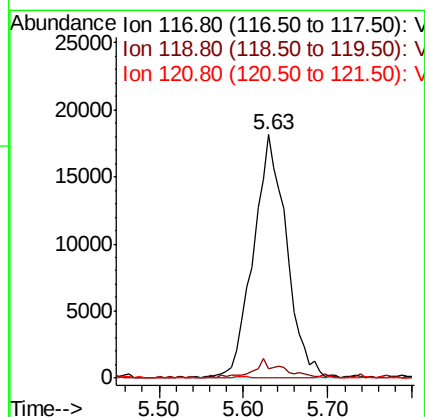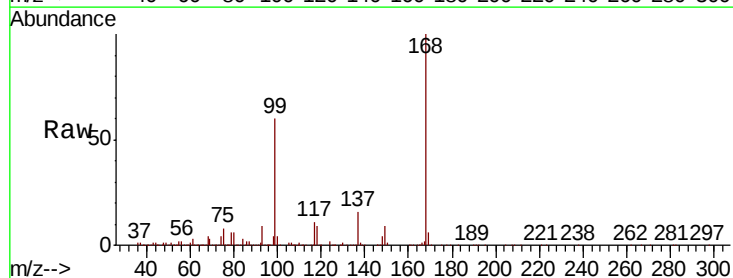



#43

Isopropyl Acetate

Concen: 10.539 ug/l

RT: 6.42 min Scan# 874

Delta R.T. -0.00 min

Lab File: VX017528.D

Acq: 24 Jul 2020 06:02

Instrument :

MSVOA_X

ClientSampleId :

357-GRID-A4-A6


Tot Ion: 43 Resp: 148845

Ion Ratio Lower Upper




43 100

61 20.4 15.5 23.3

87 12.8 10.5 15.7

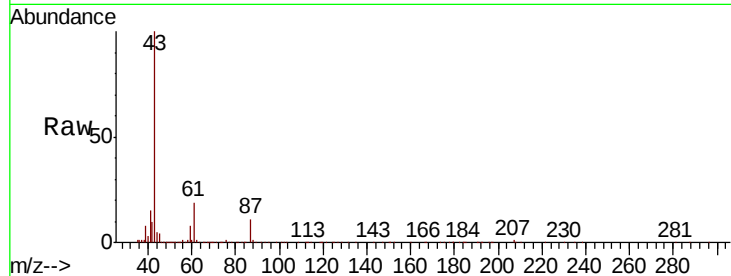

Abundance Ion 43.00 (42.70 to 43.70): VX0
Ion 61.00 (60.70 to 61.70): VX0
Ion 87.00 (86.70 to 87.70): VX0

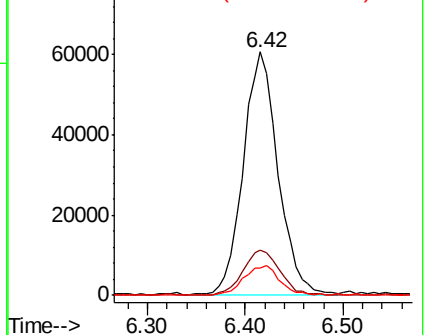

#48

Methyl methacrylate

Concen: 1.267 ug/l

RT: 7.65 min Scan# 1077

Delta R.T. -0.10 min

Lab File: VX017528.D

Acq: 24 Jul 2020 06:02


Tgt Ion: 41 Resp: 8869

Ion Ratio Lower Upper



41 100


69 4.0 63.1 94.7#

39 0.0 45.1 67.7#



Abundance Ion 41.00 (40.70 to 41.70): VX0
Ion 69.00 (68.70 to 69.70): VX0
Ion 39.00 (38.70 to 39.70): VX0

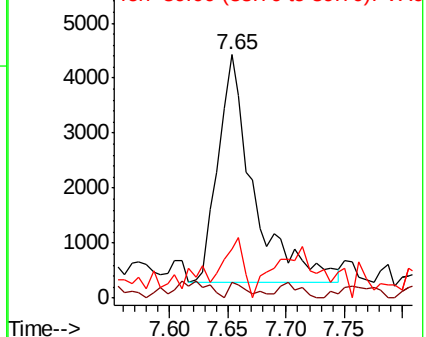







#49
1,4-Dioxane
Concen: 2.272 ug/l
RT: 7.68 min Scan# 1081
Delta R.T. -0.04 min
Lab File: VX017528.D
Acq: 24 Jul 2020 06:02

Instrument :
MSVOA_X
ClientSampleId :
357-GRID-A4-A6

Tot Ion	Ratio	Lower	Upper
88	100		
43	0.0	27.8	41.6#
58	517.0	58.3	87.5#

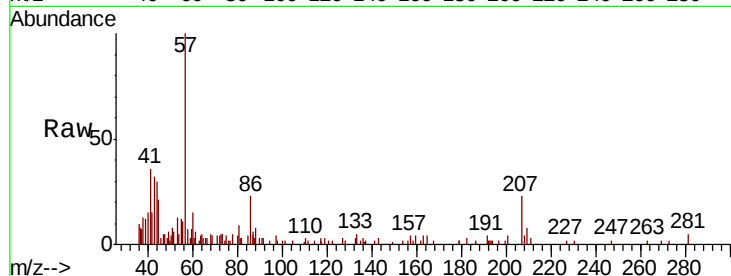


Abundance Ion 88.00 (87.70 to 88.70): VX0
Ion 43.00 (42.70 to 43.70): VX0
Ion 58.00 (57.70 to 58.70): VX0


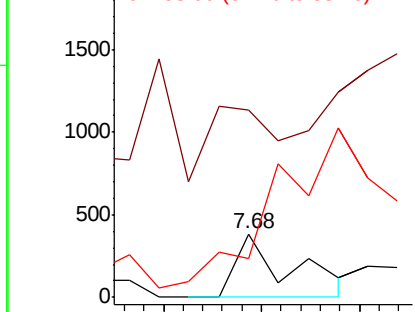



#50
Toluene-d8
Concen: 53.489 ug/l
RT: 8.70 min Scan# 1248
Delta R.T. -0.00 min
Lab File: VX017528.D
Acq: 24 Jul 2020 06:02

Tgt Ion	Ratio	Lower	Upper
98	100		
100	64.6	52.3	78.5



Abundance Ion 98.00 (97.70 to 98.70): VX0
Ion 100.00 (99.70 to 100.70): V

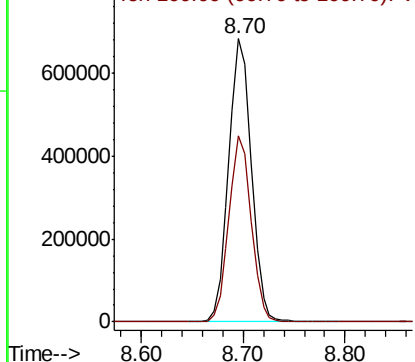

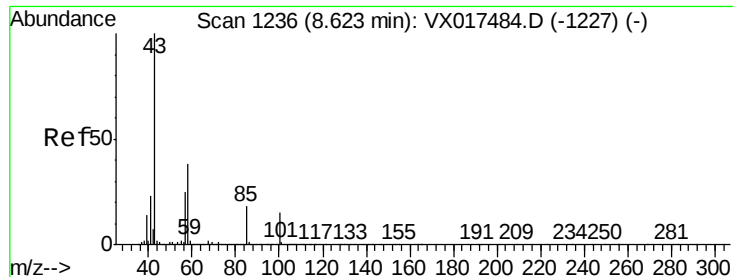

#51

4-Methyl-2-Pentanone

Concen: 16.861 ug/l

RT: 8.59 min Scan# 1231

Delta R.T. -0.03 min

Lab File: VX017528.D

Acq: 24 Jul 2020 06:02

Instrument :

MSVOA_X

ClientSampleId :





357-GRID-A4-A6

Tot Ion: 43 Resp: 142086

Ion Ratio Lower Upper

43 100

58 6.4 31.0 46.4#

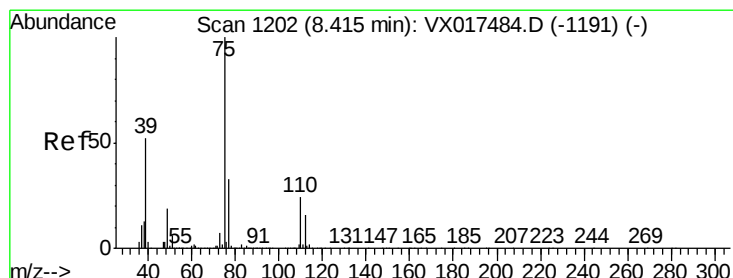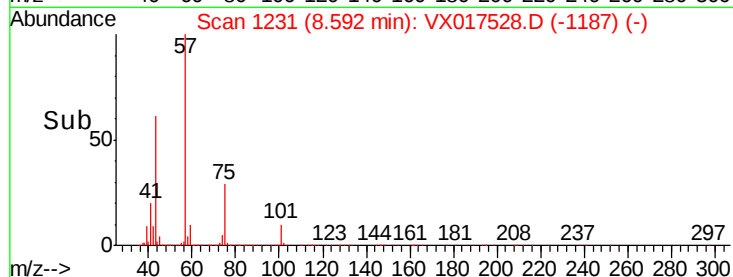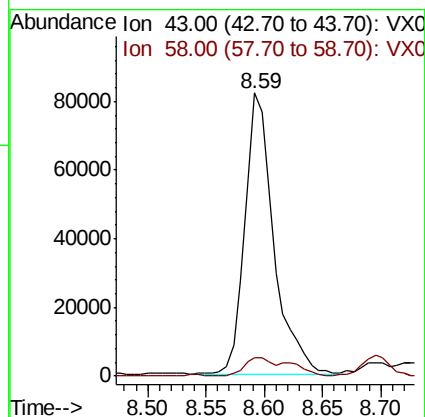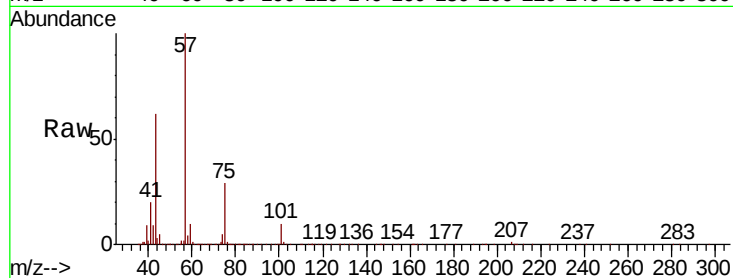

#54

cis-1,3-Dichloropropene

Concen: 5.764 ug/l

RT: 8.59 min Scan# 1231

Delta R.T. 0.18 min

Lab File: VX017528.D

Acq: 24 Jul 2020 06:02




Tgt Ion: 75 Resp: 58192


Ion Ratio Lower Upper

75 100

77 0.8 25.5 38.3#

39 30.2 41.8 62.8#

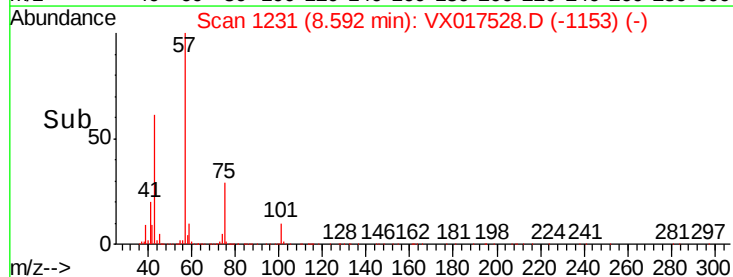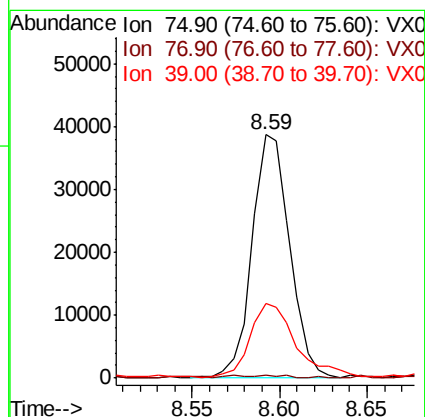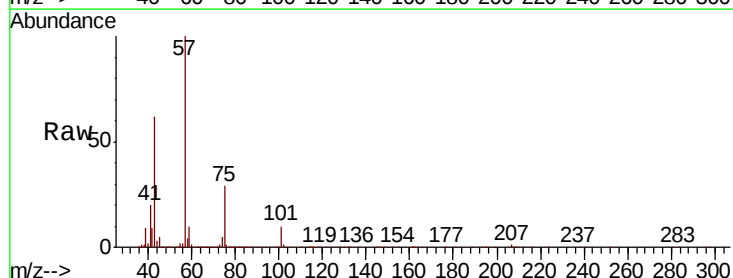

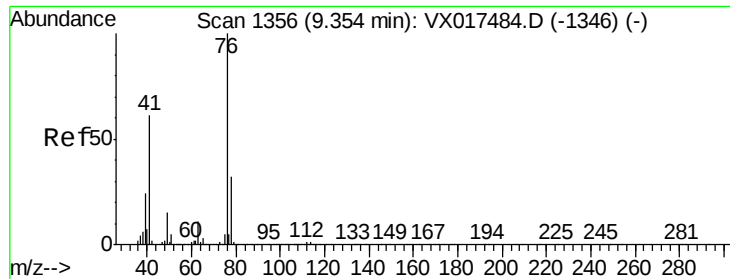

#57

1,3-Dichloropropane

Concen: 1.048 ug/l

RT: 9.52 min Scan# 1384

Delta R.T. 0.17 min

Lab File: VX017528.D

Acq: 24 Jul 2020 06:02

Instrument :

MSVOA_X

ClientSampleId :


357-GRID-A4-A6

Tot Ion: 76 Resp: 10345

Ion Ratio Lower Upper




76 100

78 2.2 25.8 38.8#

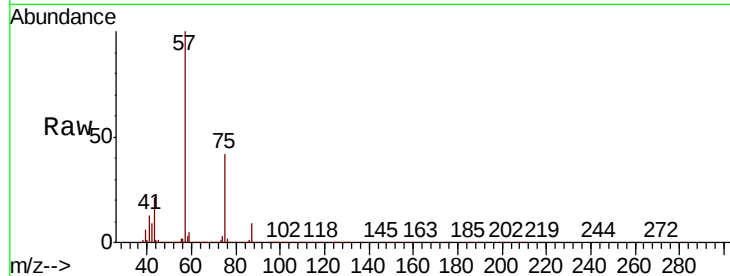

Abundance Ion 75.90 (75.60 to 76.60): VX0

Ion 77.90 (77.60 to 78.60): VX0

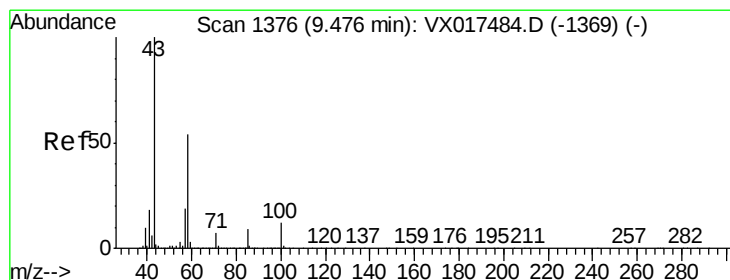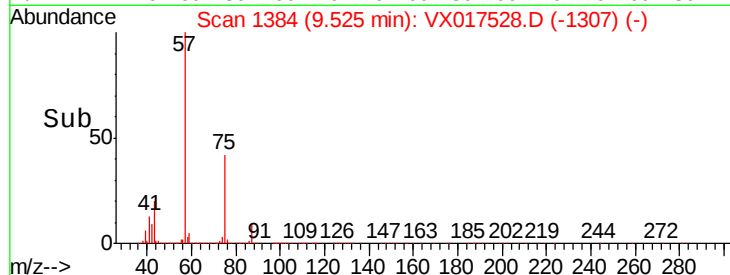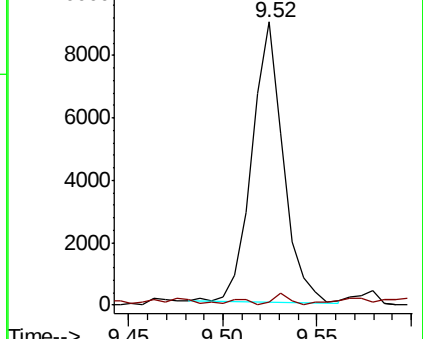

#59

2-Hexanone

Concen: 22.714 ug/l

RT: 9.52 min Scan# 1384

Delta R.T. 0.05 min

Lab File: VX017528.D


Acq: 24 Jul 2020 06:02

Tgt Ion: 43 Resp: 144109

Ion Ratio Lower Upper



43 100


58 18.5 26.6 79.8#

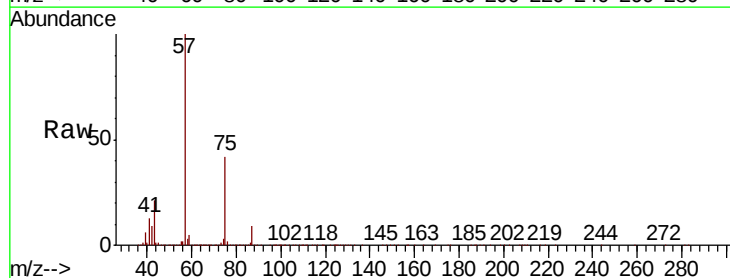

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0



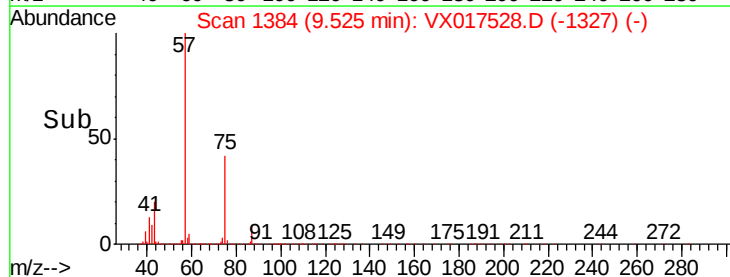
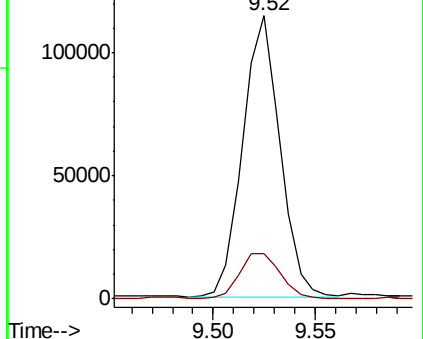




#62
4-Bromofluorobenzene
Concen: 58.921 ug/l
RT: 11.12 min Scan# 1646
Delta R.T. -0.00 min
Lab File: VX017528.D
Acq: 24 Jul 2020 06:02




Instrument :
MSVOA_X
ClientSampleId :
357-GRID-A4-A6


Tot Ion	Ratio	Lower	Upper
95	100		
174	84.0	0.0	169.0
176	80.2	0.0	161.0

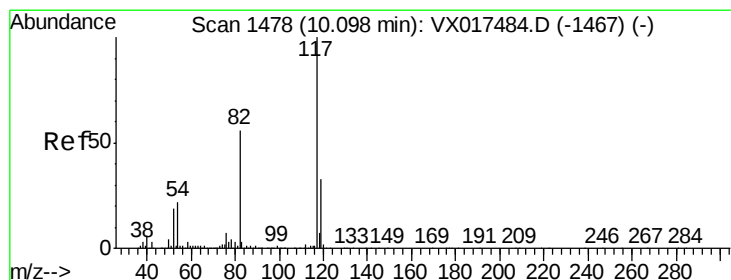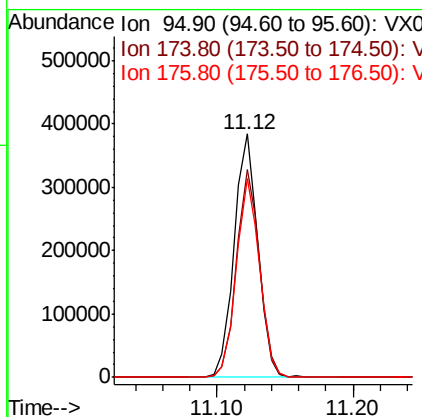

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.10 min Scan# 1478
Delta R.T. -0.00 min
Lab File: VX017528.D
Acq: 24 Jul 2020 06:02

Tgt Ion	Ratio	Lower	Upper
117	100		
82	55.6	44.0	66.0
119	31.2	25.4	38.0

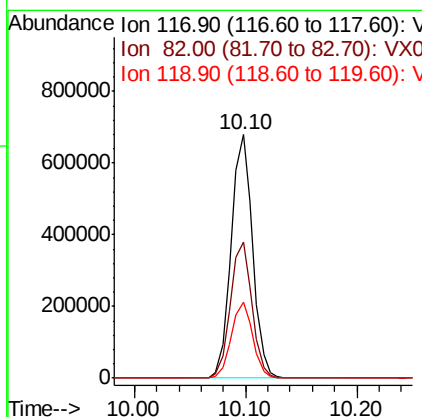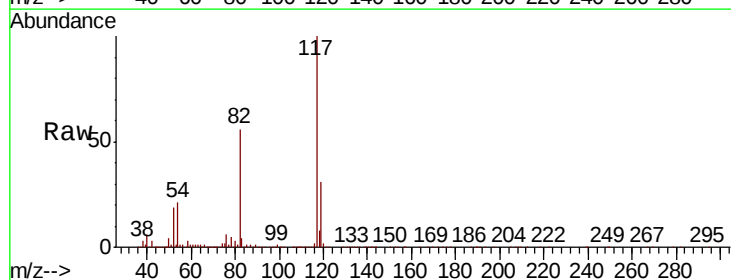

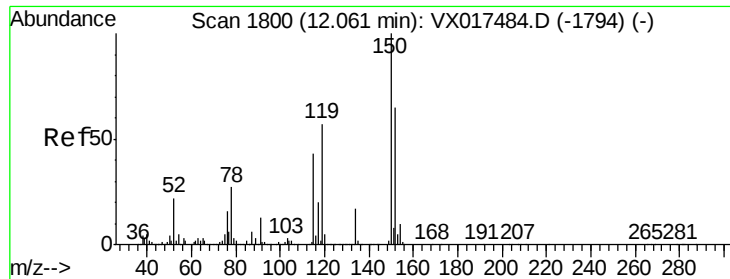

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.06 min Scan# 1800

Delta R.T. -0.00 min

Lab File: VX017528.D

Acq: 24 Jul 2020 06:02

Instrument :

MSVOA_X

ClientSampleId :

357-GRID-A4-A6


Tot Ion:152 Resp: 484611

Ion Ratio Lower Upper

152 100

115 58.2 65.5 196.6#

150 155.6 0.0 412.6



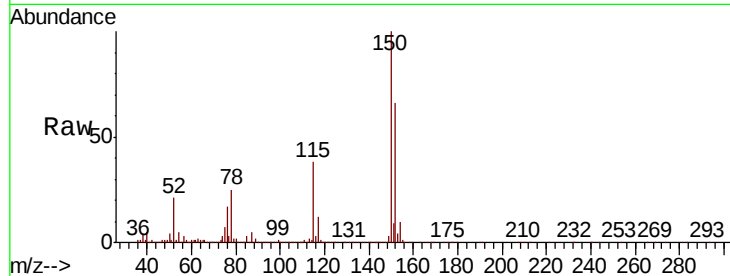


Abundance

Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

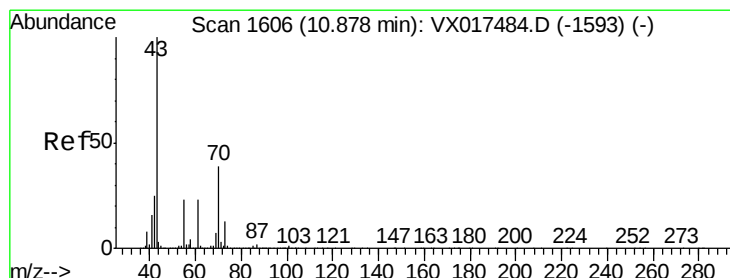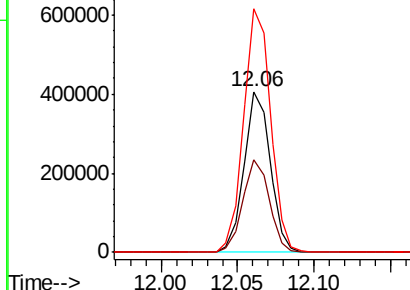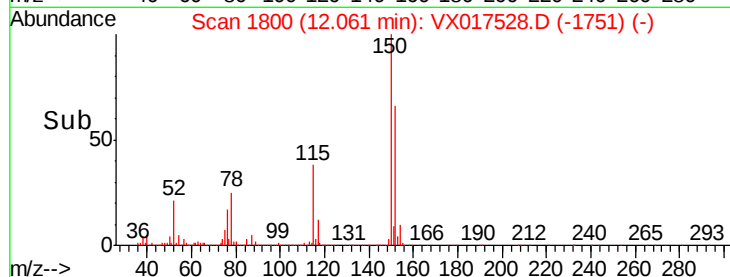

#74

N-ethyl acetate

Concen: 0.410 ug/l

RT: 10.80 min Scan# 1594

Delta R.T. -0.07 min

Lab File: VX017528.D

Acq: 24 Jul 2020 06:02

Tgt Ion: 43 Resp: 6059


Ion Ratio Lower Upper

43 100

70 7.9 32.3 48.5#

55 14.4 18.4 27.6#

61 0.0 18.6 28.0#

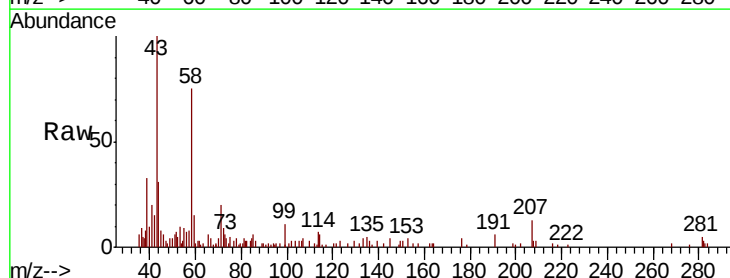



Abundance


Ion 43.00 (42.70 to 43.70): VX0

Ion 70.00 (69.70 to 70.70): VX0

Ion 55.00 (54.70 to 55.70): VX0

Ion 61.00 (60.70 to 61.70): VX0

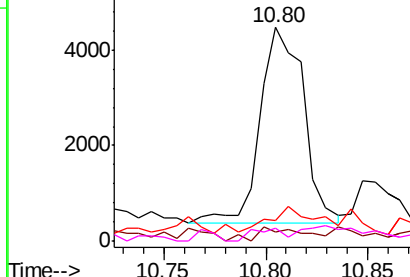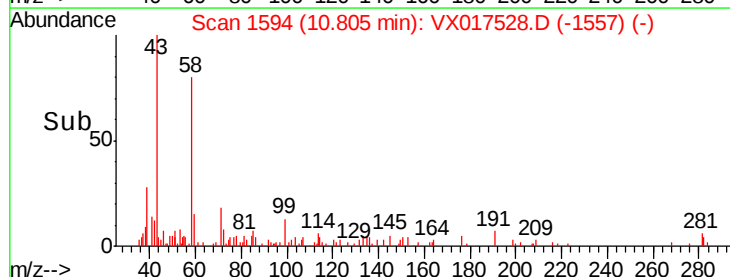



#76

1,2,3-Trichloropropane

Concen: 23.632 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. -0.16 min

Lab File: VX017528.D

Acq: 24 Jul 2020 06:02

Instrument :

MSVOA_X

ClientSampleId :





357-GRID-A4-A6

Tot Ion: 75 Resp: 235578

Ion Ratio Lower Upper

75 100

77 1.4 21.8 65.3#

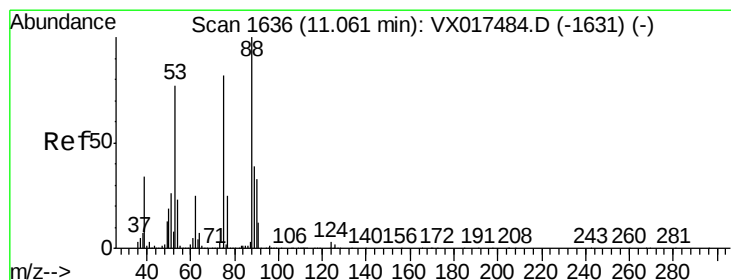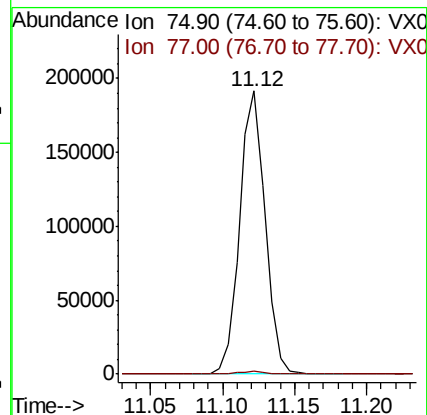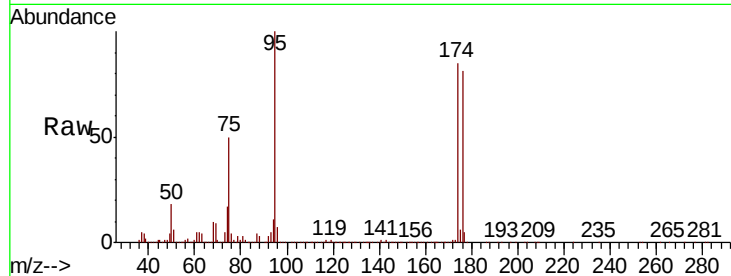

#81

trans-1,4-Dichloro-2-butene

Concen: 59.547 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. 0.06 min

Lab File: VX017528.D

Acq: 24 Jul 2020 06:02




Tgt Ion: 75 Resp: 235578


Ion Ratio Lower Upper

75 100

53 0.2 75.9 113.9#

89 0.0 37.8 56.6#

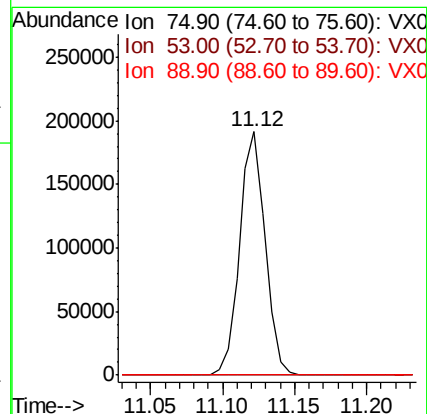



#92

1,2-Dibromo-3-Chloropropane

Concen: 2.632 ug/l

RT: 13.00 min Scan# 1954

Delta R.T. 0.02 min

Lab File: VX017528.D

Acq: 24 Jul 2020 06:02

Instrument :

MSVOA_X

ClientSampleId :

357-GRID-A4-A6


Tot Ion: 75 Resp: 170

Ion Ratio Lower Upper

75 100

155 0.0 42.3 126.8#

157 112.9 54.3 162.9



Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 154.80 (154.50 to 155.50): V

Ion 156.80 (156.50 to 157.50): V

400

300

200

100

0

12.98

13.00

Time-->

