



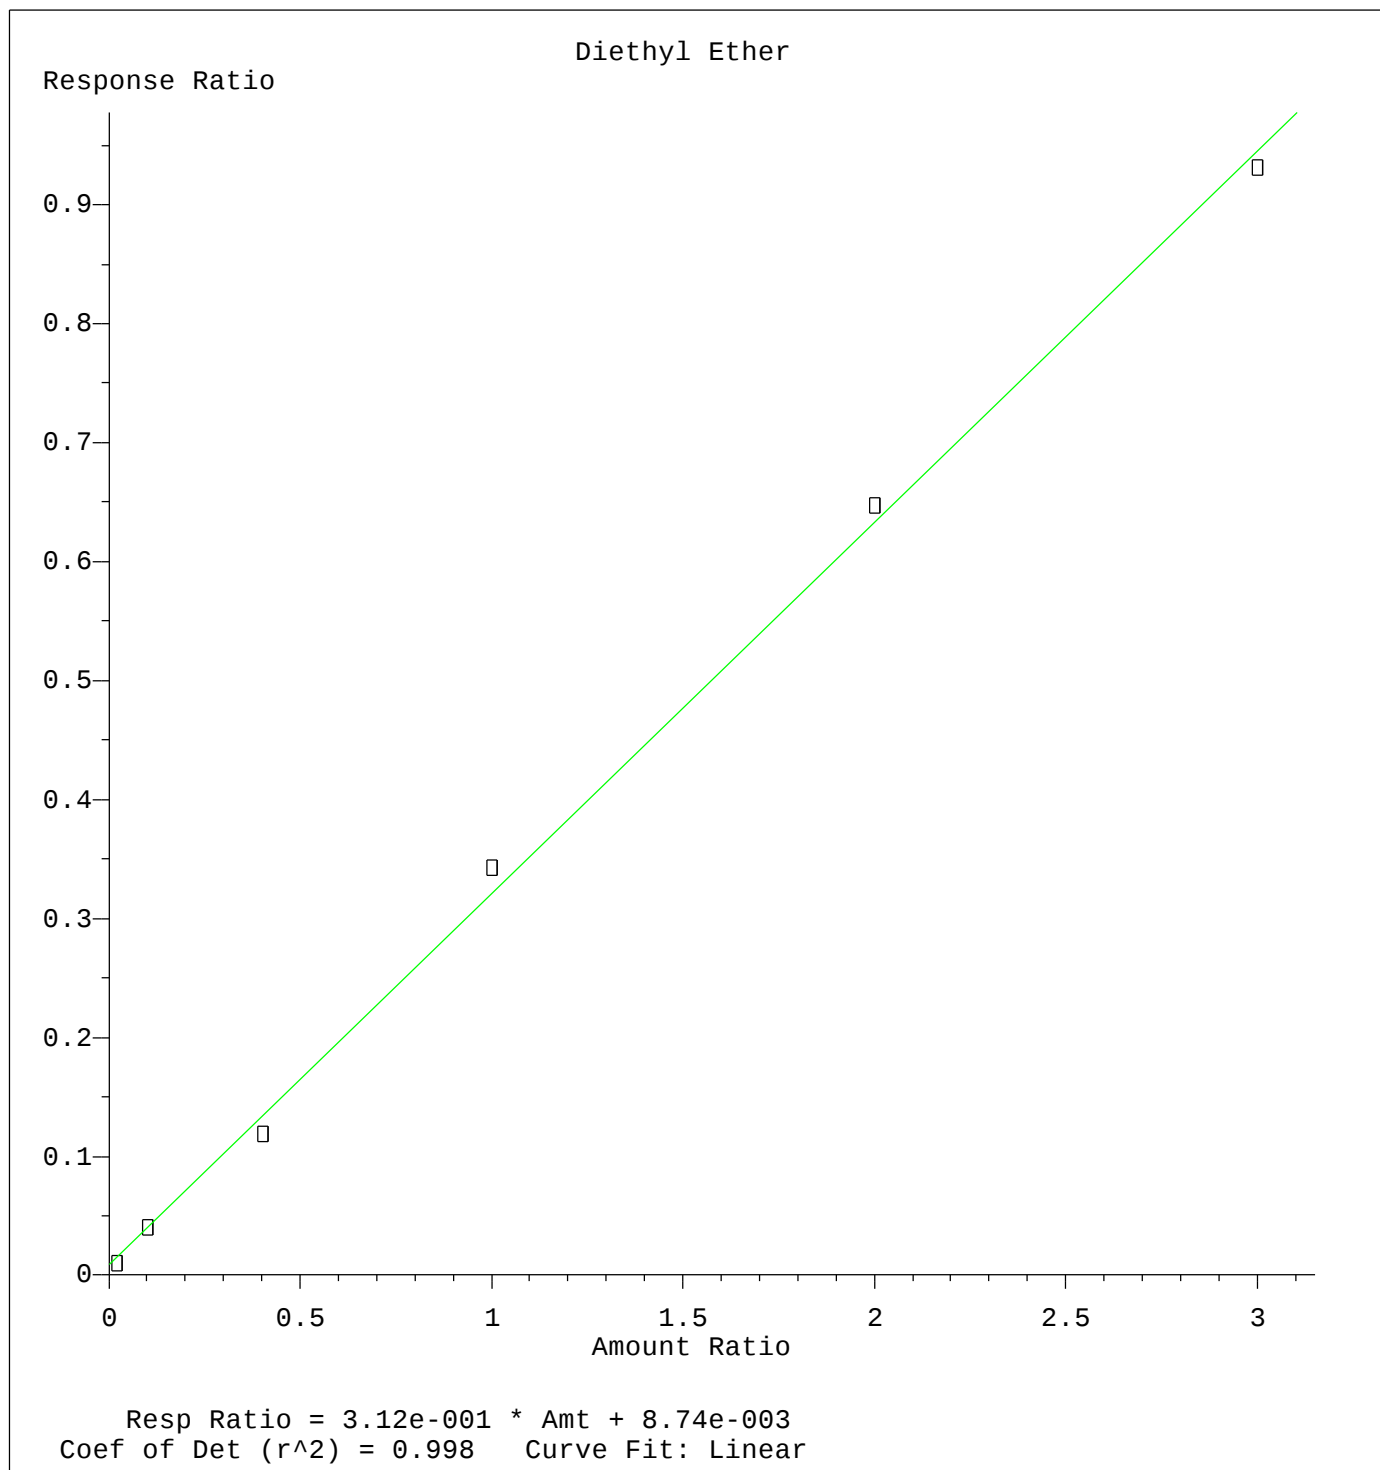

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X072320W.M  
Calibration Table Last Updated: Thu Jul 23 12:25:12 2020

# Acrolein

Response Ratio

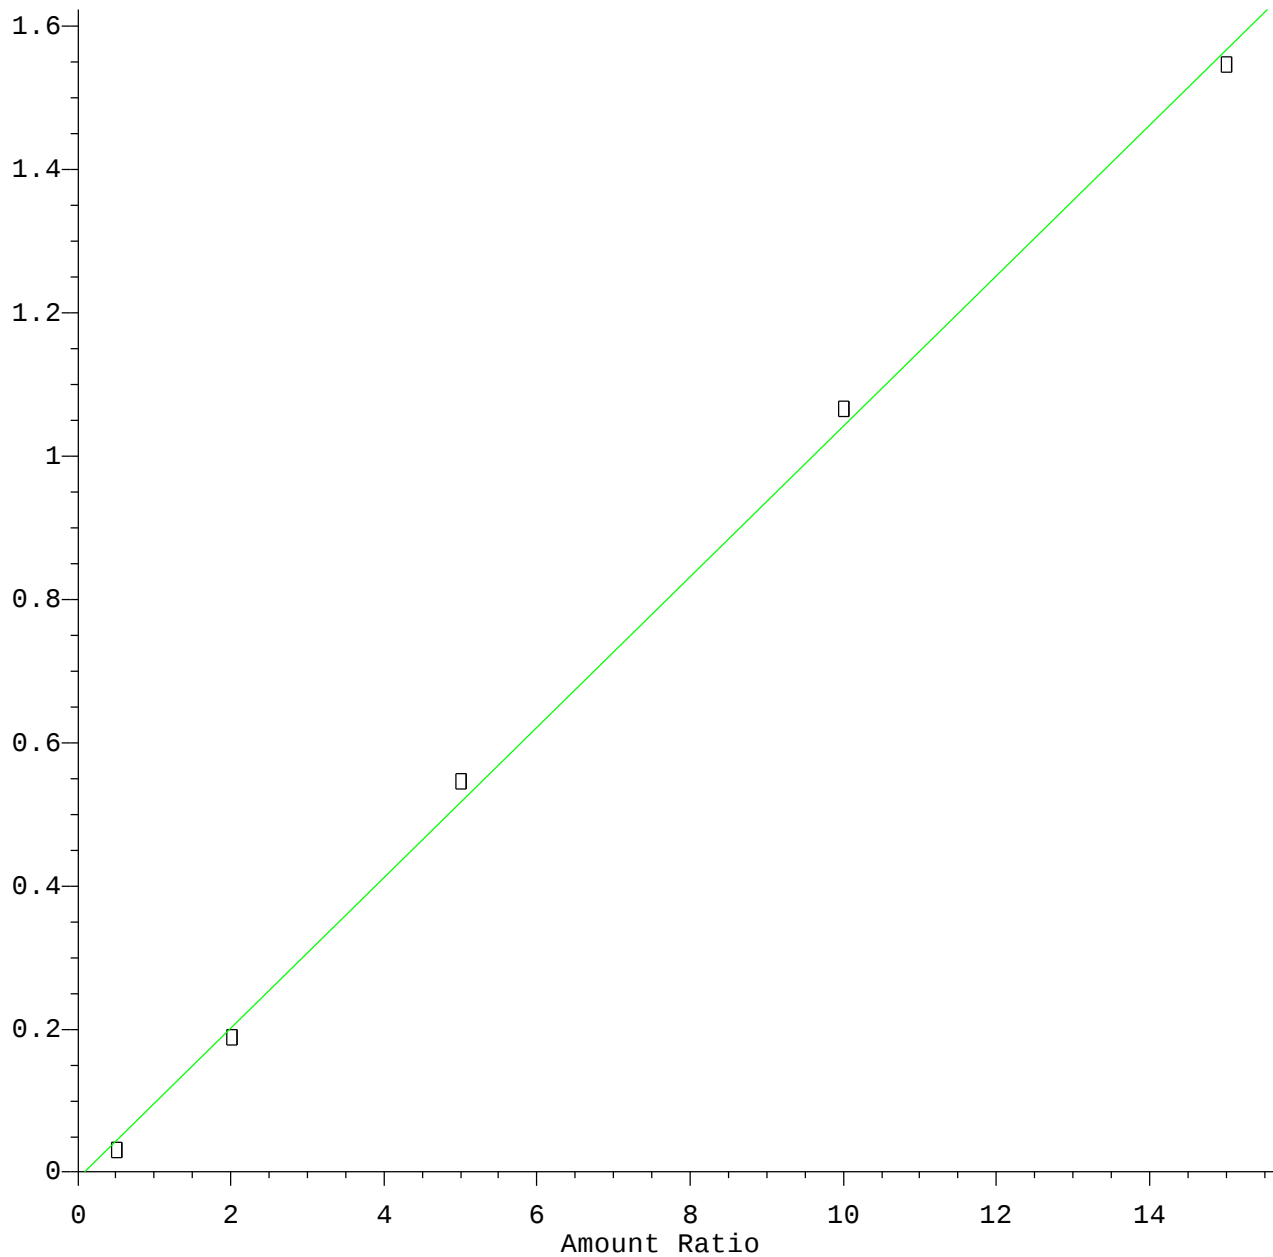


Resp Ratio = 1.05e-001 \* Amt - 8.72e-003  
Coef of Det (r<sup>2</sup>) = 0.999    Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X072320W.M  
Calibration Table Last Updated: Thu Jul 23 12:25:12 2020

# Methylene Chloride

Response Ratio

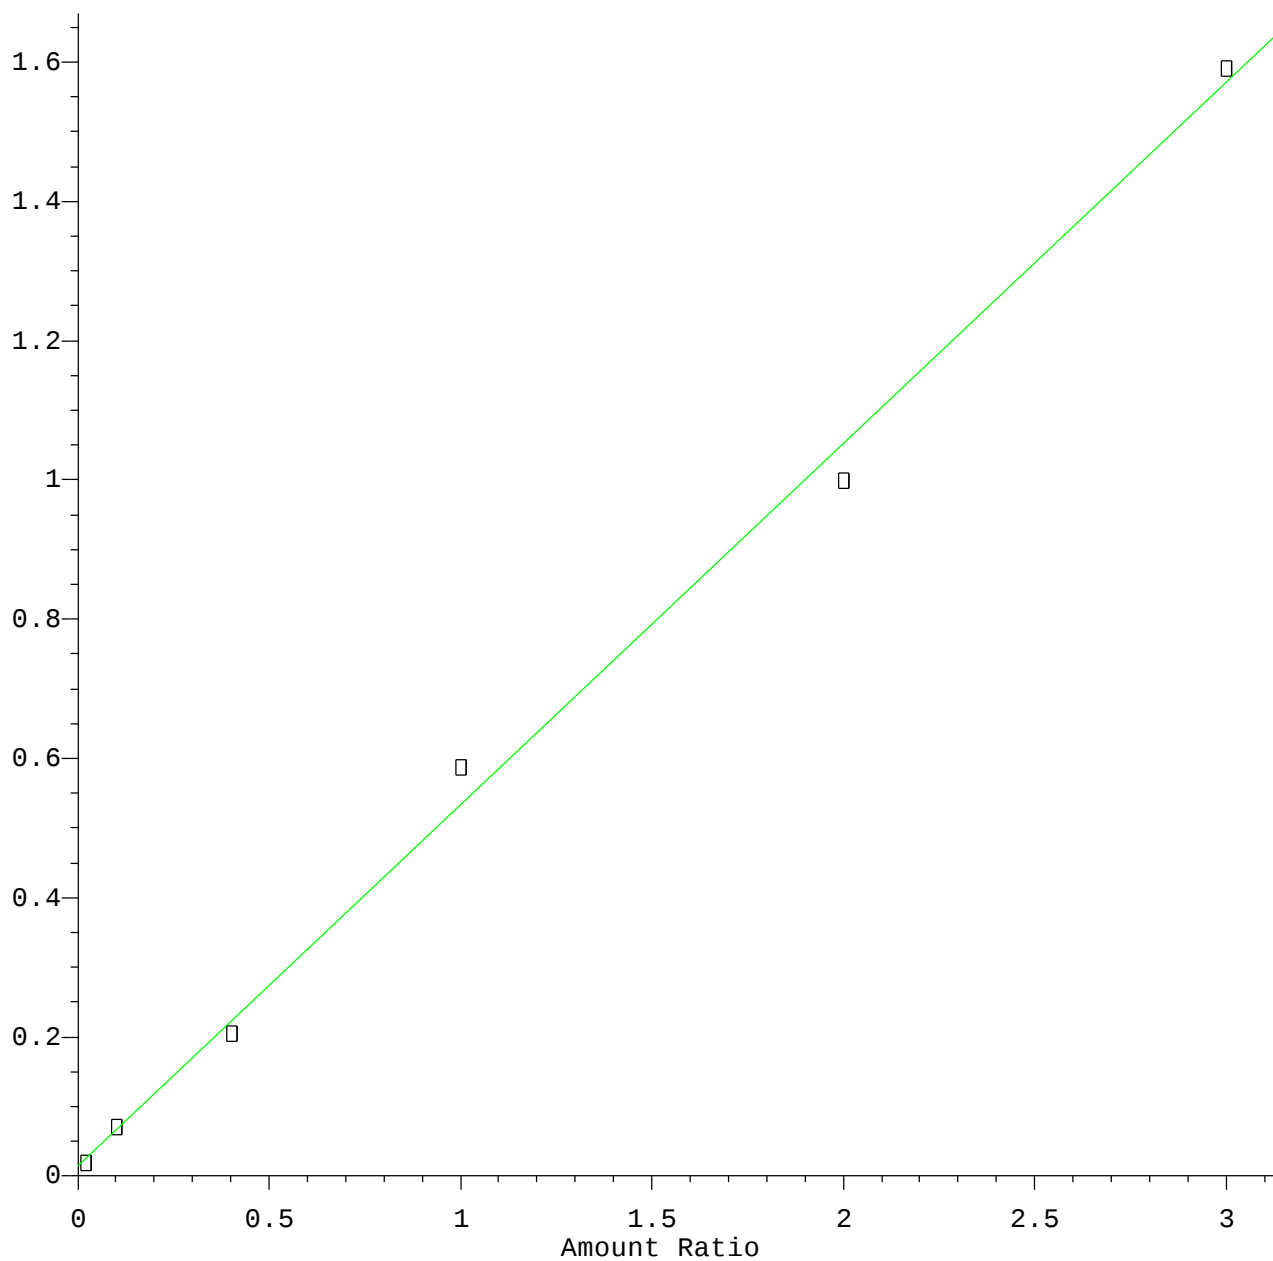


Resp Ratio =  $5.19 \times 10^{-1} \times \text{Amt} + 1.37 \times 10^{-2}$   
Coef of Det ( $r^2$ ) = 0.997    Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X072320W.M  
Calibration Table Last Updated: Thu Jul 23 12:25:12 2020


# Dichlorodifluoromethane

Response Ratio

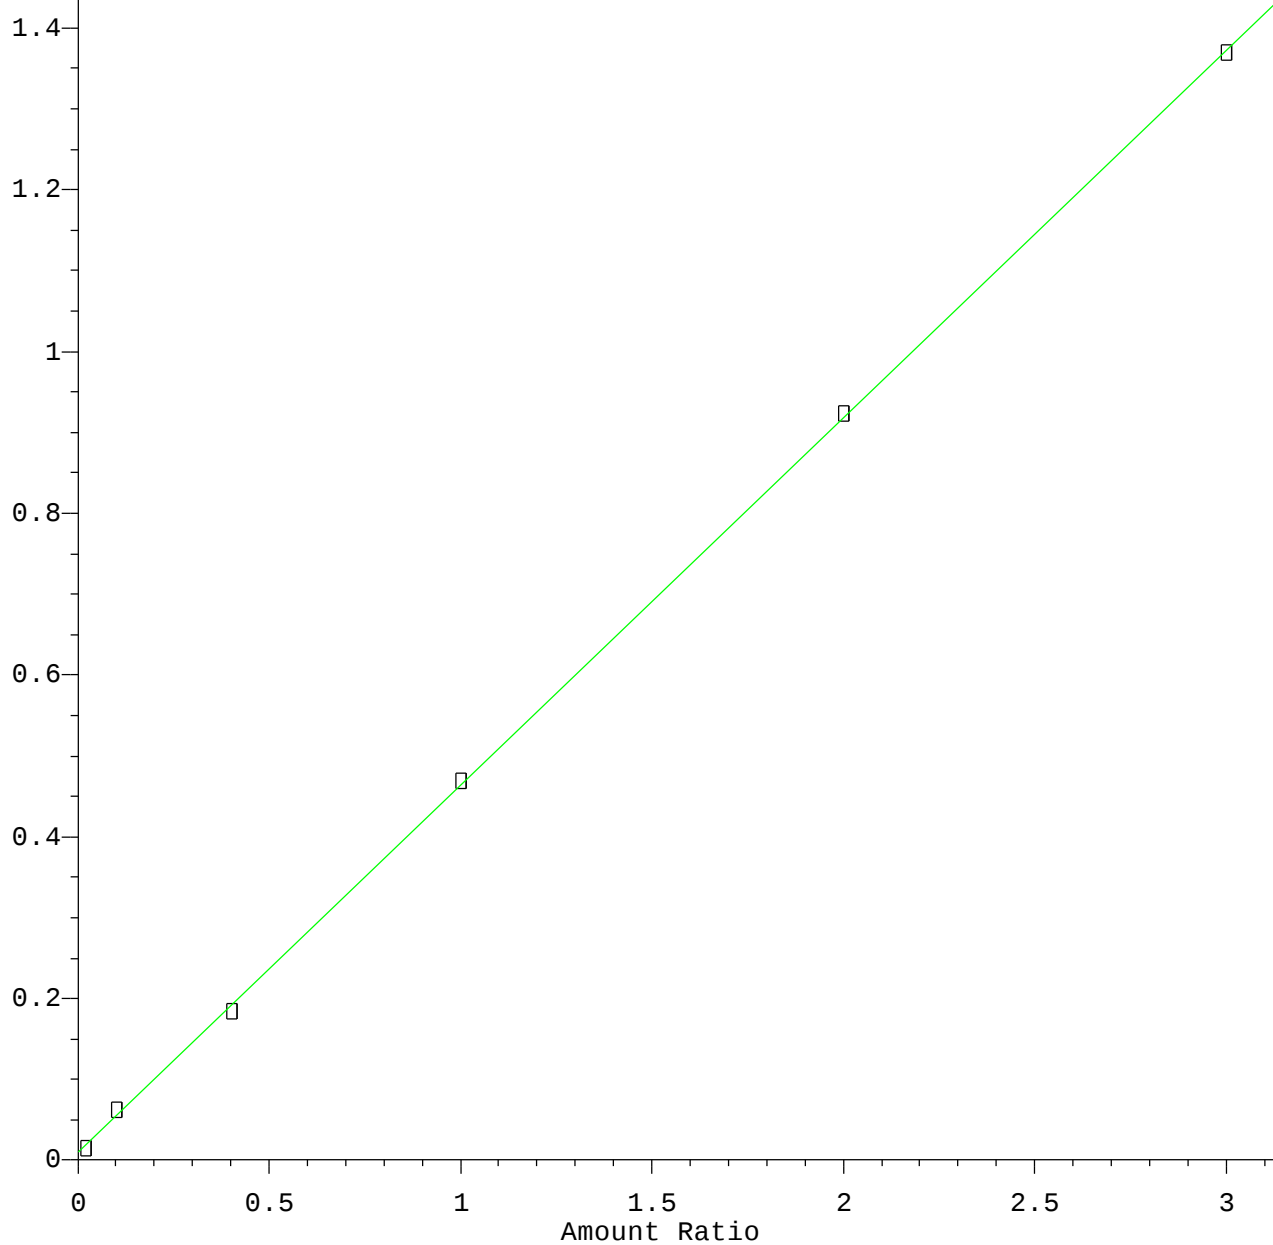


Resp Ratio =  $4.54 \times 10^{-1} \times \text{Amt} + 9.45 \times 10^{-3}$   
Coef of Det ( $r^2$ ) = 1.000    Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X072320W.M  
Calibration Table Last Updated: Thu Jul 23 12:25:12 2020

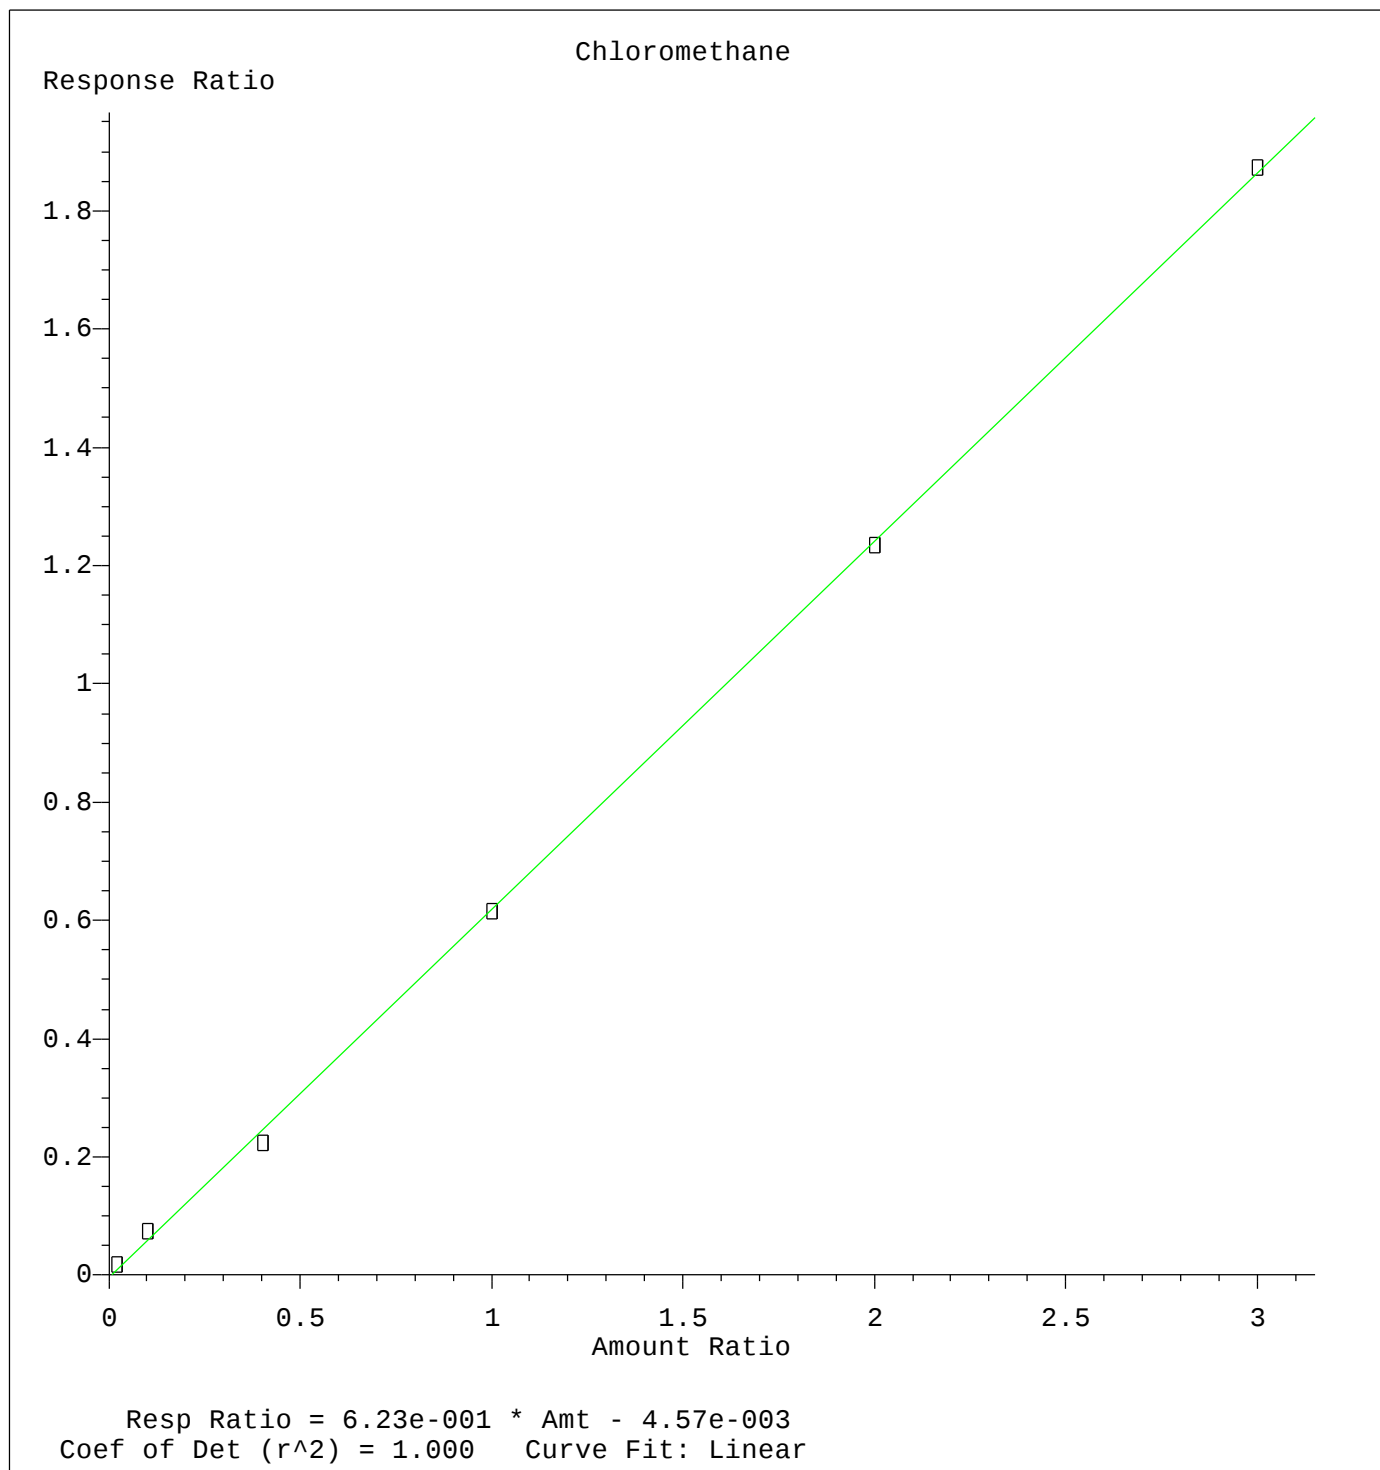


Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X072320W.M  
Calibration Table Last Updated: Thu Jul 23 12:25:12 2020

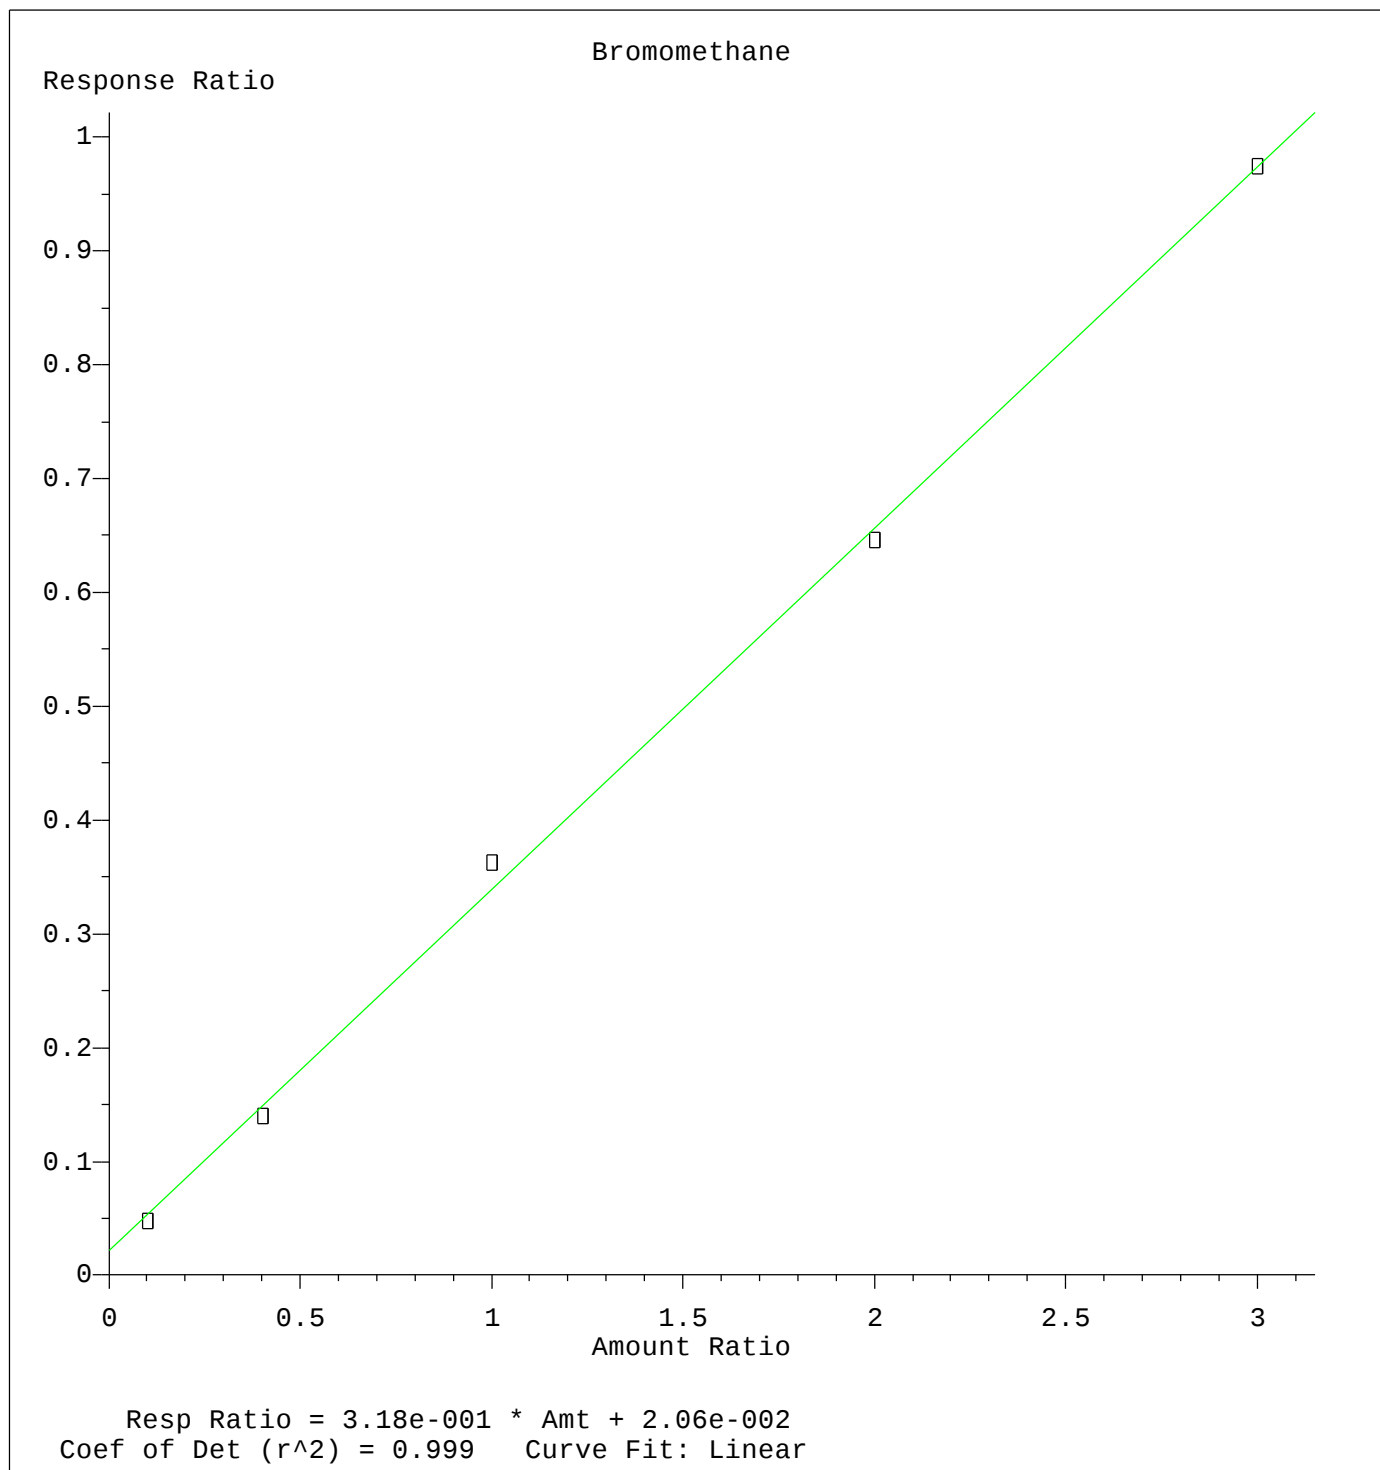

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X072320W.M  
Calibration Table Last Updated: Thu Jul 23 12:25:12 2020

# Chloroethane

Response Ratio

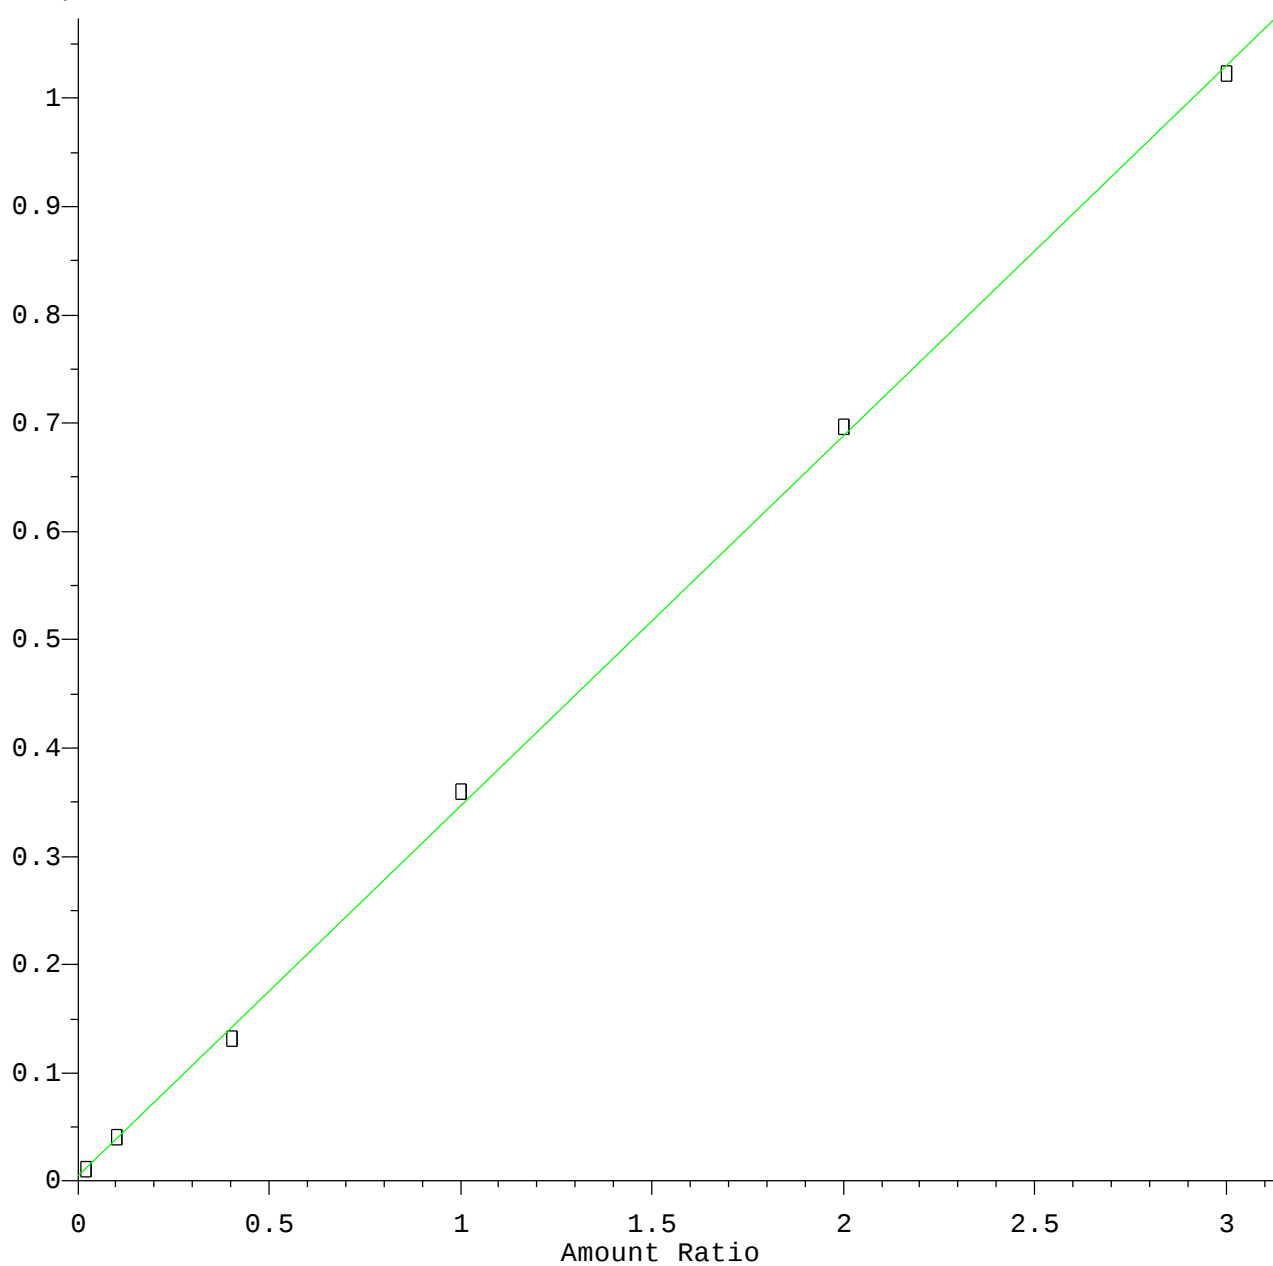

Resp Ratio = 3.42e-001 \* Amt + 5.30e-003  
Coef of Det (r<sup>2</sup>) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X072320W.M  
Calibration Table Last Updated: Thu Jul 23 12:25:12 2020