

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX072320\
 Data File : VX017524.D
 Acq On : 24 Jul 2020 04:31
 Operator : JC/SP
 Sample : PB130403ZHE#14
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 PB130403ZHE#14

Quant Time: Jul 24 07:34:44 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X072320W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jul 24 05:48:09 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.64	168	493872	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.84	114	840350	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.10	117	943217	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.06	152	490077	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.04	65	347410	54.76	ug/l	0.00
Spiked Amount 50.000			Recovery	=	109.52%	
35) Dibromofluoromethane	5.47	113	290755	51.73	ug/l	0.00
Spiked Amount 50.000			Recovery	=	103.46%	
50) Toluene-d8	8.70	98	1082604	53.40	ug/l	0.00
Spiked Amount 50.000			Recovery	=	106.80%	
62) 4-Bromofluorobenzene	11.12	95	477545	58.85	ug/l	0.00
Spiked Amount 50.000			Recovery	=	117.70%	
Target Compounds						
16) Acetone	2.42	43	74878	26.817	ug/l	96
18) Methyl Acetate	2.75	43	7194	1.094	ug/l #	83
20) Methylene Chloride	2.84	84	41974	6.874	ug/l	98
43) Isopropyl Acetate	6.42	43	163625	11.246	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX072320\
Data File : VX017524.D
Acq On : 24 Jul 2020 04:31
Operator : JC/SP
Sample : PB130403ZHE#14
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PB130403ZHE#14

Quant Time: Jul 24 07:34:44 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X072320W.M
Quant Title : SW846 8260
QLast Update : Fri Jul 24 05:48:09 2020
Response via : Initial Calibration

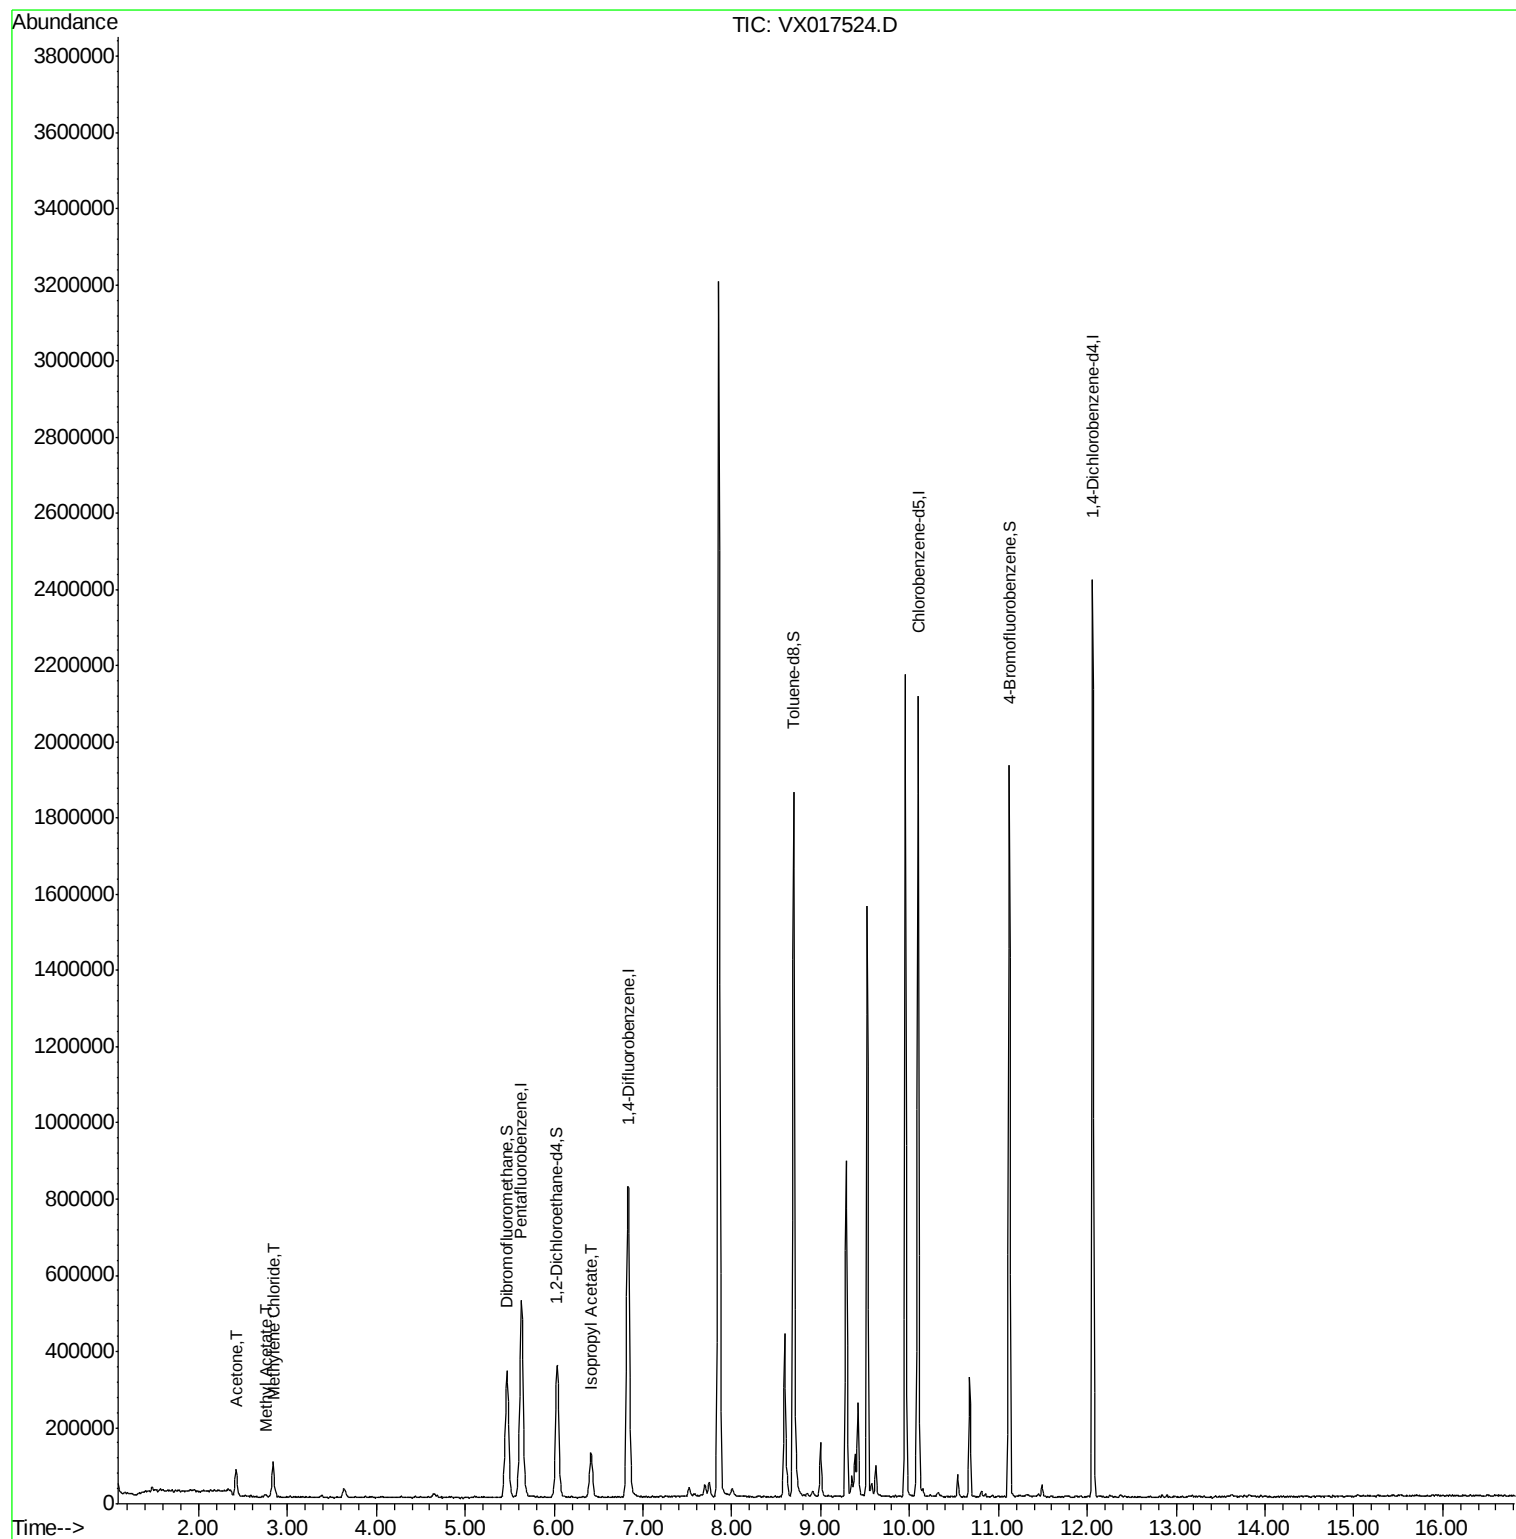

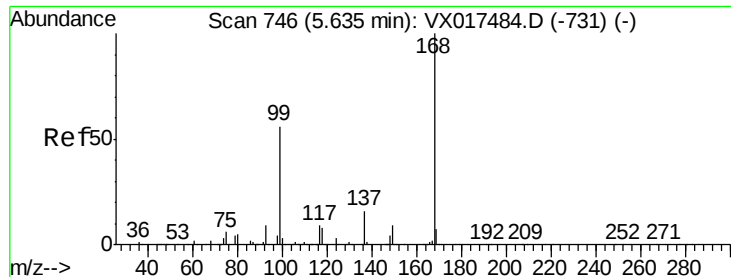

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.64 min Scan# 746

Delta R.T. -0.00 min

Lab File: VX017524.D

Acq: 24 Jul 2020 04:31

Instrument :

MSVOA_X

ClientSampleId :


PB130403ZHE#14

Tot Ion:168 Resp: 493872

Ion Ratio Lower Upper

168 100

99 59.1 43.4 65.2

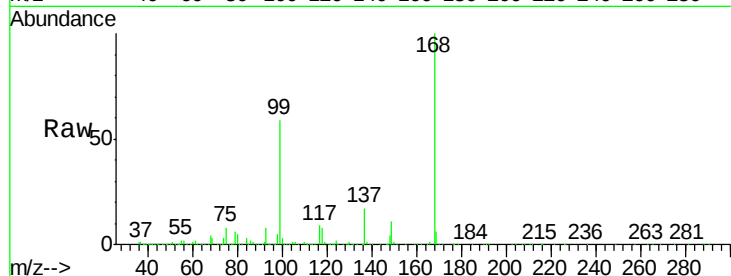

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.64

200000

150000



100000

50000

0

Time-->

5.50 5.60 5.70

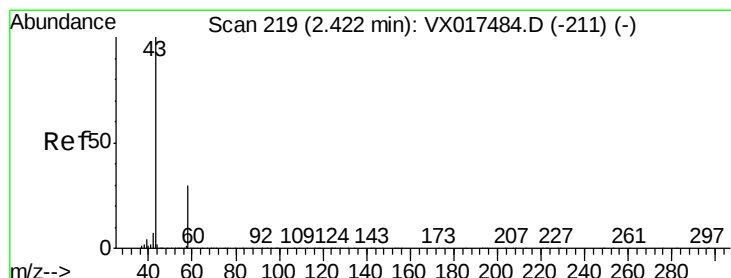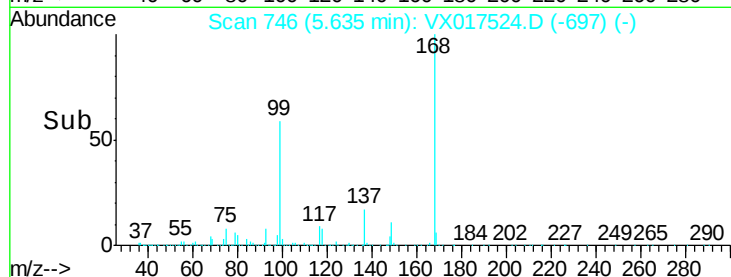

#16

Acetone

Concen: 26.817 ug/l

RT: 2.42 min Scan# 219

Delta R.T. -0.00 min

Lab File: VX017524.D


Acq: 24 Jul 2020 04:31

Tgt Ion: 43 Resp: 74878

Ion Ratio Lower Upper

43 100

58 32.4 24.2 36.4

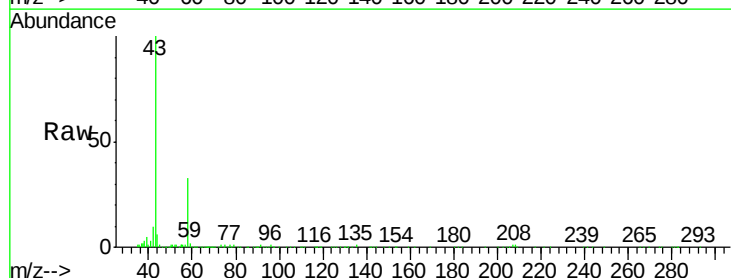

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

2.42

50000

40000

30000


20000


10000

0

Time-->

2.35 2.40 2.45 2.50




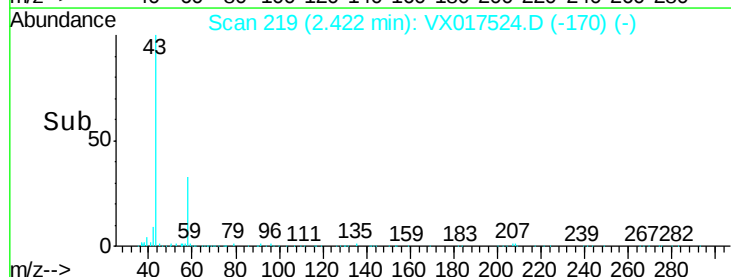


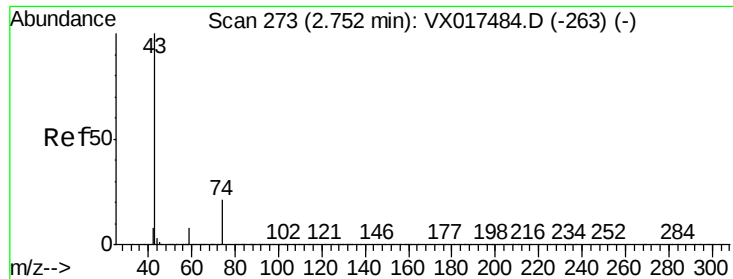

#18
Methyl Acetate
Concen: 1.094 ug/l
RT: 2.75 min Scan# 273
Delta R.T. -0.00 min
Lab File: VX017524.D
Acq: 24 Jul 2020 04:31




Instrument :
MSVOA_X
ClientSampleId :
PB130403ZHE#14


Tot Ion: 43 Resp: 7194
Ion Ratio Lower Upper
43 100
74 29.8 17.5 26.3#

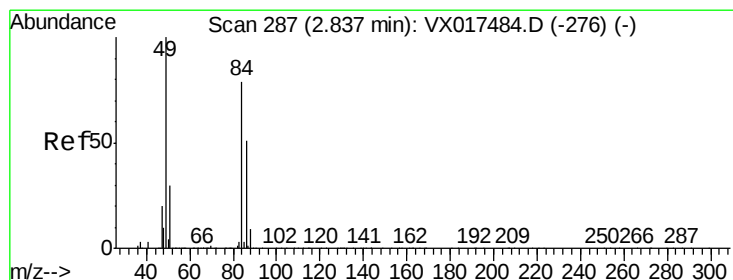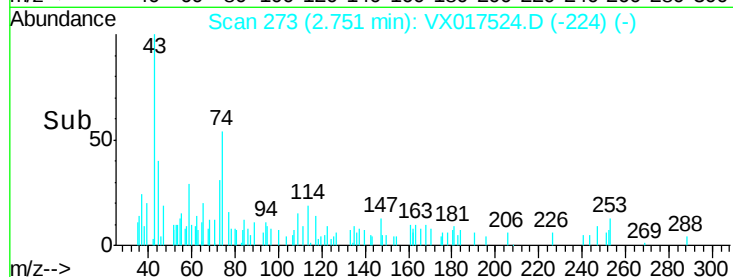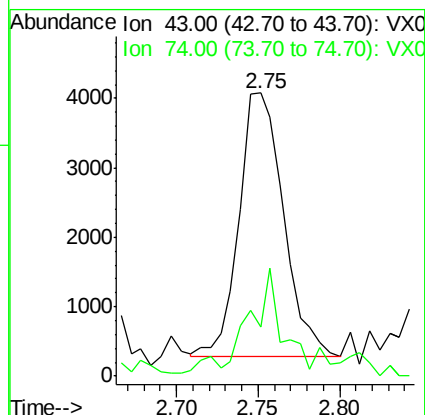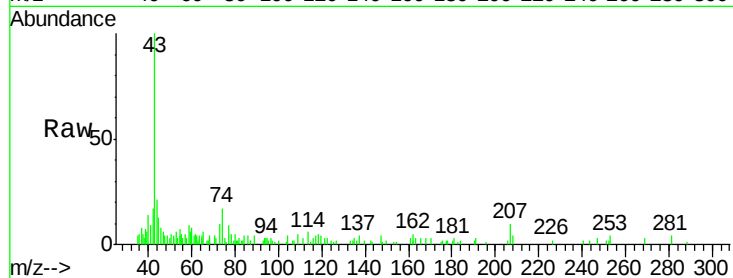

#20
Methylene Chloride
Concen: 6.874 ug/l
RT: 2.84 min Scan# 287
Delta R.T. 0.00 min
Lab File: VX017524.D
Acq: 24 Jul 2020 04:31

Tgt Ion: 84 Resp: 41974
Ion Ratio Lower Upper
84 100
49 126.1 100.3 150.5
51 35.4 30.5 45.7
86 60.9 51.1 76.7

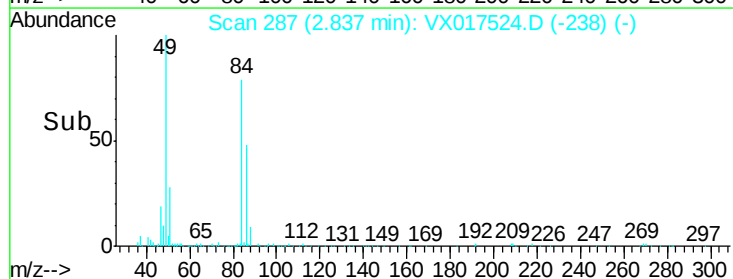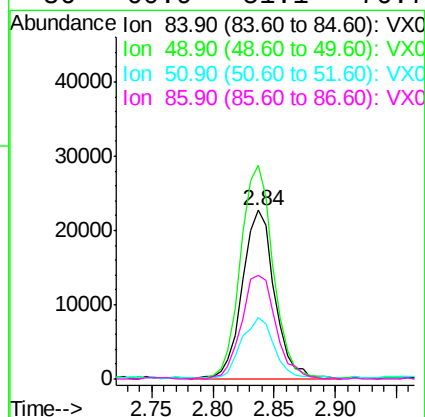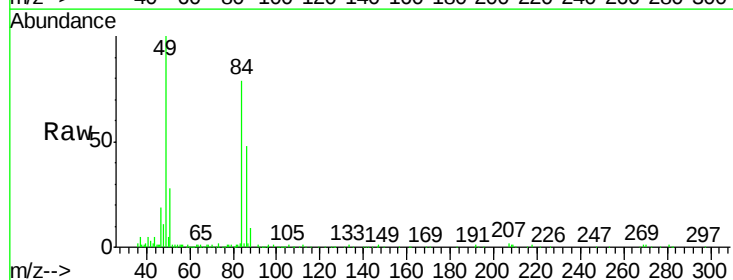

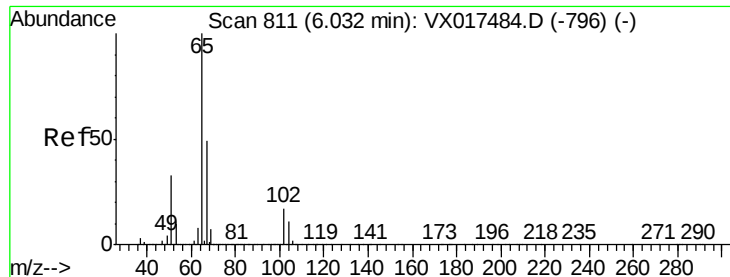

#33

1,2-Dichloroethane-d4

Concen: 54.762 ug/l

RT: 6.04 min Scan# 812

Delta R.T. 0.01 min

Lab File: VX017524.D

Acq: 24 Jul 2020 04:31

Instrument :

MSVOA_X

ClientSampleId :


PB130403ZHE#14

Tot Ion: 65 Resp: 347410

Ion Ratio Lower Upper

65 100

67 51.7 0.0 102.8

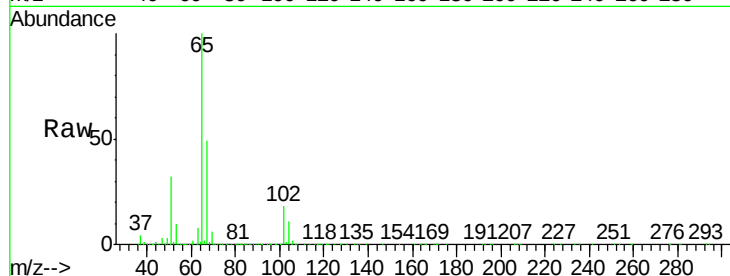

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

6.04



150000

100000

50000

0

Time--> 5.90 6.00 6.10

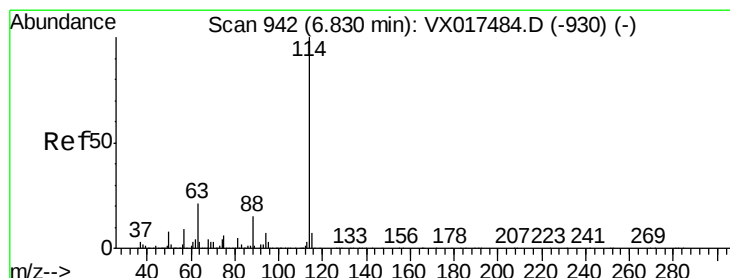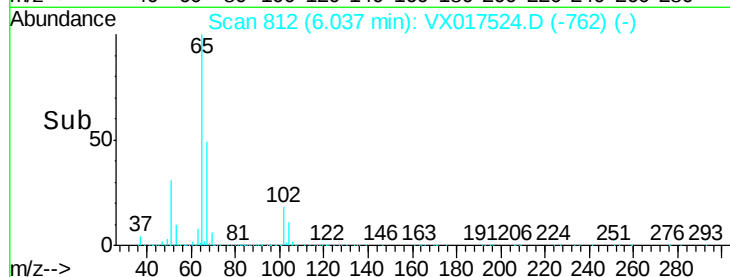

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.84 min Scan# 943

Delta R.T. 0.01 min

Lab File: VX017524.D

Acq: 24 Jul 2020 04:31


Tgt Ion: 114 Resp: 840350

Ion Ratio Lower Upper

114 100

63 19.8 0.0 40.6

88 15.2 0.0 33.4

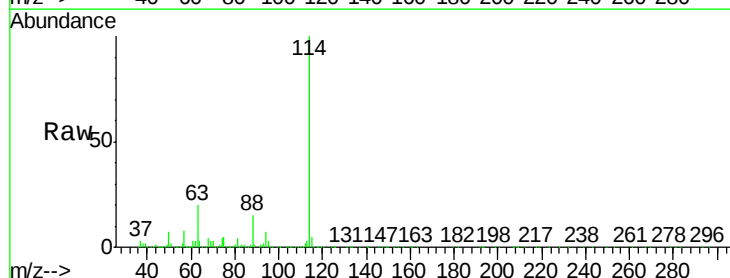

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

6.84

400000


300000


200000

100000

0

Time--> 6.70 6.80 6.90

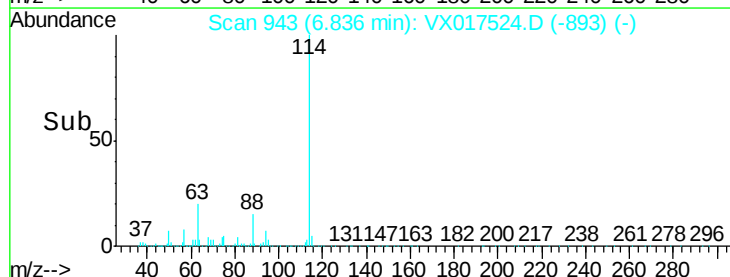

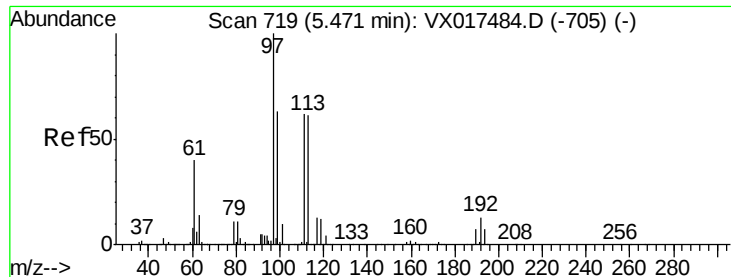

#35

Dibromofluoromethane

Concen: 51.733 ug/l

RT: 5.47 min Scan# 719

Delta R.T. -0.00 min

Lab File: VX017524.D

Acq: 24 Jul 2020 04:31

Instrument :

MSVOA_X

ClientSampleId :

PB130403ZHE#14


Tot Ion:113 Resp: 290755

Ion Ratio Lower Upper

113 100

111 100.5 80.7 121.1




192 20.3 16.9 25.3

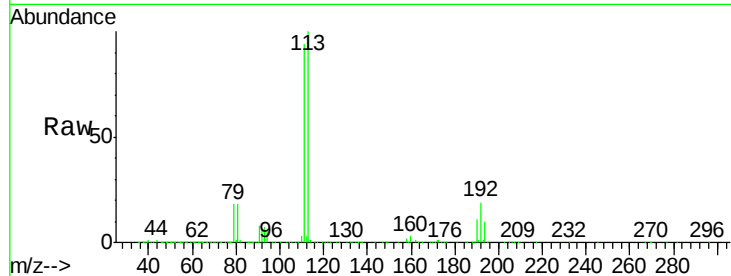

Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

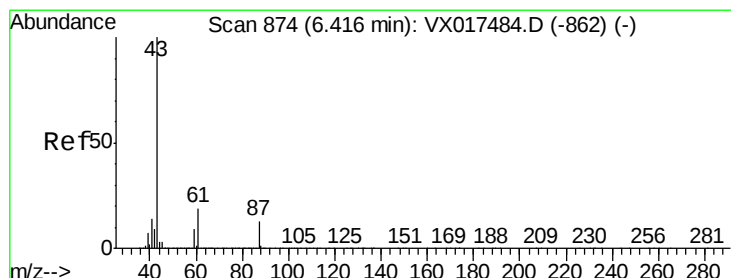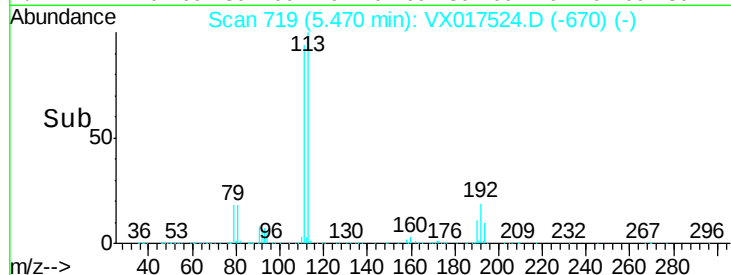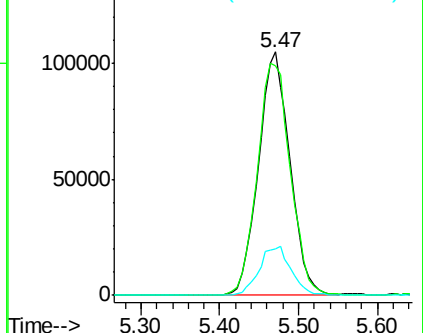

#43

Isopropyl Acetate

Concen: 11.246 ug/l

RT: 6.42 min Scan# 874

Delta R.T. -0.00 min

Lab File: VX017524.D

Acq: 24 Jul 2020 04:31


Tgt Ion: 43 Resp: 163625

Ion Ratio Lower Upper

43 100

61 19.7 15.5 23.3



87 13.8 10.5 15.7

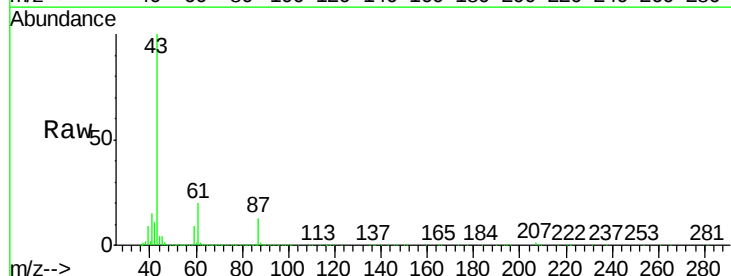


Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 61.00 (60.70 to 61.70): VX0

Ion 87.00 (86.70 to 87.70): VX0

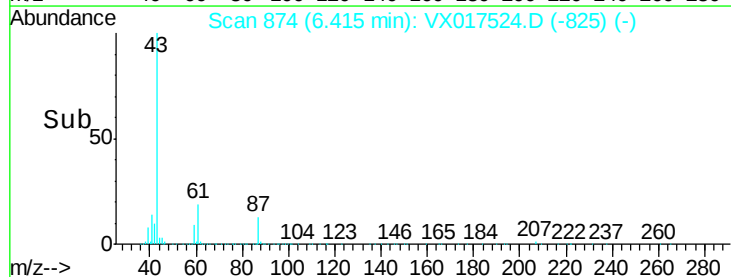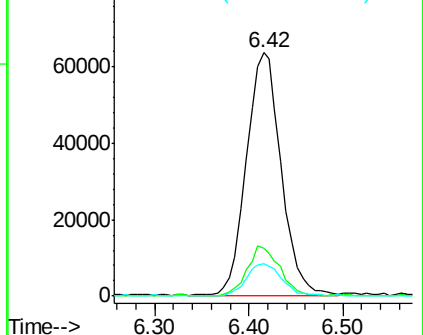

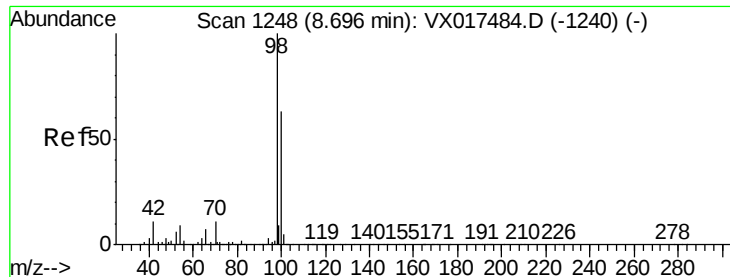

#50

Toluene-d8

Concen: 53.396 ug/l

RT: 8.70 min Scan# 1248

Delta R.T. -0.00 min

Lab File: VX017524.D

Acq: 24 Jul 2020 04:31

Instrument :

MSVOA_X

ClientSampleId :





PB130403ZHE#14

Tot Ion: 98 Resp: 1082604

Ion Ratio Lower Upper

98 100

100 64.3 52.3 78.5

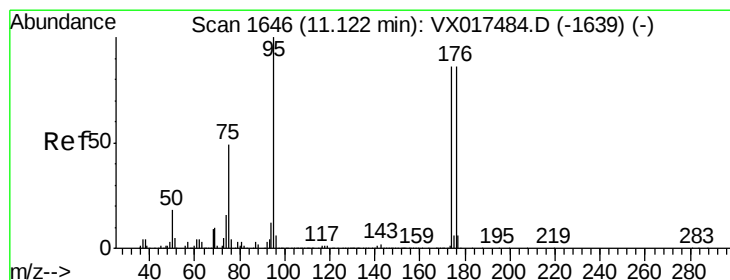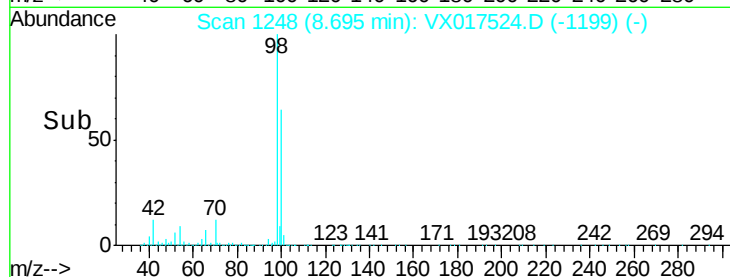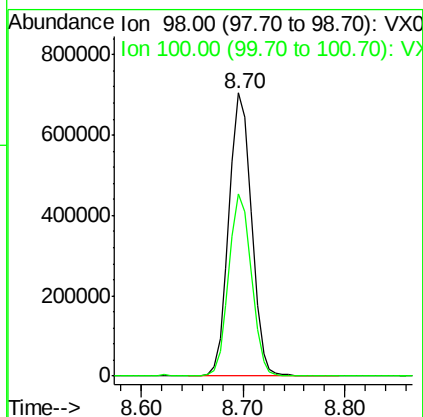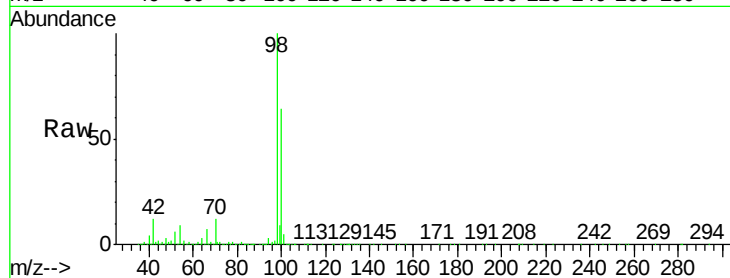

#62

4-Bromofluorobenzene

Concen: 58.853 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. -0.00 min

Lab File: VX017524.D

Acq: 24 Jul 2020 04:31




Tgt Ion: 95 Resp: 477545


Ion Ratio Lower Upper

95 100

174 83.4 0.0 169.0

176 79.9 0.0 161.0


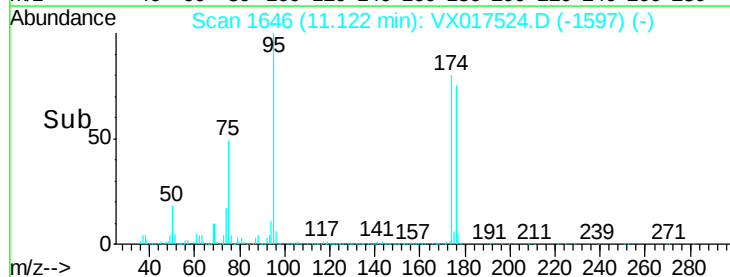
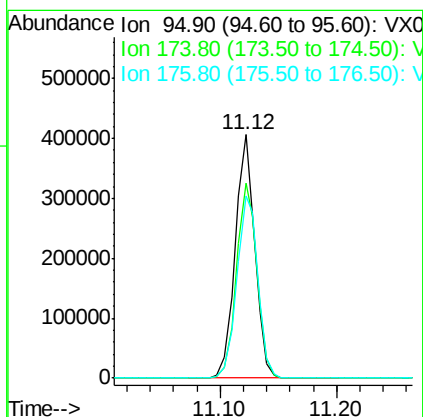
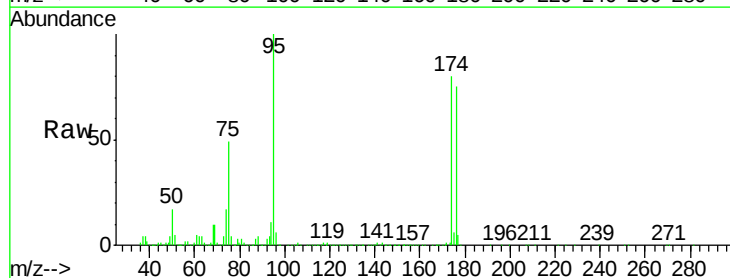


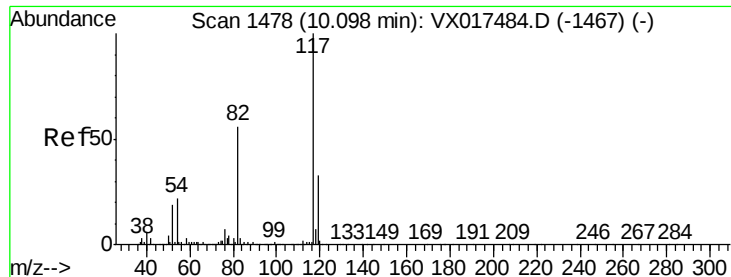

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.10 min Scan# 1478
Delta R.T. -0.00 min
Lab File: VX017524.D
Acq: 24 Jul 2020 04:31

Instrument :
MSVOA_X
ClientSampleId :
PB130403ZHE#14

Tot Ion:117 Resp: 943217
Ion Ratio Lower Upper
117 100
82 55.5 44.0 66.0
119 31.4 25.4 38.0

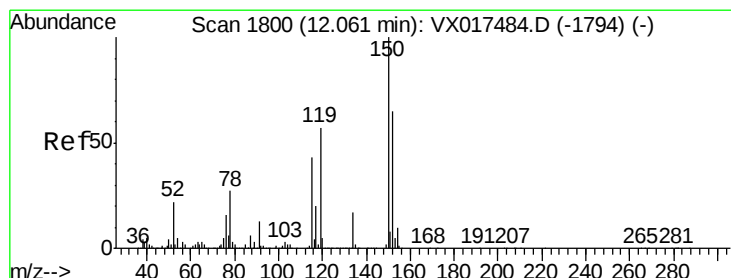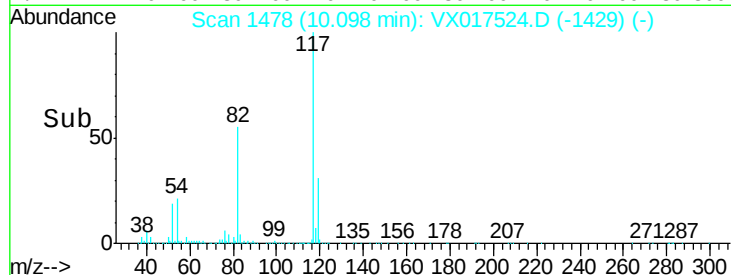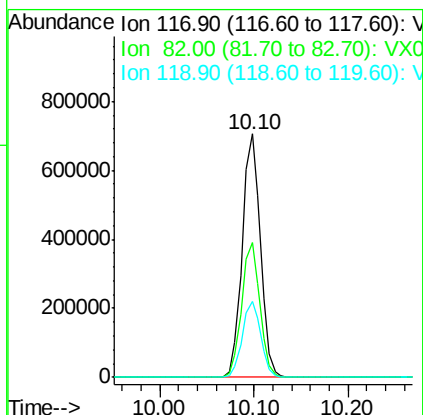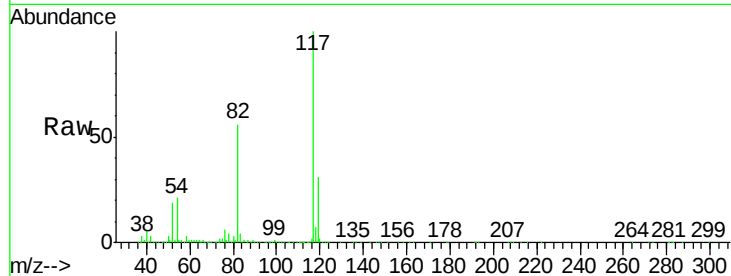

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.06 min Scan# 1800
Delta R.T. -0.00 min
Lab File: VX017524.D
Acq: 24 Jul 2020 04:31

Tgt Ion:152 Resp: 490077
Ion Ratio Lower Upper
152 100
115 59.3 65.5 196.6#
150 156.3 0.0 412.6

