

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072321\
 Data File : VX023416.D
 Acq On : 23 Jul 2021 11:29
 Operator : JC/MD
 Sample : M3145-01 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 152140-DDC-5-PS

Integration Parameters: RTEINT.P
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
 Title : SW846 8260

Signal : TIC: VX023416.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.252	24	27	33	rBV	112227	97930	10.13%	1.983%
2	1.563	70	78	81	rBV3	6652	13491	1.40%	0.273%
3	5.397	694	707	721	rBV2	112191	327838	33.91%	6.638%
4	5.562	721	734	749	rVB2	189898	535008	55.34%	10.832%
5	5.964	790	800	820	rBV	123249	323590	33.47%	6.552%
6	6.769	922	932	945	rBV	298833	709346	73.38%	14.362%
7	8.653	1234	1241	1250	rBV	631572	966714	100.00%	19.573%
8	10.055	1465	1471	1490	rBV	590125	798802	82.63%	16.173%
9	11.085	1634	1640	1650	rBV	442668	554191	57.33%	11.220%
10	12.024	1789	1794	1803	rBV	504554	612220	63.33%	12.395%




Sum of corrected areas: 4939130

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072321\
Data File : VX023416.D
Acq On : 23 Jul 2021 11:29
Operator : JC/MD
Sample : M3145-01 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-5-PS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

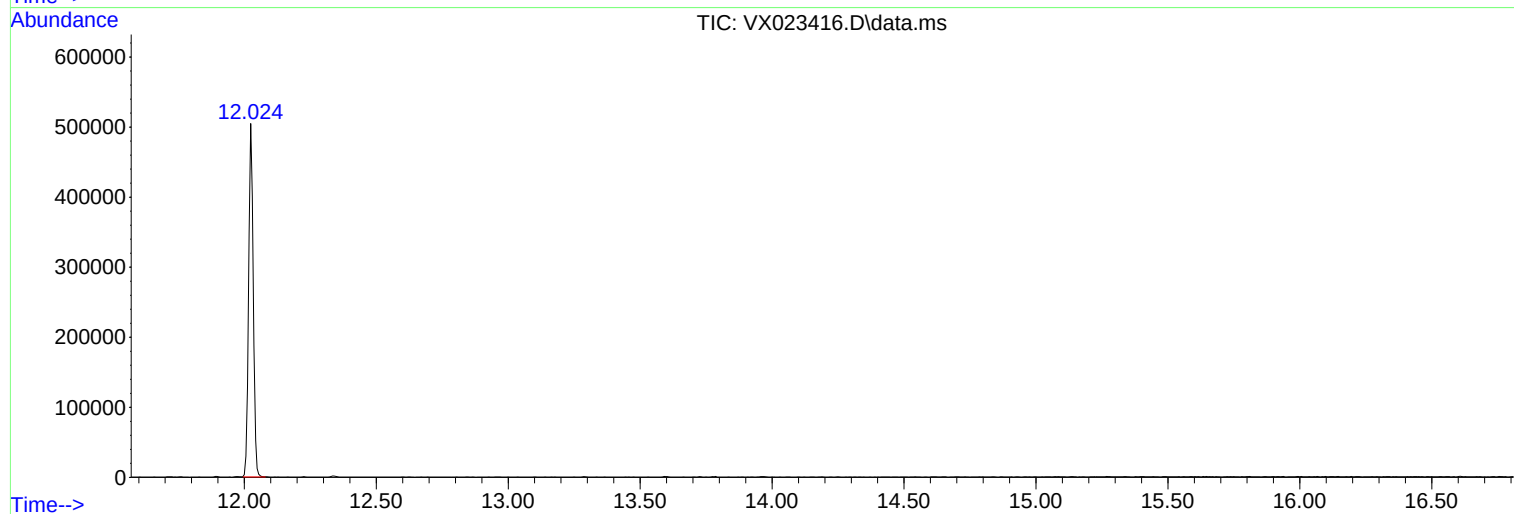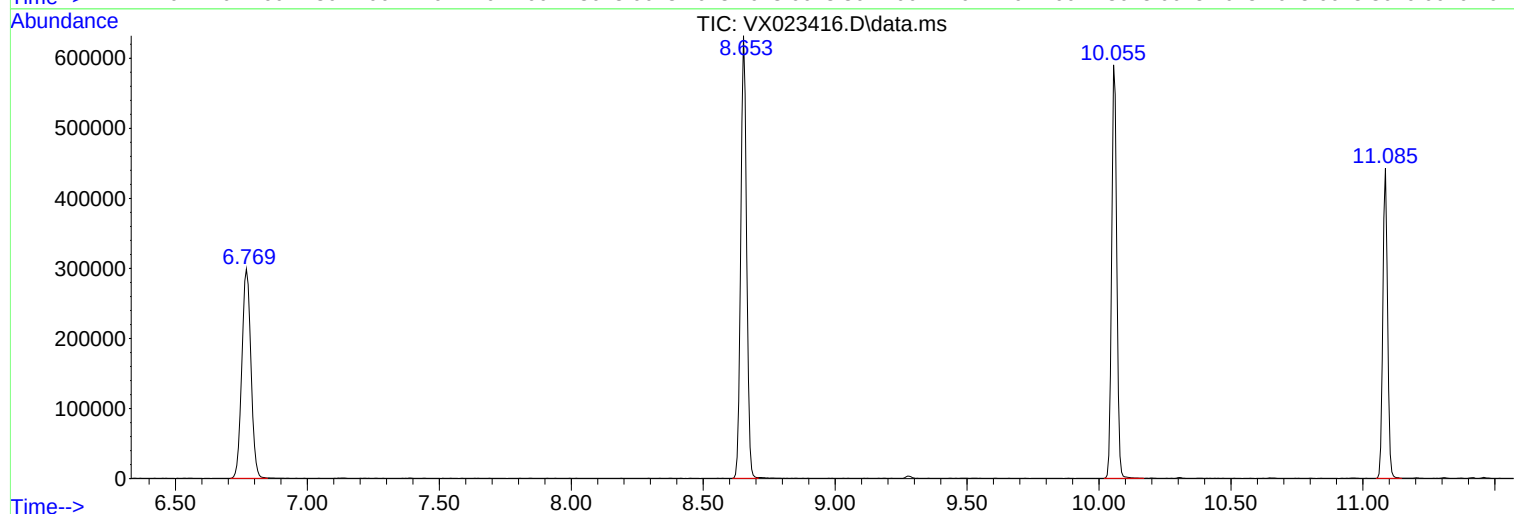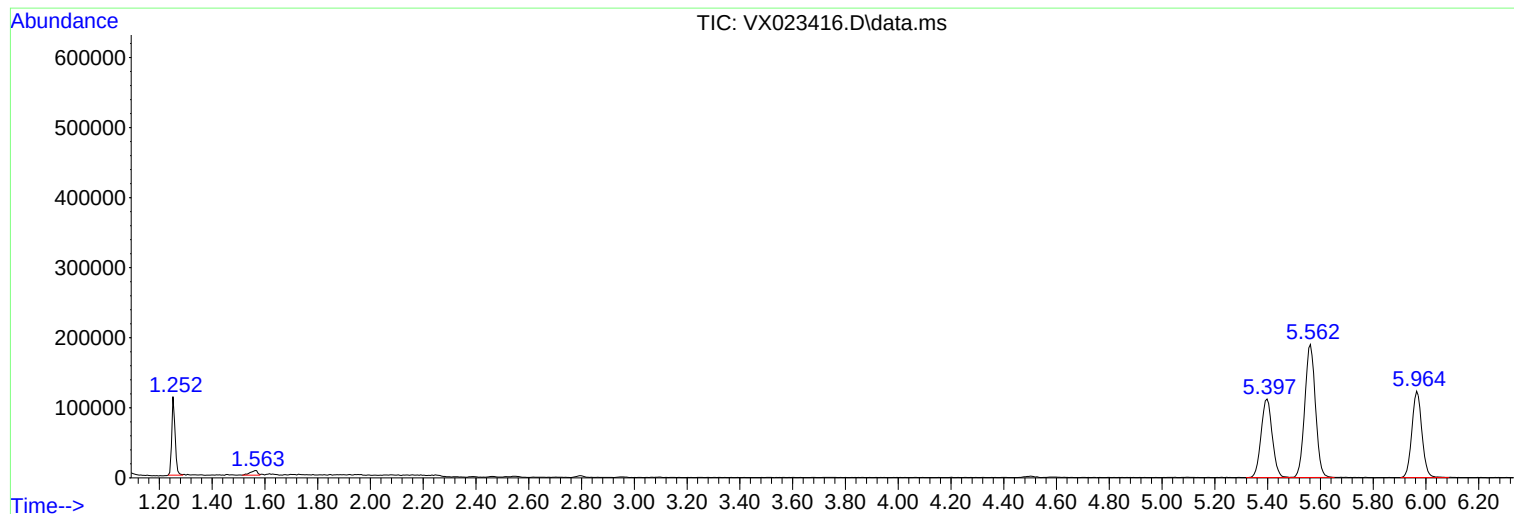

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072321\
Data File : VX023416.D
Acq On : 23 Jul 2021 11:29
Operator : JC/MD
Sample : M3145-01 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-5-PS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072321\
Data File : VX023416.D
Acq On : 23 Jul 2021 11:29
Operator : JC/MD
Sample : M3145-01 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-5-PS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
