

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072321\
 Data File : VX023417.D
 Acq On : 23 Jul 2021 11:52
 Operator : JC/MD
 Sample : M3145-02 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 152140-DDC-6-PD

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M

Title : SW846 8260

Signal : TIC: VX023417.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.252	24	27	37	rVB	135666	122648	13.80%	2.651%
2	1.556	72	77	82	rBV3	5040	9754	1.10%	0.211%
3	5.397	693	707	721	rBV2	105432	303670	34.16%	6.564%
4	5.562	721	734	751	rVB	174874	495128	55.70%	10.702%
5	5.964	789	800	815	rBV2	116629	303196	34.11%	6.554%
6	6.769	922	932	945	rBV	278089	657610	73.98%	14.215%
7	8.653	1234	1241	1255	rBV	573760	888904	100.00%	19.214%
8	10.055	1466	1471	1479	rBV	539865	731563	82.30%	15.813%
9	11.085	1634	1640	1653	rVB	417643	522560	58.79%	11.295%
10	12.024	1789	1794	1803	rBV	486848	591272	66.52%	12.781%


Sum of corrected areas: 4626305

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072321\
Data File : VX023417.D
Acq On : 23 Jul 2021 11:52
Operator : JC/MD
Sample : M3145-02 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-6-PD

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

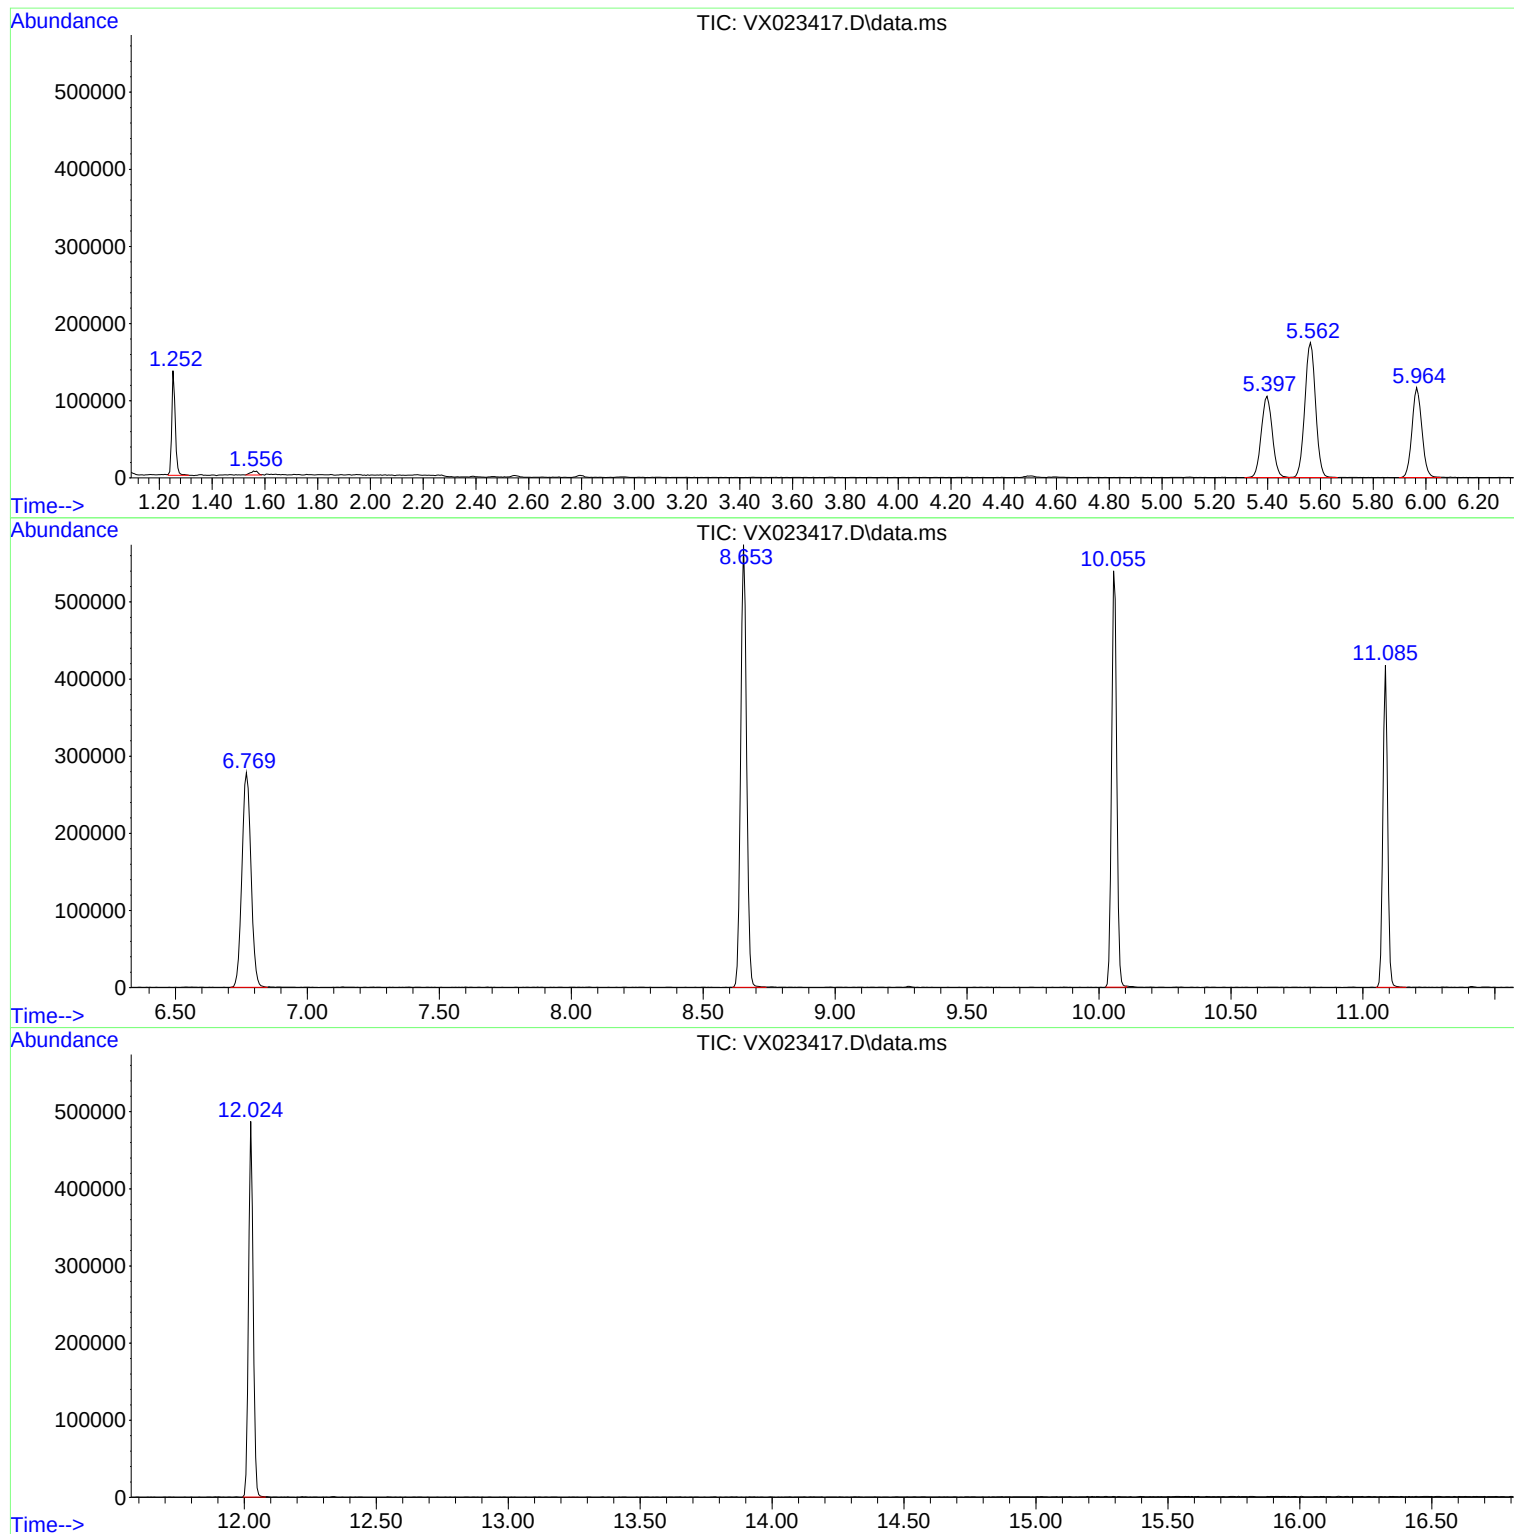

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072321\
Data File : VX023417.D
Acq On : 23 Jul 2021 11:52
Operator : JC/MD
Sample : M3145-02 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-6-PD

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072321\
Data File : VX023417.D
Acq On : 23 Jul 2021 11:52
Operator : JC/MD
Sample : M3145-02 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-6-PD

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
