

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072321\
 Data File : VX023418.D
 Acq On : 23 Jul 2021 12:16
 Operator : JC/MD
 Sample : M3145-03 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 152140-DDC-5-PD

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M

Title : SW846 8260

Signal : TIC: VX023418.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.251	24	27	33	rBV	161034	136307	14.77%	2.853%
2	1.568	70	79	83	rBV4	5328	12304	1.33%	0.258%
3	5.397	695	707	721	rBV2	106598	309389	33.52%	6.477%
4	5.562	721	734	747	rVV2	177171	505665	54.79%	10.586%
5	5.964	784	800	813	rBV2	116278	309663	33.55%	6.482%
6	6.769	921	932	945	rBV	284883	673065	72.93%	14.090%
7	8.653	1234	1241	1254	rBV	589521	922868	100.00%	19.319%
8	10.055	1465	1471	1484	rBV	568897	769366	83.37%	16.106%
9	11.085	1634	1640	1649	rBV	432854	537941	58.29%	11.261%
10	12.024	1788	1794	1802	rBV	492575	600357	65.05%	12.568%




Sum of corrected areas: 4776925

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072321\
Data File : VX023418.D
Acq On : 23 Jul 2021 12:16
Operator : JC/MD
Sample : M3145-03 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-5-PD

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

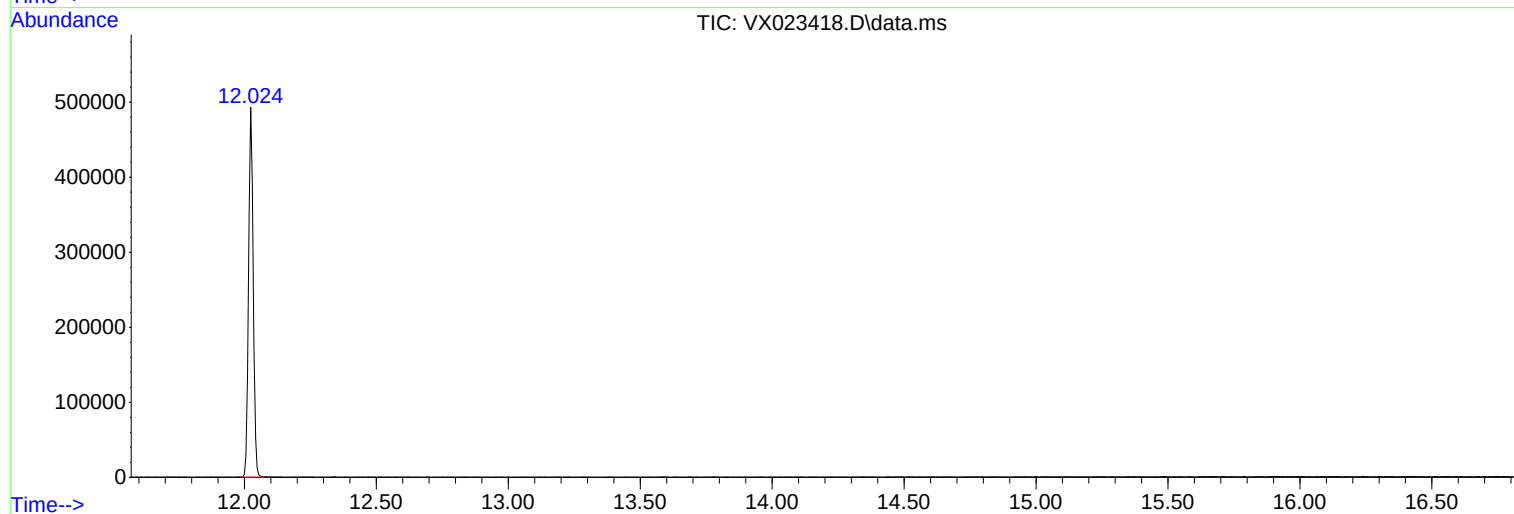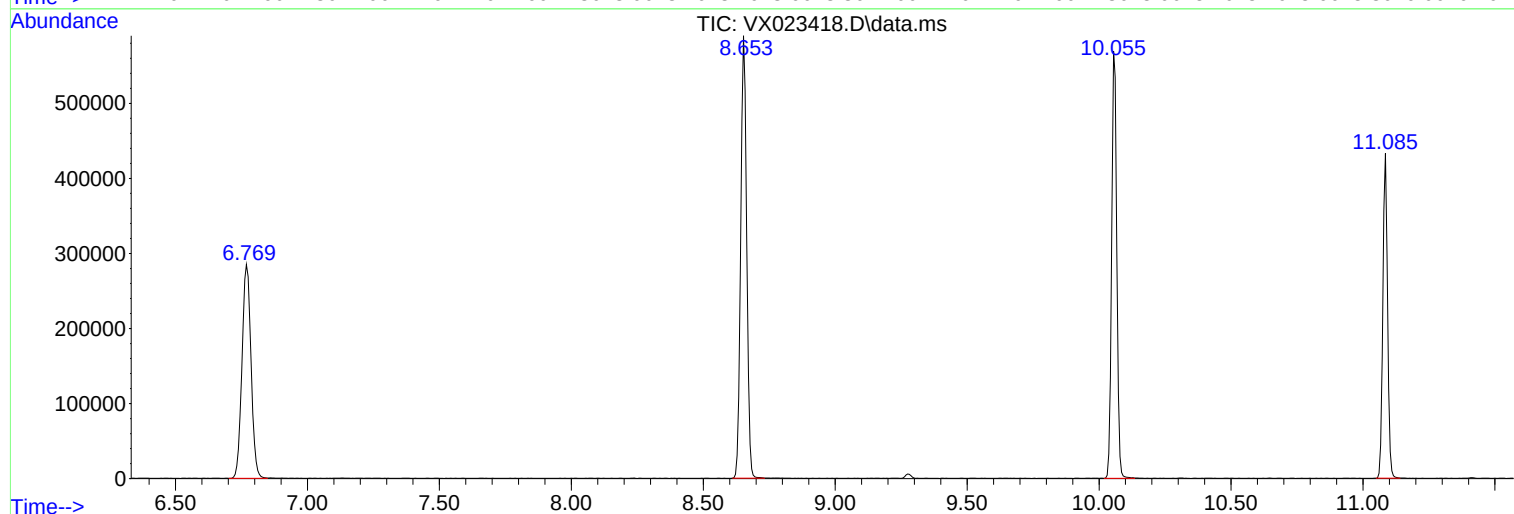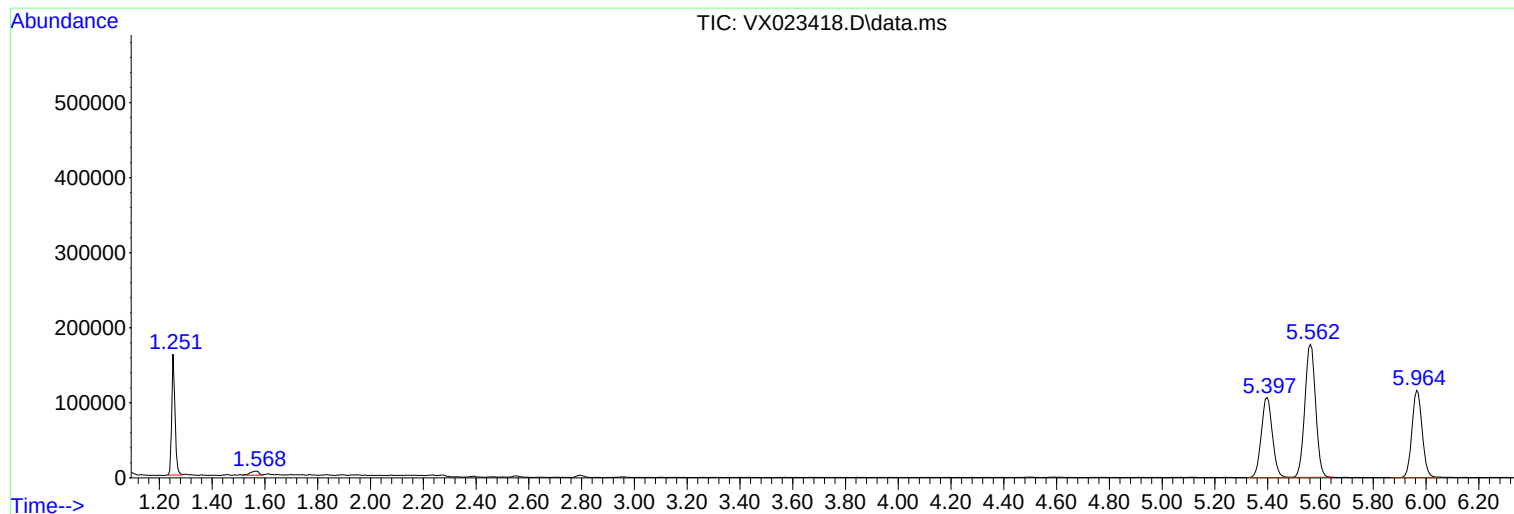

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072321\
Data File : VX023418.D
Acq On : 23 Jul 2021 12:16
Operator : JC/MD
Sample : M3145-03 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-5-PD

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072321\
Data File : VX023418.D
Acq On : 23 Jul 2021 12:16
Operator : JC/MD
Sample : M3145-03 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-5-PD

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
