

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072321\
 Data File : VX023419.D
 Acq On : 23 Jul 2021 12:40
 Operator : JC/MD
 Sample : M3145-05 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 152140-DDC-7-PS

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M

Title : SW846 8260

Signal : TIC: VX023419.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.251	24	27	33	rVB	156725	136374	15.21%	2.995%
2	1.568	70	79	83	rBV5	4879	10975	1.22%	0.241%
3	5.397	695	707	720	rBV	103374	301480	33.62%	6.622%
4	5.562	722	734	748	rVB	179369	500325	55.80%	10.989%
5	5.964	790	800	814	rBV	116276	305978	34.12%	6.721%
6	6.769	921	932	949	rBV	275249	657332	73.30%	14.438%
7	8.653	1234	1241	1252	rBV	594937	896710	100.00%	19.696%
8	10.055	1465	1471	1485	rBV	534168	728966	81.29%	16.012%
9	11.085	1634	1640	1651	rVB	394459	496324	55.35%	10.902%
10	12.024	1789	1794	1802	rBV	419726	518297	57.80%	11.384%




Sum of corrected areas: 4552761

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072321\
Data File : VX023419.D
Acq On : 23 Jul 2021 12:40
Operator : JC/MD
Sample : M3145-05 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-7-PS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

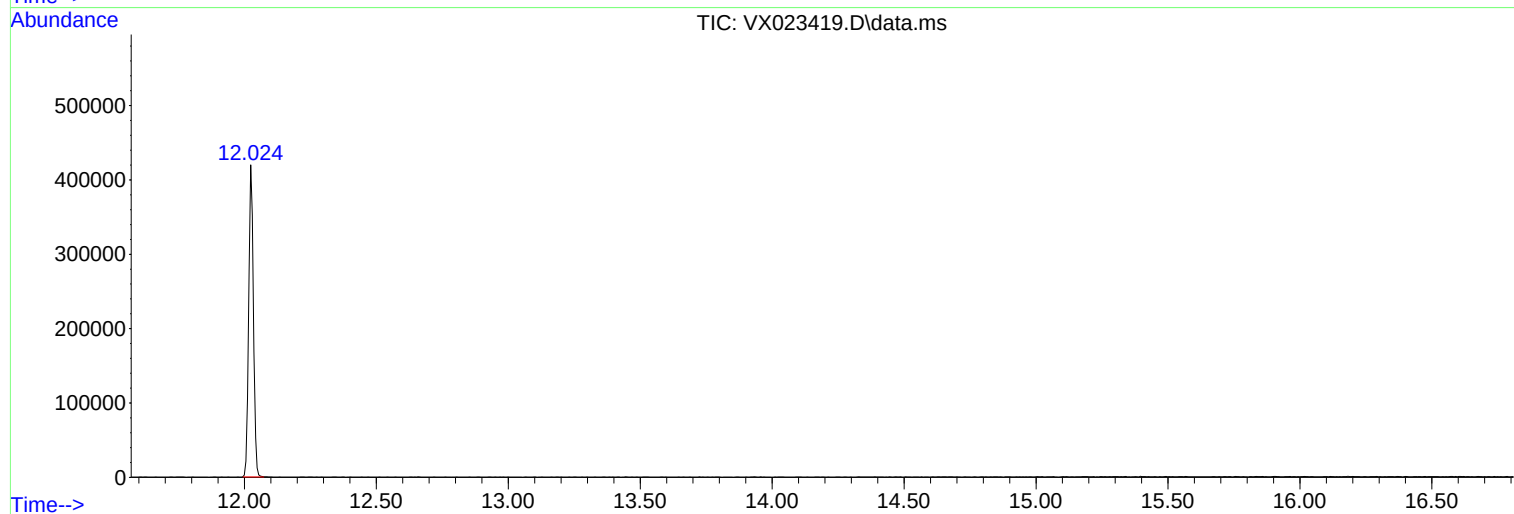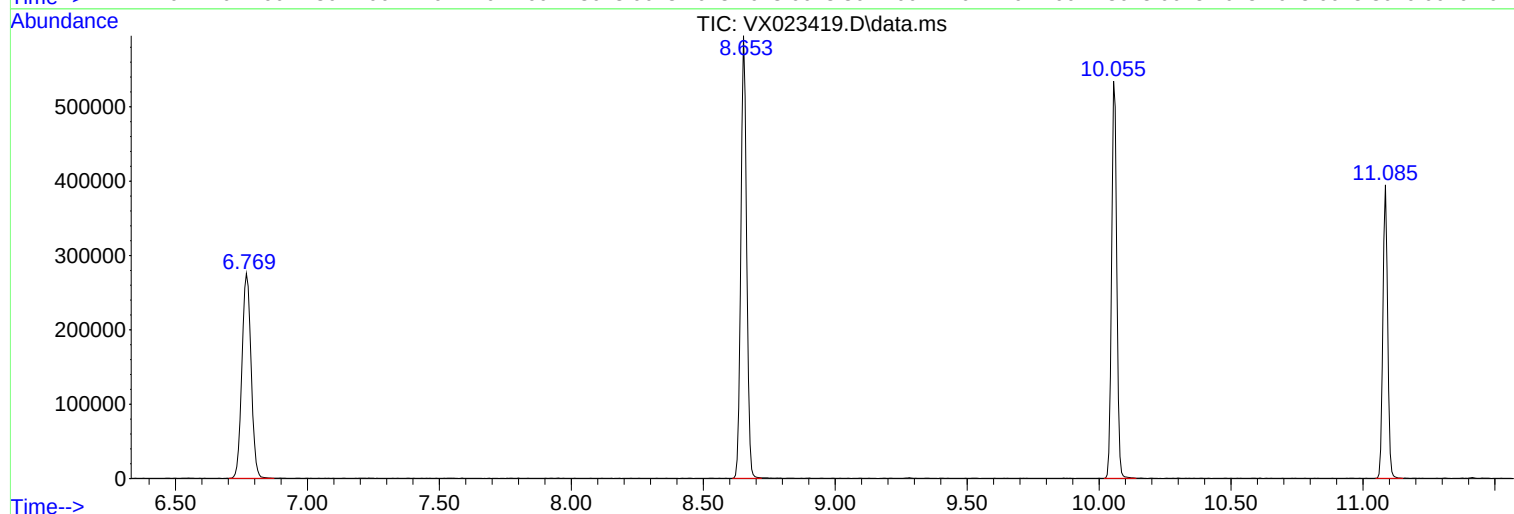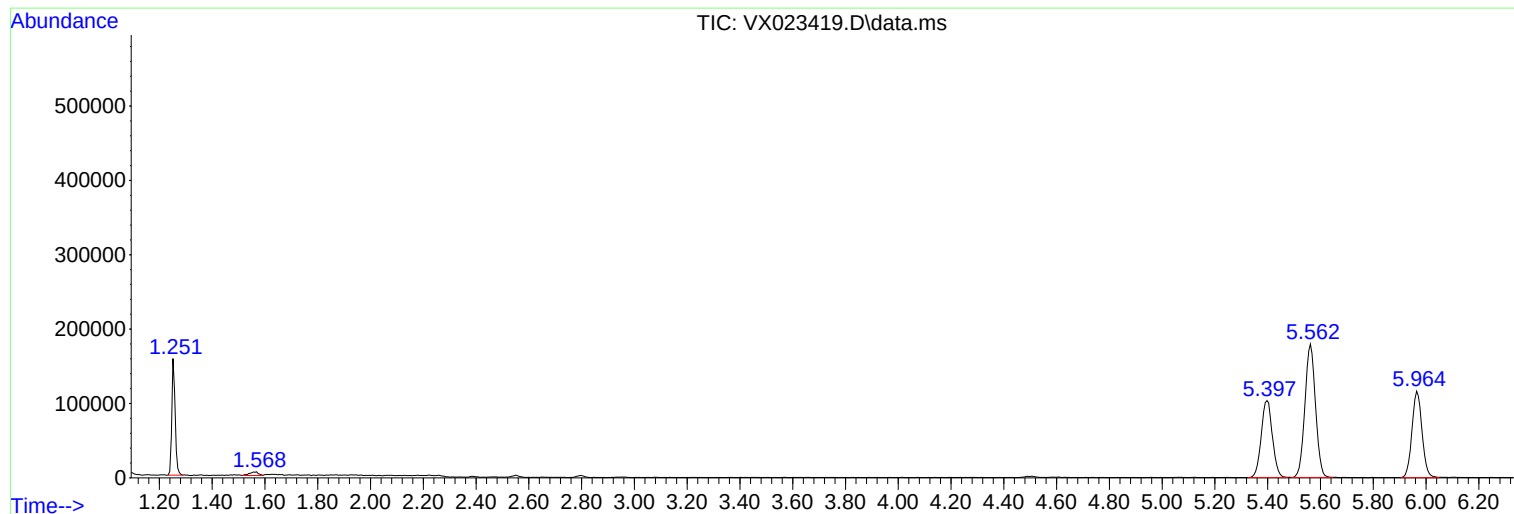

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072321\
Data File : VX023419.D
Acq On : 23 Jul 2021 12:40
Operator : JC/MD
Sample : M3145-05 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-7-PS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072321\
Data File : VX023419.D
Acq On : 23 Jul 2021 12:40
Operator : JC/MD
Sample : M3145-05 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-7-PS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------