

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072321\
 Data File : VX023420.D
 Acq On : 23 Jul 2021 13:03
 Operator : JC/MD
 Sample : M3145-09 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 152140-DDC-8-PD

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M

Title : SW846 8260

Signal : TIC: VX023420.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.252	24	27	34	rBV	166018	143963	15.76%	3.069%
2	5.397	695	707	719	rBV	106571	306297	33.53%	6.529%
3	5.562	723	734	748	rVB2	178524	498474	54.57%	10.625%
4	5.964	789	800	814	rBV	115607	310457	33.99%	6.617%
5	6.769	922	932	942	rBV	285429	673153	73.70%	14.348%
6	8.653	1234	1241	1251	rBV	595131	913410	100.00%	19.470%
7	10.055	1465	1471	1487	rVB	557748	755581	82.72%	16.105%
8	11.085	1634	1640	1652	rVB	413938	523525	57.32%	11.159%
9	12.024	1789	1794	1803	rVB	451074	566608	62.03%	12.077%




Sum of corrected areas: 4691468

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072321\
Data File : VX023420.D
Acq On : 23 Jul 2021 13:03
Operator : JC/MD
Sample : M3145-09 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-8-PD

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

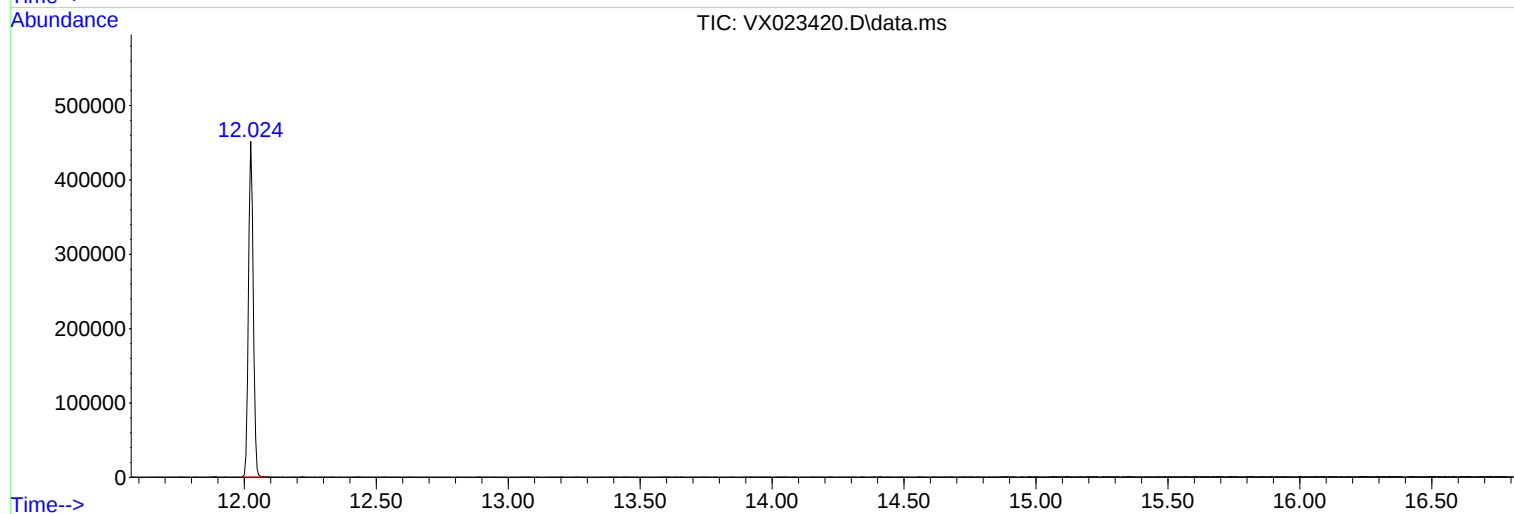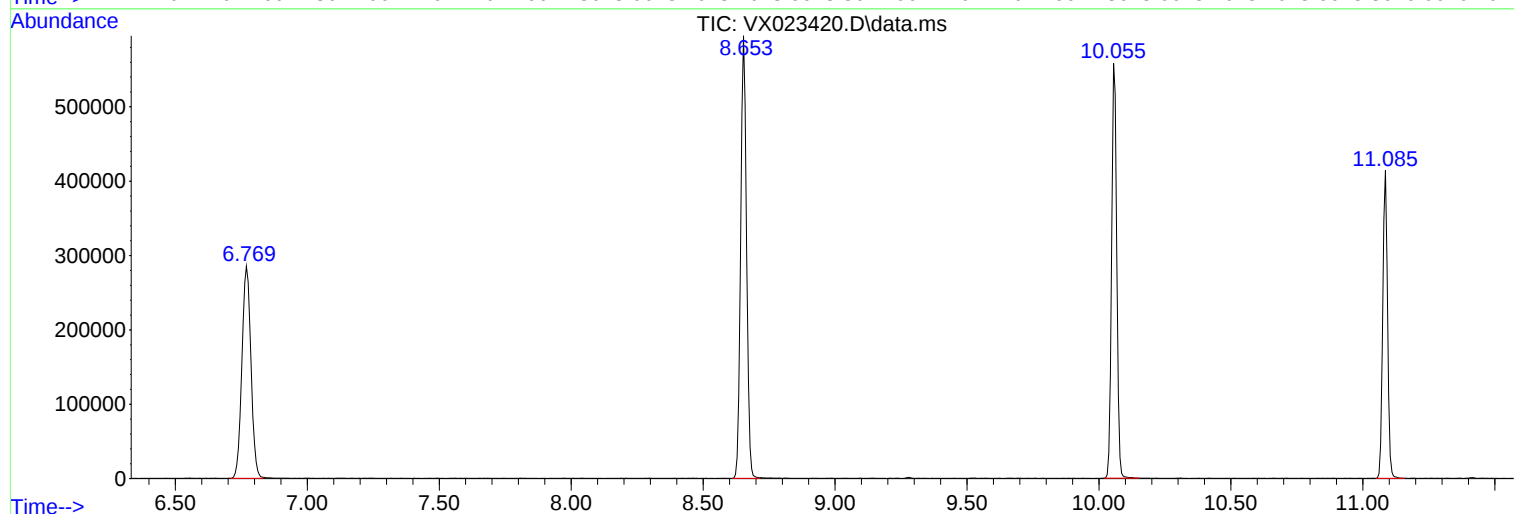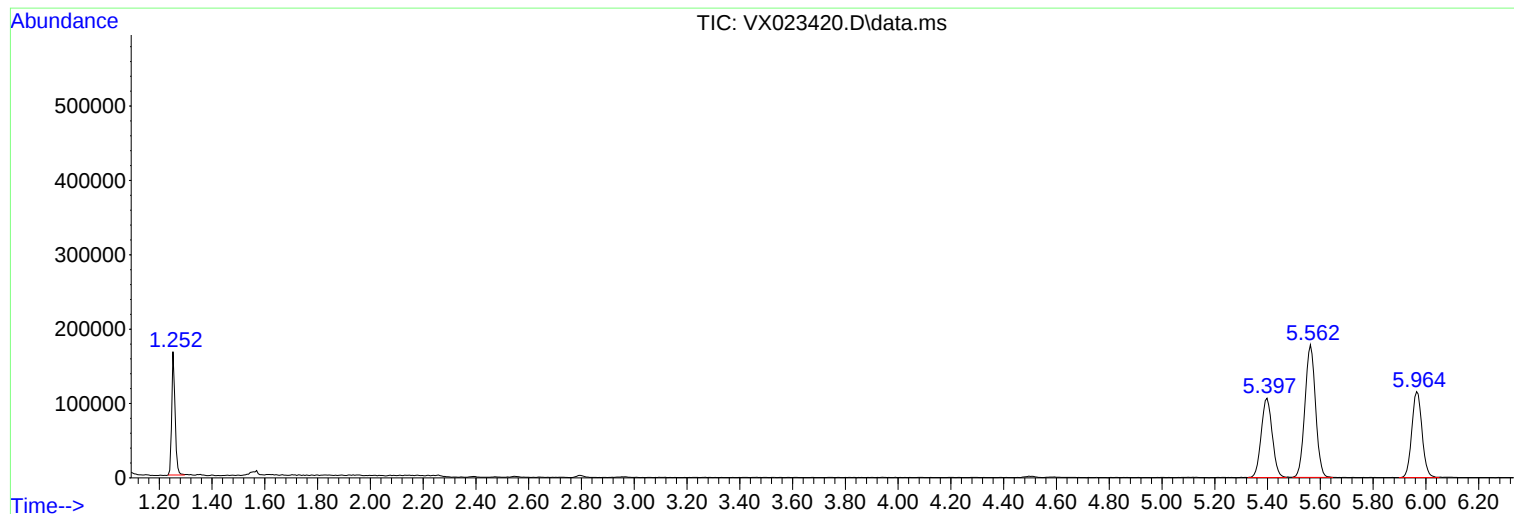

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072321\
Data File : VX023420.D
Acq On : 23 Jul 2021 13:03
Operator : JC/MD
Sample : M3145-09 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-8-PD

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072321\
Data File : VX023420.D
Acq On : 23 Jul 2021 13:03
Operator : JC/MD
Sample : M3145-09 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-8-PD

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
