

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072321\
 Data File : VX023421.D
 Acq On : 23 Jul 2021 13:50
 Operator : JC/MD
 Sample : M3145-15 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 152140-DDC-10-PS

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M

Title : SW846 8260

Signal : TIC: VX023421.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.252	24	27	33	rVB	149492	128968	13.95%	2.681%
2	1.569	68	79	83	rBV5	5367	11313	1.22%	0.235%
3	5.397	693	707	721	rBV	105901	308958	33.42%	6.423%
4	5.562	721	734	747	rVB	181466	506412	54.78%	10.527%
5	5.964	790	800	812	rBV	115968	306020	33.11%	6.362%
6	6.769	921	932	943	rBV	289321	672137	72.71%	13.972%
7	8.653	1234	1241	1251	rBV	605897	924365	100.00%	19.216%
8	9.275	1339	1343	1351	rVB2	9260	14386	1.56%	0.299%
9	10.055	1465	1471	1487	rVB	568832	778257	84.19%	16.178%
10	11.085	1634	1640	1649	rBV	445201	551018	59.61%	11.455%
11	12.024	1789	1794	1805	rVB	504137	608619	65.84%	12.652%


Sum of corrected areas: 4810453

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072321\
Data File : VX023421.D
Acq On : 23 Jul 2021 13:50
Operator : JC/MD
Sample : M3145-15 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-10-PS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

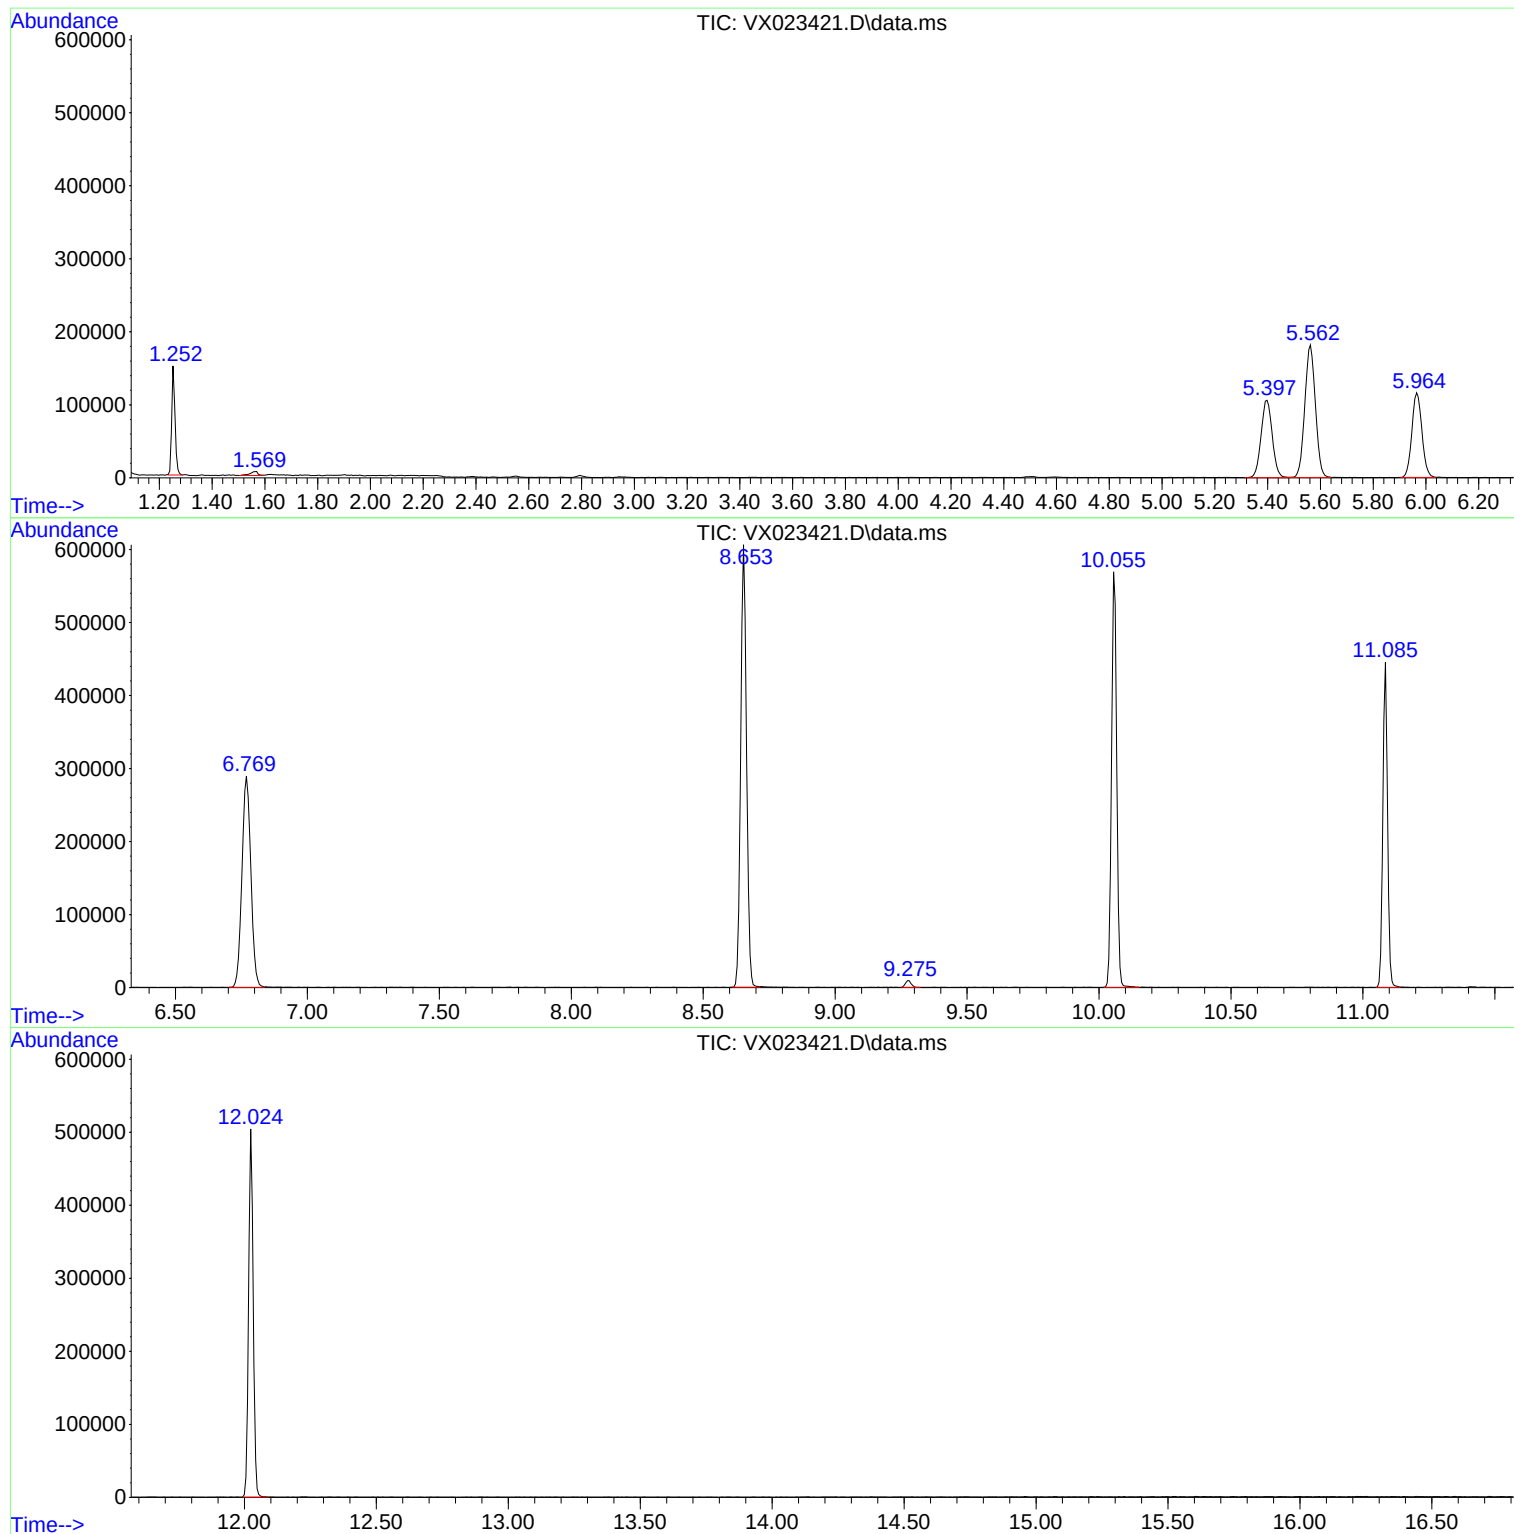

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072321\
Data File : VX023421.D
Acq On : 23 Jul 2021 13:50
Operator : JC/MD
Sample : M3145-15 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-10-PS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072321\
Data File : VX023421.D
Acq On : 23 Jul 2021 13:50
Operator : JC/MD
Sample : M3145-15 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-10-PS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------