

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072321\
 Data File : VX023425.D
 Acq On : 23 Jul 2021 15:48
 Operator : JC/MD
 Sample : M3146-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 152140-MW-1D(OFFSITE)

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M

Title : SW846 8260

Signal : TIC: VX023425.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.550	233	240	252	rBV	22408	40277	4.49%	0.780%
2	4.495	547	559	570	rBV	83072	230453	25.69%	4.464%
3	5.397	694	707	721	rBV2	104392	301918	33.65%	5.849%
4	5.562	723	734	747	rVV	176449	492301	54.88%	9.537%
5	5.964	788	800	812	rBV	113240	301439	33.60%	5.840%
6	6.769	921	932	945	rBV	278455	657708	73.31%	12.741%
7	7.135	979	992	1002	rBV	41275	90944	10.14%	1.762%
8	8.653	1234	1241	1253	rBV	588917	897127	100.00%	17.380%
9	9.275	1337	1343	1353	rVB	164882	244217	27.22%	4.731%
10	10.055	1465	1471	1487	rVB	549923	762726	85.02%	14.776%
11	11.085	1634	1640	1651	rBV	435358	540752	60.28%	10.476%
12	12.024	1789	1794	1802	rBV	488213	602119	67.12%	11.664%


Sum of corrected areas: 5161981

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072321\
Data File : VX023425.D
Acq On : 23 Jul 2021 15:48
Operator : JC/MD
Sample : M3146-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-MW-1D(OFFSITE)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

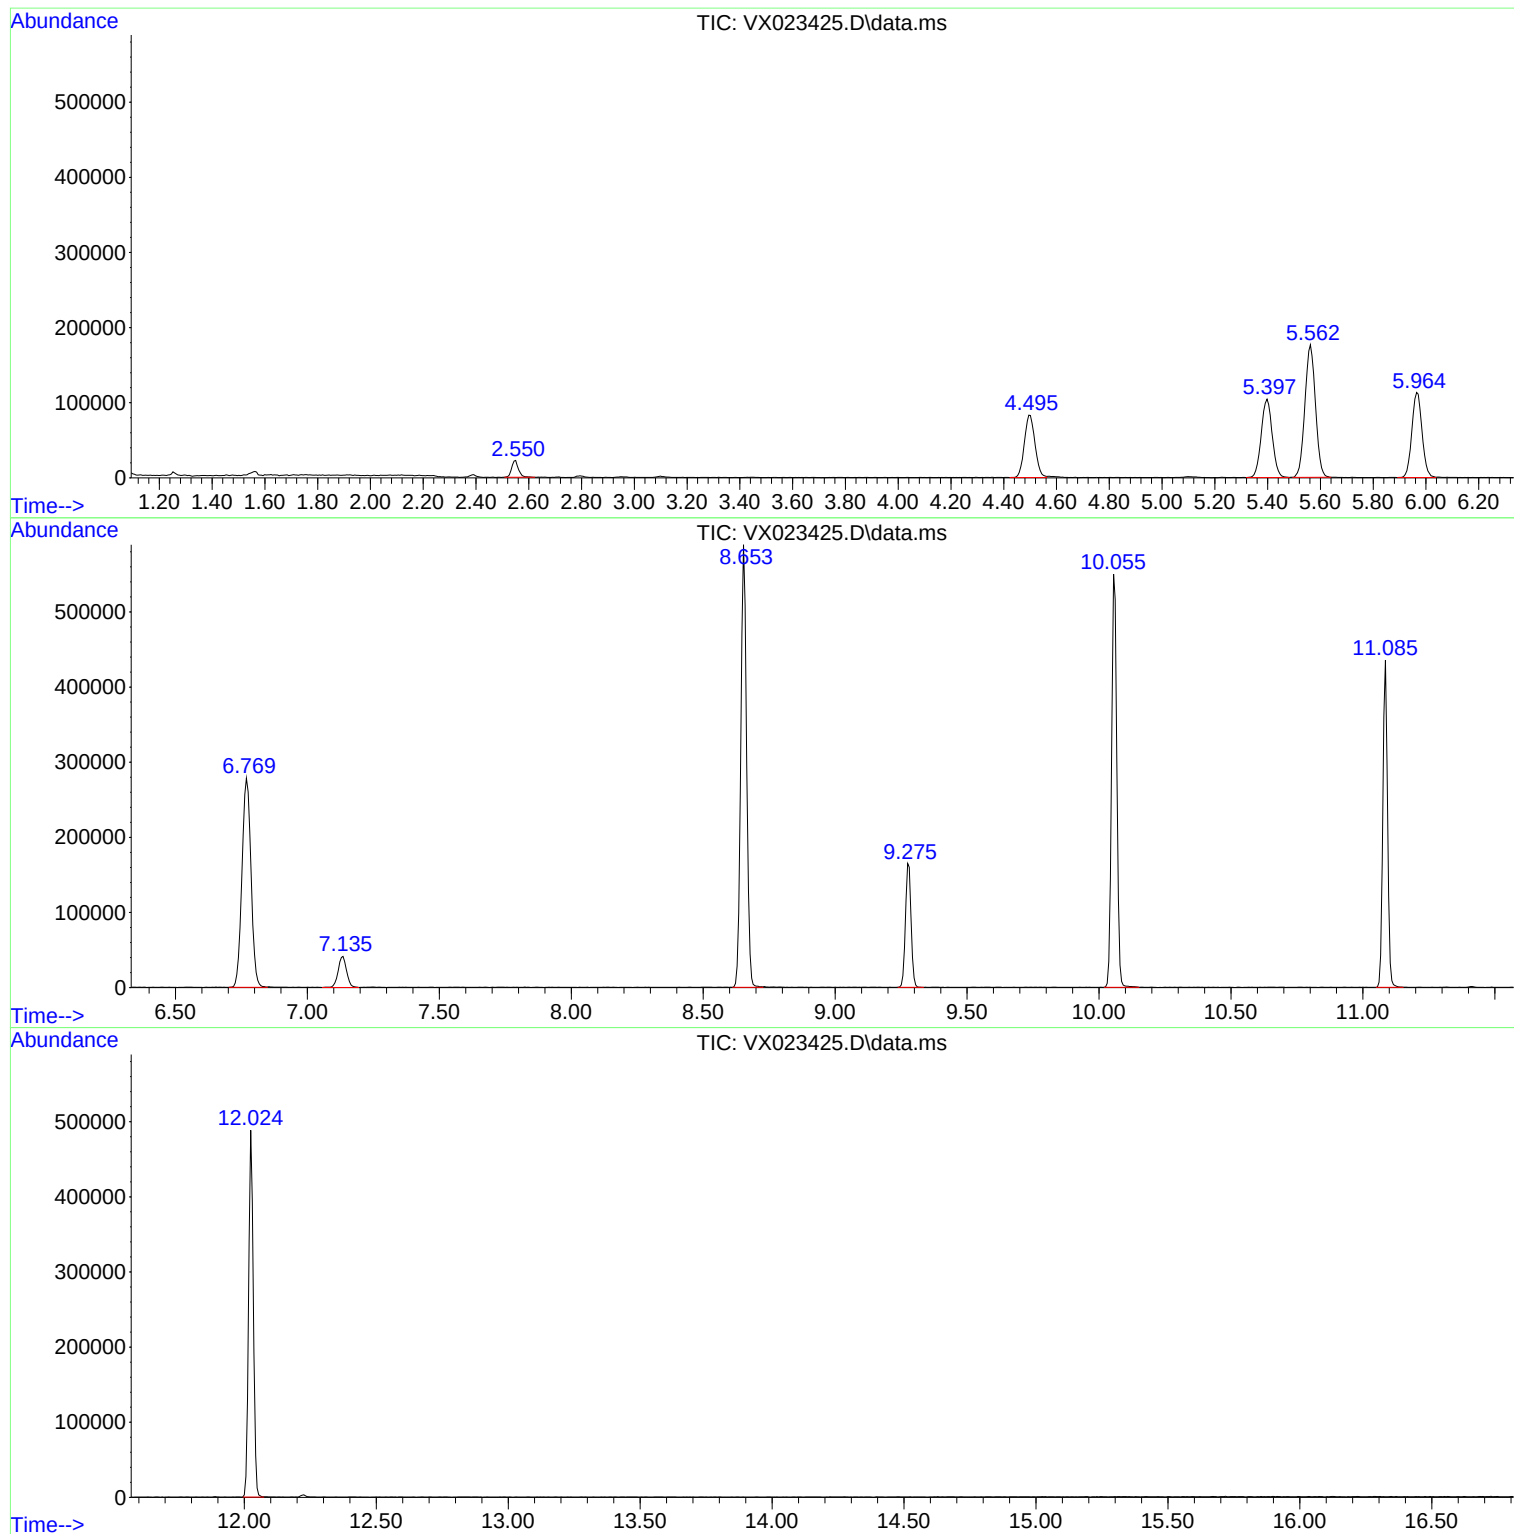

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072321\
Data File : VX023425.D
Acq On : 23 Jul 2021 15:48
Operator : JC/MD
Sample : M3146-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-MW-1D(OFFSITE)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072321\
Data File : VX023425.D
Acq On : 23 Jul 2021 15:48
Operator : JC/MD
Sample : M3146-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-MW-1D(OFFSITE)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
