

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072321\
 Data File : VX023430.D
 Acq On : 23 Jul 2021 17:46
 Operator : JC/MD
 Sample : M3145-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 152140-DDC-5-PS

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M

Title : SW846 8260

Signal : TIC: VX023430.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	21	26	33	rBV	24218	36029	4.02%	0.773%
2	1.557	69	77	82	rBV4	6444	13539	1.51%	0.290%
3	2.550	235	240	246	rVB	7401	12706	1.42%	0.273%
4	4.495	551	559	572	rBV2	15783	42570	4.75%	0.913%
5	5.397	695	707	720	rBV	105767	303009	33.81%	6.501%
6	5.562	723	734	746	rBV	172171	491551	54.85%	10.546%
7	5.964	788	800	816	rBV	117415	307681	34.33%	6.601%
8	6.769	920	932	946	rBV	278027	663841	74.08%	14.242%
9	8.653	1233	1241	1258	rBV	584232	896158	100.00%	19.226%
10	9.275	1338	1343	1349	rVB2	19227	28216	3.15%	0.605%
11	10.055	1465	1471	1487	rBV	545351	746353	83.28%	16.012%
12	11.085	1634	1640	1650	rBV	417186	527214	58.83%	11.311%
13	12.024	1789	1794	1802	rVB	472068	592307	66.09%	12.707%


Sum of corrected areas: 4661174

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072321\
Data File : VX023430.D
Acq On : 23 Jul 2021 17:46
Operator : JC/MD
Sample : M3145-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-5-PS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

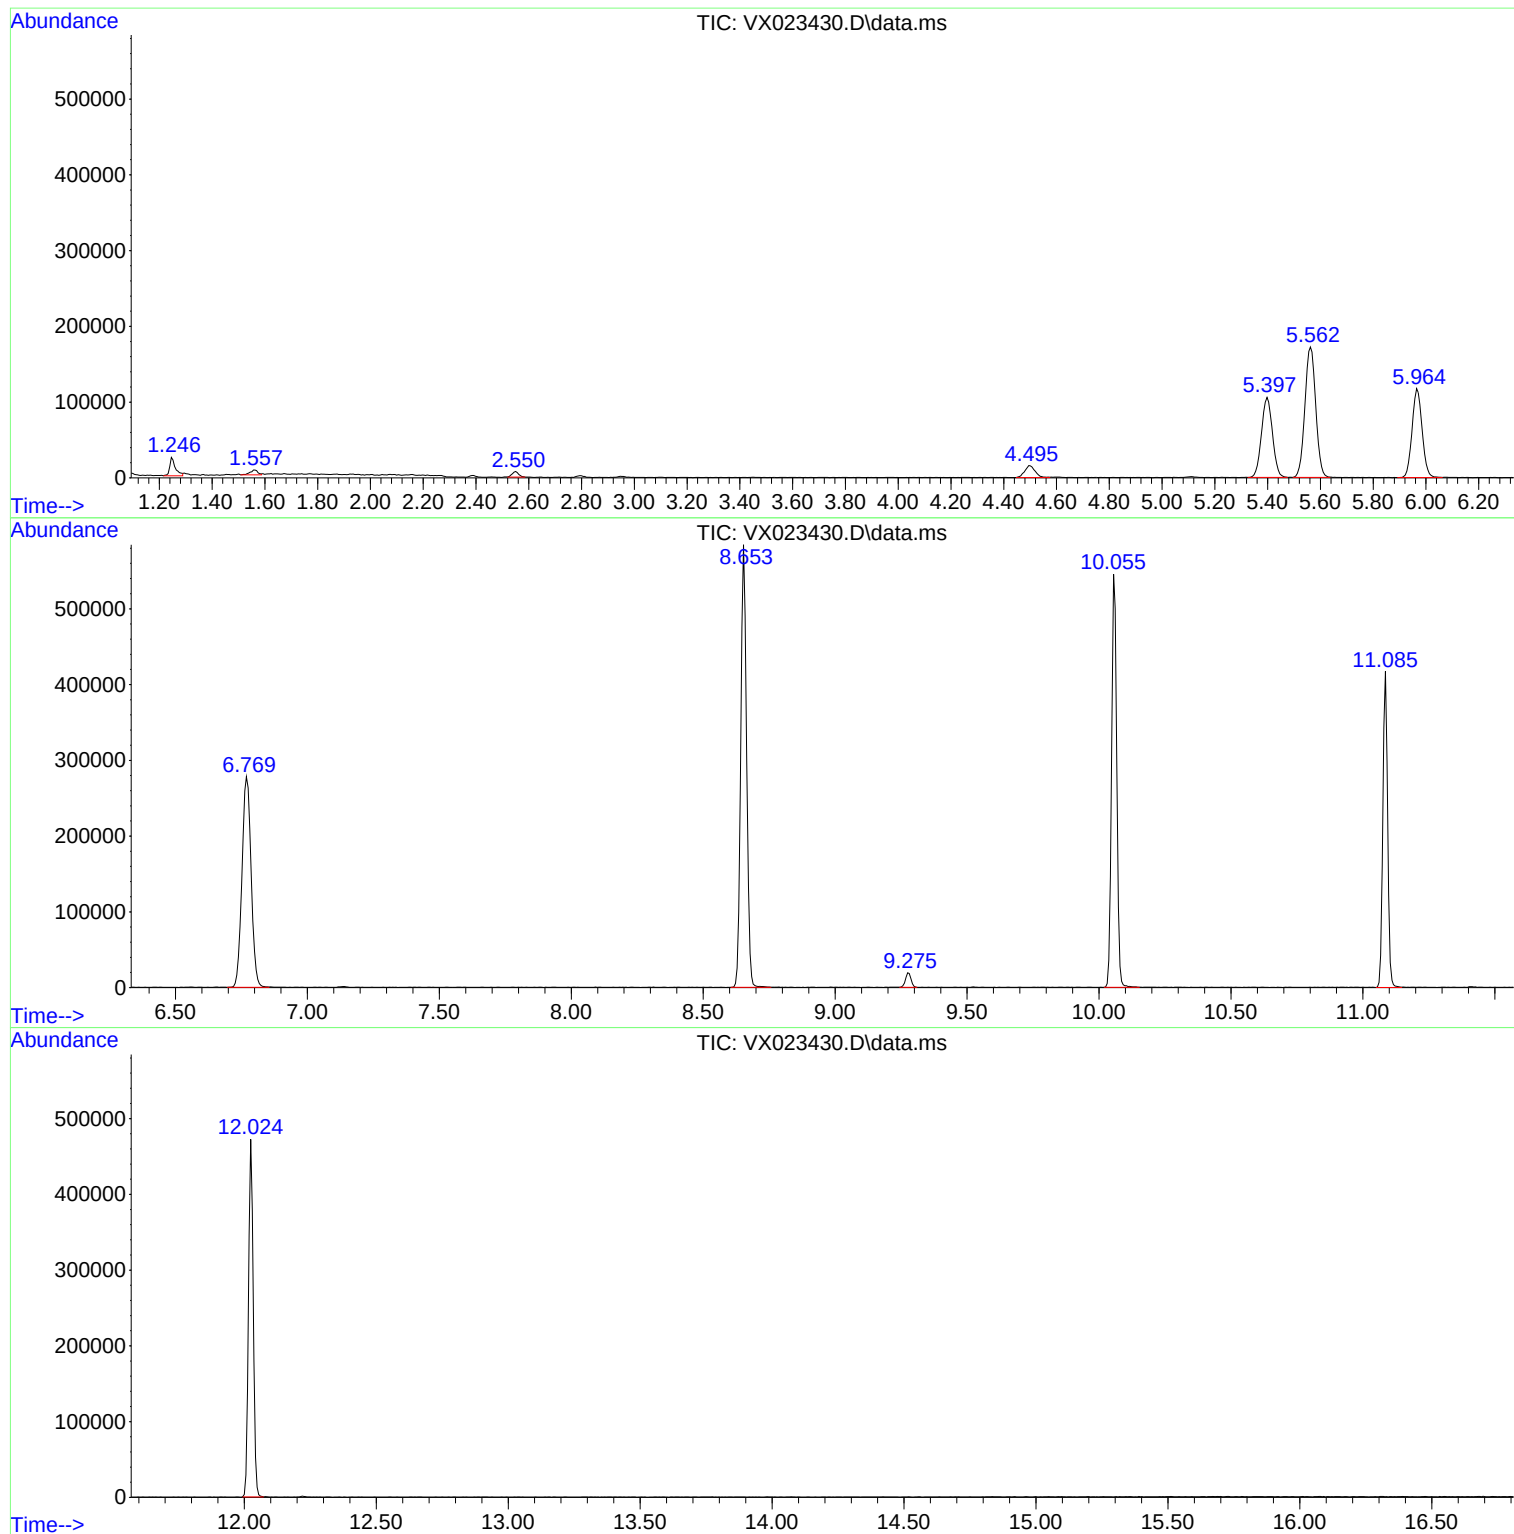

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072321\
Data File : VX023430.D
Acq On : 23 Jul 2021 17:46
Operator : JC/MD
Sample : M3145-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-5-PS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072321\
Data File : VX023430.D
Acq On : 23 Jul 2021 17:46
Operator : JC/MD
Sample : M3145-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-5-PS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
