

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072321\
 Data File : VX023433.D
 Acq On : 23 Jul 2021 18:57
 Operator : JC/MD
 Sample : M3145-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 152140-DDC-7-PS

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
 Title : SW846 8260

Signal : TIC: VX023433.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.251	23	27	32	rBV	7868	12492	1.38%	0.270%
2	1.562	71	78	84	rVB4	4874	9551	1.06%	0.206%
3	4.495	550	559	570	rBV2	15163	42353	4.69%	0.916%
4	5.397	696	707	720	rBV2	104865	301850	33.42%	6.525%
5	5.562	722	734	747	rVB	176141	492720	54.55%	10.651%
6	5.964	790	800	813	rBV	115650	307228	34.01%	6.642%
7	6.769	922	932	947	rBV	276786	659535	73.01%	14.258%
8	8.653	1234	1241	1250	rBV	593060	903301	100.00%	19.527%
9	10.055	1463	1471	1482	rBV	552786	762243	84.38%	16.478%
10	11.085	1634	1640	1650	rBV	431428	534132	59.13%	11.547%
11	12.024	1789	1794	1801	rBV	486416	600428	66.47%	12.980%


Sum of corrected areas: 4625833

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072321\
Data File : VX023433.D
Acq On : 23 Jul 2021 18:57
Operator : JC/MD
Sample : M3145-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-7-PS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

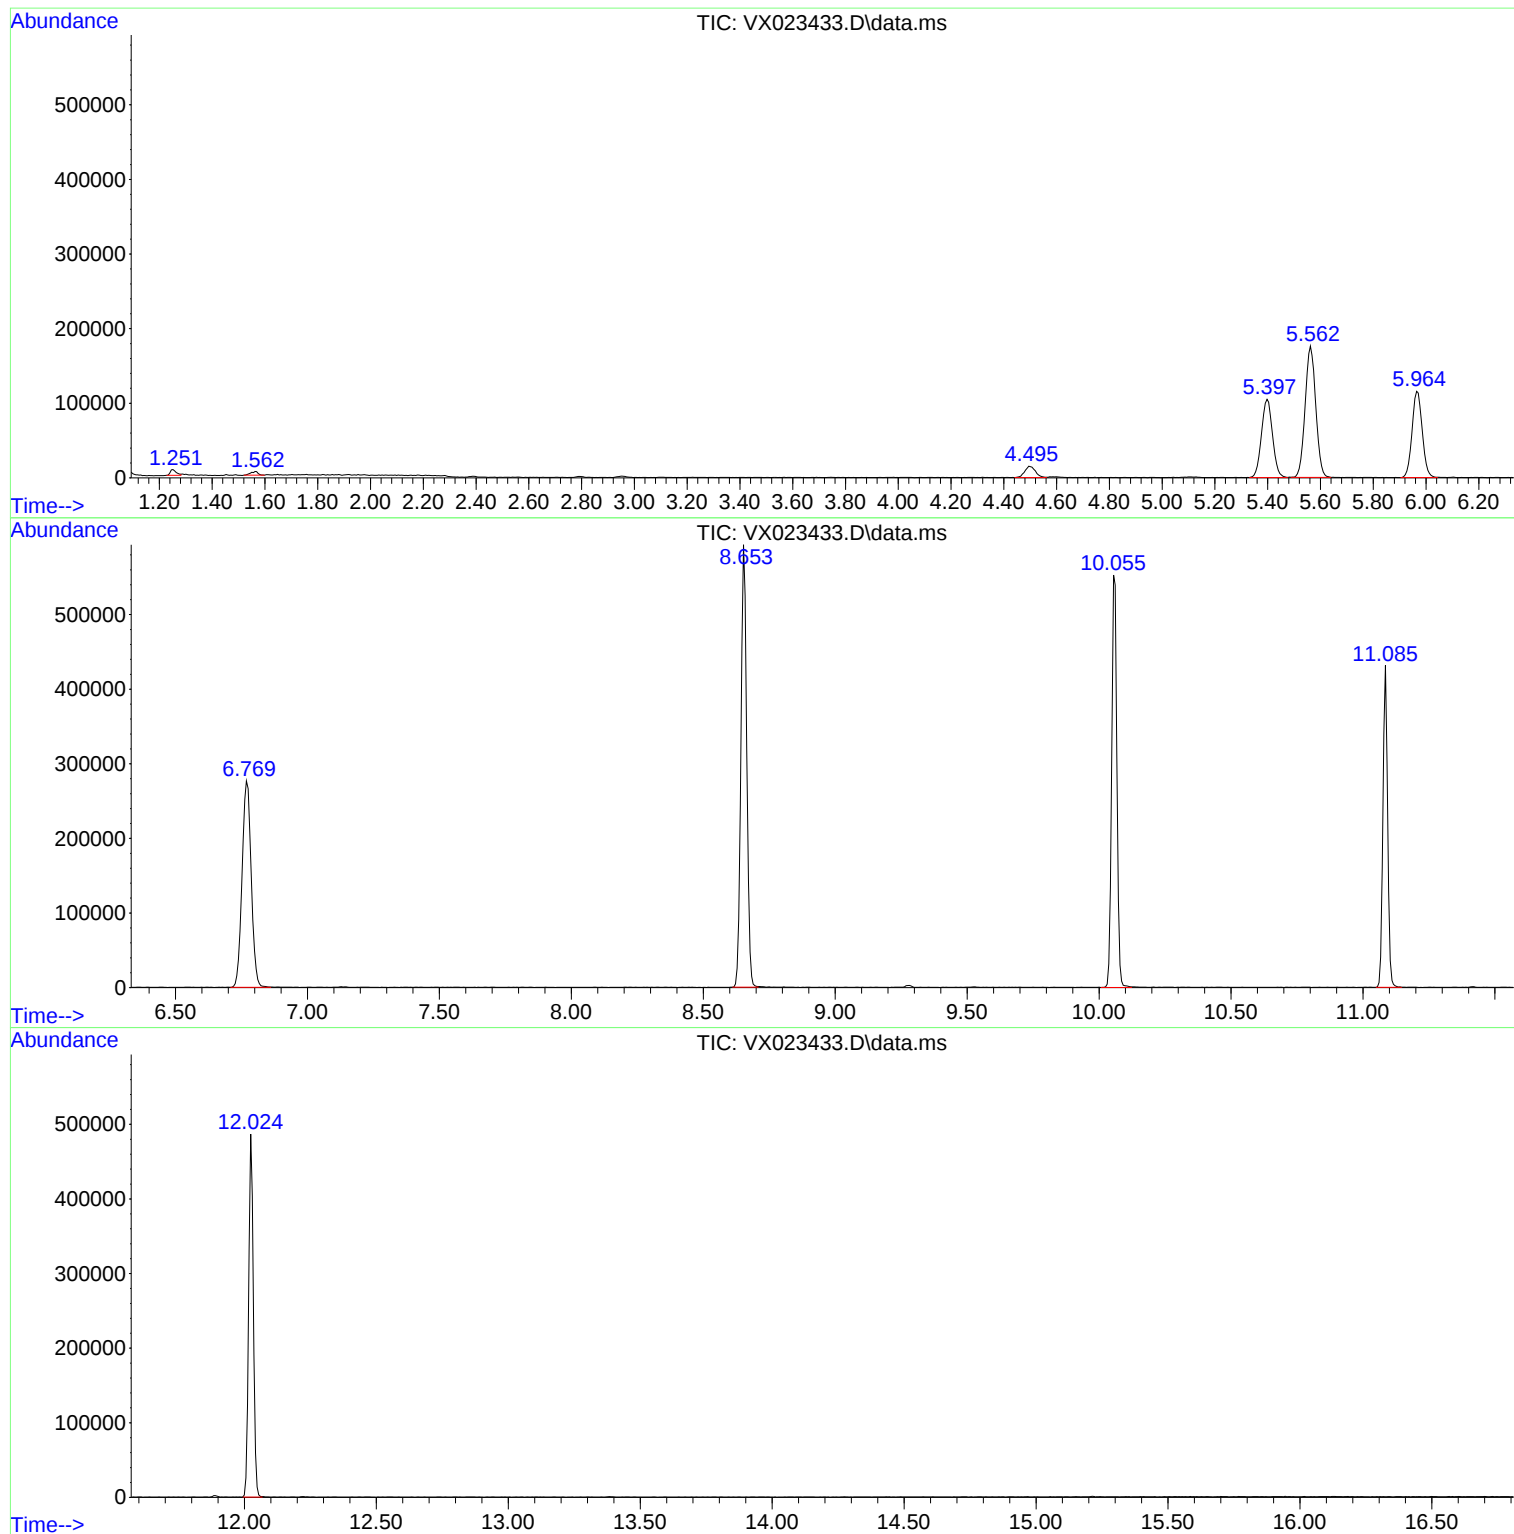

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072321\
Data File : VX023433.D
Acq On : 23 Jul 2021 18:57
Operator : JC/MD
Sample : M3145-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-7-PS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072321\
Data File : VX023433.D
Acq On : 23 Jul 2021 18:57
Operator : JC/MD
Sample : M3145-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-7-PS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
