


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX072419\
 Data File : VX011054.D
 Acq On : 24 Jul 2019 09:25
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\624X071919W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Fri Jul 19 03:27:28 2019

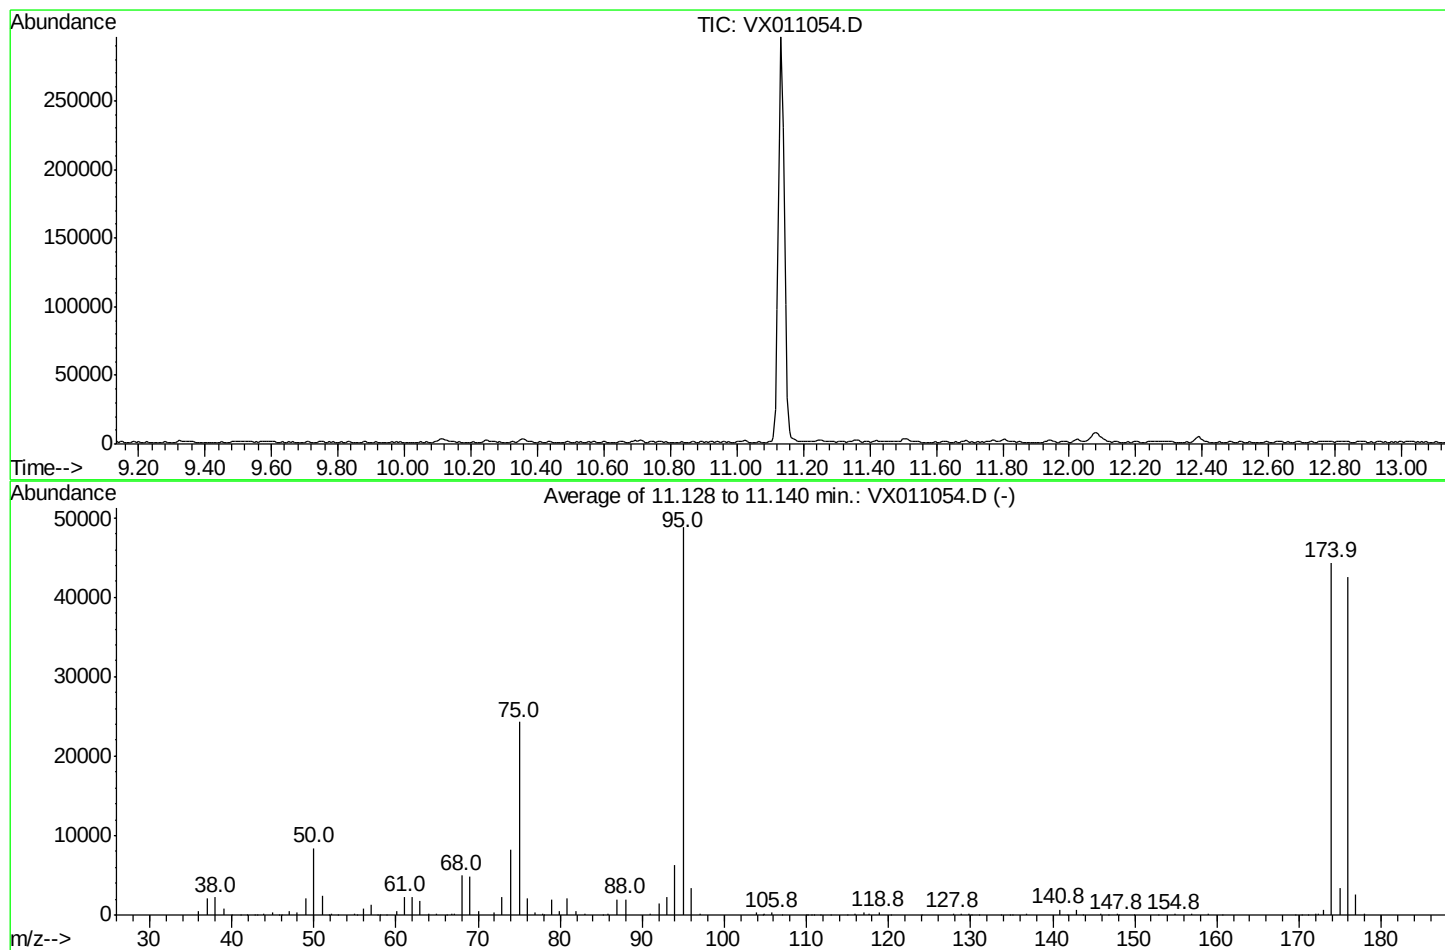

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1631

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	8397	PASS
75	95	30	60	49.8	24312	PASS
95	95	100	100	100.0	48792	PASS
96	95	5	9	6.8	3337	PASS
173	174	0.00	2	1.3	586	PASS
174	95	50	100	91.0	44378	PASS
175	174	5	9	7.8	3462	PASS
176	174	95	101	95.7	42490	PASS
177	176	5	9	6.1	2571	PASS