

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\WX072420\
 Data File : VX017552.D
 Acq On : 24 Jul 2020 18:47
 Operator : JC/SP
 Sample : L3381-21
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VNJ-225-GRID-B5

Quant Time: Jul 25 01:53:25 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X072320W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jul 24 05:48:09 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.63	168	481683	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.83	114	723336	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.10	117	781431	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.06	152	439663	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.04	65	331268	53.54	ug/l	0.00
Spiked Amount			Recovery	=	107.08%	
35) Dibromofluoromethane	5.46	113	280530	57.99	ug/l	0.00
Spiked Amount			Recovery	=	115.98%	
50) Toluene-d8	8.70	98	976127	55.93	ug/l	0.00
Spiked Amount			Recovery	=	111.86%	
62) 4-Bromofluorobenzene	11.12	95	432048	61.86	ug/l	0.00
Spiked Amount			Recovery	=	123.72%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) Dichlorodifluoromethane	1.17	85	347	Below Cal	#	1
3) Chloromethane	1.32	50	1585	0.631	ug/l #	81
5) Bromomethane	1.64	94	760	Below Cal	#	28
6) Chloroethane	1.69	64	162	Below Cal		89
8) Diethyl Ether	2.12	74	426	Below Cal		90
11) Tert butyl alcohol	2.98	59	333	0.255	ug/l #	1
13) Acrolein	2.28	56	798	4.937	ug/l #	14
15) Acrylonitrile	3.12	53	726	0.258	ug/l #	72
16) Acetone	2.42	43	37013	13.591	ug/l	90
18) Methyl Acetate	2.75	43	7620	1.188	ug/l #	79
20) Methylene Chloride	2.84	84	39190	6.524	ug/l #	91
25) 2-Butanone	4.65	43	7899	2.042	ug/l #	90
29) Tetrahydrofuran	5.26	42	486	0.203	ug/l	94
31) Cyclohexane	5.64	56	9870	1.293	ug/l #	9
36) 1,1-Dichloropropene	5.62	75	35370	5.098	ug/l #	47
38) Carbon Tetrachloride	5.64	117	49050	5.822	ug/l #	18
43) Isopropyl Acetate	6.42	43	145620	11.627	ug/l	99
48) Methyl methacrylate	7.66	41	7999	1.288	ug/l #	17
49) 1,4-Dioxane	7.71	88	245	2.058	ug/l #	1
51) 4-Methyl-2-Pentanone	8.59	43	151915	20.329	ug/l #	46
54) cis-1,3-Dichloropropene	8.59	75	64606	7.217	ug/l #	59
59) 2-Hexanone	9.52	43	146449	26.030	ug/l #	51
76) 1,2,3-Trichloropropane	11.12	75	222346	24.585	ug/l #	34
81) trans-1,4-Dichloro-2-buten	11.12	75	222346	61.948	ug/l #	11
92) 1,2-Dibromo-3-Chloropropan	13.01	75	225	2.657	ug/l #	17


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX072420\
Data File : VX017552.D
Acq On : 24 Jul 2020 18:47
Operator : JC/SP
Sample : L3381-21
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VNJ-225-GRID-B5

Quant Time: Jul 25 01:53:25 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X072320W.M
Quant Title : SW846 8260
QLast Update : Fri Jul 24 05:48:09 2020
Response via : Initial Calibration





#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.63 min Scan# 745

Delta R.T. -0.01 min

Lab File: VX017552.D

Acq: 24 Jul 2020 18:47

Instrument :

MSVOA_X

ClientSampleId :


VNJ-225-GRID-B5

Tot Ion:168 Resp: 481683

Ion Ratio Lower Upper

168 100

99 57.2 43.4 65.2



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.63

150000



100000

50000

0

Time-->

5.50 5.60 5.70



#2

Dichlorodifluoromethane

Concen: Below Cal

RT: 1.17 min Scan# 13

Delta R.T. -0.02 min

Lab File: VX017552.D


Acq: 24 Jul 2020 18:47

Tgt Ion: 85 Resp: 347

Ion Ratio Lower Upper

85 100

87 108.4 16.1 48.3#



Abundance Ion 84.90 (84.60 to 85.60): VX0

Ion 86.90 (86.60 to 87.60): VX0

1.17

300


200


100

0

Time-->

1.15 1.20





#3

Chloromethane

Concen: 0.631 ug/l

RT: 1.32 min Scan# 38

Delta R.T. 0.01 min

Lab File: VX017552.D

Acq: 24 Jul 2020 18:47

Instrument :

MSVOA_X

ClientSampleId :


VNJ-225-GRID-B5

Tot Ion: 50 Resp: 1585

Ion Ratio Lower Upper




50 100

52 43.0 25.9 38.9#



Abundance Ion 49.90 (49.60 to 50.60): VX0

Ion 51.90 (51.60 to 52.60): VX0



#5

Bromomethane

Concen: Below Cal

RT: 1.64 min Scan# 90

Delta R.T. 0.01 min

Lab File: VX017552.D


Acq: 24 Jul 2020 18:47

Tgt Ion: 94 Resp: 760

Ion Ratio Lower Upper



94 100


96 23.7 74.1 111.1#



Abundance Ion 93.90 (93.60 to 94.60): VX0

Ion 95.90 (95.60 to 96.60): VX0





#6

Chloroethane

Concen: Below Cal

RT: 1.69 min Scan# 99

Delta R.T. -0.02 min

Lab File: VX017552.D

Acq: 24 Jul 2020 18:47

Instrument :

MSVOA_X

ClientSampleId :





VNJ-225-GRID-B5

Tot Ion: 64 Resp: 162

Ion Ratio Lower Upper

64 100

66 25.0 24.9 37.3



#8

Diethyl Ether

Concen: Below Cal

RT: 2.12 min Scan# 170

Delta R.T. -0.04 min

Lab File: VX017552.D




Acq: 24 Jul 2020 18:47


Tgt Ion: 74 Resp: 426

Ion Ratio Lower Upper

74 100

45 92.0 50.8 152.5









#11

Tert butyl alcohol
Concen: 0.255 ug/l
RT: 2.98 min Scan# 311
Delta R.T. -0.04 min
Lab File: VX017552.D
Acq: 24 Jul 2020 18:47

Instrument :
MSVOA_X
ClientSampled :
VNJ-225-GRID-B5




Tot Ion: 59 Resp: 333
Ion Ratio Lower Upper
59 100
57 54.4 8.6 12.8#




#13

Acrolein
Concen: 4.937 ug/l
RT: 2.28 min Scan# 196
Delta R.T. 0.01 min
Lab File: VX017552.D
Acq: 24 Jul 2020 18:47

Tgt Ion: 56 Resp: 798
Ion Ratio Lower Upper
56 100
55 0.0 57.4 86.2#





#15

Acrylonitrile

Concen: 0.258 ug/l

RT: 3.12 min Scan# 333

Delta R.T. -0.00 min

Lab File: VX017552.D

Acq: 24 Jul 2020 18:47

Instrument :

MSVOA_X

ClientSampleId :

VNJ-225-GRID-B5


Tot Ion: 53 Resp: 726

Ion Ratio Lower Upper

53 100

52 71.5 66.6 99.8




51 0.0 29.4 44.2#



Abundance Ion 53.00 (52.70 to 53.70): VX0

Ion 52.00 (51.70 to 52.70): VX0

Ion 51.00 (50.70 to 51.70): VX0



#16

Acetone

Concen: 13.591 ug/l

RT: 2.42 min Scan# 219

Delta R.T. -0.00 min

Lab File: VX017552.D


Acq: 24 Jul 2020 18:47

Tgt Ion: 43 Resp: 37013

Ion Ratio Lower Upper



43 100


58 24.9 24.2 36.4



Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0









#18
Methyl Acetate
Concen: 1.188 ug/l
RT: 2.75 min Scan# 273
Delta R.T. -0.00 min
Lab File: VX017552.D
Acq: 24 Jul 2020 18:47




Instrument :
MSVOA_X
ClientSampleId :
VNJ-225-GRID-B5


Tot Ion: 43 Resp: 7620
Ion Ratio Lower Upper
43 100
74 32.0 17.5 26.3#



#20
Methylene Chloride
Concen: 6.524 ug/l
RT: 2.84 min Scan# 287
Delta R.T. 0.00 min
Lab File: VX017552.D
Acq: 24 Jul 2020 18:47

Tgt Ion: 84 Resp: 39190
Ion Ratio Lower Upper
84 100
49 135.6 100.3 150.5
51 47.8 30.5 45.7#
86 60.4 51.1 76.7





#25

2-Butanone

Concen: 2.042 ug/l

RT: 4.65 min Scan# 584

Delta R.T. 0.01 min

Lab File: VX017552.D

Acq: 24 Jul 2020 18:47

Instrument :

MSVOA_X

ClientSampleId :


VNJ-225-GRID-B5

Tot Ion: 43 Resp: 7899

Ion Ratio Lower Upper




43 100

72 18.9 19.0 28.4#



Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 72.00 (71.70 to 72.70): VX0



#29

Tetrahydrofuran

Concen: 0.203 ug/l

RT: 5.26 min Scan# 684

Delta R.T. 0.16 min

Lab File: VX017552.D

Acq: 24 Jul 2020 18:47


Tgt Ion: 42 Resp: 486

Ion Ratio Lower Upper

42 100

72 50.2 35.5 53.3



71 38.9 33.0 49.4




Abundance Ion 42.00 (41.70 to 42.70): VX0

Ion 72.00 (71.70 to 72.70): VX0

Ion 71.00 (70.70 to 71.70): VX0





#31

Cyclohexane

Concen: 1.293 ug/l

RT: 5.64 min Scan# 746

Delta R.T. 0.08 min

Lab File: VX017552.D

Acq: 24 Jul 2020 18:47

Instrument :

MSVOA_X

ClientSampleId :

VNJ-225-GRID-B5


Tot Ion: 56 Resp: 9870

Ion Ratio Lower Upper




56 100

69 173.6 24.2 36.4#

84 114.1 69.0 103.6#



Abundance Ion 56.00 (55.70 to 56.70): VX0
Ion 69.00 (68.70 to 69.70): VX0
Ion 84.00 (83.70 to 84.70): VX0



#33

1,2-Dichloroethane-d4

Concen: 53.539 ug/l

RT: 6.04 min Scan# 812

Delta R.T. 0.01 min

Lab File: VX017552.D


Acq: 24 Jul 2020 18:47

Tgt Ion: 65 Resp: 331268



Ion Ratio Lower Upper


65 100

67 50.6 0.0 102.8



Abundance Ion 64.90 (64.60 to 65.60): VX0
Ion 66.90 (66.60 to 67.60): VX0



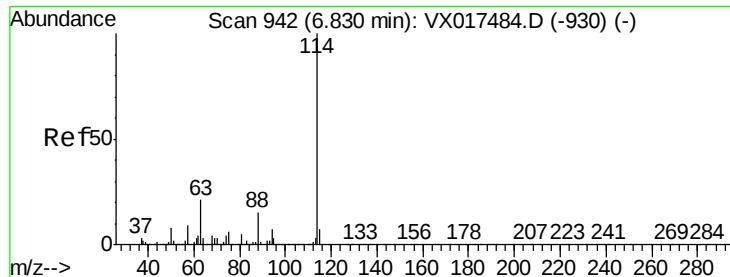

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.83 min Scan# 942

Delta R.T. -0.00 min

Lab File: VX017552.D

Acq: 24 Jul 2020 18:47

Instrument :

MSVOA_X

ClientSampleId :

VNJ-225-GRID-B5


Tot Ion:114 Resp: 723336

Ion Ratio Lower Upper

114 100

63 19.7 0.0 40.6




88 15.5 0.0 33.4



Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0



#35

Dibromofluoromethane

Concen: 57.988 ug/l

RT: 5.46 min Scan# 718

Delta R.T. -0.01 min

Lab File: VX017552.D

Acq: 24 Jul 2020 18:47


Tgt Ion:113 Resp: 280530

Ion Ratio Lower Upper

113 100

111 102.3 80.7 121.1



192 20.8 16.9 25.3




Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V





#36

1,1-Dichloropropene

Concen: 5.098 ug/l

RT: 5.62 min Scan# 744

Delta R.T. -0.15 min

Lab File: VX017552.D

Acq: 24 Jul 2020 18:47

Instrument :

MSVOA_X

ClientSampleId :

VNJ-225-GRID-B5


Tot Ion: 75 Resp: 35370

Ion Ratio Lower Upper

75 100

110 6.1 18.1 54.3#




77 0.0 24.6 37.0#



Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 109.90 (109.60 to 110.60): V

Ion 76.90 (76.60 to 77.60): VX0



#38

Carbon Tetrachloride

Concen: 5.822 ug/l

RT: 5.64 min Scan# 746

Delta R.T. -0.12 min

Lab File: VX017552.D

Acq: 24 Jul 2020 18:47


Tgt Ion: 117 Resp: 49050

Ion Ratio Lower Upper

117 100

119 6.7 75.4 113.0#



121 0.0 24.3 36.5#




Abundance Ion 116.80 (116.50 to 117.50): V

Ion 118.80 (118.50 to 119.50): V

Ion 120.80 (120.50 to 121.50): V









#43

Isopropyl Acetate
 Concen: 11.627 ug/l
 RT: 6.42 min Scan# 874
 Delta R.T. -0.00 min
 Lab File: VX017552.D
 Acq: 24 Jul 2020 18:47

Instrument :
 MSVOA_X
 ClientSampleId :
 VNJ-225-GRID-B5




Tot Ion	43	Resp	145620
Ion Ratio	Lower	Upper	
43	100		
61	20.4	15.5	23.3
87	13.2	10.5	15.7




#48

Methyl methacrylate
 Concen: 1.288 ug/l
 RT: 7.66 min Scan# 1078
 Delta R.T. -0.09 min
 Lab File: VX017552.D
 Acq: 24 Jul 2020 18:47

Tgt Ion	41	Resp	7999
Ion Ratio	Lower	Upper	
41	100		
69	2.4	63.1	94.7#
39	0.0	45.1	67.7#









#49
1,4-Dioxane
Concen: 2.058 ug/l
RT: 7.71 min Scan# 1086
Delta R.T. -0.01 min
Lab File: VX017552.D
Acq: 24 Jul 2020 18:47

Instrument :
MSVOA_X
ClientSampleId :
VNJ-225-GRID-B5

Tot Ion: 88 Resp: 245
Ion Ratio Lower Upper
88 100
43 0.0 27.8 41.6#
58 402.0 58.3 87.5#




Abundance Ion 88.00 (87.70 to 88.70): VX0
Ion 43.00 (42.70 to 43.70): VX0
Ion 58.00 (57.70 to 58.70): VX0






#50
Toluene-d8
Concen: 55.932 ug/l
RT: 8.70 min Scan# 1248
Delta R.T. -0.00 min
Lab File: VX017552.D
Acq: 24 Jul 2020 18:47

Tgt Ion: 98 Resp: 976127
Ion Ratio Lower Upper
98 100
100 64.5 52.3 78.5



Abundance Ion 98.00 (97.70 to 98.70): VX0
Ion 100.00 (99.70 to 100.70): VX0





#51

4-Methyl-2-Pentanone

Concen: 20.329 ug/l

RT: 8.59 min Scan# 1231

Delta R.T. -0.03 min

Lab File: VX017552.D

Acq: 24 Jul 2020 18:47

Instrument :

MSVOA_X

ClientSampleId :





VNJ-225-GRID-B5

Tot Ion: 43 Resp: 151915

Ion Ratio Lower Upper

43 100

58 5.9 31.0 46.4#



#54

cis-1,3-Dichloropropene

Concen: 7.217 ug/l

RT: 8.59 min Scan# 1231

Delta R.T. 0.18 min

Lab File: VX017552.D

Acq: 24 Jul 2020 18:47




Tgt Ion: 75 Resp: 64606


Ion Ratio Lower Upper

75 100

77 0.5 25.5 38.3#

39 29.8 41.8 62.8#









#59
2-Hexanone
Concen: 26.030 ug/l
RT: 9.52 min Scan# 1384
Delta R.T. 0.05 min
Lab File: VX017552.D
Acq: 24 Jul 2020 18:47




Instrument :
MSVOA_X
ClientSampleId :
VNJ-225-GRID-B5


Tot Ion: 43 Resp: 146449
Ion Ratio Lower Upper
43 100
58 18.5 26.6 79.8#

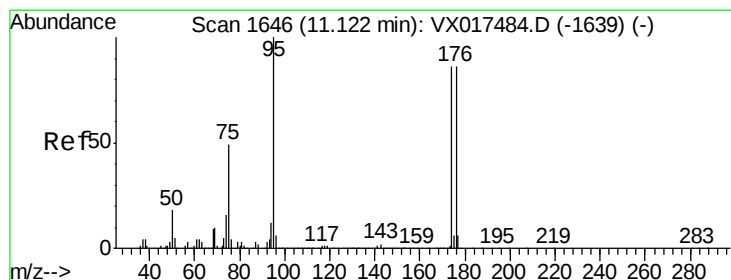

#62
4-Bromofluorobenzene
Concen: 61.860 ug/l
RT: 11.12 min Scan# 1646
Delta R.T. -0.00 min
Lab File: VX017552.D
Acq: 24 Jul 2020 18:47

Tgt Ion: 95 Resp: 432048
Ion Ratio Lower Upper
95 100
174 85.5 0.0 169.0
176 83.1 0.0 161.0









#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.10 min Scan# 1478
Delta R.T. -0.00 min
Lab File: VX017552.D
Acq: 24 Jul 2020 18:47




Instrument :
MSVOA_X
ClientSampleId :
VNJ-225-GRID-B5


Tot Ion	Ratio	Lower	Upper
117	100		
82	55.3	44.0	66.0
119	33.3	25.4	38.0



#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.06 min Scan# 1800
Delta R.T. -0.00 min
Lab File: VX017552.D
Acq: 24 Jul 2020 18:47

Tgt Ion	Ratio	Lower	Upper
152	100		
115	57.9	65.5	196.6#
150	155.0	0.0	412.6









#76
 1,2,3-Trichloropropane
 Concen: 24.585 ug/l
 RT: 11.12 min Scan# 1646
 Delta R.T. -0.16 min
 Lab File: VX017552.D
 Acq: 24 Jul 2020 18:47




Instrument :
 MSVOA_X
 ClientSampleId :
 VNJ-225-GRID-B5


Tot Ion: 75 Resp: 222346
 Ion Ratio Lower Upper
 75 100
 77 1.2 21.8 65.3#



#81
 trans-1,4-Dichloro-2-butene
 Concen: 61.948 ug/l
 RT: 11.12 min Scan# 1646
 Delta R.T. 0.06 min
 Lab File: VX017552.D
 Acq: 24 Jul 2020 18:47

Tgt Ion: 75 Resp: 222346
 Ion Ratio Lower Upper
 75 100
 53 0.1 75.9 113.9#
 89 0.1 37.8 56.6#





#92

1,2-Dibromo-3-Chloropropane

Concen: 2.657 ug/l

RT: 13.01 min Scan# 1956

Delta R.T. 0.03 min

Lab File: VX017552.D

Acq: 24 Jul 2020 18:47

Instrument :

MSVOA_X

ClientSampleId :

VNJ-225-GRID-B5


Tot Ion: 75 Resp: 225

Ion Ratio Lower Upper

75 100

155 0.0 42.3 126.8#

157 28.9 54.3 162.9#



Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 154.80 (154.50 to 155.50): V

Ion 156.80 (156.50 to 157.50): V

