

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\WX072420\
 Data File : VX017555.D
 Acq On : 24 Jul 2020 19:56
 Operator : JC/SP
 Sample : L3402-02
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BUS-WASH

Quant Time: Jul 25 01:54:26 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X072320W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jul 24 05:48:09 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.63	168	496278	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.83	114	785791	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.10	117	890251	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.06	152	514247	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.03	65	315589	49.50	ug/l	0.00
Spiked Amount			Recovery	=	99.00%	
35) Dibromofluoromethane	5.46	113	286383	54.49	ug/l	0.00
Spiked Amount			Recovery	=	108.98%	
50) Toluene-d8	8.70	98	1025834	54.11	ug/l	0.00
Spiked Amount			Recovery	=	108.22%	
62) 4-Bromofluorobenzene	11.12	95	428027	56.41	ug/l	0.00
Spiked Amount			Recovery	=	112.82%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) Dichlorodifluoromethane	1.20	85	446	Below Cal	#	42
3) Chloromethane	1.31	50	1293	0.576	ug/l	100
5) Bromomethane	1.63	94	427	Below Cal	#	3
6) Chloroethane	1.72	64	179	Below Cal	#	13
8) Diethyl Ether	2.17	74	1827	Below Cal		99
11) Tert butyl alcohol	3.03	59	3445	2.564	ug/l #	72
13) Acrolein	2.27	56	471	4.600	ug/l #	4
16) Acetone	2.42	43	249933	89.077	ug/l	99
17) Carbon Disulfide	2.56	76	5186	0.333	ug/l #	85
18) Methyl Acetate	2.75	43	6586	0.997	ug/l #	91
20) Methylene Chloride	2.84	84	43862	7.201	ug/l	90
25) 2-Butanone	4.64	43	37873	9.502	ug/l	94
29) Tetrahydrofuran	5.10	42	3501	1.418	ug/l #	85
36) 1,1-Dichloropropene	5.64	75	37655	4.996	ug/l #	42
37) Ethyl Acetate	4.64	43	37873	4.593	ug/l #	69
38) Carbon Tetrachloride	5.63	117	49842	5.446	ug/l #	16
41) Methacrylonitrile	4.98	41	1007	0.213	ug/l #	59
43) Isopropyl Acetate	6.42	43	63447	4.663	ug/l	98
48) Methyl methacrylate	7.66	41	10478	1.554	ug/l #	26
49) 1,4-Dioxane	7.70	88	166	1.284	ug/l #	1
51) 4-Methyl-2-Pentanone	8.62	43	219645	27.057	ug/l #	77
52) Toluene	8.77	92	4615	0.333	ug/l	76
54) cis-1,3-Dichloropropene	8.59	75	46722	4.804	ug/l #	58
59) 2-Hexanone	9.52	43	58524	9.576	ug/l #	53
76) 1,2,3-Trichloropropane	11.12	75	218877	20.691	ug/l #	35
81) trans-1,4-Dichloro-2-buten	11.12	75	218877	52.137	ug/l #	11
92) 1,2-Dibromo-3-Chloropropan	12.93	75	339	2.680	ug/l	61
95) Naphthalene	13.82	128	7437	0.219	ug/l #	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX072420\
Data File : VX017555.D
Acq On : 24 Jul 2020 19:56
Operator : JC/SP
Sample : L3402-02
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BUS-WASH

Quant Time: Jul 25 01:54:26 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X072320W.M
Quant Title : SW846 8260
QLast Update : Fri Jul 24 05:48:09 2020
Response via : Initial Calibration

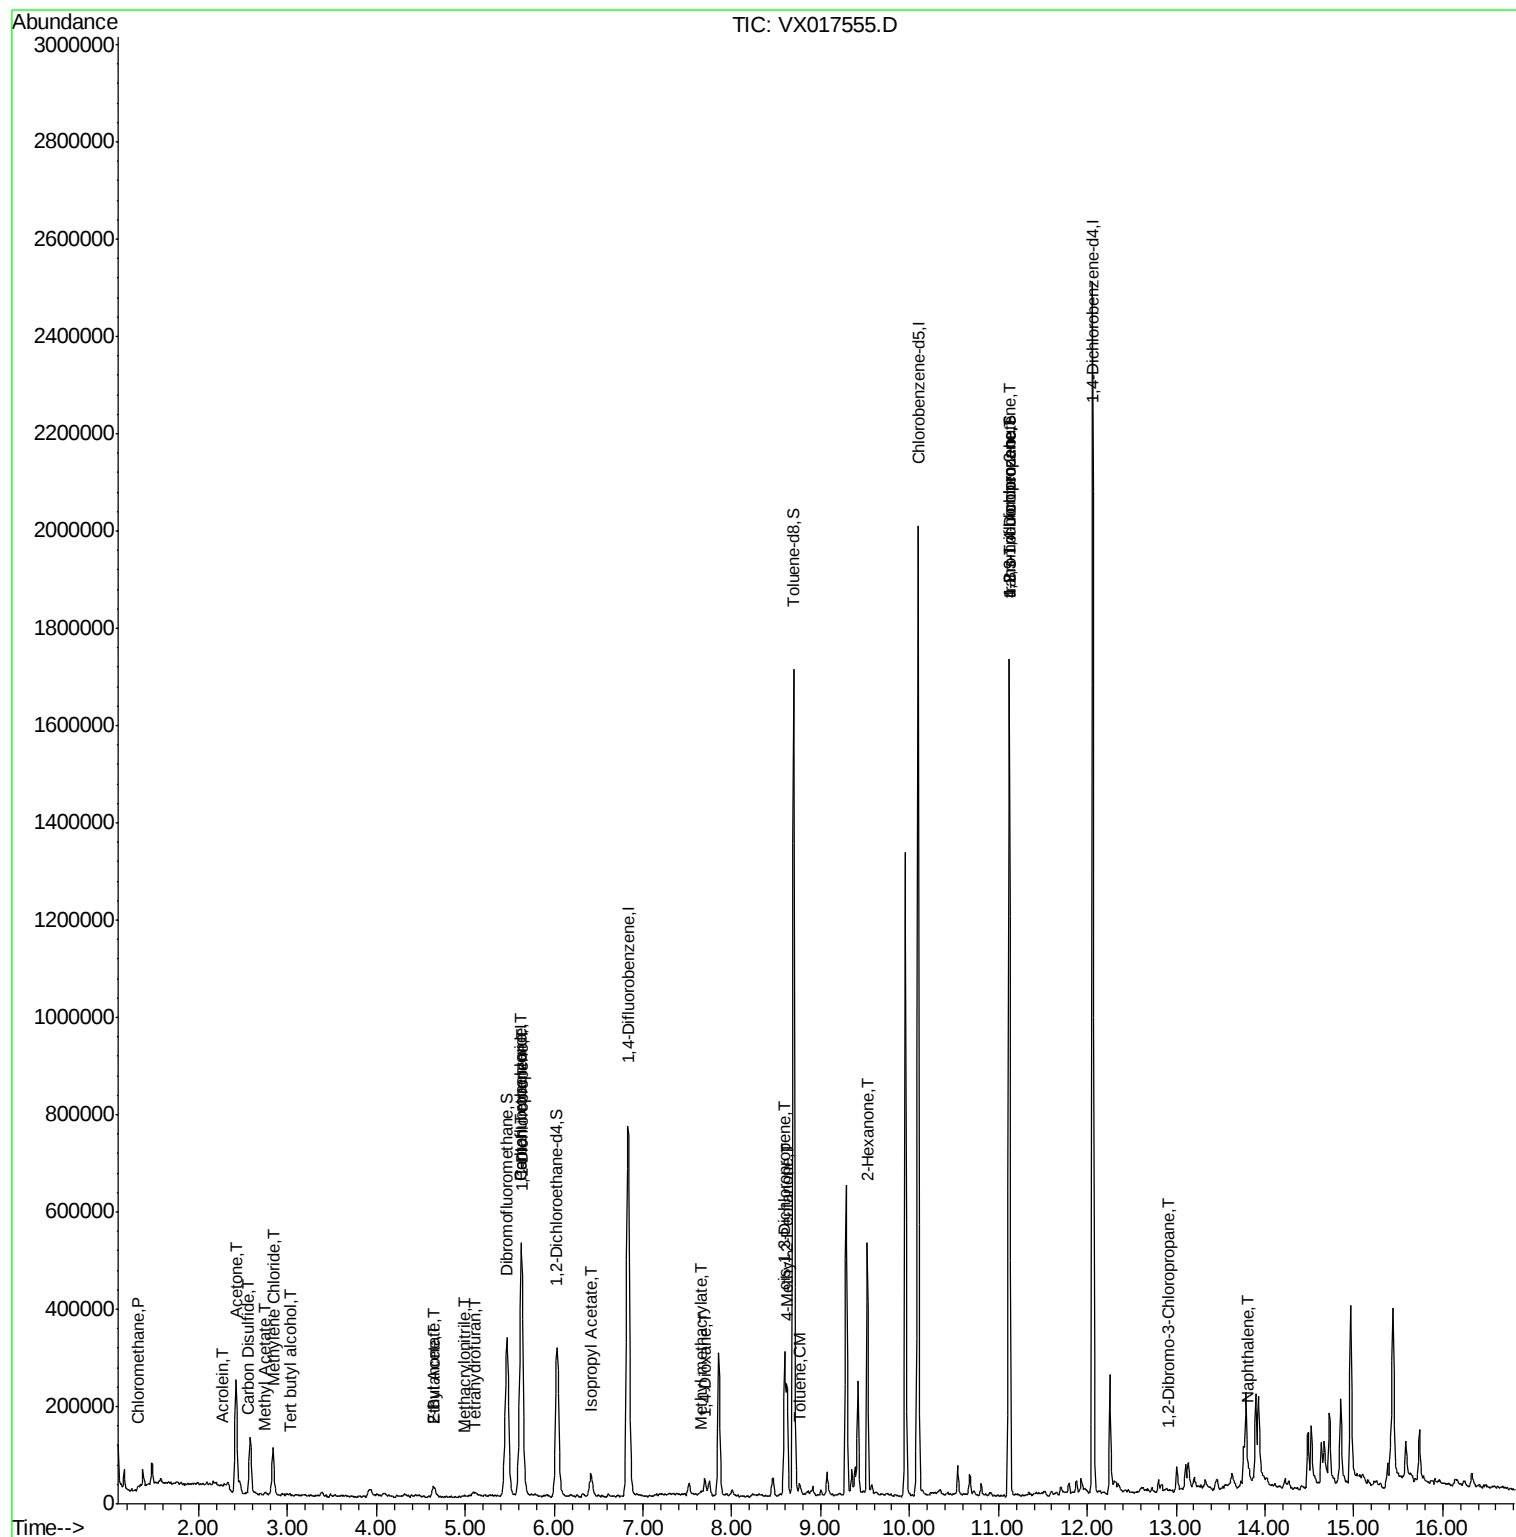



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.63 min Scan# 745

Delta R.T. -0.01 min

Lab File: VX017555.D

Acq: 24 Jul 2020 19:56

Instrument :

MSVOA_X

ClientSampleId :


BUS-WASH

Tot Ion:168 Resp: 496278

Ion Ratio Lower Upper

168 100

99 59.1 43.4 65.2



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.63

200000

150000

100000

50000

0



Time-->

5.50

5.60

5.70

5.80



#2

Dichlorodifluoromethane

Concen: Below Cal

RT: 1.20 min Scan# 18

Delta R.T. 0.01 min

Lab File: VX017555.D


Acq: 24 Jul 2020 19:56

Tgt Ion: 85 Resp: 446

Ion Ratio Lower Upper

85 100

87 0.0 16.1 48.3#



Abundance Ion 84.90 (84.60 to 85.60): VX0

Ion 86.90 (86.60 to 87.60): VX0

1.20

300

200


100


0

Time-->

1.15

1.20



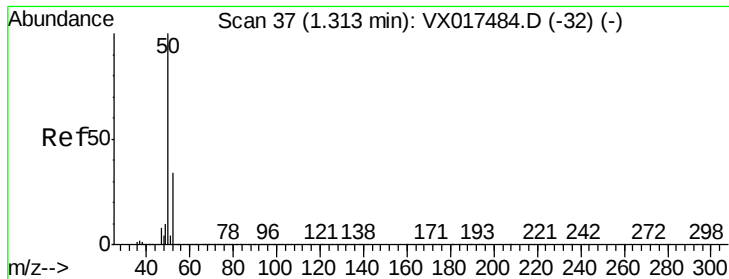

#3

Chloromethane

Concen: 0.576 ug/l

RT: 1.31 min Scan# 37

Delta R.T. 0.00 min

Lab File: VX017555.D

Acq: 24 Jul 2020 19:56

Instrument :

MSVOA_X

ClientSampleId :


BUS-WASH

Tot Ion: 50 Resp: 1293

Ion Ratio Lower Upper

50 100

52 32.3 25.9 38.9

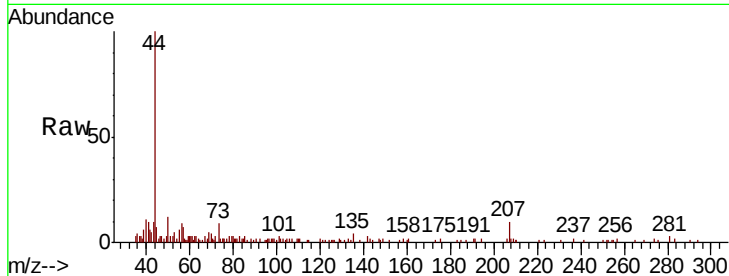

Abundance Ion 49.90 (49.60 to 50.60): VX0

Ion 51.90 (51.60 to 52.60): VX0

1.31

800

600



400

200

0

Time-->

1.30 1.35

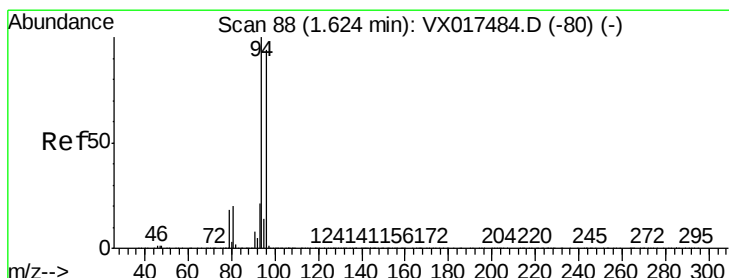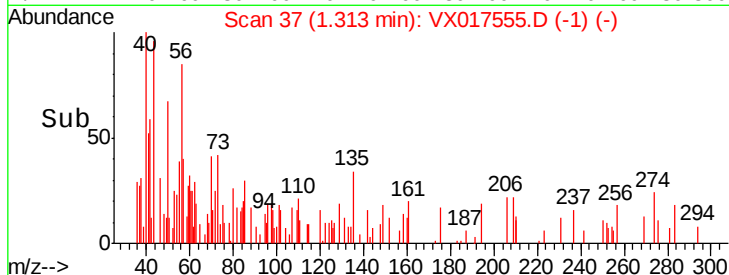

#5

Bromomethane

Concen: Below Cal

RT: 1.63 min Scan# 89

Delta R.T. 0.01 min

Lab File: VX017555.D


Acq: 24 Jul 2020 19:56

Tgt Ion: 94 Resp: 427

Ion Ratio Lower Upper

94 100

96 0.0 74.1 111.1#

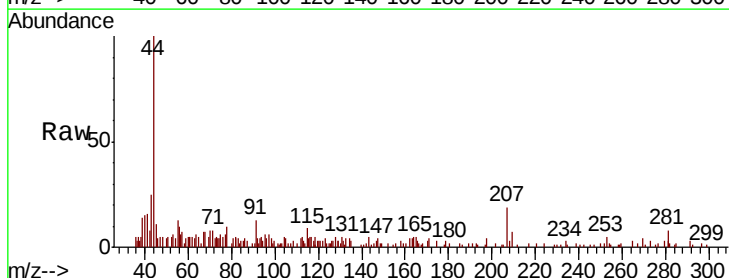

Abundance Ion 93.90 (93.60 to 94.60): VX0

Ion 95.90 (95.60 to 96.60): VX0

1.63

600


400


200

0

Time-->

1.60 1.62 1.64

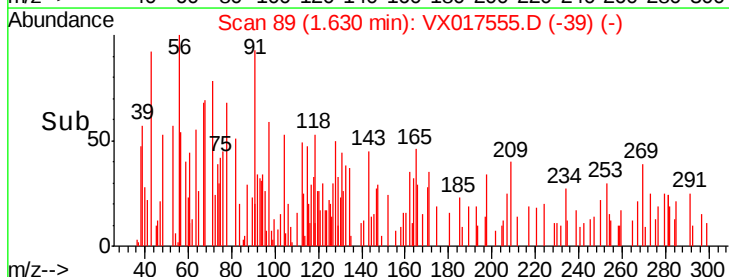



#6

Chloroethane

Concen: Below Cal

RT: 1.72 min Scan# 103

Delta R.T. 0.01 min

Lab File: VX017555.D

Acq: 24 Jul 2020 19:56

Instrument :

MSVOA_X

ClientSampled :


BUS-WASH

Tot Ion: 64 Resp: 179

Ion Ratio Lower Upper




64 100

66 79.1 24.9 37.3#



Abundance Ion 63.90 (63.60 to 64.60): VX0

Ion 65.90 (65.60 to 66.60): VX0

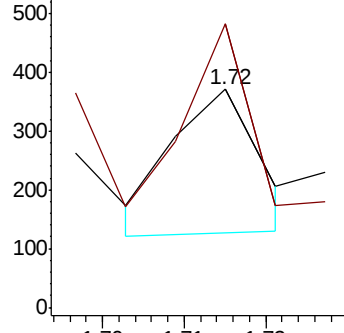

#8

Diethyl Ether

Concen: Below Cal

RT: 2.17 min Scan# 177

Delta R.T. 0.00 min

Lab File: VX017555.D


Acq: 24 Jul 2020 19:56

Tgt Ion: 74 Resp: 1827

Ion Ratio Lower Upper



74 100


45 100.7 50.8 152.5



Abundance Ion 74.00 (73.70 to 74.70): VX0

Ion 45.00 (44.70 to 45.70): VX0

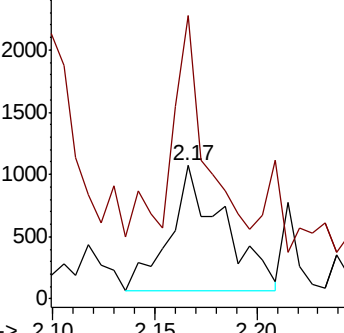







#11

Tert butyl alcohol
 Concen: 2.564 ug/l
 RT: 3.03 min Scan# 318
 Delta R.T. 0.01 min
 Lab File: VX017555.D
 Acq: 24 Jul 2020 19:56

Instrument :
 MSVOA_X
 ClientSampled :
 BUS-WASH




Tot Ion: 59 Resp: 3445
 Ion Ratio Lower Upper
 59 100
 57 0.0 8.6 12.8#

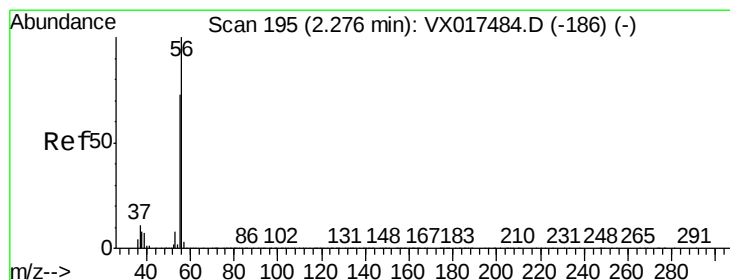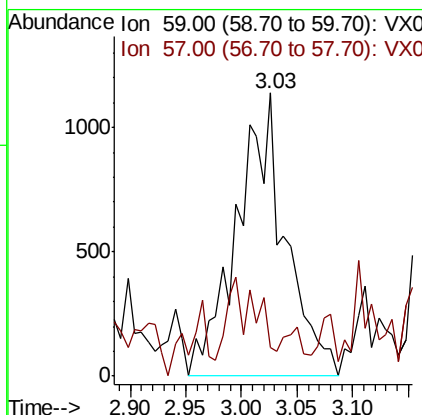


#13

Acrolein
 Concen: 4.600 ug/l
 RT: 2.27 min Scan# 194
 Delta R.T. -0.01 min
 Lab File: VX017555.D
 Acq: 24 Jul 2020 19:56

Tgt Ion: 56 Resp: 471
 Ion Ratio Lower Upper
 56 100
 55 151.8 57.4 86.2#



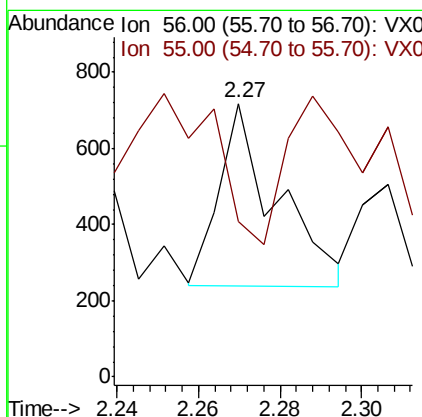





#16
Acetone
Concen: 89.077 ug/l
RT: 2.42 min Scan# 219
Delta R.T. -0.00 min
Lab File: VX017555.D
Acq: 24 Jul 2020 19:56




Instrument :
MSVOA_X
ClientSampleId :
BUS-WASH


Tot Ion: 43 Resp: 249933
Ion Ratio Lower Upper
43 100
58 30.7 24.2 36.4

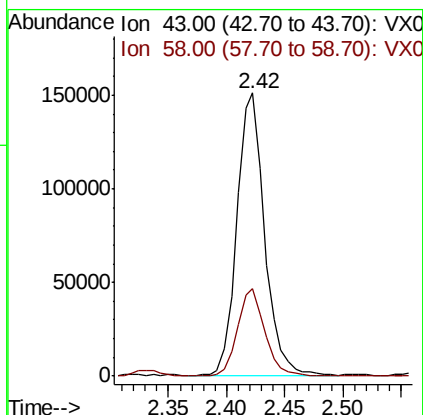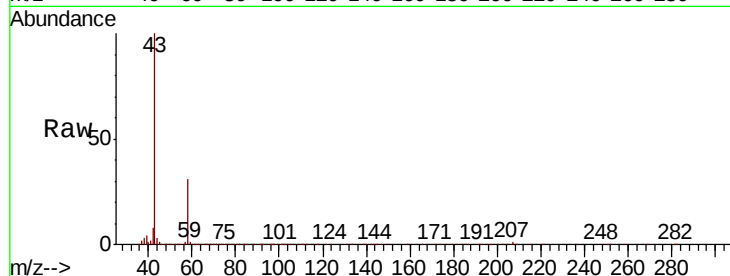

#17
Carbon Disulfide
Concen: 0.333 ug/l
RT: 2.56 min Scan# 241
Delta R.T. 0.01 min
Lab File: VX017555.D
Acq: 24 Jul 2020 19:56

Tgt Ion: 76 Resp: 5186
Ion Ratio Lower Upper
76 100
78 4.0 7.5 11.3#


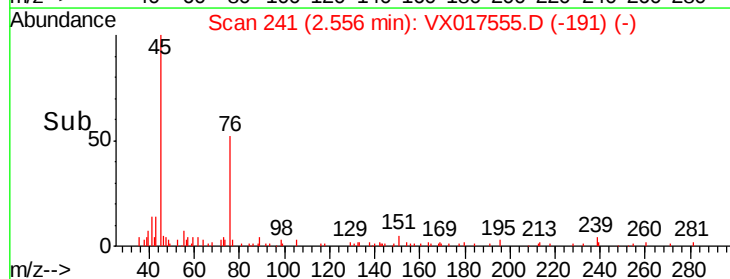
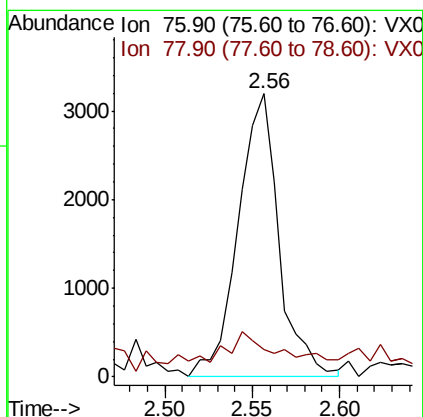



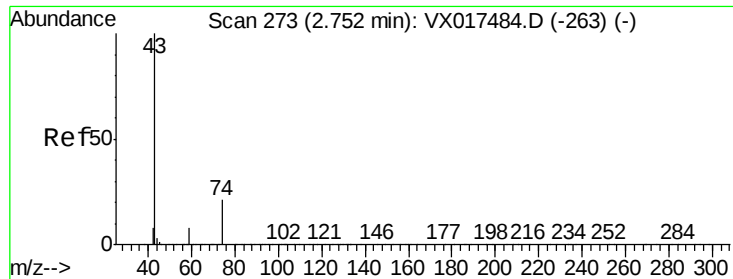

#18
Methyl Acetate
Concen: 0.997 ug/l
RT: 2.75 min Scan# 273
Delta R.T. -0.00 min
Lab File: VX017555.D
Acq: 24 Jul 2020 19:56




Instrument :
MSVOA_X
ClientSampleId :
BUS-WASH


Tot Ion: 43 Resp: 6586
Ion Ratio Lower Upper
43 100
74 26.4 17.5 26.3#

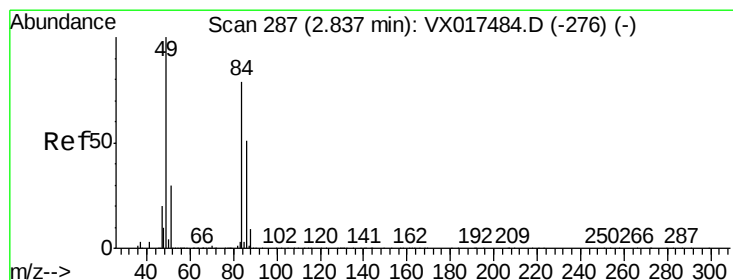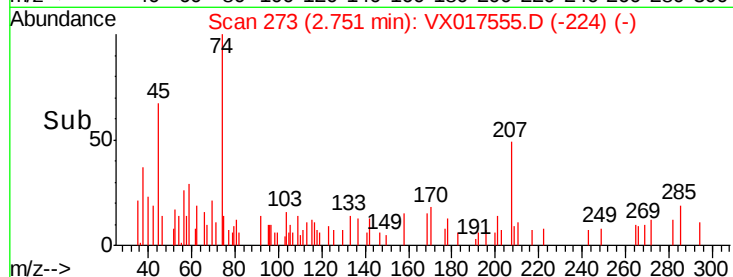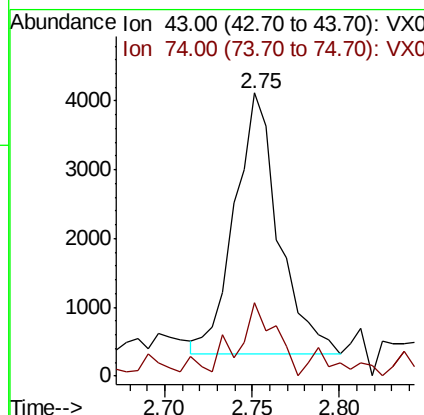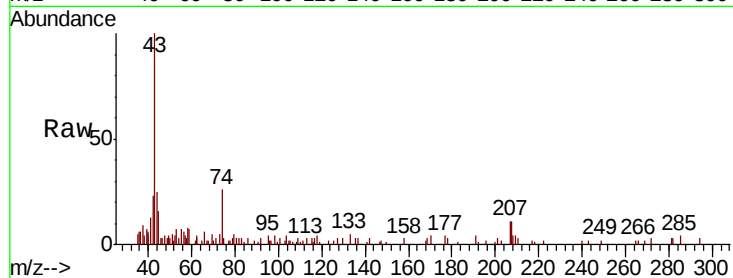

#20
Methylene Chloride
Concen: 7.201 ug/l
RT: 2.84 min Scan# 287
Delta R.T. 0.00 min
Lab File: VX017555.D
Acq: 24 Jul 2020 19:56

Tgt Ion: 84 Resp: 43862
Ion Ratio Lower Upper
84 100
49 137.1 100.3 150.5
51 44.4 30.5 45.7
86 69.9 51.1 76.7

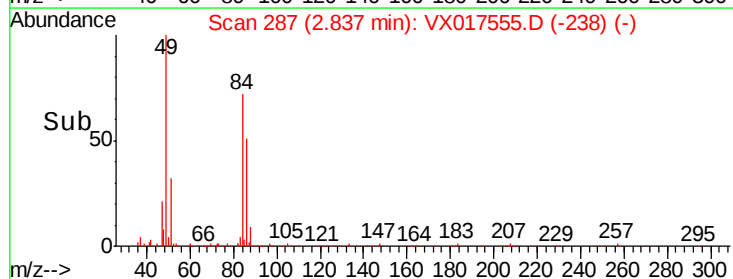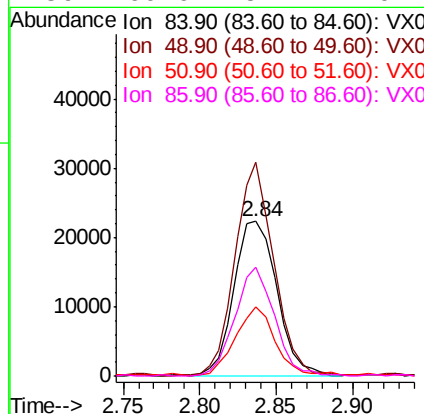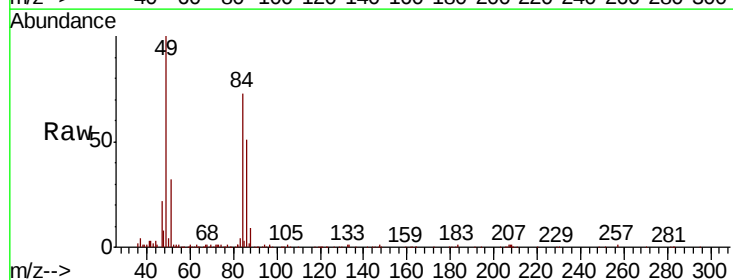

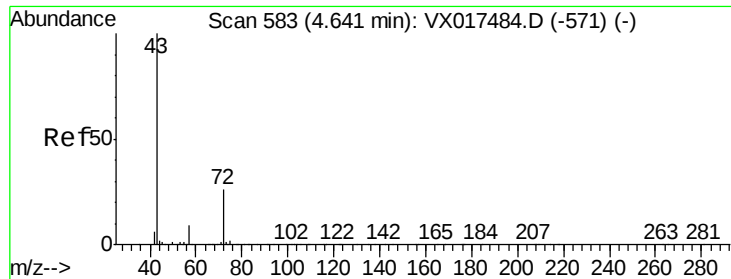

#25

2-Butanone

Concen: 9.502 ug/l

RT: 4.64 min Scan# 583

Delta R.T. -0.00 min

Lab File: VX017555.D

Acq: 24 Jul 2020 19:56

Instrument :

MSVOA_X

ClientSampleId :





BUS-WASH

Tot Ion: 43 Resp: 37873

Ion Ratio Lower Upper

43 100

72 26.4 19.0 28.4

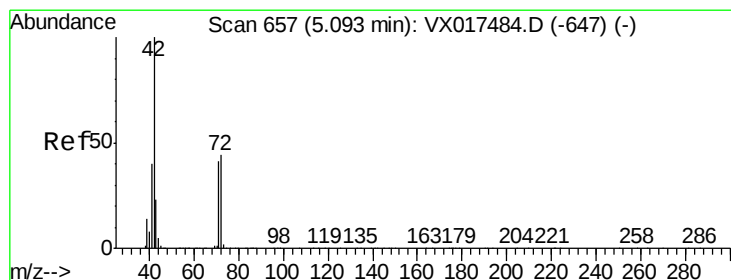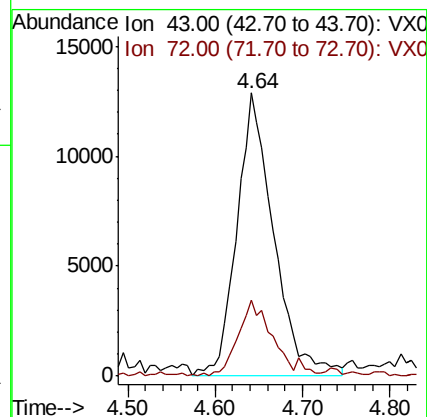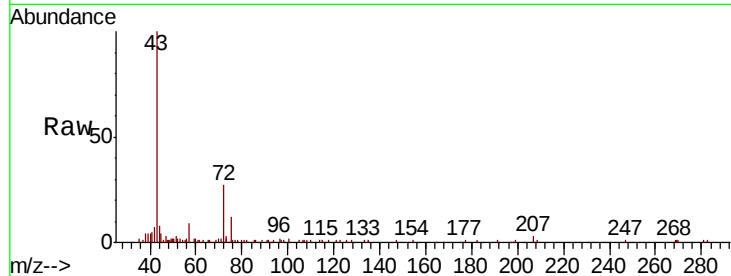

#29

Tetrahydrofuran

Concen: 1.418 ug/l

RT: 5.10 min Scan# 659

Delta R.T. 0.01 min

Lab File: VX017555.D

Acq: 24 Jul 2020 19:56




Tgt Ion: 42 Resp: 3501


Ion Ratio Lower Upper

42 100

72 37.2 35.5 53.3

71 53.4 33.0 49.4#

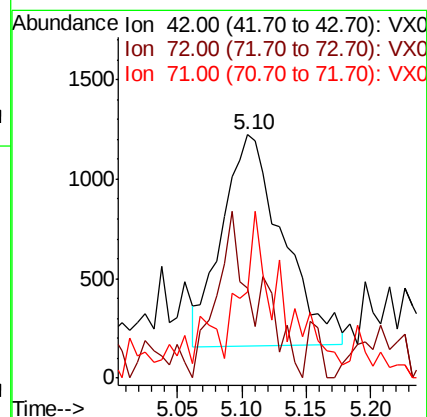

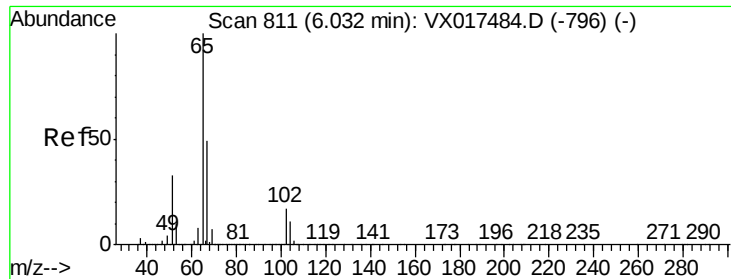

#33

1,2-Dichloroethane-d4

Concen: 49.505 ug/l

RT: 6.03 min Scan# 811

Delta R.T. -0.00 min

Lab File: VX017555.D

Acq: 24 Jul 2020 19:56

Instrument :

MSVOA_X

ClientSampleId :


BUS-WASH

Tot Ion: 65 Resp: 315589

Ion Ratio Lower Upper




65 100

67 51.1 0.0 102.8

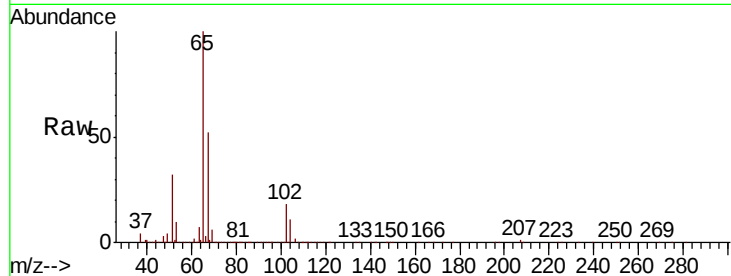

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

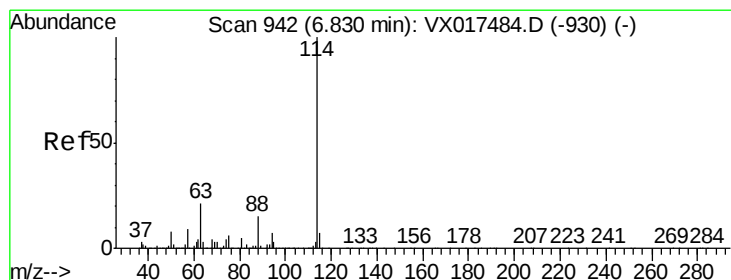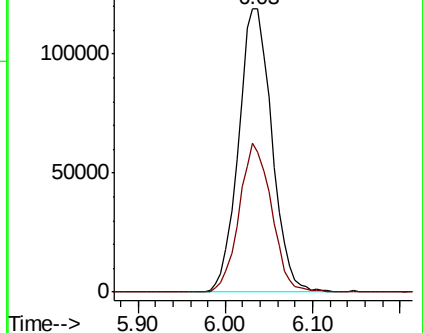

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.83 min Scan# 942

Delta R.T. -0.00 min

Lab File: VX017555.D

Acq: 24 Jul 2020 19:56


Tgt Ion: 114 Resp: 785791

Ion Ratio Lower Upper

114 100

63 21.6 0.0 40.6



88 16.3 0.0 33.4




Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0




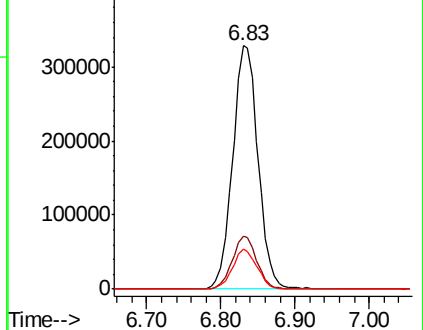


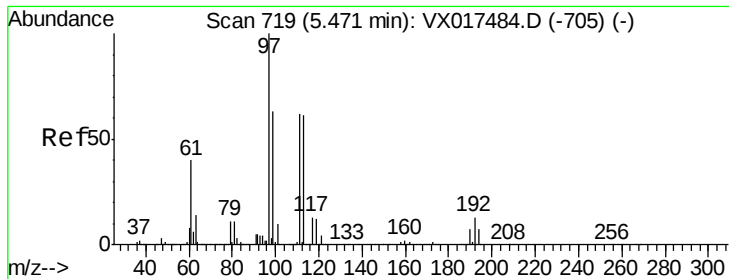

#35
 Dibromofluoromethane
 Concen: 54.493 ug/l
 RT: 5.46 min Scan# 718
 Delta R.T. -0.01 min
 Lab File: VX017555.D
 Acq: 24 Jul 2020 19:56




Instrument :
 MSVOA_X
 ClientSampleId :
 BUS-WASH


Tot Ion	Ratio	Lower	Upper
113	100		
111	101.2	80.7	121.1
192	20.6	16.9	25.3

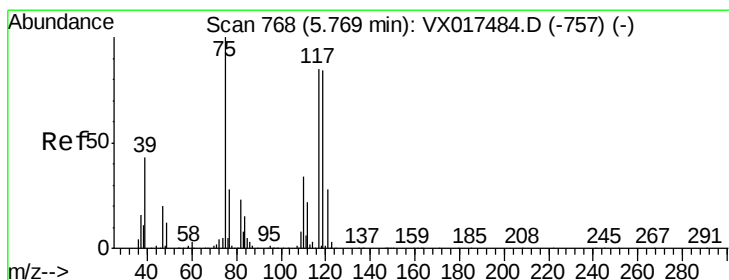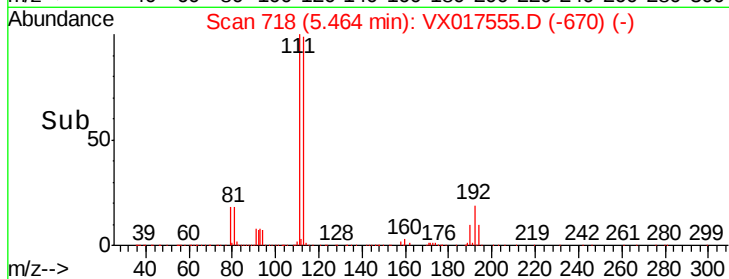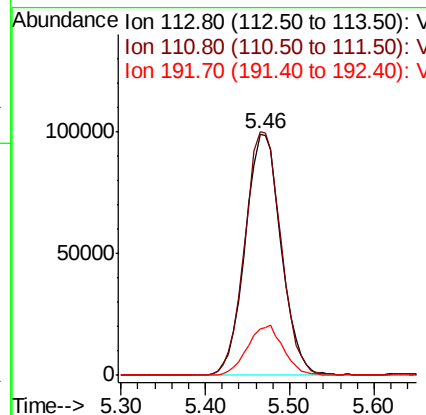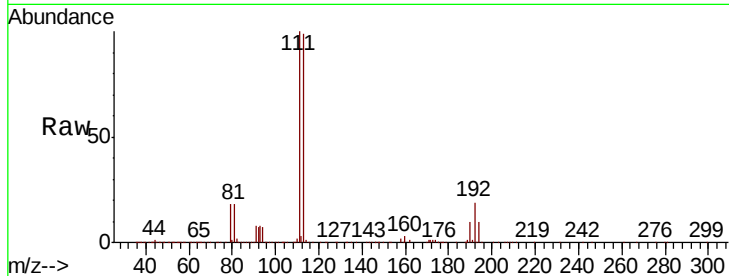

#36
 1,1-Dichloropropene
 Concen: 4.996 ug/l
 RT: 5.64 min Scan# 747
 Delta R.T. -0.13 min
 Lab File: VX017555.D
 Acq: 24 Jul 2020 19:56

Tgt Ion	Ratio	Lower	Upper
75	100		
110	0.0	18.1	54.3#
77	1.2	24.6	37.0#

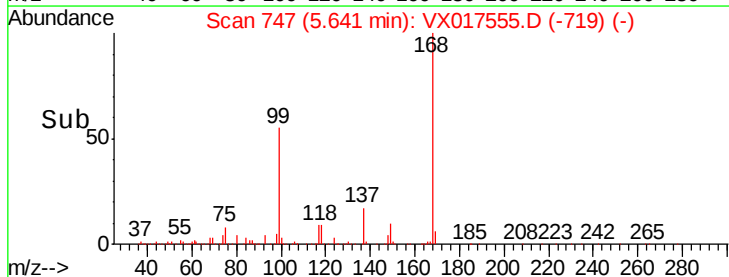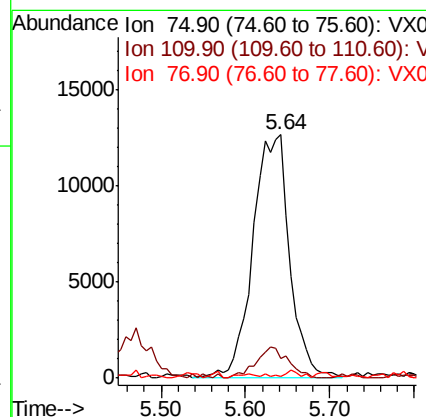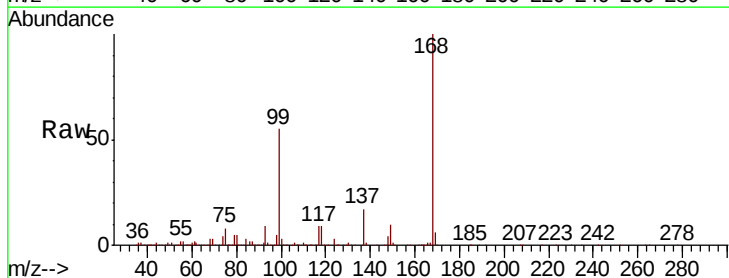


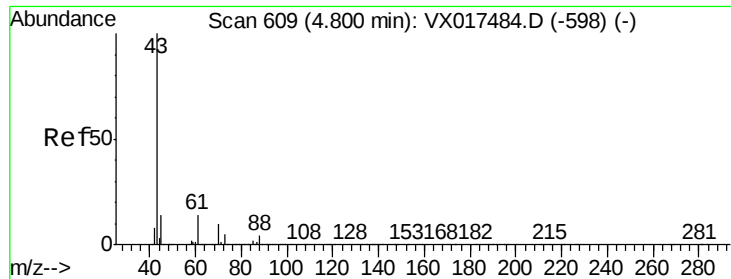




#37
Ethyl Acetate
Concen: 4.593 ug/l
RT: 4.64 min Scan# 583
Delta R.T. -0.16 min
Lab File: VX017555.D
Acq: 24 Jul 2020 19:56

Instrument :
MSVOA_X
ClientSampleId :
BUS-WASH

Tot Ion	Ratio	Lower	Upper
43	100		
61	0.0	10.7	16.1#
70	0.4	8.5	12.7#




Abundance Ion 43.00 (42.70 to 43.70): VX0
Ion 60.90 (60.60 to 61.60): VX0
Ion 70.00 (69.70 to 70.70): VX0

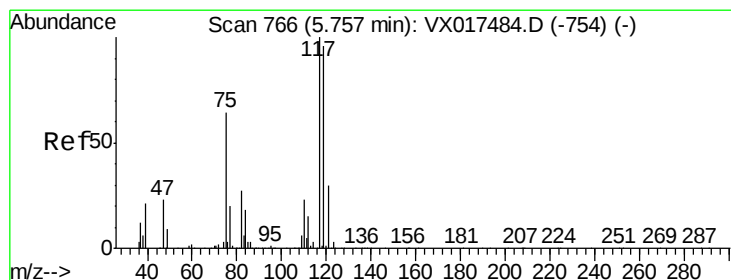
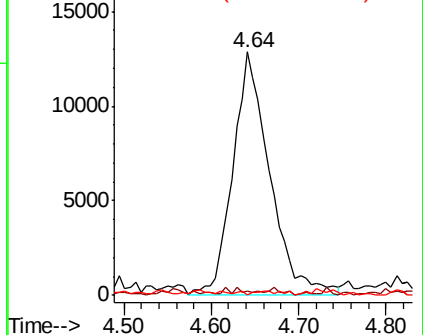



#38
Carbon Tetrachloride
Concen: 5.446 ug/l
RT: 5.63 min Scan# 745
Delta R.T. -0.13 min
Lab File: VX017555.D
Acq: 24 Jul 2020 19:56

Tgt Ion	Ratio	Lower	Upper
117	100		
119	4.0	75.4	113.0#
121	0.0	24.3	36.5#



Abundance Ion 116.80 (116.50 to 117.50): V
Ion 118.80 (118.50 to 119.50): V
Ion 120.80 (120.50 to 121.50): V




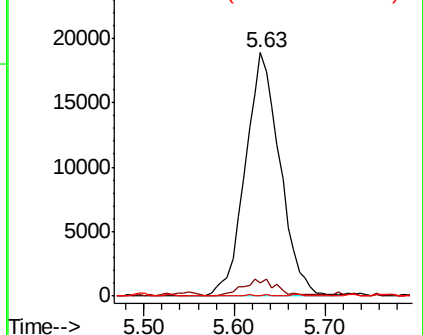




#41
Methacrylonitrile
Concen: 0.213 ug/l
RT: 4.98 min Scan# 639
Delta R.T. -0.02 min
Lab File: VX017555.D
Acq: 24 Jul 2020 19:56




Instrument :
MSVOA_X
ClientSampleId :
BUS-WASH


Tot Ion:	41	Resp:	1007
Ion	Ratio	Lower	Upper
41	100		
39	28.7	43.9	65.9#
67	28.5	54.0	81.0#
52	44.8	23.0	34.6#

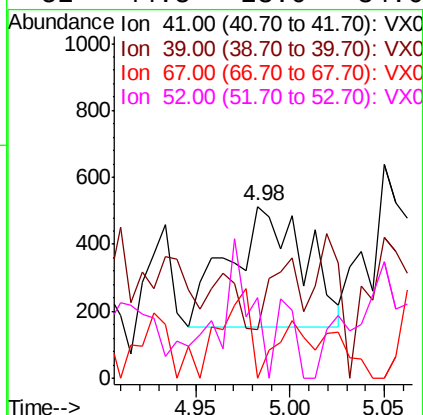

#43
Isopropyl Acetate
Concen: 4.663 ug/l
RT: 6.42 min Scan# 874
Delta R.T. -0.00 min
Lab File: VX017555.D
Acq: 24 Jul 2020 19:56

Tgt Ion:	43	Resp:	63447
Ion	Ratio	Lower	Upper
43	100		
61	20.3	15.5	23.3
87	13.8	10.5	15.7


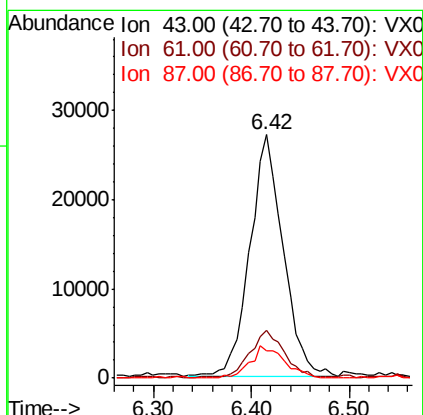




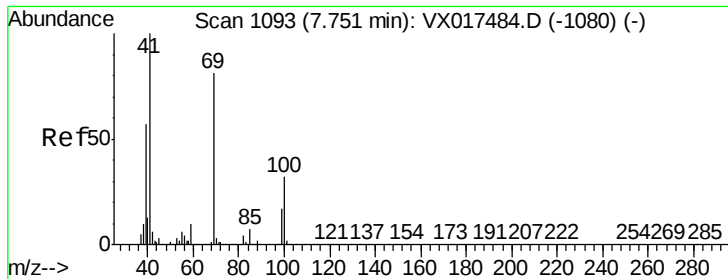

#48
Methvl methacrylate
Concen: 1.554 ug/l
RT: 7.66 min Scan# 1078
Delta R.T. -0.09 min
Lab File: VX017555.D
Acq: 24 Jul 2020 19:56




Instrument :
MSVOA_X
ClientSampleId :
BUS-WASH


Tot Ion	Ratio	Lower	Upper
41	100		
69	0.0	63.1	94.7#
39	18.6	45.1	67.7#

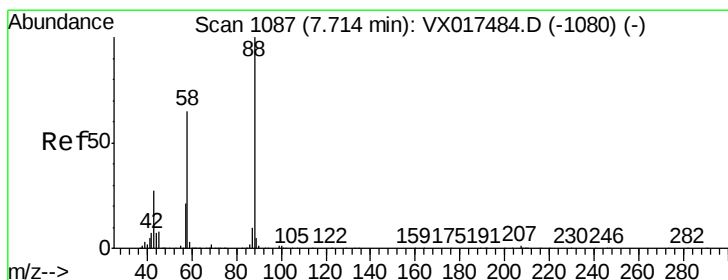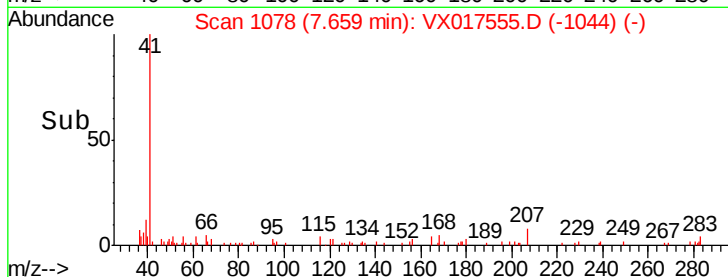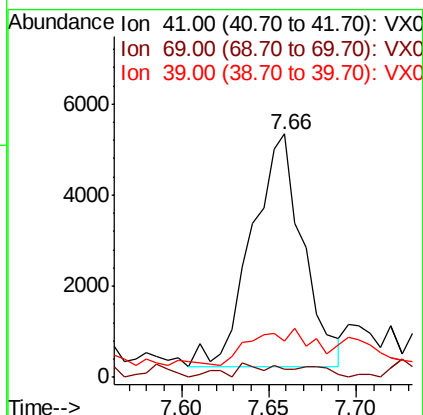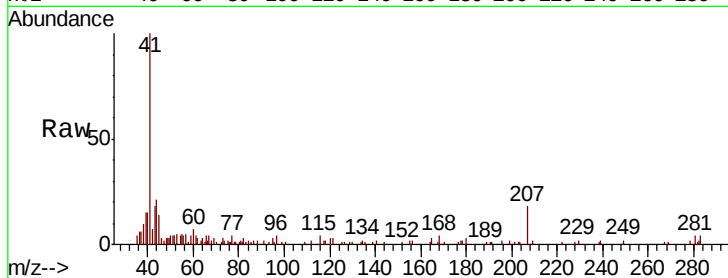

#49
1,4-Dioxane
Concen: 1.284 ug/l
RT: 7.70 min Scan# 1084
Delta R.T. -0.02 min
Lab File: VX017555.D
Acq: 24 Jul 2020 19:56

Tgt Ion	Ratio	Lower	Upper
88	100		
43	0.0	27.8	41.6#
58	1077.7	58.3	87.5#

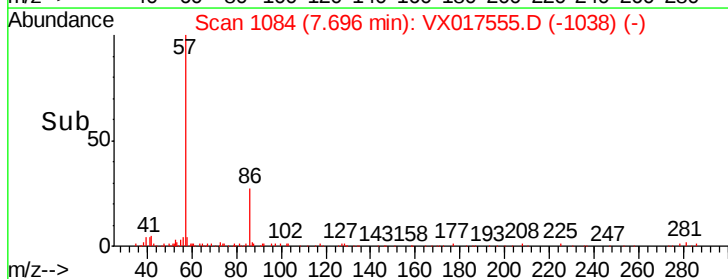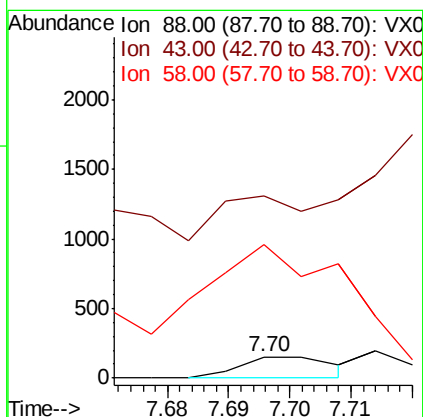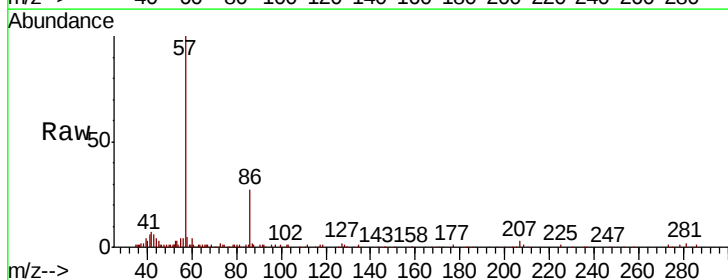



#50

Toluene-d8

Concen: 54.109 ug/l

RT: 8.70 min Scan# 1248

Delta R.T. -0.00 min

Lab File: VX017555.D

Acq: 24 Jul 2020 19:56

Instrument :

MSVOA_X

ClientSampleId :





BUS-WASH

Tot Ion: 98 Resp: 1025834

Ion Ratio Lower Upper

98 100

100 64.3 52.3 78.5

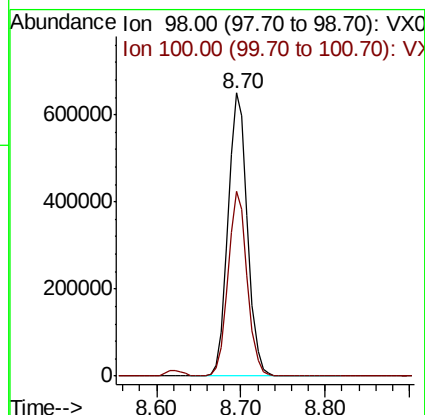

#51

4-Methyl-2-Pentanone

Concen: 27.057 ug/l

RT: 8.62 min Scan# 1235

Delta R.T. -0.01 min

Lab File: VX017555.D




Acq: 24 Jul 2020 19:56


Tgt Ion: 43 Resp: 219645

Ion Ratio Lower Upper

43 100

58 24.9 31.0 46.4#

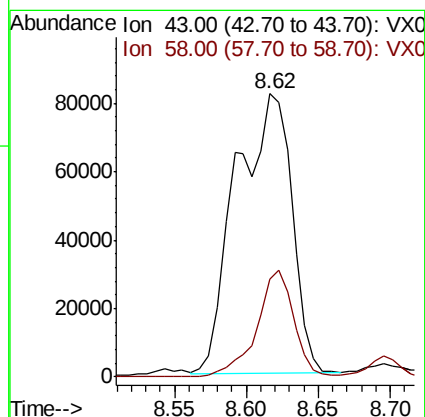



#52

Toluene

Concen: 0.333 ug/l

RT: 8.77 min Scan# 1260

Delta R.T. -0.00 min

Lab File: VX017555.D

Acq: 24 Jul 2020 19:56

Instrument :

MSVOA_X

ClientSampleId :





BUS-WASH

Tot Ion: 92 Resp: 4615

Ion Ratio Lower Upper

92 100

91 205.3 137.6 206.4

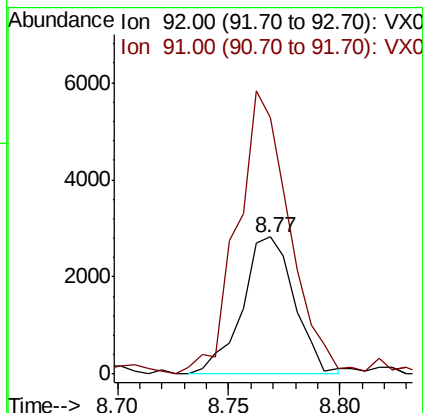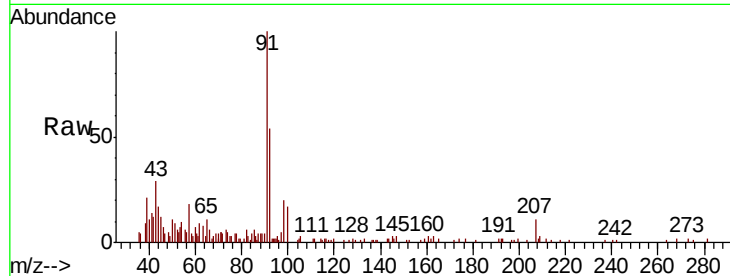

#54

cis-1,3-Dichloropropene

Concen: 4.804 ug/l

RT: 8.59 min Scan# 1231

Delta R.T. 0.18 min

Lab File: VX017555.D

Acq: 24 Jul 2020 19:56




Tgt Ion: 75 Resp: 46722


Ion Ratio Lower Upper

75 100

77 0.3 25.5 38.3#

39 29.6 41.8 62.8#



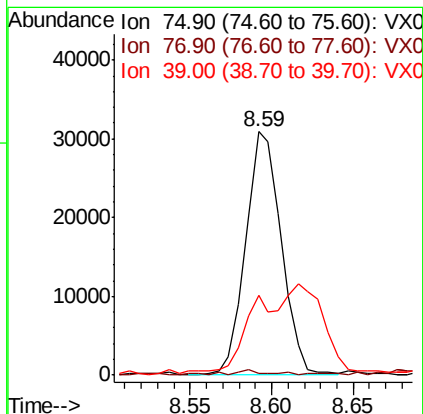
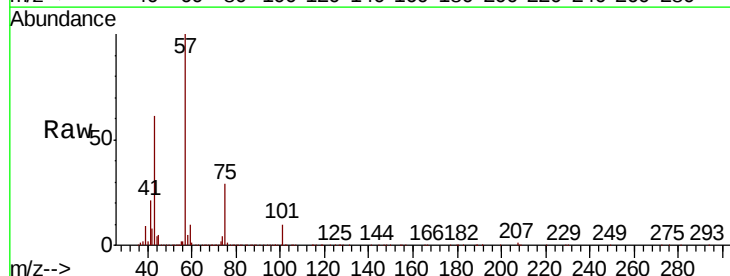


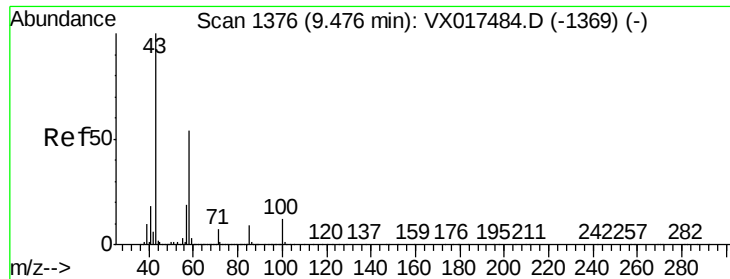

#59
2-Hexanone
Concen: 9.576 ug/l
RT: 9.52 min Scan# 1384
Delta R.T. 0.05 min
Lab File: VX017555.D
Acq: 24 Jul 2020 19:56




Instrument :
MSVOA_X
ClientSampled :
BUS-WASH


Tot Ion: 43 Resp: 58524
Ion Ratio Lower Upper
43 100
58 19.6 26.6 79.8#

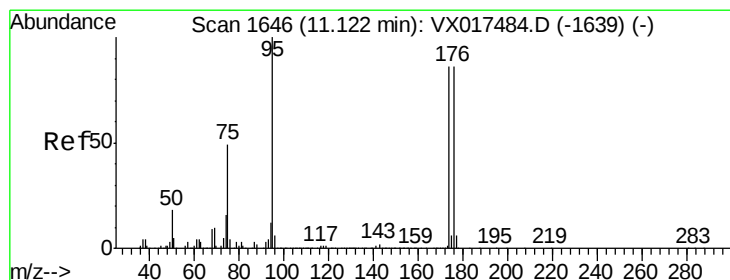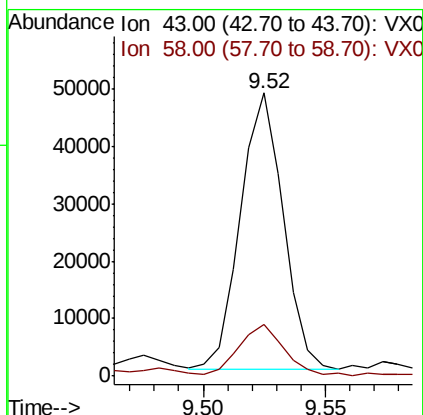

#62
4-Bromofluorobenzene
Concen: 56.413 ug/l
RT: 11.12 min Scan# 1646
Delta R.T. -0.00 min
Lab File: VX017555.D
Acq: 24 Jul 2020 19:56

Tgt Ion: 95 Resp: 428027
Ion Ratio Lower Upper
95 100
174 85.2 0.0 169.0
176 82.8 0.0 161.0


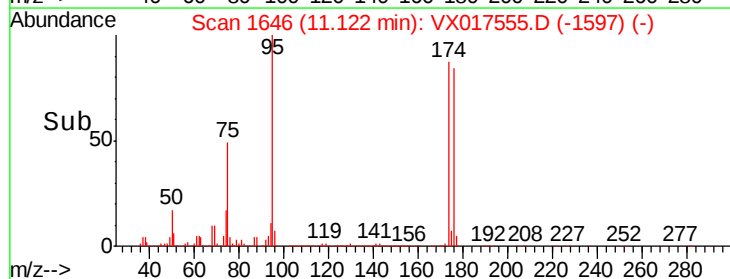
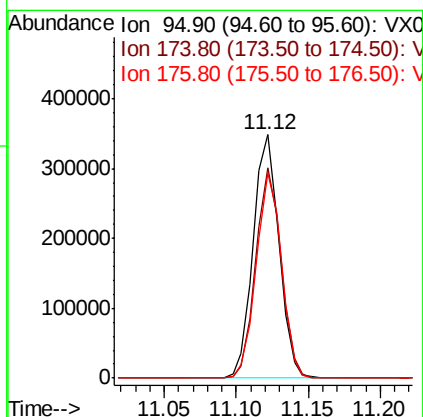
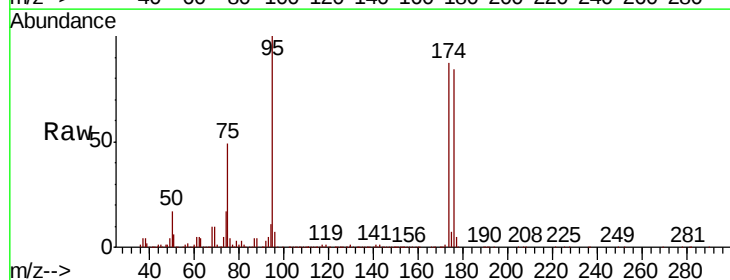




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.10 min Scan# 1478
Delta R.T. -0.00 min
Lab File: VX017555.D
Acq: 24 Jul 2020 19:56




Instrument :
MSVOA_X
ClientSampleId :
BUS-WASH


Tot Ion	Ratio	Lower	Upper
117	100		
82	53.5	44.0	66.0
119	32.4	25.4	38.0

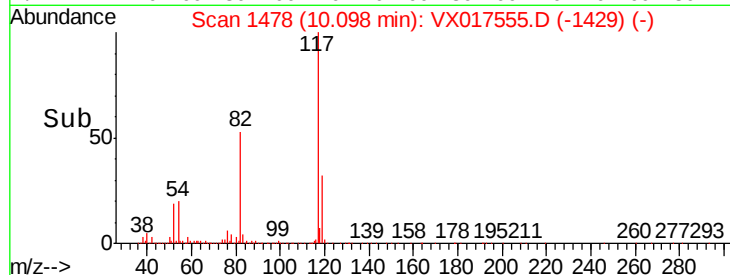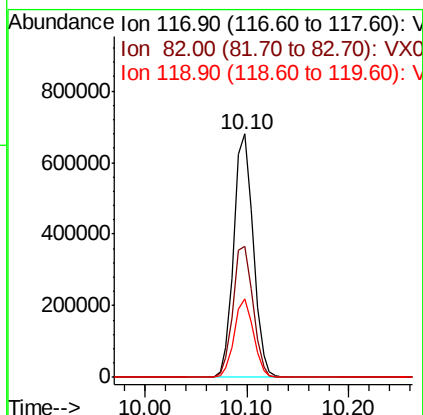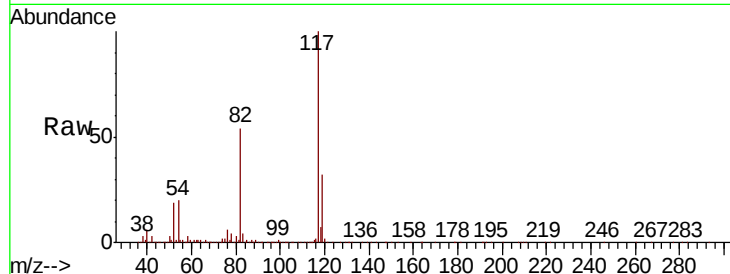

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.06 min Scan# 1800
Delta R.T. -0.00 min
Lab File: VX017555.D
Acq: 24 Jul 2020 19:56

Tgt Ion	Ratio	Lower	Upper
152	100		
115	57.8	65.5	196.6#
150	155.0	0.0	412.6

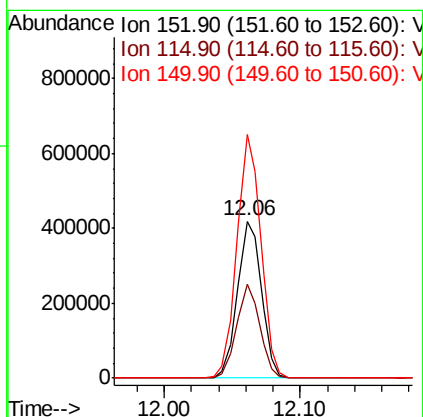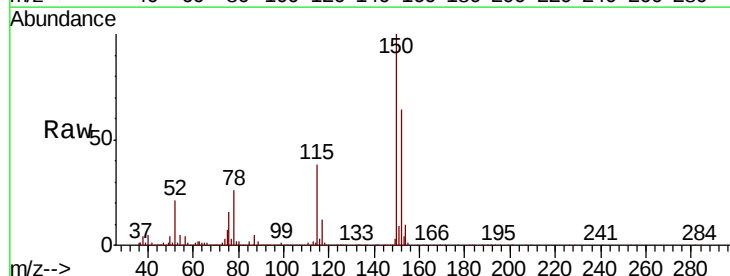

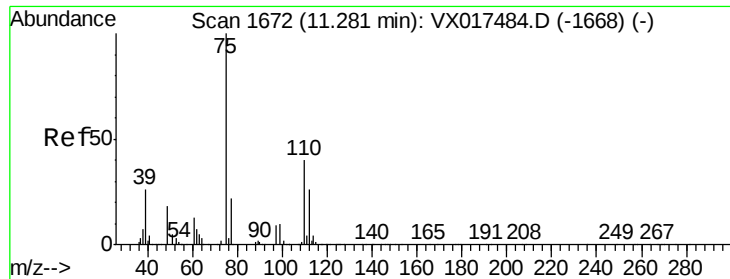

#76

1,2,3-Trichloropropane

Concen: 20.691 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. -0.16 min

Lab File: VX017555.D

Acq: 24 Jul 2020 19:56

Instrument :

MSVOA_X

ClientSampleId :


BUS-WASH

Tot Ion: 75 Resp: 218877

Ion Ratio Lower Upper

75 100

77 1.4 21.8 65.3#

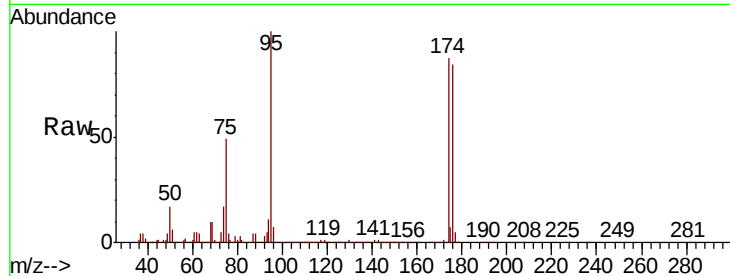

Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 77.00 (76.70 to 77.70): VX0

11.12



150000

100000

50000

0

Time-->

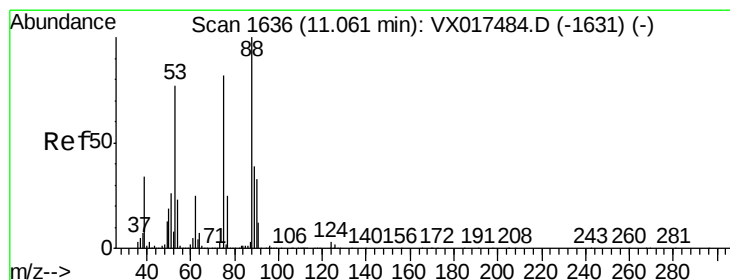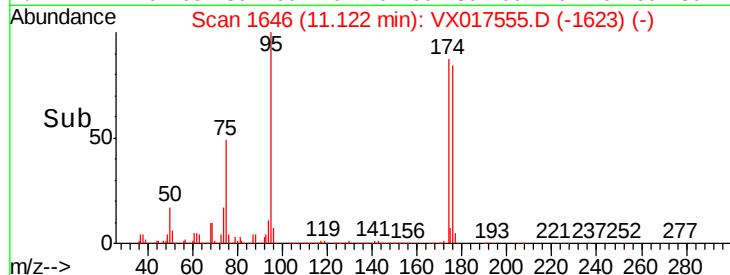

#81

trans-1,4-Dichloro-2-butene

Concen: 52.137 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. 0.06 min

Lab File: VX017555.D

Acq: 24 Jul 2020 19:56


Tgt Ion: 75 Resp: 218877

Ion Ratio Lower Upper

75 100

53 0.0 75.9 113.9#

89 0.0 37.8 56.6#



Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 53.00 (52.70 to 53.70): VX0

Ion 88.90 (88.60 to 89.60): VX0

11.12


150000


100000

50000

0

Time-->







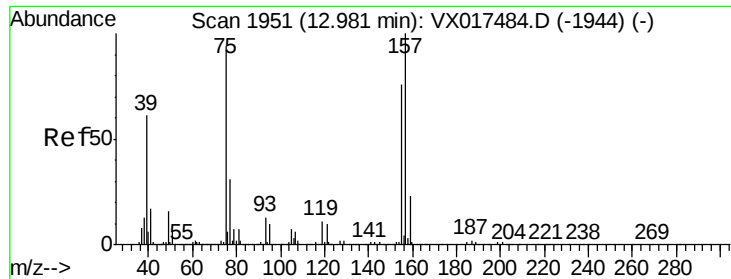

#92
 1,2-Dibromo-3-Chloropropane
 Concen: 2.680 ug/l
 RT: 12.93 min Scan# 1942
 Delta R.T. -0.05 min
 Lab File: VX017555.D
 Acq: 24 Jul 2020 19:56

Instrument :
 MSVOA_X
 ClientSampleId :
 BUS-WASH

Tot Ion: 75 Resp: 339
 Ion Ratio Lower Upper
 75 100
 155 48.7 42.3 126.8
 157 68.4 54.3 162.9

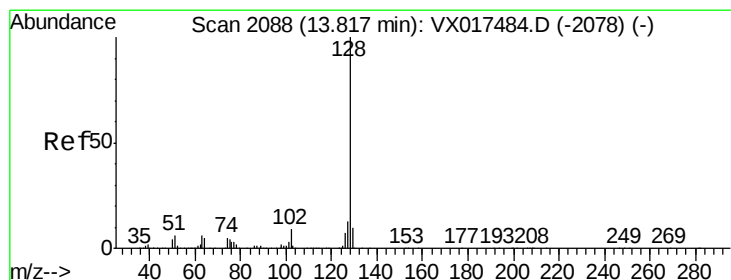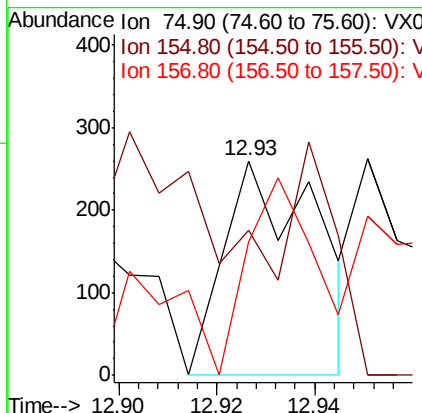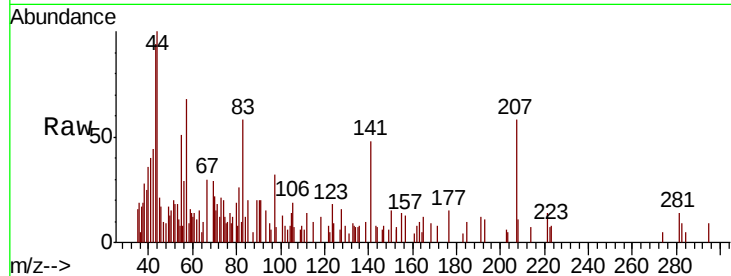

#95
 Naphthalene
 Concen: 0.219 ug/l
 RT: 13.82 min Scan# 2088
 Delta R.T. -0.00 min
 Lab File: VX017555.D
 Acq: 24 Jul 2020 19:56

Tgt Ion: 128 Resp: 7437
 Ion Ratio Lower Upper
 128 100
 127 17.8 10.4 15.6#
 129 15.0 8.9 13.3#

