

Data Path : Z:\VOASRV\HPCHEM1\MSVOA\_X\DATA\VX072420\  
 Data File : VX017546.D  
 Acq On : 24 Jul 2020 16:30  
 Operator : JC/SP  
 Sample : L3410-03  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 16 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 FM-FRAC

Integration Parameters: RTEINT.P

Integrator: RTE  
 Smoothing : ON Filtering: 5  
 Sampling : 1 Min Area: 3 % of largest Peak  
 Start Thrs: 0.2 Max Peaks: 100  
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X072320W.M  
 Title : SW846 8260

Signal : TIC

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 2.422       | 214           | 219         | 226          | rVB      | 47665          | 75451         | 3.06%           | 0.548%        |
| 2         | 2.581       | 240           | 245         | 255          | rVB      | 29963          | 57546         | 2.33%           | 0.418%        |
| 3         | 5.470       | 704           | 719         | 731          | rBV2     | 306923         | 874700        | 35.48%          | 6.351%        |
| 4         | 5.629       | 733           | 745         | 758          | rVV      | 477519         | 1295901       | 52.57%          | 9.410%        |
| 5         | 6.031       | 803           | 811         | 822          | rBV      | 303292         | 769262        | 31.20%          | 5.586%        |
| 6         | 6.830       | 932           | 942         | 955          | rBV2     | 706001         | 1689926       | 68.55%          | 12.271%       |
| 7         | 8.695       | 1241          | 1248        | 1257         | rBV      | 1610219        | 2465305       | 100.00%         | 17.901%       |
| 8         | 10.098      | 1470          | 1478        | 1488         | rBV      | 1658716        | 2270323       | 92.09%          | 16.485%       |
| 9         | 11.122      | 1640          | 1646        | 1652         | rBV      | 1532669        | 1924671       | 78.07%          | 13.976%       |
| 10        | 12.061      | 1794          | 1800        | 1808         | rVB      | 1949257        | 2348634       | 95.27%          | 17.054%       |


Sum of corrected areas: 13771719

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA\_X\DATA\VX072420\  
Data File : VX017546.D  
Acq On : 24 Jul 2020 16:30  
Operator : JC/SP  
Sample : L3410-03  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 16 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
FM-FRAC

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X072320W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

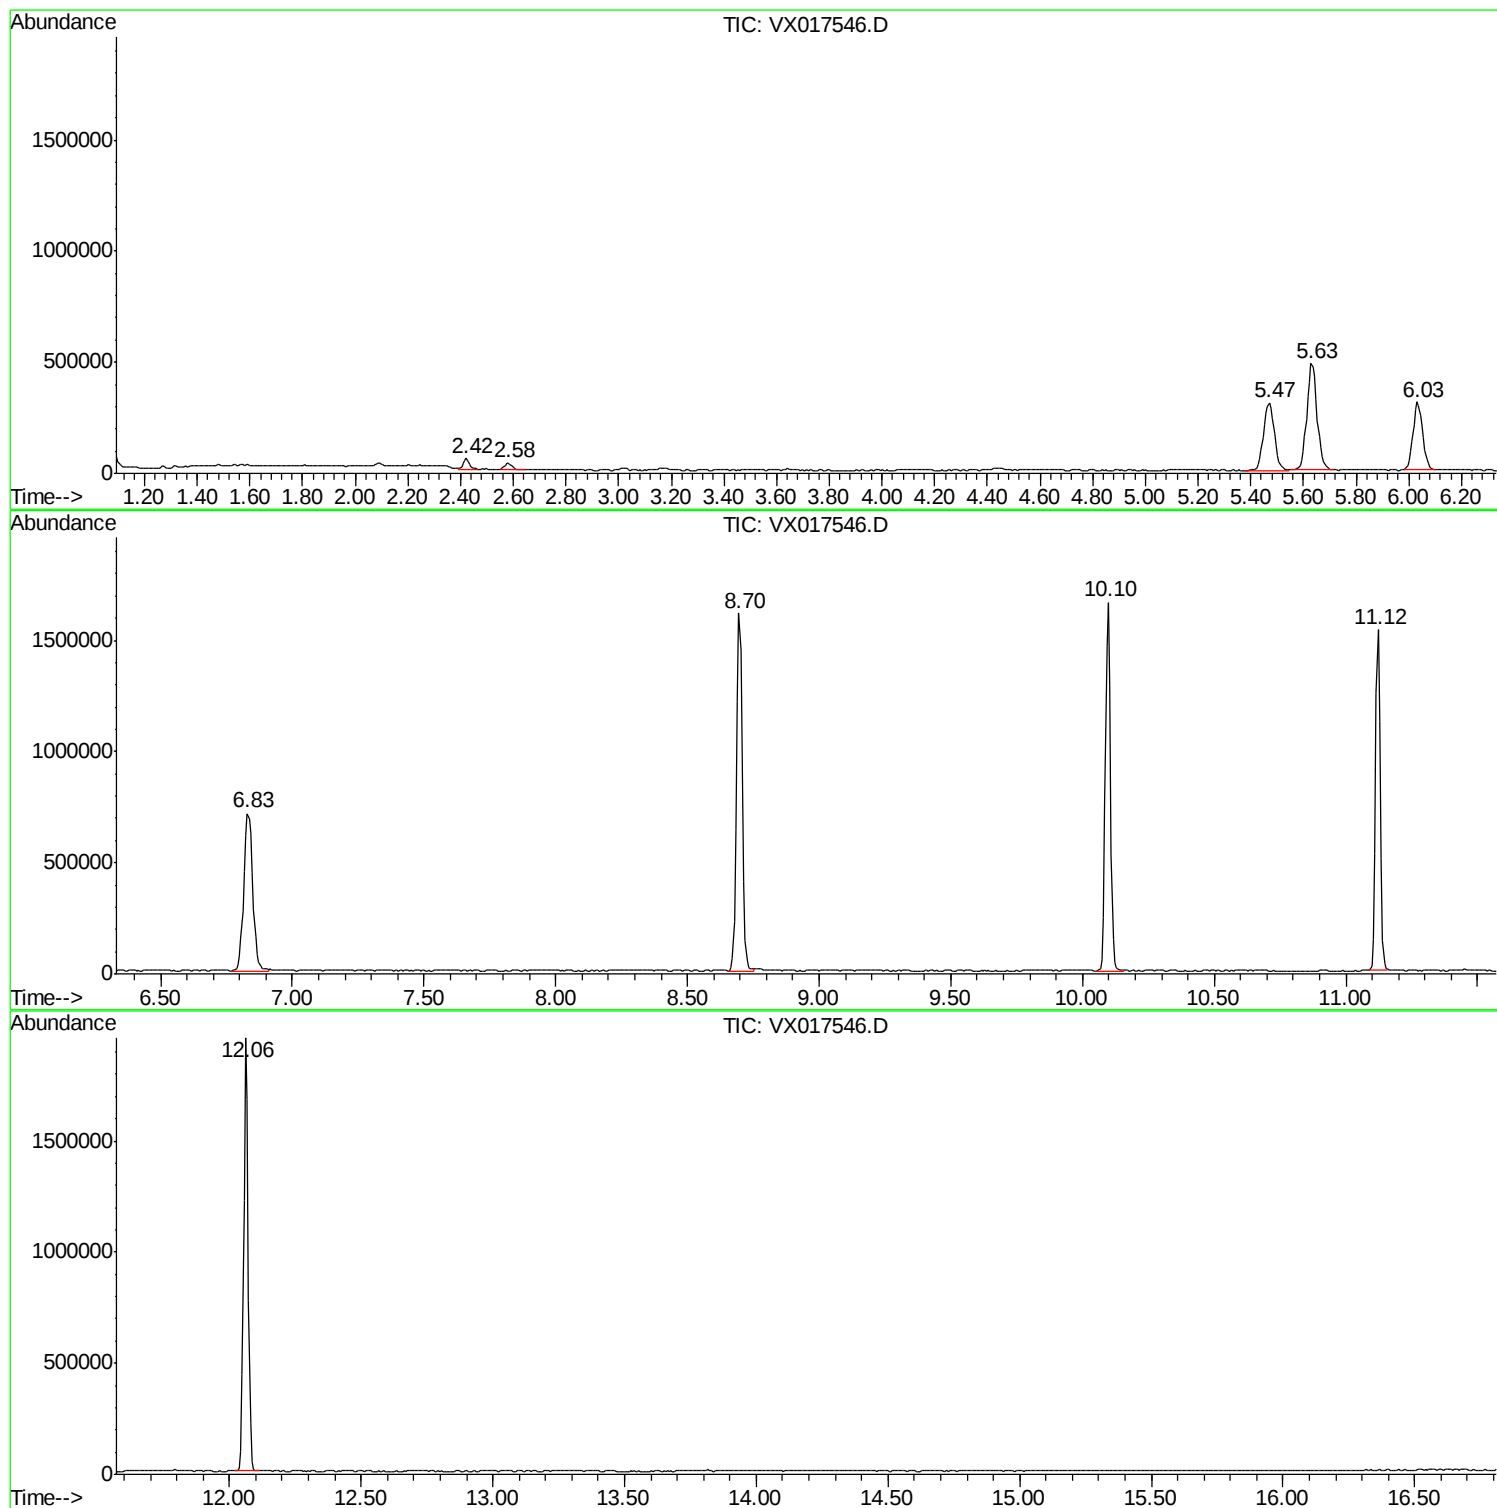

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA\_X\DATA\VX072420\  
Data File : VX017546.D  
Acq On : 24 Jul 2020 16:30  
Operator : JC/SP  
Sample : L3410-03  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 16 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
FM-FRAC

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X072320W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA\_X\DATA\VX072420\  
Data File : VX017546.D  
Acq On : 24 Jul 2020 16:30  
Operator : JC/SP  
Sample : L3410-03  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 16 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
FM-FRAC

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X072320W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |
|------------------|----|---------|-------|----------|-----------------------|
|                  |    |         |       |          | # RT Resp Conc        |