


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX072420\
 Data File : VX017585.D
 Acq On : 25 Jul 2020 10:41
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X072320W.M
 Title : SW846 8260
 Last Update : Fri Jul 24 05:48:09 2020

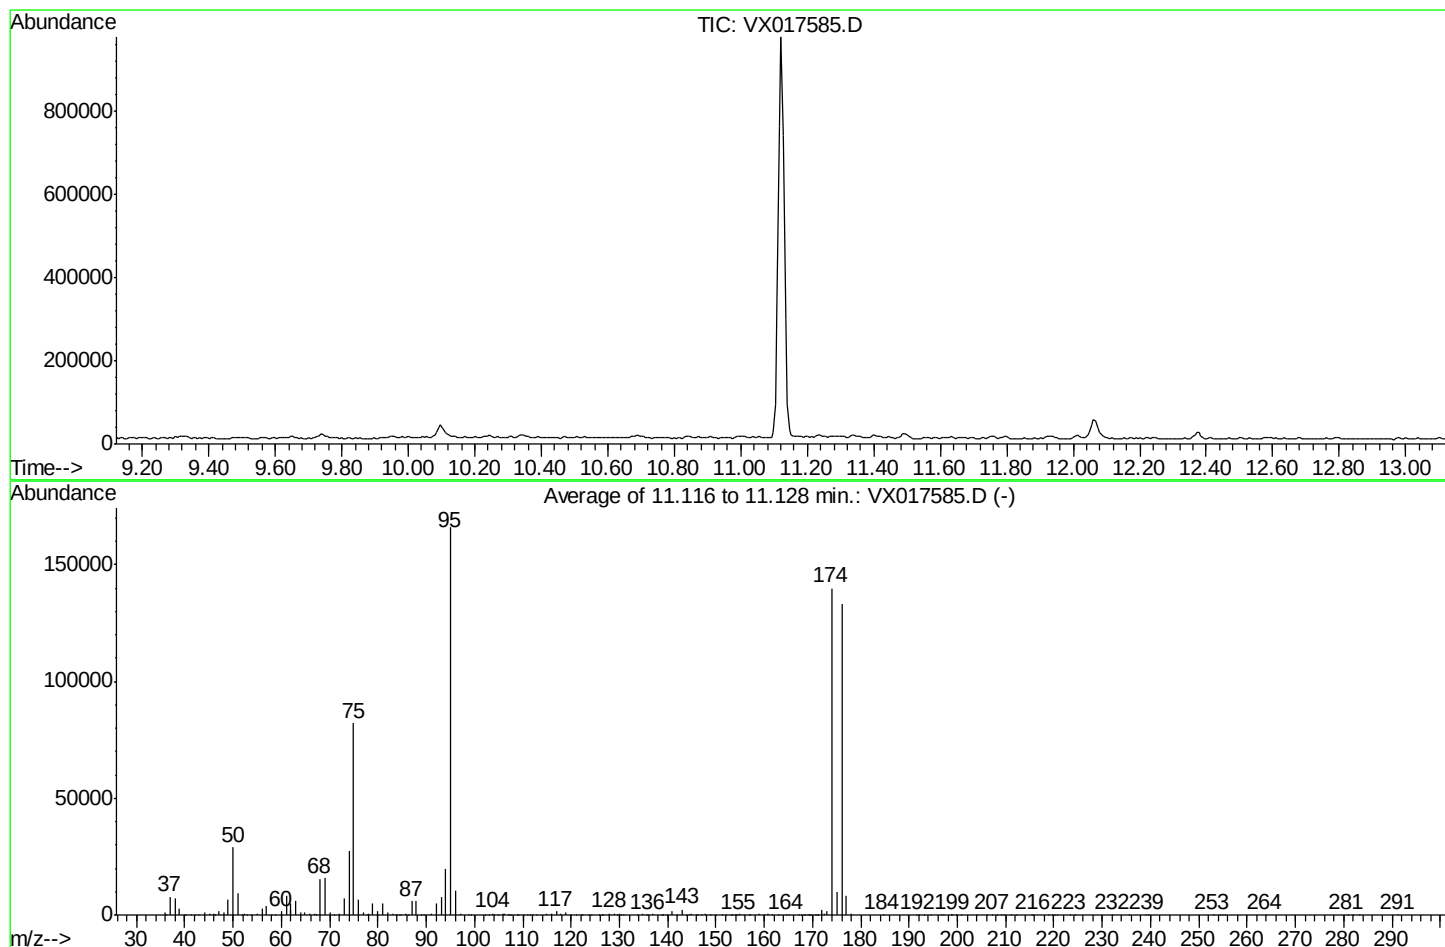

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1636

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	28952	PASS
75	95	30	60	49.4	81959	PASS
95	95	100	100	100.0	165952	PASS
96	95	5	9	6.4	10702	PASS
173	174	0.00	2	1.3	1887	PASS
174	95	50	100	84.3	139968	PASS
175	174	5	9	7.2	10106	PASS
176	174	95	101	95.0	132970	PASS
177	176	5	9	6.2	8215	PASS