

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072423\
 Data File : VX036634.D
 Acq On : 24 Jul 2023 16:57
 Operator : JC/MD
 Sample : 03722-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 33712

Quant Time: Jul 25 06:37:35 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072123W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jul 21 12:14:12 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) Pentafluorobenzene	5.550	168	158014	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	280805	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	261850	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	121921	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	107534	45.993	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	91.980%
35) Dibromofluoromethane	5.385	113	89541	46.392	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	92.780%
50) Toluene-d8	8.647	98	335089	48.957	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	97.920%
62) 4-Bromofluorobenzene	11.079	95	132394	51.269	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	102.540%
Target Compounds						
					Qvalue	
11) Tert butyl alcohol	2.965	59	3592	6.489	ug/l #	74
13) Acrolein	2.239	56	228	0.722	ug/l #	14
16) Acetone	2.380	43	25211	25.985	ug/l	92
17) Carbon Disulfide	2.514	76	4674	0.957	ug/l	97
25) 2-Butanone	4.574	43	5701	3.622	ug/l	99
36) 1,1-Dichloropropene	5.556	75	13343	4.638	ug/l #	50
37) Ethyl Acetate	4.574	43	5696	1.749	ug/l #	69
38) Carbon Tetrachloride	5.550	117	16711	5.464	ug/l #	16
51) 4-Methyl-2-Pentanone	8.574	43	4825	1.556	ug/l	97
52) Toluene	8.720	92	2366	0.451	ug/l	91
59) 2-Hexanone	9.439	43	915	0.397	ug/l	96
67) Ethyl Benzene	10.195	91	11675	1.107	ug/l	100
68) m/p-Xylenes	10.299	106	26808	6.814	ug/l	99
69) o-Xylene	10.640	106	26149	6.659	ug/l	99
70) Styrene	10.646	104	1508	0.233	ug/l #	1
73) Isopropylbenzene	10.963	105	9578	0.949	ug/l	100
74) N-amyl acetate	10.854	43	1657	0.352	ug/l #	21
76) 1,2,3-Trichloropropane	11.079	75	68103	23.748	ug/l #	39
78) n-propylbenzene	11.305	91	21629	1.854	ug/l	98
79) 2-Chlorotoluene	11.378	91	19279	2.726	ug/l #	42
80) 1,3,5-Trimethylbenzene	11.451	105	49287	5.839	ug/l	100
81) trans-1,4-Dichloro-2-b...	11.079	75	68103	53.827	ug/l #	5
82) 4-Chlorotoluene	11.451	91	5550	0.689	ug/l #	46
83) tert-Butylbenzene	11.750	119	23582	2.844	ug/l #	56
84) 1,2,4-Trimethylbenzene	11.750	105	202553	23.994	ug/l	96
85) sec-Butylbenzene	11.890	105	12970	1.254	ug/l	90
86) p-Isopropyltoluene	12.006	119	8491	0.998	ug/l	94
89) n-Butylbenzene	12.329	91	22854	3.000	ug/l #	28
90) Hexachloroethane	12.530	117	4732	2.743	ug/l #	17
92) 1,2-Dibromo-3-Chloropr...	12.920	75	391	0.494	ug/l #	9
95) Naphthalene	13.774	128	163700	18.566	ug/l	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072423\
Data File : VX036634.D
Acq On : 24 Jul 2023 16:57
Operator : JC/MD
Sample : 03722-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
33712


Quant Time: Jul 25 06:37:35 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072123W.M
Quant Title : SW846 8260
QLast Update : Fri Jul 21 12:14:12 2023
Response via : Initial Calibration

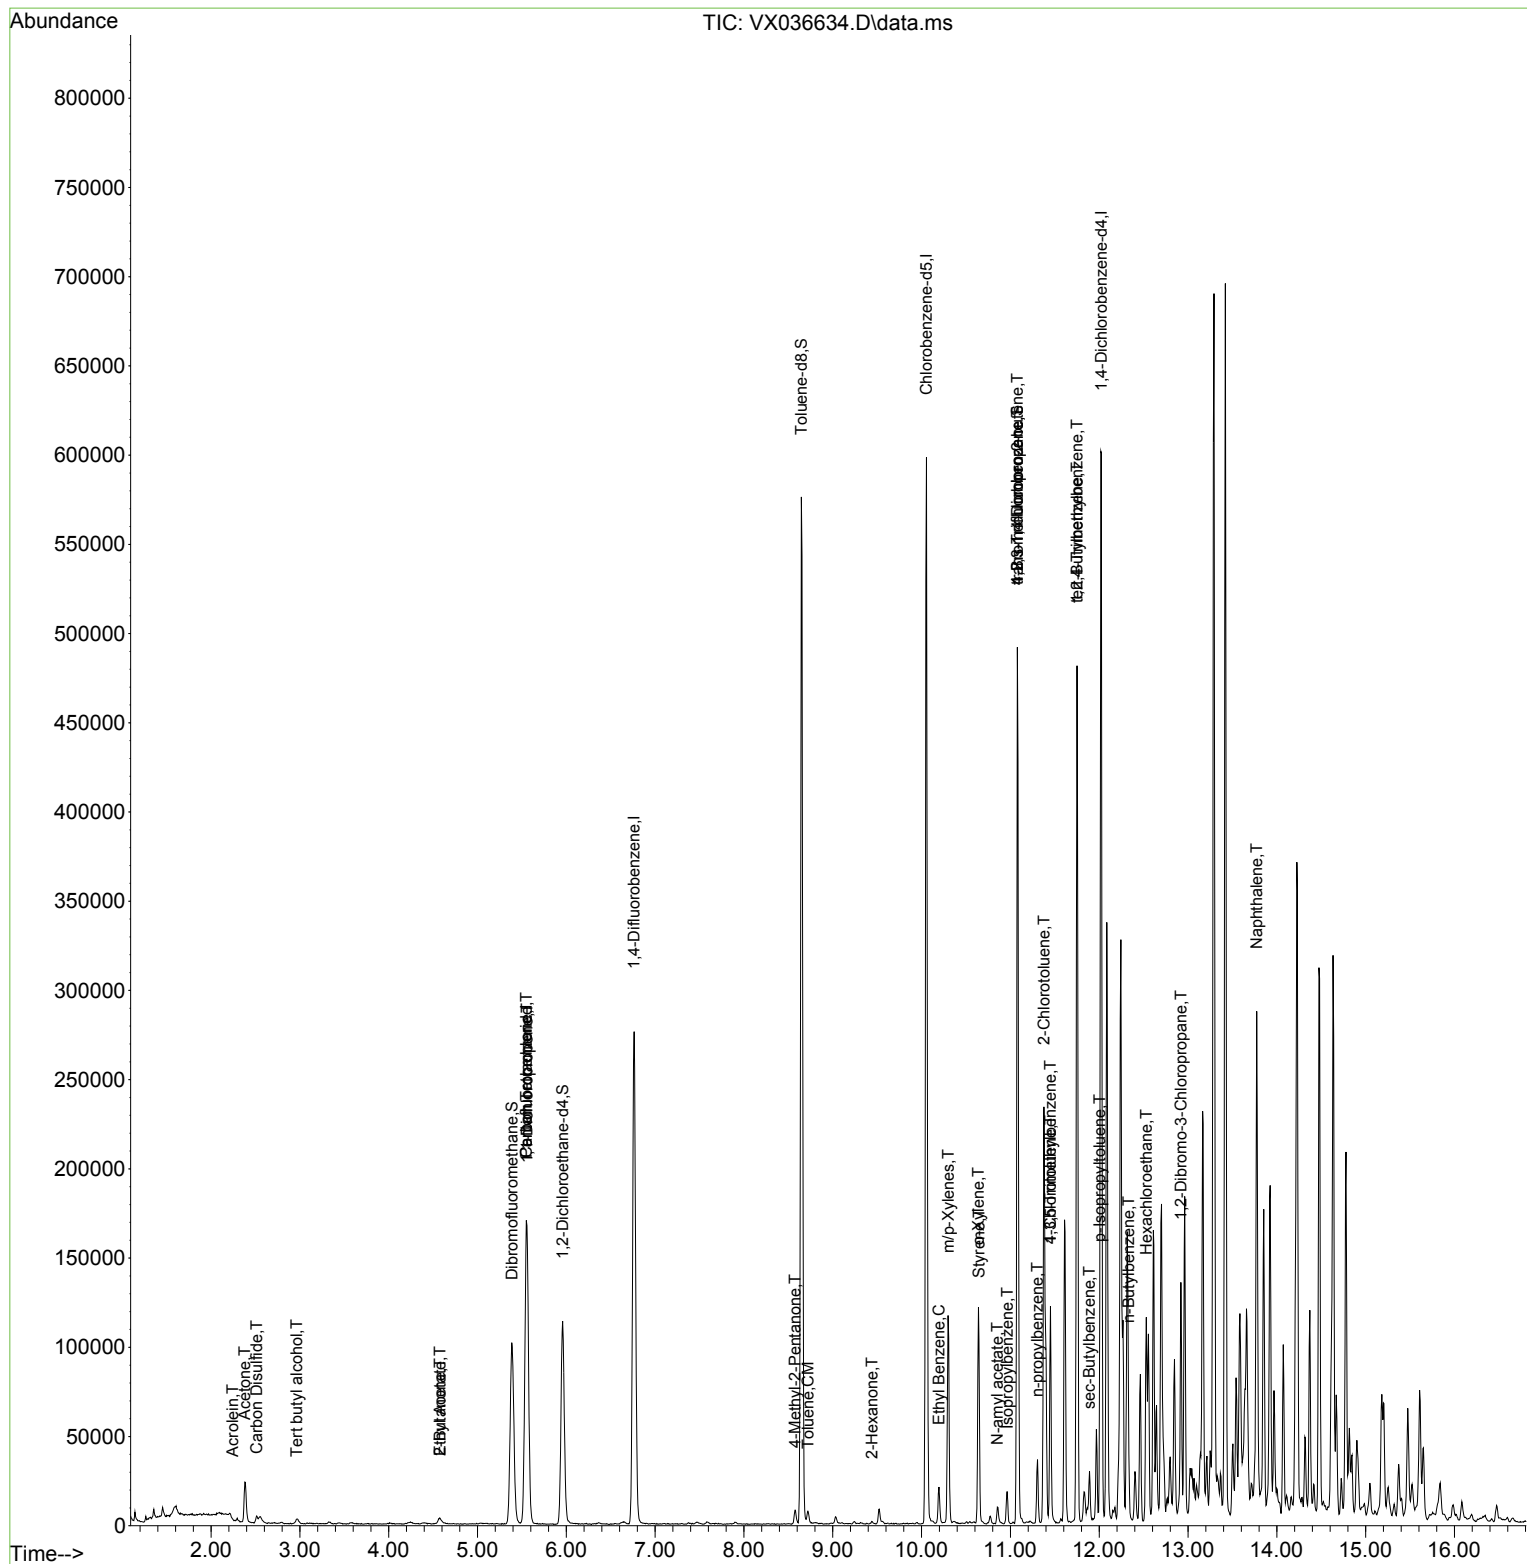



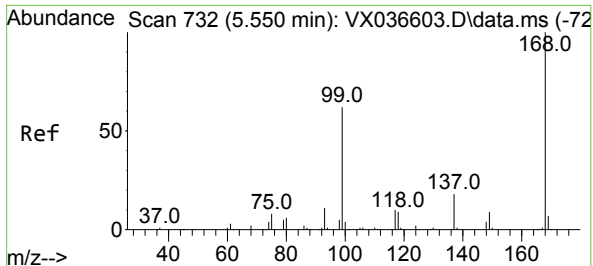


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 712
Delta R.T. -0.000 min
Lab File: VX036634.D
Acq: 24 Jul 2023 16:57

Instrument :
MSVOA_X
ClientSampleId :
33712



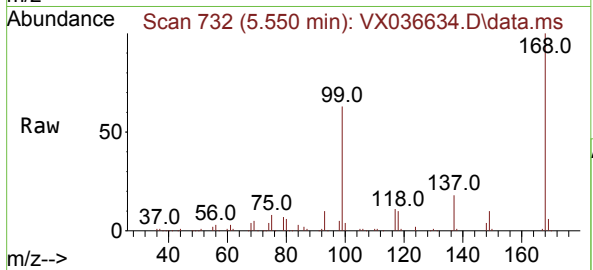



Tgt Ion:168 Resp: 158014
Ion Ratio Lower Upper
168 100
99 63.4 56.6 85.0

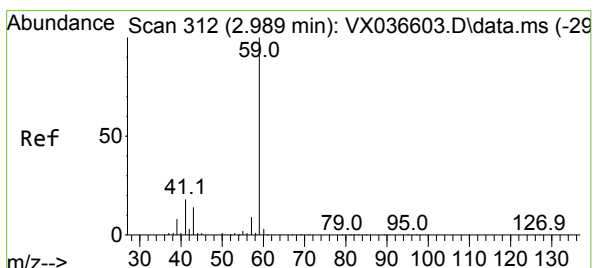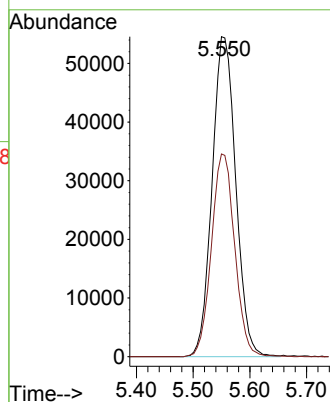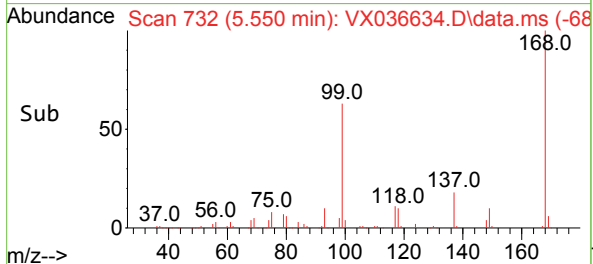

#11
Tert butyl alcohol
Concen: 6.489 ug/l
RT: 2.965 min Scan# 308
Delta R.T. -0.024 min
Lab File: VX036634.D
Acq: 24 Jul 2023 16:57

Tgt Ion: 59 Resp: 3592
Ion Ratio Lower Upper
59 100
57 16.7 6.0 9.0#

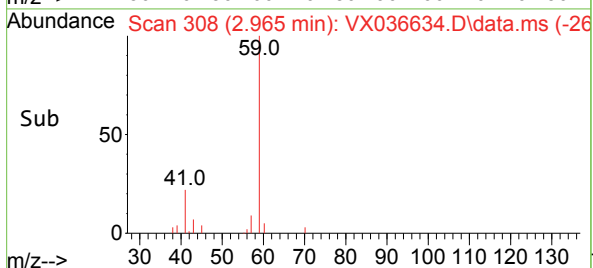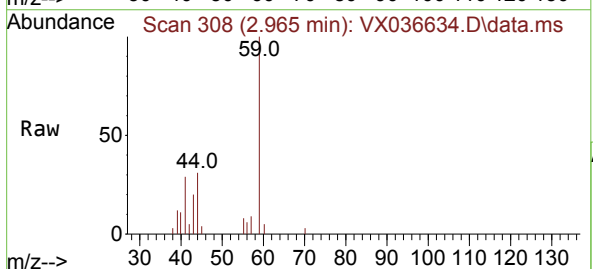



#13

Acrolein

Concen: 0.722 ug/l

RT: 2.239 min Scan# 11

Delta R.T. 0.000 min

Lab File: VX036634.D

Acq: 24 Jul 2023 16:57

Instrument :

MSVOA_X

ClientSampleId :





33712

Tgt Ion: 56 Resp: 228

Ion Ratio Lower Upper

56 100

55 0.0 57.1 85.7#

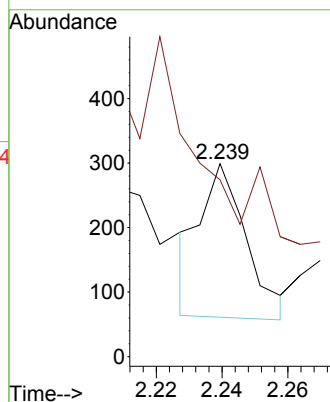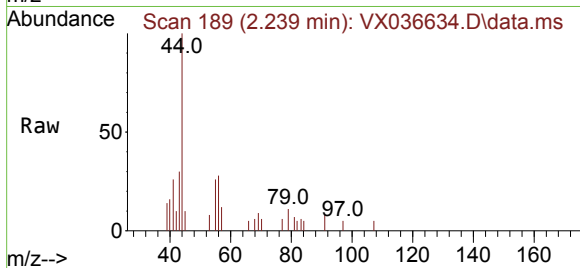

#16

Acetone

Concen: 25.985 ug/l

RT: 2.380 min Scan# 212

Delta R.T. -0.012 min

Lab File: VX036634.D




Acq: 24 Jul 2023 16:57


Tgt Ion: 43 Resp: 25211

Ion Ratio Lower Upper

43 100

58 31.8 21.9 32.9




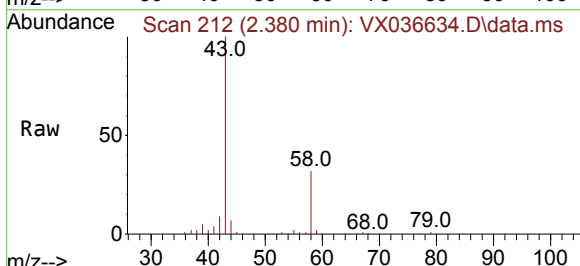




#17
Carbon Disulfide
Concen: 0.957 ug/l
RT: 2.514 min Scan# 21
Delta R.T. 0.000 min
Lab File: VX036634.D
Acq: 24 Jul 2023 16:57




Instrument :
MSVOA_X
ClientSampleId :
33712


Tgt Ion: 76 Resp: 4674
Ion Ratio Lower Upper
76 100
78 9.8 7.0 10.6



#25
2-Butanone
Concen: 3.622 ug/l
RT: 4.574 min Scan# 572
Delta R.T. 0.012 min
Lab File: VX036634.D
Acq: 24 Jul 2023 16:57

Tgt Ion: 43 Resp: 5701
Ion Ratio Lower Upper
43 100
72 23.8 19.4 29.2









#33
 1,2-Dichloroethane-d4
 Concen: 45.993 ug/l
 RT: 5.958 min Scan# 798
 Delta R.T. 0.006 min
 Lab File: VX036634.D
 Acq: 24 Jul 2023 16:57




Instrument :
 MSVOA_X
 ClientSampleId :
 33712


Tgt Ion: 65 Resp: 107534
 Ion Ratio Lower Upper
 65 100
 67 52.0 0.0 100.2



#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.763 min Scan# 931
 Delta R.T. 0.000 min
 Lab File: VX036634.D
 Acq: 24 Jul 2023 16:57

Tgt Ion: 114 Resp: 280805
 Ion Ratio Lower Upper
 114 100
 63 21.3 0.0 45.0
 88 16.9 0.0 36.6









#35
Dibromofluoromethane
Concen: 46.392 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX036634.D
Acq: 24 Jul 2023 16:57




Instrument :
MSVOA_X
ClientSampleId :
33712


Tgt Ion:113 Resp: 89541
Ion Ratio Lower Upper
113 100
111 103.6 82.9 124.3
192 17.9 13.3 19.9

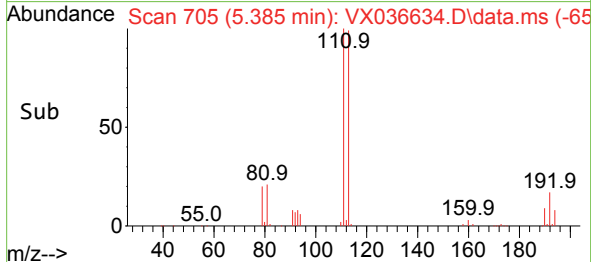

#36
1,1-Dichloropropene
Concen: 4.638 ug/l
RT: 5.556 min Scan# 733
Delta R.T. -0.140 min
Lab File: VX036634.D
Acq: 24 Jul 2023 16:57

Tgt Ion: 75 Resp: 13343
Ion Ratio Lower Upper
75 100
110 8.9 17.0 50.9#
77 0.0 24.7 37.1#


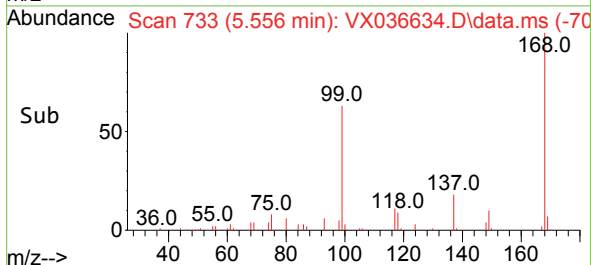
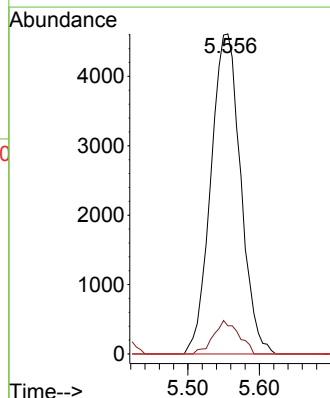
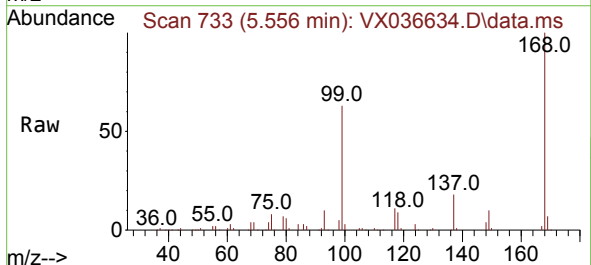




#37
Ethyl Acetate
Concen: 1.749 ug/l
RT: 4.574 min Scan# 51
Delta R.T. -0.140 min
Lab File: VX036634.D
Acq: 24 Jul 2023 16:57




Instrument :
MSVOA_X
ClientSampleId :
33712


Tgt Ion: 43 Resp: 5696
Ion Ratio Lower Upper
43 100
61 0.0 10.6 16.0#
70 0.0 8.3 12.5#



#38
Carbon Tetrachloride
Concen: 5.464 ug/l
RT: 5.550 min Scan# 732
Delta R.T. -0.128 min
Lab File: VX036634.D
Acq: 24 Jul 2023 16:57

Tgt Ion: 117 Resp: 16711
Ion Ratio Lower Upper
117 100
119 5.6 78.2 117.2#
121 0.0 24.4 36.6#

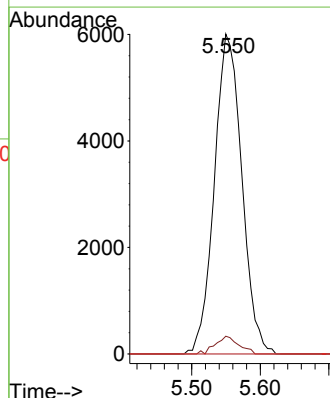



#50

Toluene-d8

Concen: 48.957 ug/l

RT: 8.647 min Scan# 11

Delta R.T. 0.000 min

Lab File: VX036634.D

Acq: 24 Jul 2023 16:57

Instrument :

MSVOA_X

ClientSampleId :





33712

Tgt Ion: 98 Resp: 335089

Ion Ratio Lower Upper

98 100

100 66.1 53.1 79.7

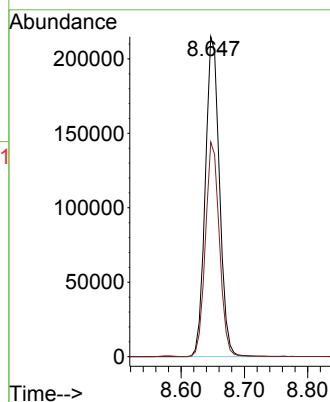

#51

4-Methyl-2-Pentanone

Concen: 1.556 ug/l

RT: 8.574 min Scan# 1228

Delta R.T. 0.000 min

Lab File: VX036634.D




Acq: 24 Jul 2023 16:57


Tgt Ion: 43 Resp: 4825

Ion Ratio Lower Upper

43 100

58 39.5 30.4 45.6



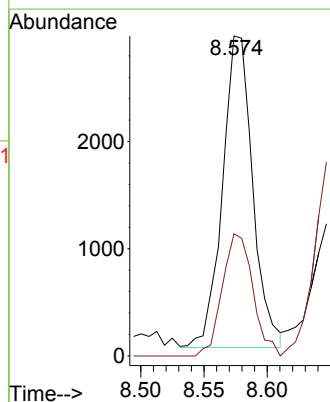





#52
Toluene
Concen: 0.451 ug/l
RT: 8.720 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX036634.D
Acq: 24 Jul 2023 16:57




Instrument :
MSVOA_X
ClientSampleId :
33712


Tgt Ion: 92 Resp: 2366
Ion Ratio Lower Upper
92 100
91 179.8 134.2 201.2



#59
2-Hexanone
Concen: 0.397 ug/l
RT: 9.439 min Scan# 1370
Delta R.T. 0.012 min
Lab File: VX036634.D
Acq: 24 Jul 2023 16:57

Tgt Ion: 43 Resp: 915
Ion Ratio Lower Upper
43 100
58 49.6 26.2 78.5



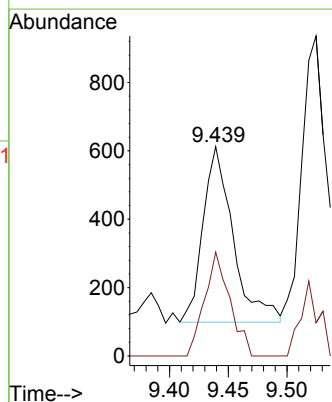





#62
4-Bromofluorobenzene
Concen: 51.269 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX036634.D
Acq: 24 Jul 2023 16:57




Instrument :
MSVOA_X
ClientSampleId :
33712


Tgt Ion: 95 Resp: 132394
Ion Ratio Lower Upper
95 100
174 71.1 0.0 135.6
176 69.8 0.0 131.0



#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX036634.D
Acq: 24 Jul 2023 16:57

Tgt Ion: 117 Resp: 261850
Ion Ratio Lower Upper
117 100
82 57.1 46.2 69.4
119 32.1 25.5 38.3


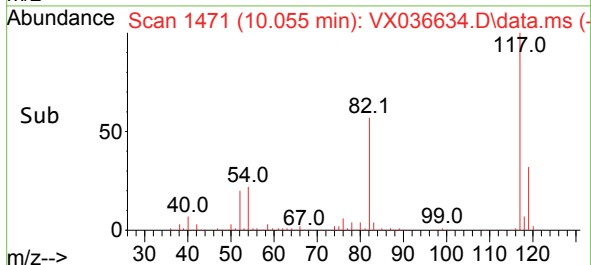






#67
Ethyl Benzene
Concen: 1.107 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX036634.D
Acq: 24 Jul 2023 16:57




Instrument :
MSVOA_X
ClientSampleId :
33712


Tgt Ion: 91 Resp: 11675
Ion Ratio Lower Upper
91 100
106 31.0 24.9 37.3



#68
m/p-Xylenes
Concen: 6.814 ug/l
RT: 10.299 min Scan# 1511
Delta R.T. 0.000 min
Lab File: VX036634.D
Acq: 24 Jul 2023 16:57

Tgt Ion: 106 Resp: 26808
Ion Ratio Lower Upper
106 100
91 208.1 165.5 248.3





#69

o-Xylene

Concen: 6.659 ug/l

RT: 10.640 min Scan# 1567

Delta R.T. 0.000 min

Lab File: VX036634.D

Acq: 24 Jul 2023 16:57

Instrument :

MSVOA_X

ClientSampleId :





33712

Tgt Ion:106 Resp: 26149

Ion Ratio Lower Upper

106 100

91 215.6 108.9 326.8



#70

Styrene

Concen: 0.233 ug/l

RT: 10.646 min Scan# 1568

Delta R.T. -0.006 min

Lab File: VX036634.D

Acq: 24 Jul 2023 16:57




Tgt Ion:104 Resp: 1508


Ion Ratio Lower Upper

104 100

78 281.5 43.6 65.4#

103 234.9 43.6 65.4#









#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX036634.D
Acq: 24 Jul 2023 16:57




Instrument :
MSVOA_X
ClientSampleId :
33712


Tgt Ion:152 Resp: 121921
Ion Ratio Lower Upper
152 100
115 63.3 43.3 129.9
150 157.3 0.0 345.0

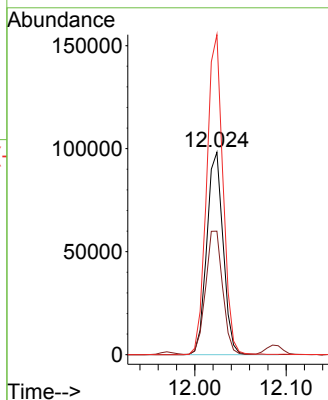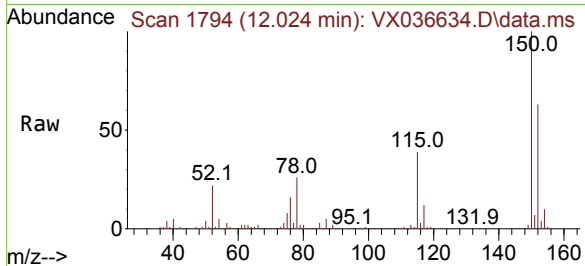

#73
Isopropylbenzene
Concen: 0.949 ug/l
RT: 10.963 min Scan# 1620
Delta R.T. 0.000 min
Lab File: VX036634.D
Acq: 24 Jul 2023 16:57

Tgt Ion:105 Resp: 9578
Ion Ratio Lower Upper
105 100
120 25.6 12.9 38.6



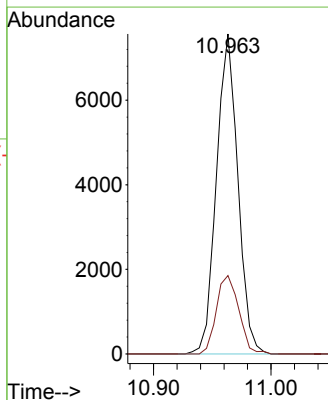
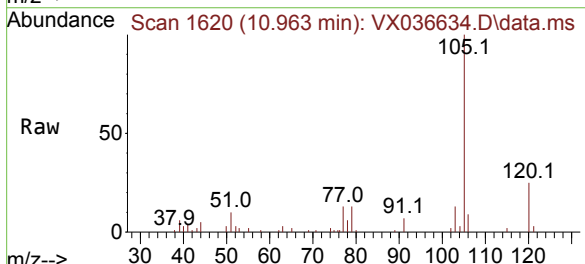




#74
N-amy1 acetate
Concen: 0.352 ug/l
RT: 10.854 min Scan# 1657
Delta R.T. 0.012 min
Lab File: VX036634.D
Acq: 24 Jul 2023 16:57




Instrument :
MSVOA_X
ClientSampleId :
33712


Tgt Ion: 43	Resp: 1657
Ion Ratio	Lower Upper
43	100
70	90.7 32.9 49.3#
55	77.5 19.3 28.9#
61	0.0 18.8 28.2#



#76
1,2,3-Trichloropropane
Concen: 23.748 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.159 min
Lab File: VX036634.D
Acq: 24 Jul 2023 16:57

Tgt Ion: 75	Resp: 68103
Ion Ratio	Lower Upper
75	100
77	1.1 19.1 57.5#







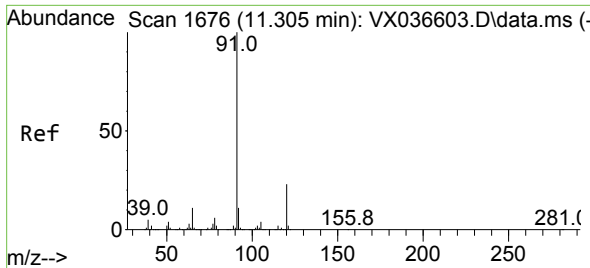

#78
n-propylbenzene
Concen: 1.854 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. 0.000 min
Lab File: VX036634.D
Acq: 24 Jul 2023 16:57




Instrument :
MSVOA_X
ClientSampleId :
33712


Tgt Ion: 91 Resp: 21629
Ion Ratio Lower Upper
91 100
120 21.9 11.5 34.4

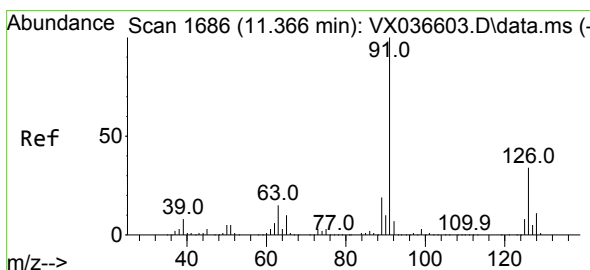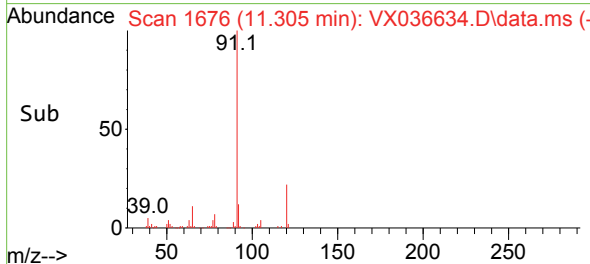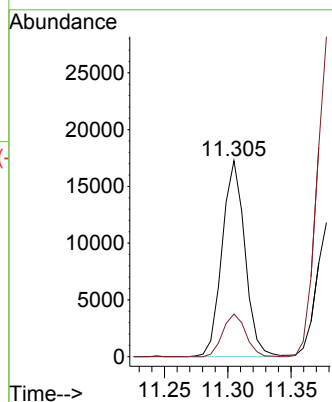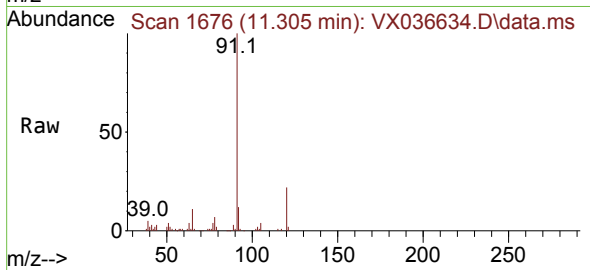

#79
2-Chlorotoluene
Concen: 2.726 ug/l
RT: 11.378 min Scan# 1688
Delta R.T. 0.012 min
Lab File: VX036634.D
Acq: 24 Jul 2023 16:57

Tgt Ion: 91 Resp: 19279
Ion Ratio Lower Upper
91 100
126 0.0 16.3 48.8#

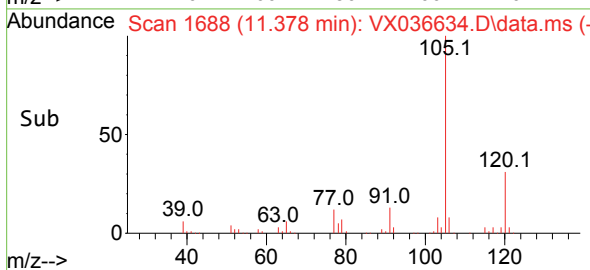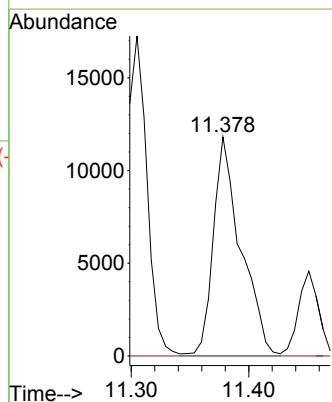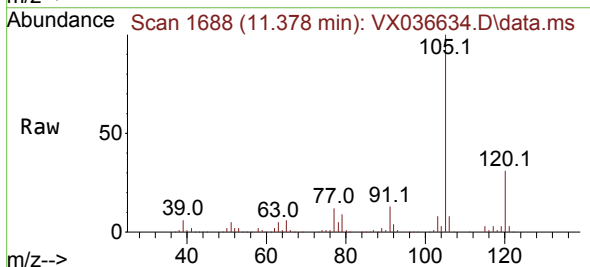



#80

1,3,5-Trimethylbenzene

Concen: 5.839 ug/l

RT: 11.451 min Scan# 11

Delta R.T. 0.000 min

Lab File: VX036634.D

Acq: 24 Jul 2023 16:57

Instrument :

MSVOA_X

ClientSampleId :





33712

Tgt Ion:105 Resp: 49287

Ion Ratio Lower Upper

105 100

120 48.5 24.1 72.3

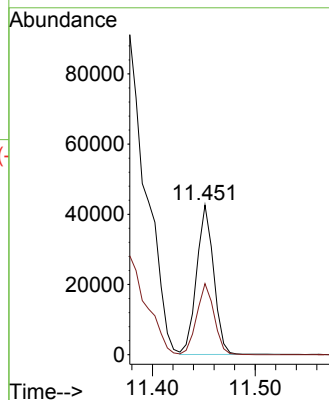

#81

trans-1,4-Dichloro-2-butene

Concen: 53.827 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.061 min

Lab File: VX036634.D

Acq: 24 Jul 2023 16:57




Tgt Ion: 75 Resp: 68103


Ion Ratio Lower Upper

75 100

53 0.0 90.5 135.7#

89 0.0 36.9 55.3#

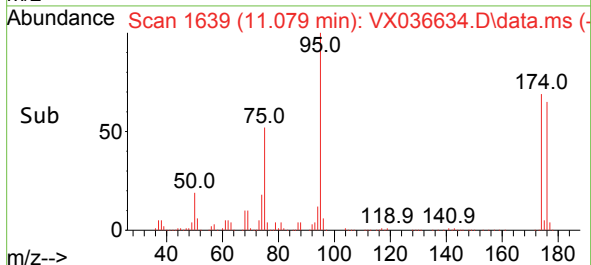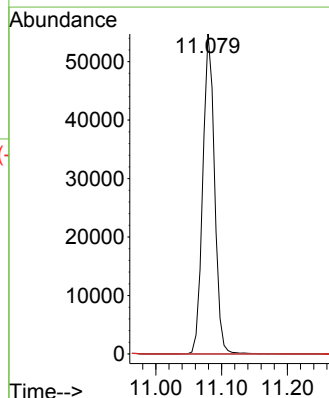



#82

4-Chlorotoluene

Concen: 0.689 ug/l

RT: 11.451 min Scan# 11

Delta R.T. 0.000 min

Lab File: VX036634.D

Acq: 24 Jul 2023 16:57

Instrument :

MSVOA_X

ClientSampleId :





33712

Tgt Ion: 91 Resp: 5550

Ion Ratio Lower Upper

91 100

126 0.0 14.2 42.6#

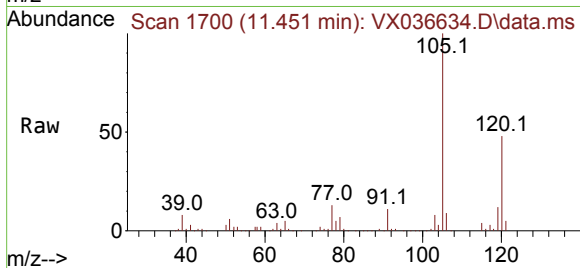

#83

tert-Butylbenzene

Concen: 2.844 ug/l

RT: 11.750 min Scan# 1749

Delta R.T. 0.037 min

Lab File: VX036634.D

Acq: 24 Jul 2023 16:57




Tgt Ion: 119 Resp: 23582


Ion Ratio Lower Upper

119 100

91 95.6 31.2 93.6#

134 0.0 11.7 35.0#




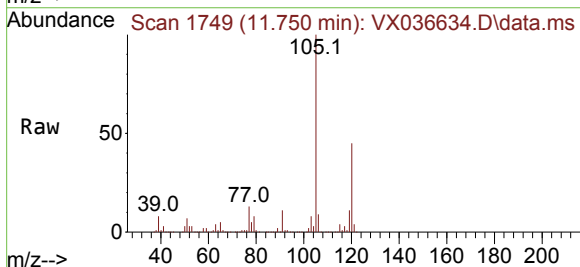




#84
1,2,4-Trimethylbenzene
Concen: 23.994 ug/l
RT: 11.750 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX036634.D
Acq: 24 Jul 2023 16:57




Instrument :
MSVOA_X
ClientSampleId :
33712


Tgt Ion:105 Resp: 202553
Ion Ratio Lower Upper
105 100
120 45.0 21.2 63.6

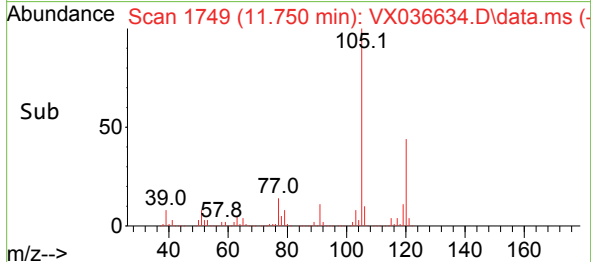

#85
sec-Butylbenzene
Concen: 1.254 ug/l
RT: 11.890 min Scan# 1772
Delta R.T. 0.000 min
Lab File: VX036634.D
Acq: 24 Jul 2023 16:57

Tgt Ion:105 Resp: 12970
Ion Ratio Lower Upper
105 100
134 24.1 9.8 29.4









#86
p-Isopropyltoluene
Concen: 0.998 ug/l
RT: 12.006 min Scan# 1791
Delta R.T. 0.000 min
Lab File: VX036634.D
Acq: 24 Jul 2023 16:57




Instrument :
MSVOA_X
ClientSampleId :
33712


Tgt Ion:119 Resp: 8491
Ion Ratio Lower Upper
119 100
134 27.3 12.8 38.3
91 30.6 13.1 39.3

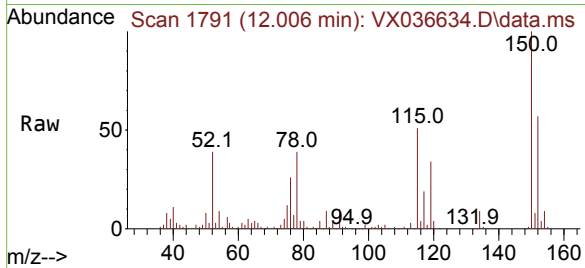

#89
n-Butylbenzene
Concen: 3.000 ug/l
RT: 12.329 min Scan# 1844
Delta R.T. 0.000 min
Lab File: VX036634.D
Acq: 24 Jul 2023 16:57

Tgt Ion: 91 Resp: 22854
Ion Ratio Lower Upper
91 100
92 32.3 27.4 82.0
134 106.1 12.6 37.8#




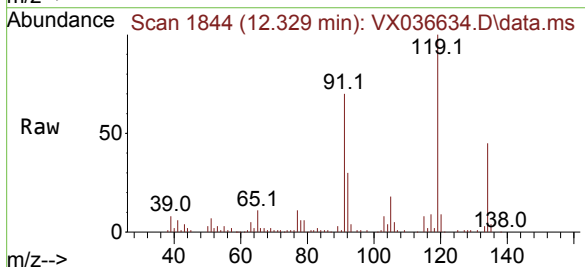




#90
Hexachloroethane
Concen: 2.743 ug/l
RT: 12.530 min Scan# 117
Delta R.T. -0.006 min
Lab File: VX036634.D
Acq: 24 Jul 2023 16:57




Instrument :
MSVOA_X
ClientSampleId :
33712


Tgt Ion:117 Resp: 4732
Ion Ratio Lower Upper
117 100
201 0.0 32.9 98.6#

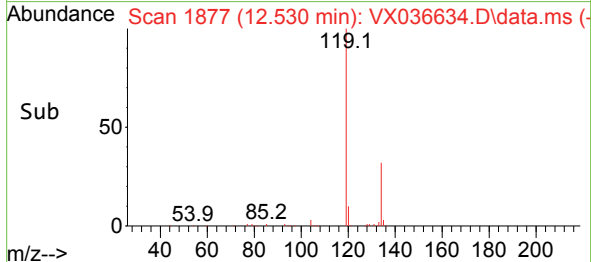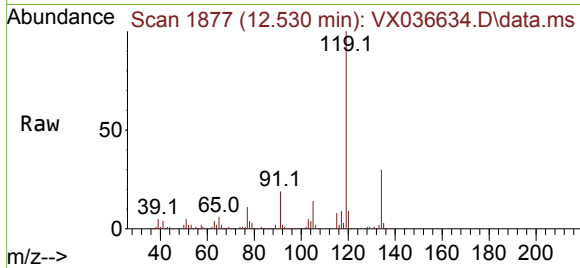

#92
1,2-Dibromo-3-Chloropropane
Concen: 0.494 ug/l
RT: 12.920 min Scan# 1941
Delta R.T. -0.018 min
Lab File: VX036634.D
Acq: 24 Jul 2023 16:57

Tgt Ion: 75 Resp: 391
Ion Ratio Lower Upper
75 100
155 0.0 36.1 108.5#
157 0.0 44.9 134.7#

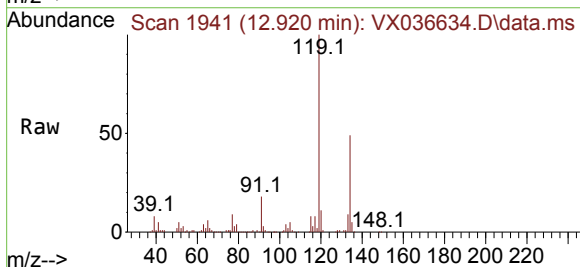



#95
Naphthalene
Concen: 18.566 ug/l
RT: 13.774 min Scan# 2081
Delta R.T. 0.000 min
Lab File: VX036634.D
Acq: 24 Jul 2023 16:57

Instrument :
MSVOA_X
ClientSampleId :
33712

Tgt Ion:	128	Resp:	163700
Ion	Ratio	Lower	Upper
128	100		
127	13.0	10.3	15.5
129	12.2	8.8	13.2

