

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072424\
 Data File : VX042479.D
 Acq On : 23 Jul 2024 18:04
 Operator : JC/MD
 Sample : P3327-10
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jul 24 03:50:54 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jul 24 03:44:32 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	210675	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	188797	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	90393	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	56438	46.025	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	92.040%
7) Chloroethane-d5	1.648	69	35358	45.795	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	91.600%
11) 1,1-Dichloroethene-d2	2.294	65	24835	46.275	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	92.560%
21) 2-Butanone-d5	4.464	46	96265	108.935	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	108.930%
24) Chloroform-d	5.056	84	123343	50.026	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	100.060%
26) 1,2-Dichloroethane-d4	5.952	65	79351	54.526	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	109.060%
32) Benzene-d6	5.970	84	255460	52.349	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	104.700%
36) 1,2-Dichloropropane-d6	7.305	67	79692	54.264	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	108.520%
41) Toluene-d8	8.647	98	221402	48.685	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	97.380%
43) trans-1,3-Dichloroprop...	8.951	79	30578	48.176	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	96.360%
47) 2-Hexanone-d5	9.384	63	72420	108.638	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	108.640%
56) 1,1,2,2-Tetrachloroeth...	11.189	84	125707	57.899	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	115.800%
66) 1,2-Dichlorobenzene-d4	12.323	152	97493	55.529	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	111.060%
Target Compounds						
					Qvalue	
13) Acetone	2.392	43	3403	5.645	ug/L	96
37) 1,2-Dichloropropane	7.305	63	8595	6.345	ug/L #	84
61) 1,2,3-Trichloropropane	12.018	75	9123	5.684	ug/L #	61


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072424\
Data File : VX042479.D
Acq On : 23 Jul 2024 18:04
Operator : JC/MD
Sample : P3327-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Jul 24 03:50:54 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jul 24 03:44:32 2024
Response via : Initial Calibration

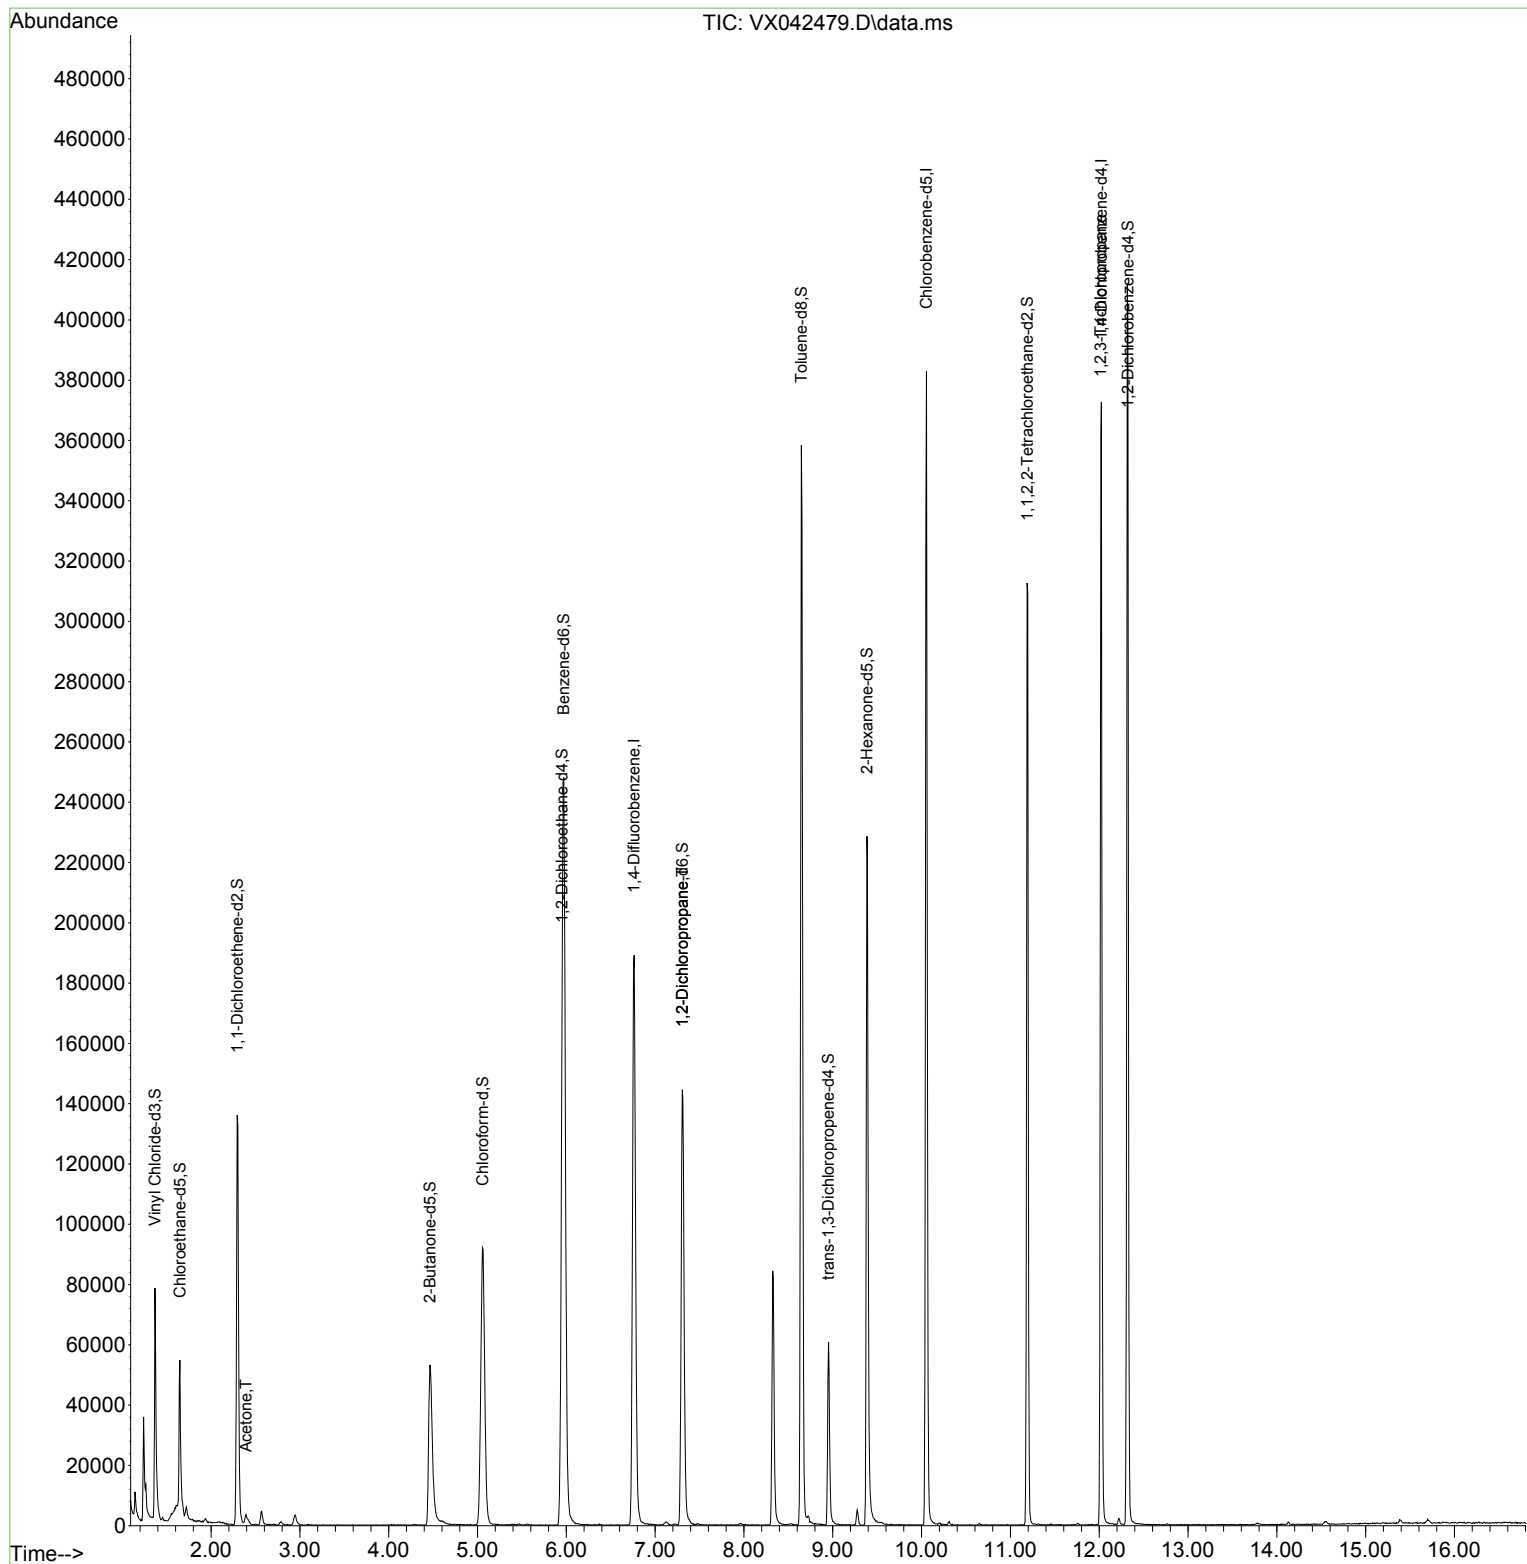

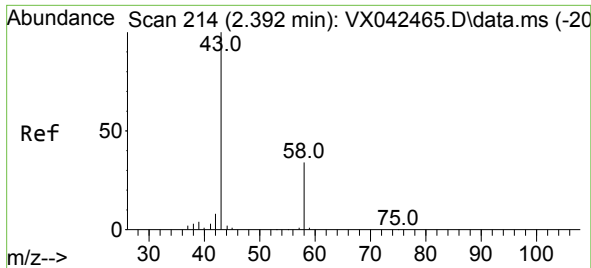

#13

Acetone

Concen: 5.645 ug/L

RT: 2.392 min Scan# 214

Delta R.T. -0.000 min

Lab File: VX042479.D

Acq: 23 Jul 2024 18:04

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 43 Resp: 3403

Ion Ratio Lower Upper

43 100

58 33.6 0.0 62.6

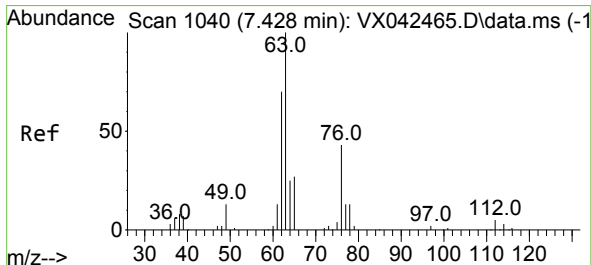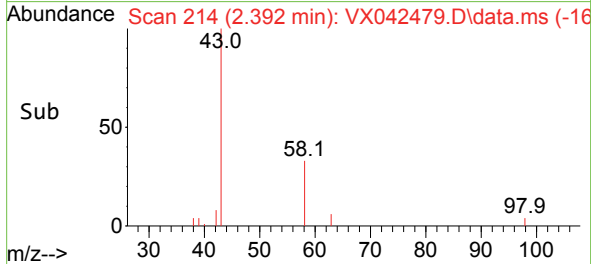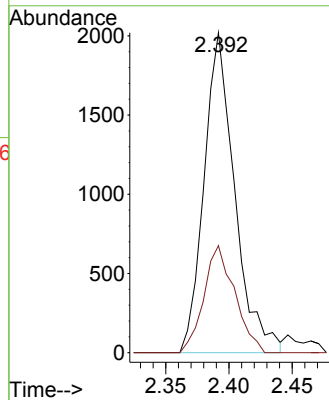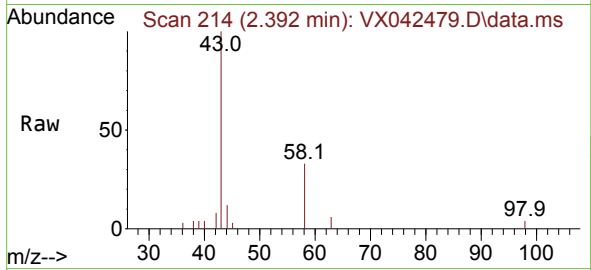

#37

1,2-Dichloropropane

Concen: 6.345 ug/L

RT: 7.305 min Scan# 1020

Delta R.T. -0.122 min

Lab File: VX042479.D




Acq: 23 Jul 2024 18:04


Tgt Ion: 63 Resp: 8595

Ion Ratio Lower Upper

63 100


112 0.0 4.3 6.5#

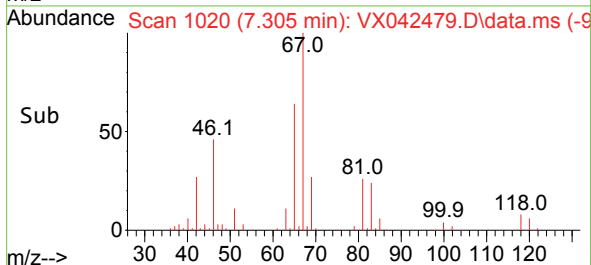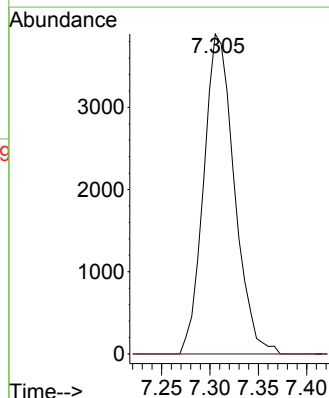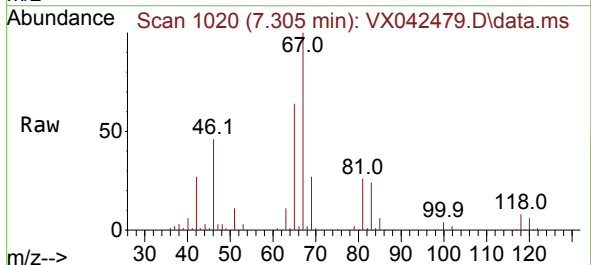

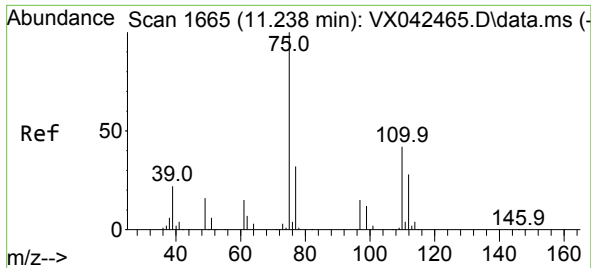

#61
1,2,3-Trichloropropane
Concen: 5.684 ug/L
RT: 12.018 min Scan# 11
Delta R.T. 0.780 min
Lab File: VX042479.D
Acq: 23 Jul 2024 18:04

Instrument :
MSVOA_X
ClientSampleId :

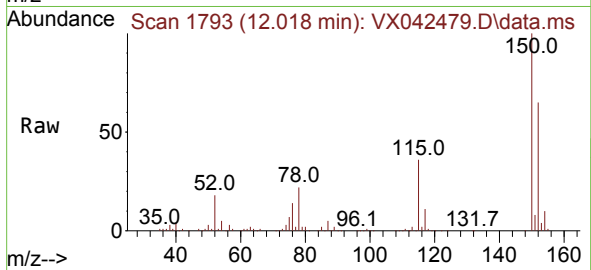

Tgt Ion:	75	Resp:	9123
Ion	Ratio	Lower	Upper
75	100		
77	29.8	25.8	38.8
110	2.8	35.4	53.0#

