

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072424\
 Data File : VX042480.D
 Acq On : 23 Jul 2024 18:27
 Operator : JC/MD
 Sample : P3327-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jul 24 03:51:11 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jul 24 03:44:32 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	187269	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	167669	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	77570	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	62114	56.984	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 113.960%			
7) Chloroethane-d5	1.648	69	32619	47.528	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery = 95.060%			
11) 1,1-Dichloroethene-d2	2.294	65	23255	48.747	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 97.500%			
21) 2-Butanone-d5	4.465	46	80969	103.078	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery = 103.080%			
24) Chloroform-d	5.056	84	108213	49.375	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 98.740%			
26) 1,2-Dichloroethane-d4	5.952	65	69546	53.761	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 107.520%			
32) Benzene-d6	5.970	84	222311	51.296	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 102.600%			
36) 1,2-Dichloropropane-d6	7.306	67	68208	52.297	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 104.600%			
41) Toluene-d8	8.647	98	199514	49.401	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 98.800%			
43) trans-1,3-Dichloroprop...	8.952	79	27010	47.917	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 95.840%			
47) 2-Hexanone-d5	9.384	63	60589	102.343	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery = 102.340%			
56) 1,1,2,2-Tetrachloroeth...	11.189	84	96253	49.919	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 99.840%			
66) 1,2-Dichlorobenzene-d4	12.317	152	81166	53.872	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 107.740%			
Target Compounds					Qvalue	
13) Acetone	2.398	43	2423	4.522	ug/L	98
61) 1,2,3-Trichloropropane	12.018	75	7055	5.122	ug/L #	63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072424\
Data File : VX042480.D
Acq On : 23 Jul 2024 18:27
Operator : JC/MD
Sample : P3327-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Jul 24 03:51:11 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jul 24 03:44:32 2024
Response via : Initial Calibration

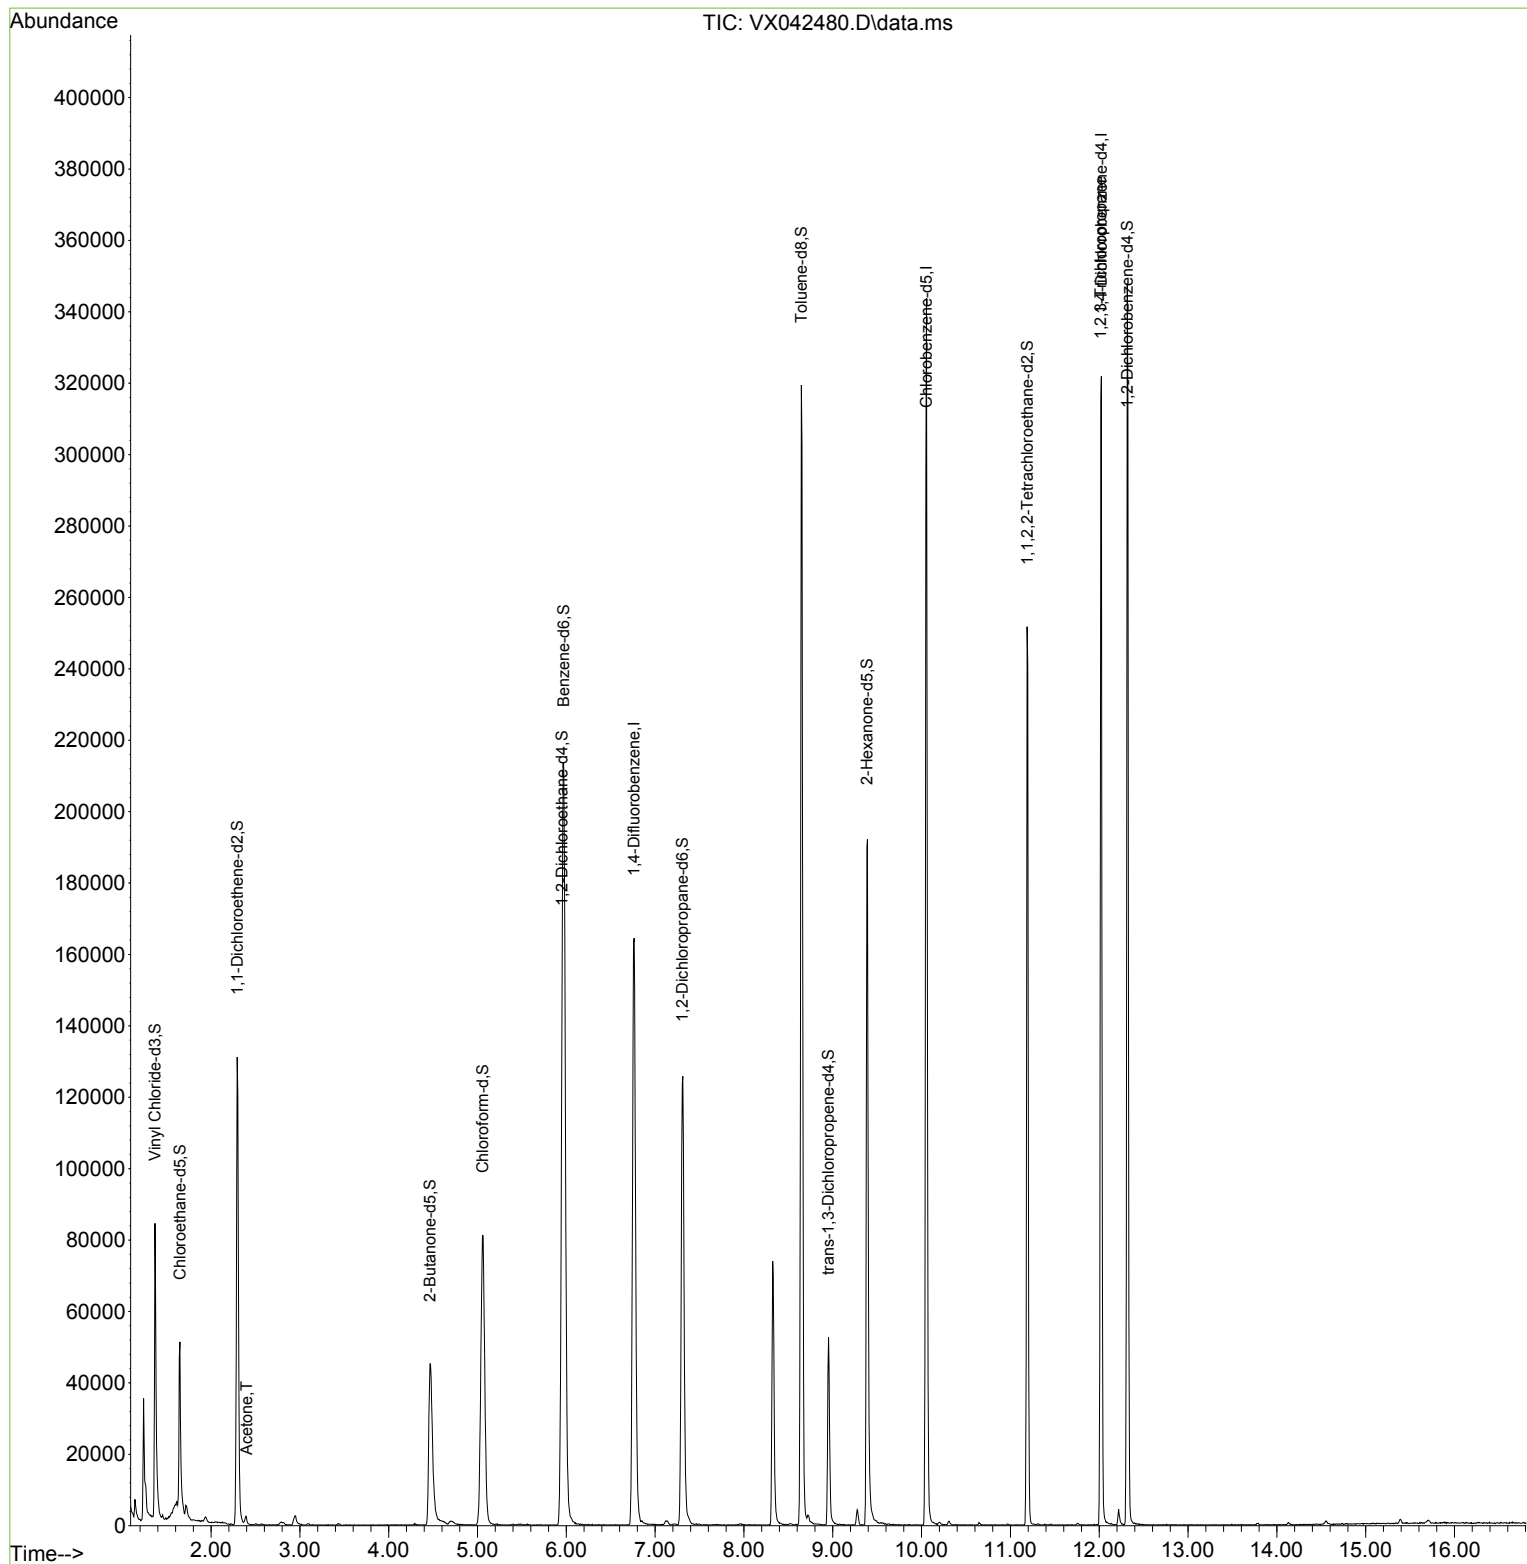

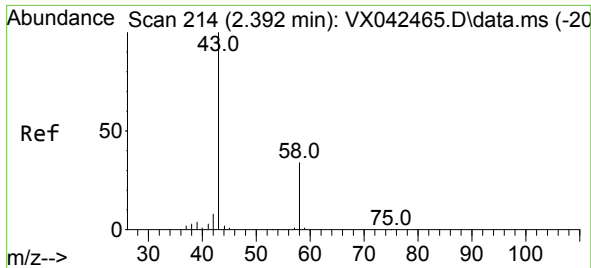

#13

Acetone

Concen: 4.522 ug/L

RT: 2.398 min Scan# 214

Delta R.T. 0.006 min

Lab File: VX042480.D

Acq: 23 Jul 2024 18:27

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 43 Resp: 2423

Ion Ratio Lower Upper

43 100

58 30.3 0.0 62.6

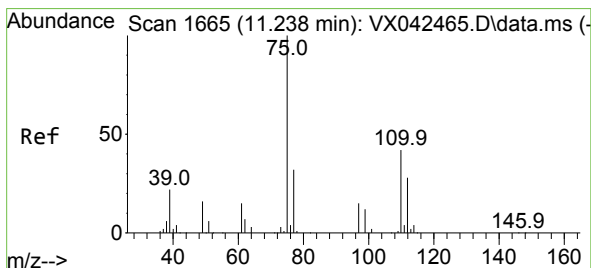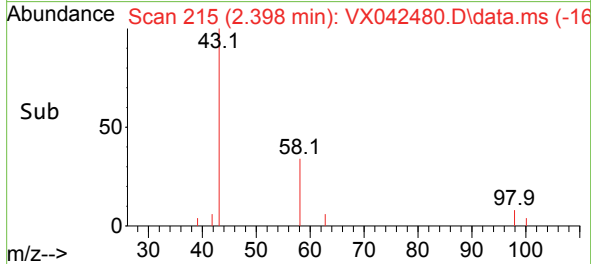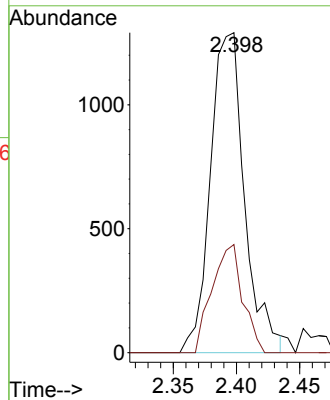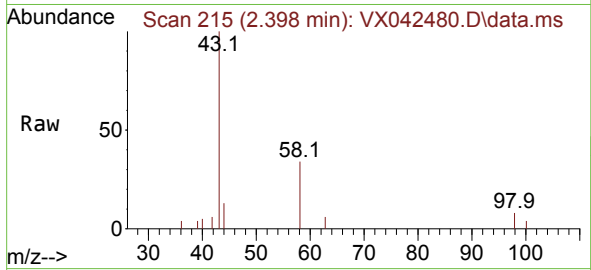

#61

1,2,3-Trichloropropane

Concen: 5.122 ug/L

RT: 12.018 min Scan# 1793

Delta R.T. 0.780 min

Lab File: VX042480.D

Acq: 23 Jul 2024 18:27

Tgt Ion: 75 Resp: 7055

Ion Ratio Lower Upper

75 100

77 32.2 25.8 38.8

110 2.6 35.4 53.0

