

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX072424\  
 Data File : VX042480.D  
 Acq On : 23 Jul 2024 18:27  
 Operator : JC/MD  
 Sample : P3327-11  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 17 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 E1ZW6

Quant Time: Jul 24 03:51:11 2024  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\SFAMXML070324WMA.M  
 Quant Title : VOC Analysis  
 QLast Update : Wed Jul 24 03:44:32 2024  
 Response via : Initial Calibration


| Compound                      | R.T.           | QIon | Response            | Conc    | Units  | Dev(Min) |
|-------------------------------|----------------|------|---------------------|---------|--------|----------|
| -----                         |                |      |                     |         |        |          |
| Internal Standards            |                |      |                     |         |        |          |
| 1) 1,4-Difluorobenzene        | 6.763          | 114  | 187269              | 50.000  | ug/L   | 0.00     |
| 28) Chlorobenzene-d5          | 10.055         | 117  | 167669              | 50.000  | ug/L   | 0.00     |
| 58) 1,4-Dichlorobenzene-d4    | 12.024         | 152  | 77570               | 50.000  | ug/L   | 0.00     |
|                               |                |      |                     |         |        |          |
| System Monitoring Compounds   |                |      |                     |         |        |          |
| 4) Vinyl Chloride-d3          | 1.368          | 65   | 62114               | 56.984  | ug/L   | 0.00     |
| Spiked Amount 50.000          | Range 60 - 135 |      | Recovery = 113.960% |         |        |          |
| 7) Chloroethane-d5            | 1.648          | 69   | 32619               | 47.528  | ug/L   | 0.00     |
| Spiked Amount 50.000          | Range 70 - 130 |      | Recovery = 95.060%  |         |        |          |
| 11) 1,1-Dichloroethene-d2     | 2.294          | 65   | 23255               | 48.747  | ug/L   | 0.00     |
| Spiked Amount 50.000          | Range 60 - 125 |      | Recovery = 97.500%  |         |        |          |
| 21) 2-Butanone-d5             | 4.465          | 46   | 80969               | 103.078 | ug/L   | 0.00     |
| Spiked Amount 100.000         | Range 40 - 130 |      | Recovery = 103.080% |         |        |          |
| 24) Chloroform-d              | 5.056          | 84   | 108213              | 49.375  | ug/L   | 0.00     |
| Spiked Amount 50.000          | Range 70 - 125 |      | Recovery = 98.740%  |         |        |          |
| 26) 1,2-Dichloroethane-d4     | 5.952          | 65   | 69546               | 53.761  | ug/L   | 0.00     |
| Spiked Amount 50.000          | Range 70 - 125 |      | Recovery = 107.520% |         |        |          |
| 32) Benzene-d6                | 5.970          | 84   | 222311              | 51.296  | ug/L   | 0.00     |
| Spiked Amount 50.000          | Range 70 - 125 |      | Recovery = 102.600% |         |        |          |
| 36) 1,2-Dichloropropane-d6    | 7.306          | 67   | 68208               | 52.297  | ug/L   | 0.00     |
| Spiked Amount 50.000          | Range 70 - 120 |      | Recovery = 104.600% |         |        |          |
| 41) Toluene-d8                | 8.647          | 98   | 199514              | 49.401  | ug/L   | 0.00     |
| Spiked Amount 50.000          | Range 80 - 120 |      | Recovery = 98.800%  |         |        |          |
| 43) trans-1,3-Dichloroprop... | 8.952          | 79   | 27010               | 47.917  | ug/L   | 0.00     |
| Spiked Amount 50.000          | Range 60 - 125 |      | Recovery = 95.840%  |         |        |          |
| 47) 2-Hexanone-d5             | 9.384          | 63   | 60589               | 102.343 | ug/L   | 0.00     |
| Spiked Amount 100.000         | Range 45 - 130 |      | Recovery = 102.340% |         |        |          |
| 56) 1,1,2,2-Tetrachloroeth... | 11.189         | 84   | 96253               | 49.919  | ug/L   | 0.00     |
| Spiked Amount 50.000          | Range 65 - 120 |      | Recovery = 99.840%  |         |        |          |
| 66) 1,2-Dichlorobenzene-d4    | 12.317         | 152  | 81166               | 53.872  | ug/L   | 0.00     |
| Spiked Amount 50.000          | Range 80 - 120 |      | Recovery = 107.740% |         |        |          |
|                               |                |      |                     |         |        |          |
| Target Compounds              |                |      |                     |         | Qvalue |          |
| 13) Acetone                   | 2.398          | 43   | 2423                | 4.522   | ug/L   | 98       |
| -----                         |                |      |                     |         |        |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX072424\  
Data File : VX042480.D  
Acq On : 23 Jul 2024 18:27  
Operator : JC/MD  
Sample : P3327-11  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 17 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
E1ZW6

Quant Time: Jul 24 03:51:11 2024  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\SFAMXML070324WMA.M  
Quant Title : VOC Analysis  
QLast Update : Wed Jul 24 03:44:32 2024  
Response via : Initial Calibration

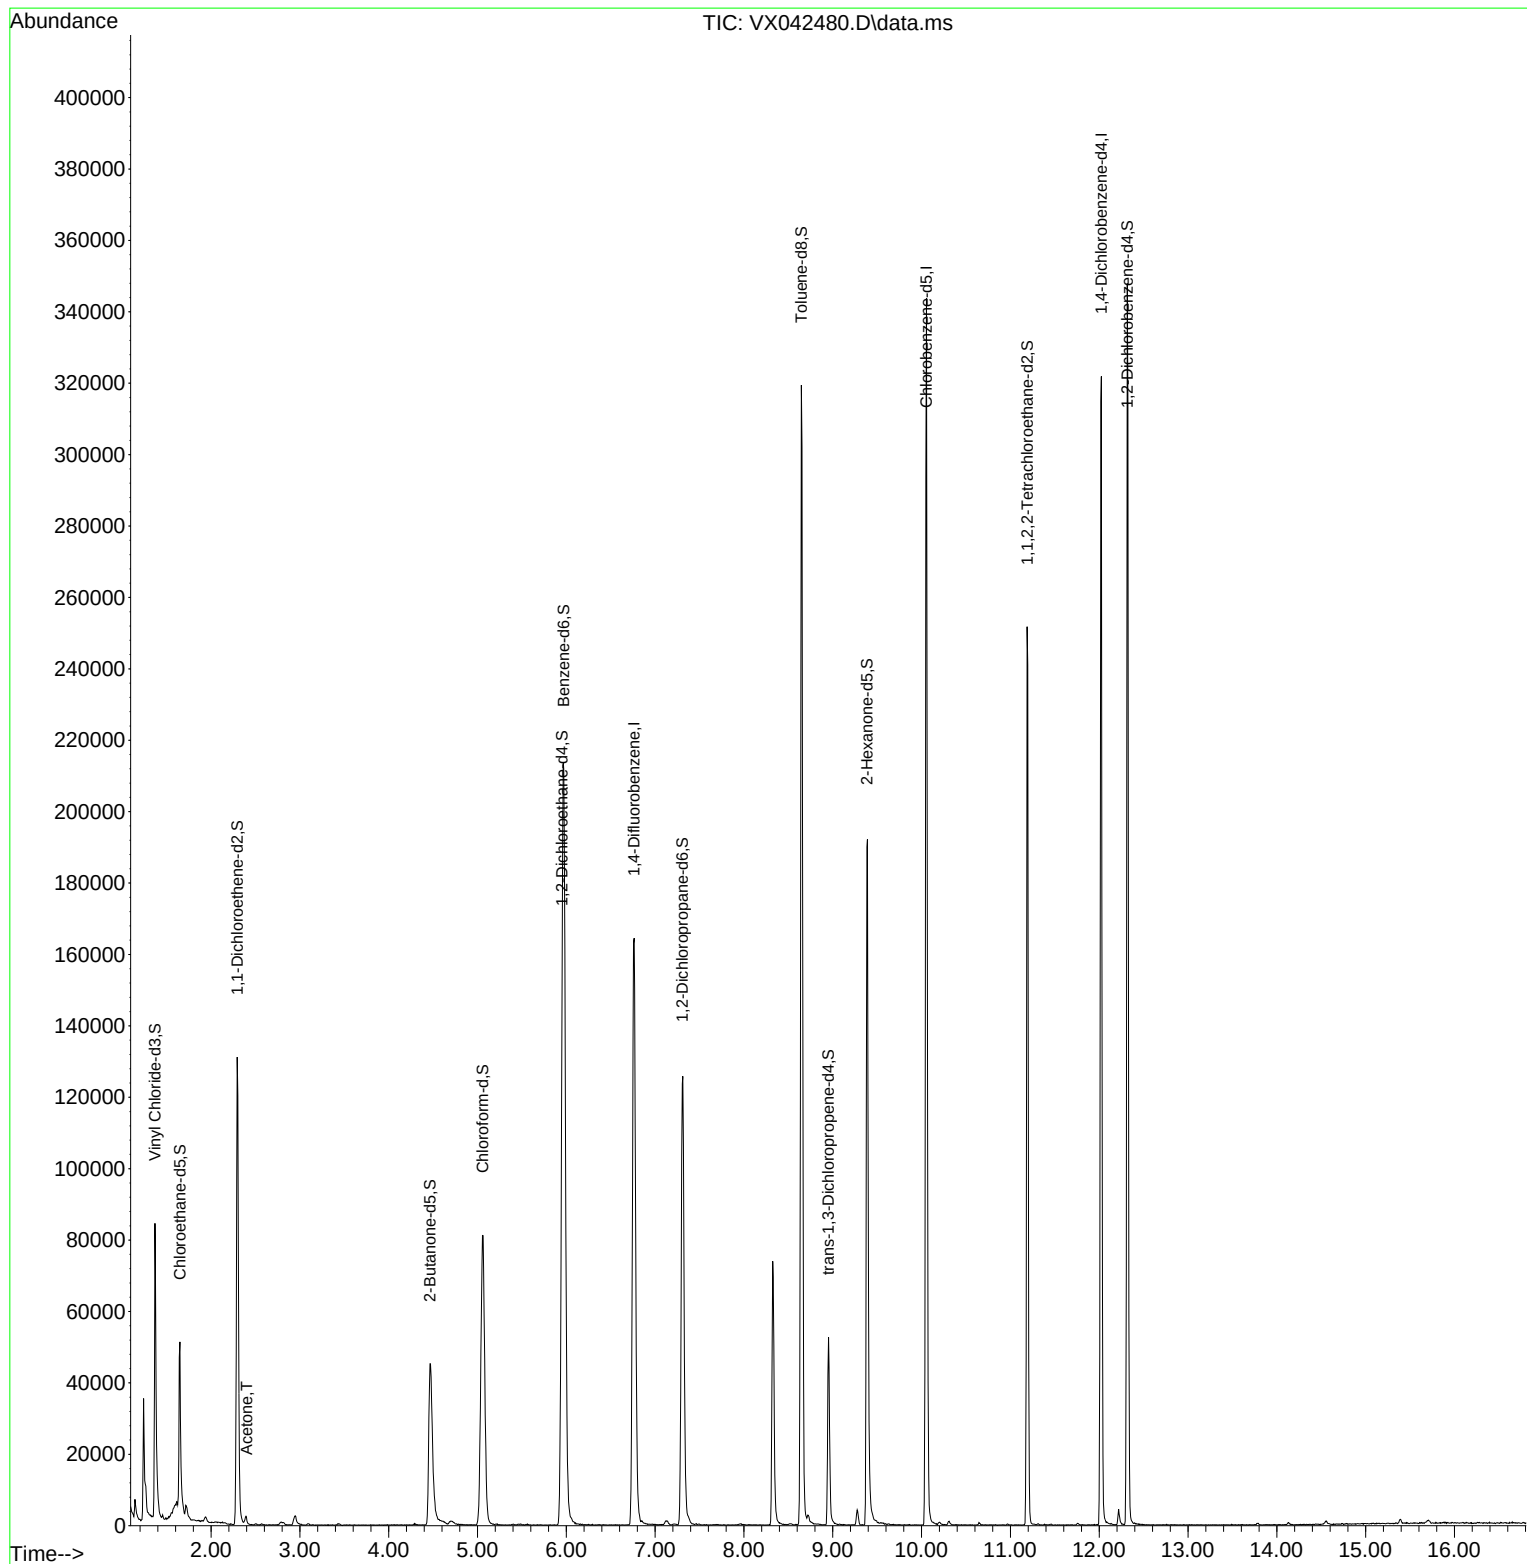

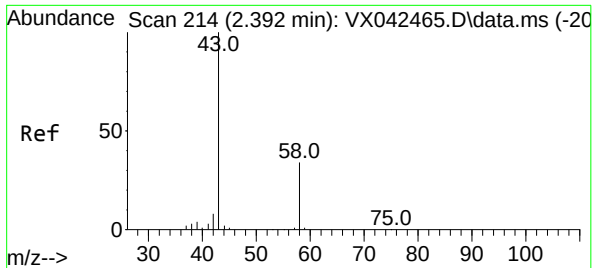

#13  
 Acetone  
 Concen: 4.522 ug/L  
 RT: 2.398 min Scan# 21  
 Delta R.T. 0.006 min  
 Lab File: VX042480.D  
 Acq: 23 Jul 2024 18:27

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 E1ZW6

Tgt Ion: 43 Resp: 2423  
 Ion Ratio Lower Upper  
 43 100  
 58 30.3 0.0 62.6

