

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072424\
 Data File : VX042482.D
 Acq On : 23 Jul 2024 19:13
 Operator : JC/MD
 Sample : P3327-13
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E1ZW8

Quant Time: Jul 24 03:51:41 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jul 24 03:44:32 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	188985	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	166937	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	71628	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	46838	42.580	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	85.160%		
7) Chloroethane-d5	1.648	69	32400	46.780	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	93.560%		
11) 1,1-Dichloroethene-d2	2.294	65	23380	48.564	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	97.120%		
21) 2-Butanone-d5	4.465	46	87605	110.513	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	110.510%		
24) Chloroform-d	5.056	84	114953	51.974	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	103.940%		
26) 1,2-Dichloroethane-d4	5.958	65	73573	56.358	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	112.720%		
32) Benzene-d6	5.971	84	233675	54.155	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	108.300%		
36) 1,2-Dichloropropane-d6	7.306	67	72964	56.189	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	112.380%		
41) Toluene-d8	8.647	98	204710	50.910	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	101.820%		
43) trans-1,3-Dichloroprop...	8.952	79	28169	50.192	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	100.380%		
47) 2-Hexanone-d5	9.385	63	64535	109.487	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	109.490%		
56) 1,1,2,2-Tetrachloroeth...	11.189	84	102690	53.491	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	106.980%		
66) 1,2-Dichlorobenzene-d4	12.323	152	78978	56.768	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	113.540%		
Target Compounds					Qvalue	
13) Acetone	2.392	43	3183	5.886	ug/L	98
34) Trichloroethene	7.129	95	8624	7.053	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072424\
Data File : VX042482.D
Acq On : 23 Jul 2024 19:13
Operator : JC/MD
Sample : P3327-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E1ZW8

Quant Time: Jul 24 03:51:41 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jul 24 03:44:32 2024
Response via : Initial Calibration

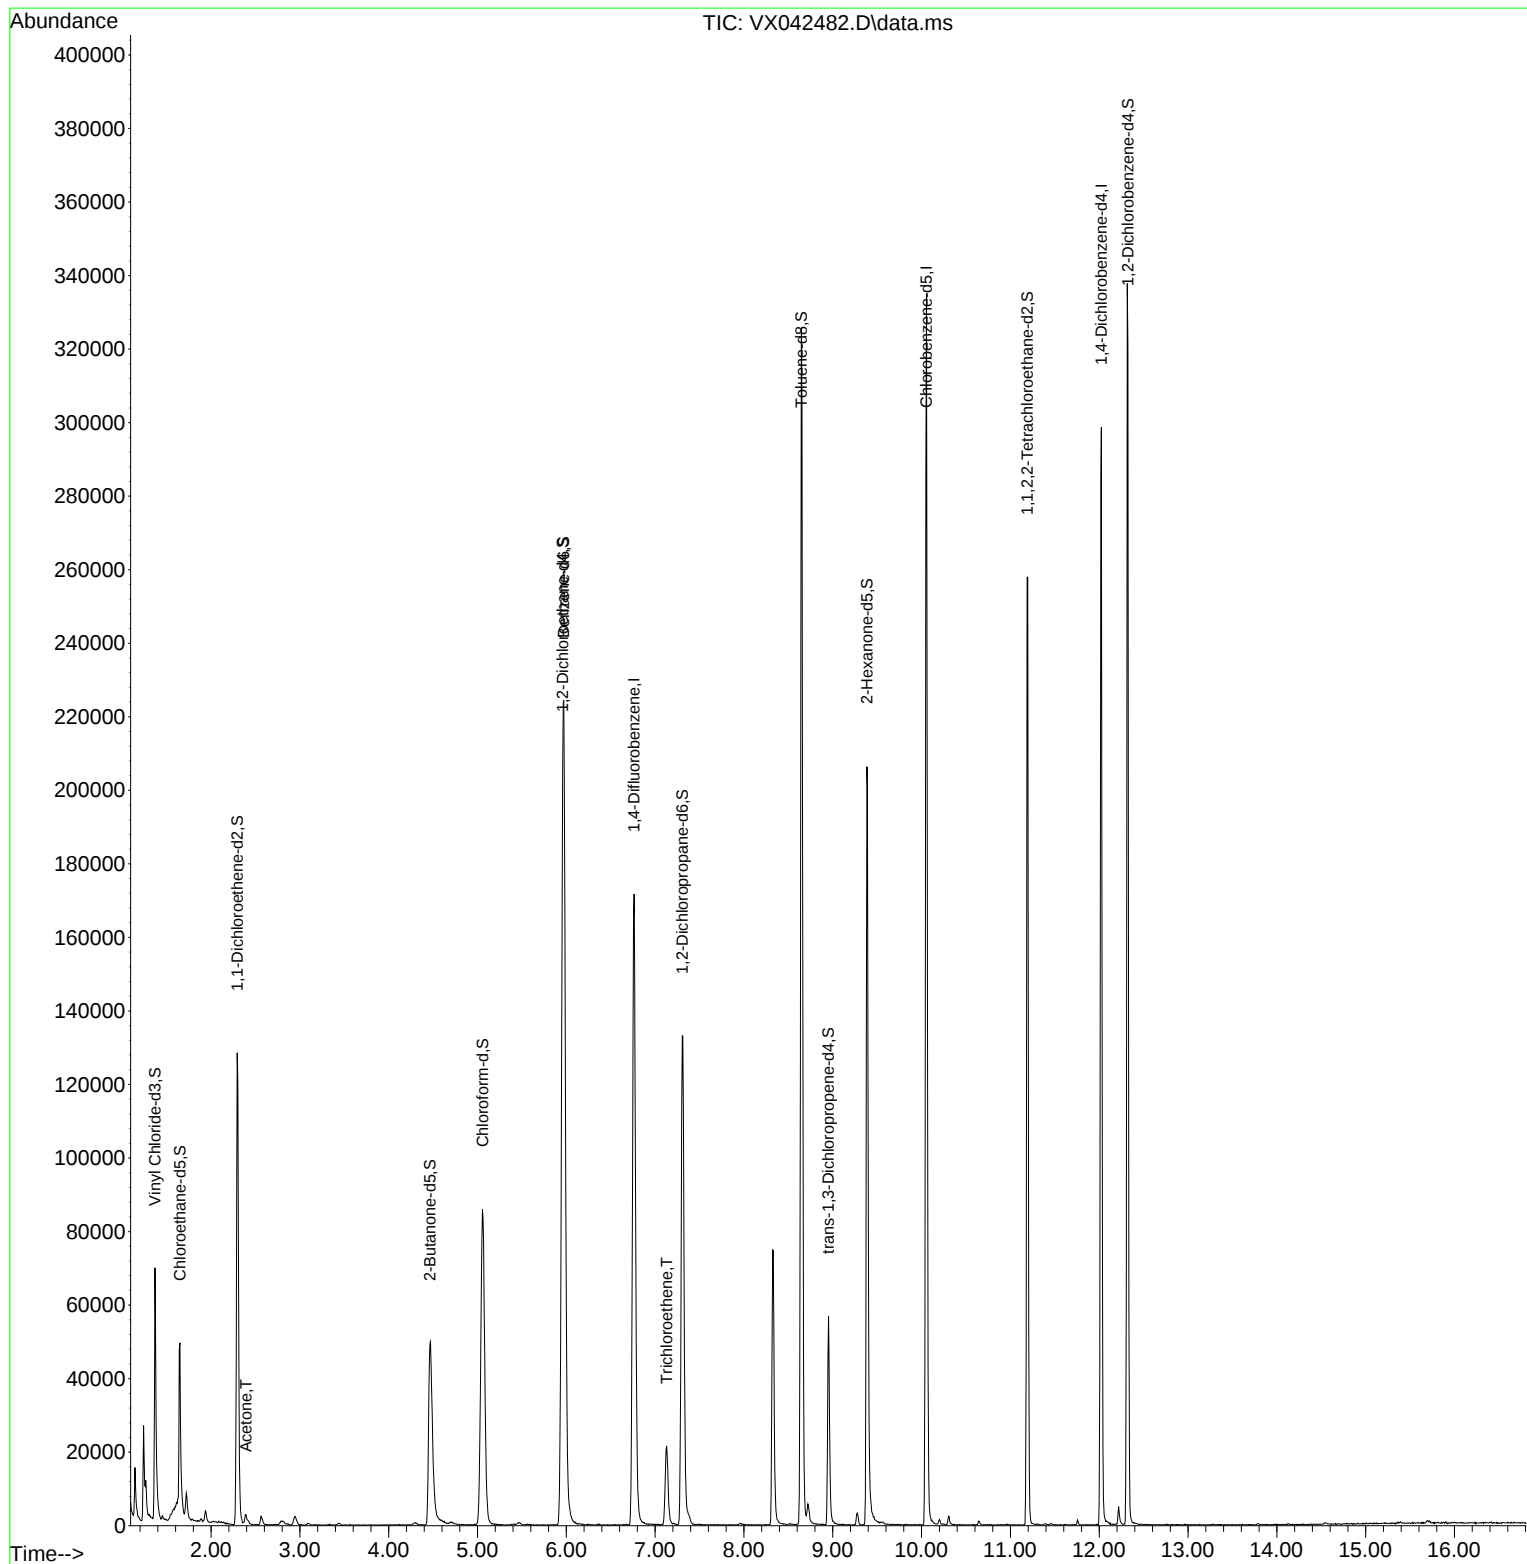

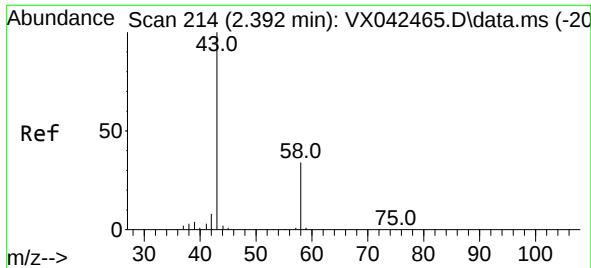

#13

Acetone

Concen: 5.886 ug/L

RT: 2.392 min Scan# 214

Delta R.T. 0.000 min

Lab File: VX042482.D

Acq: 23 Jul 2024 19:13

Instrument :

MSVOA_X

ClientSampleId :





E1ZW8

Tgt Ion: 43 Resp: 3183

Ion Ratio Lower Upper

43 100

58 30.0 0.0 62.6

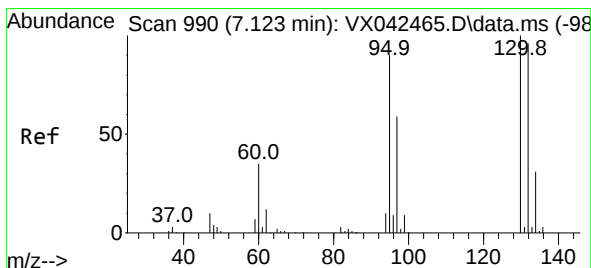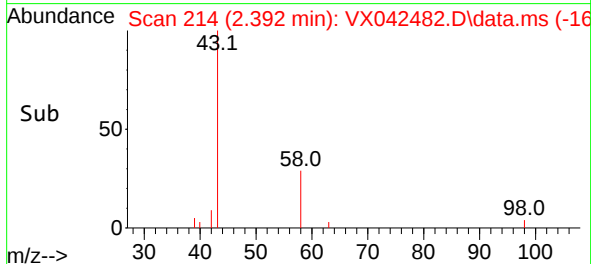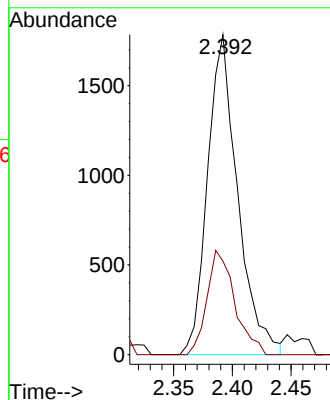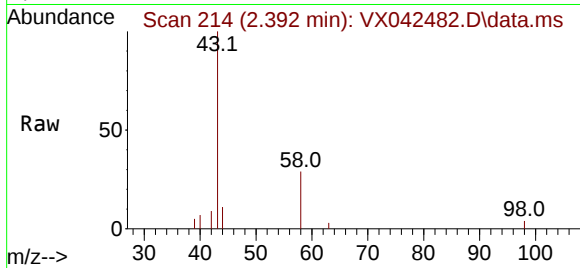

#34

Trichloroethene

Concen: 7.053 ug/L

RT: 7.129 min Scan# 991

Delta R.T. 0.006 min

Lab File: VX042482.D

Acq: 23 Jul 2024 19:13

Tgt Ion: 95 Resp: 8624

Ion Ratio Lower Upper

95 100

97 65.8 45.1 83.7

132 110.5 77.2 143.4

130 119.0 80.3 149.1

