

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072424\
 Data File : VX042486.D
 Acq On : 23 Jul 2024 20:46
 Operator : JC/MD
 Sample : P3327-17
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E1ZX2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

Signal : TIC: VX042486.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	7	9	18	rVB	12926	16940	0.04%	0.033%
2	1.239	22	25	27	rBV	19296	18954	0.05%	0.037%
3	1.264	27	29	35	rVB2	10369	11722	0.03%	0.023%
4	1.374	43	47	58	rBV2	189195	232084	0.60%	0.449%
5	1.550	72	76	77	rBV2	1883	2208	0.01%	0.004%
6	1.648	88	92	100	rVB	38120	53008	0.14%	0.102%
7	1.727	100	105	111	rVB2	8681	13582	0.04%	0.026%
8	1.941	136	140	147	rVB	5463	7796	0.02%	0.015%
9	2.300	193	199	213	rBV3	92607	184236	0.48%	0.356%
10	2.495	230	231	233	rBV2	207	194	0.00%	0.000%
11	2.562	237	242	248	rBV2	963	1780	0.00%	0.003%
12	2.818	273	284	289	rBV6	1807	5407	0.01%	0.010%
13	2.946	299	305	310	rBV	1227	2460	0.01%	0.005%
14	3.093	321	329	342	rBV	50360	117324	0.30%	0.227%
15	3.349	366	371	373	rBV2	236	371	0.00%	0.001%
16	3.446	377	387	393	rVB5	1240	2930	0.01%	0.006%
17	3.507	393	397	401	rBV2	132	205	0.00%	0.000%
18	3.611	406	414	422	rVB2	2727	6051	0.02%	0.012%
19	3.739	433	435	438	rVB	187	200	0.00%	0.000%
20	3.855	451	454	456	rBV2	133	200	0.00%	0.000%
21	4.300	516	527	535	rBB5	1021	2704	0.01%	0.005%
22	4.489	545	558	601	rBV	2963030	8270299	21.37%	15.986%
23	4.934	629	631	634	rVB2	302	282	0.00%	0.001%
24	5.056	639	651	666	rBV	73173	228774	0.59%	0.442%
25	5.196	672	674	677	rBV3	244	245	0.00%	0.000%
26	5.227	677	679	681	rVB	318	210	0.00%	0.000%
27	5.269	685	686	690	rVB2	214	217	0.00%	0.000%
28	5.385	696	705	713	rBV6	1842	5533	0.01%	0.011%
29	5.476	713	720	727	rVB6	1006	2962	0.01%	0.006%
30	5.562	731	734	739	rVB3	304	433	0.00%	0.001%
31	5.885	785	787	790	rBV	176	190	0.00%	0.000%
32	5.964	790	800	826	rBV2	189949	572060	1.48%	1.106%
33	6.165	831	833	838	rVB2	227	218	0.00%	0.000%
34	6.263	846	849	854	rBV2	176	292	0.00%	0.001%
35	6.336	858	861	862	rBV2	281	268	0.00%	0.001%
36	6.556	894	897	898	rBV	221	241	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072424\
 Data File : VX042486.D
 Acq On : 23 Jul 2024 20:46
 Operator : JC/MD
 Sample : P3327-17
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E1ZX2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

37	6.610	904	906	911	rBV2	176	202	0.00%	0.000%
38	6.763	922	931	947	rBV	168999	413790	1.07%	0.800%
39	7.135	980	992	1014	rBV	16954909	38702487	100.00%	74.809%
40	7.312	1014	1021	1030	rVB	113691	247725	0.64%	0.479%
41	7.818	1102	1104	1107	rBV3	228	188	0.00%	0.000%
42	7.946	1123	1125	1127	rBV3	449	525	0.00%	0.001%
43	8.025	1137	1138	1142	rVB3	199	229	0.00%	0.000%
44	8.324	1182	1187	1200	rBV	65652	112700	0.29%	0.218%
45	8.525	1213	1220	1223	rBV4	773	1563	0.00%	0.003%
46	8.598	1230	1232	1234	rBV	465	483	0.00%	0.001%
47	8.647	1234	1240	1248	rVV	275189	436320	1.13%	0.843%
48	8.720	1248	1252	1262	rVB	8032	15623	0.04%	0.030%
49	8.951	1285	1290	1304	rBV	47965	74212	0.19%	0.143%
50	9.165	1320	1325	1329	rBV3	1032	1462	0.00%	0.003%
51	9.275	1339	1343	1349	rVB2	4756	7290	0.02%	0.014%
52	9.384	1356	1361	1380	rBV	194890	294286	0.76%	0.569%
53	9.561	1388	1390	1393	rVB2	703	588	0.00%	0.001%
54	9.616	1397	1399	1402	rVB3	227	207	0.00%	0.000%
55	9.659	1404	1406	1408	rBV3	196	191	0.00%	0.000%
56	10.055	1465	1471	1485	rBV	352294	478414	1.24%	0.925%
57	10.195	1491	1494	1501	rVB	2427	3842	0.01%	0.007%
58	10.305	1507	1512	1519	rVV2	4280	6037	0.02%	0.012%
59	10.646	1564	1568	1578	rVV2	1327	2049	0.01%	0.004%
60	10.933	1611	1615	1618	rBV2	154	311	0.00%	0.001%
61	10.957	1618	1619	1621	rBV2	245	214	0.00%	0.000%
62	11.091	1639	1641	1648	rVB2	135	191	0.00%	0.000%
63	11.189	1652	1657	1668	rVV	229366	309716	0.80%	0.599%
64	11.268	1668	1670	1672	rVV	315	286	0.00%	0.001%
65	11.311	1672	1677	1682	rVV5	494	794	0.00%	0.002%
66	11.384	1684	1689	1693	rVV2	521	814	0.00%	0.002%
67	11.457	1697	1701	1707	rVB4	867	1181	0.00%	0.002%
68	11.616	1724	1727	1732	rVB2	311	455	0.00%	0.001%
69	11.670	1732	1736	1737	rBV	140	182	0.00%	0.000%
70	11.756	1746	1750	1758	rVB	1939	2477	0.01%	0.005%
71	12.024	1788	1794	1802	rBV	336793	437076	1.13%	0.845%
72	12.219	1821	1826	1834	rVV	6353	9335	0.02%	0.018%
73	12.317	1837	1842	1854	rVV	302845	400374	1.03%	0.774%
74	12.420	1857	1859	1862	rVB3	265	297	0.00%	0.001%
75	12.530	1873	1877	1879	rBV	152	223	0.00%	0.000%
76	12.622	1889	1892	1894	rBV2	231	184	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072424\
 Data File : VX042486.D
 Acq On : 23 Jul 2024 20:46
 Operator : JC/MD
 Sample : P3327-17
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E1ZX2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

77	12.762	1911	1915	1918	rVB3	320	429	0.00%	0.001%
78	13.225	1988	1991	1994	rVB2	169	239	0.00%	0.000%
79	13.292	1999	2002	2004	rVB2	203	195	0.00%	0.000%
80	13.353	2007	2012	2013	rBV2	174	266	0.00%	0.001%
81	13.585	2047	2050	2051	rBV2	185	183	0.00%	0.000%
82	13.786	2080	2083	2085	rBV3	262	420	0.00%	0.001%
83	14.060	2124	2128	2131	rVB2	143	252	0.00%	0.000%
84	14.103	2131	2135	2136	rBV	157	244	0.00%	0.000%
85	14.133	2136	2140	2144	rVB2	794	1025	0.00%	0.002%
86	14.402	2178	2184	2186	rBV2	183	285	0.00%	0.001%
87	14.676	2225	2229	2231	rBV4	197	245	0.00%	0.000%
88	14.761	2240	2243	2244	rBV2	202	234	0.00%	0.000%
89	15.030	2283	2287	2288	rBV2	229	286	0.00%	0.001%
90	15.316	2332	2334	2335	rBV2	301	236	0.00%	0.000%
91	15.383	2342	2345	2346	rBV2	622	675	0.00%	0.001%
92	15.572	2373	2376	2378	rBV3	312	445	0.00%	0.001%
93	15.645	2386	2388	2390	rBV3	258	241	0.00%	0.000%
94	15.694	2394	2396	2397	rVV2	309	184	0.00%	0.000%
95	15.792	2410	2412	2414	rVB2	320	213	0.00%	0.000%
96	15.816	2414	2416	2418	rVB2	296	218	0.00%	0.000%
97	15.840	2418	2420	2422	rBV3	432	409	0.00%	0.001%
98	16.151	2469	2471	2473	rBV2	242	215	0.00%	0.000%
99	16.346	2501	2503	2504	rBV2	343	284	0.00%	0.001%
100	16.584	2538	2542	2544	rBV2	255	362	0.00%	0.001%




Sum of corrected areas: 51734888

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072424\
Data File : VX042486.D
Acq On : 23 Jul 2024 20:46
Operator : JC/MD
Sample : P3327-17
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E1ZX2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

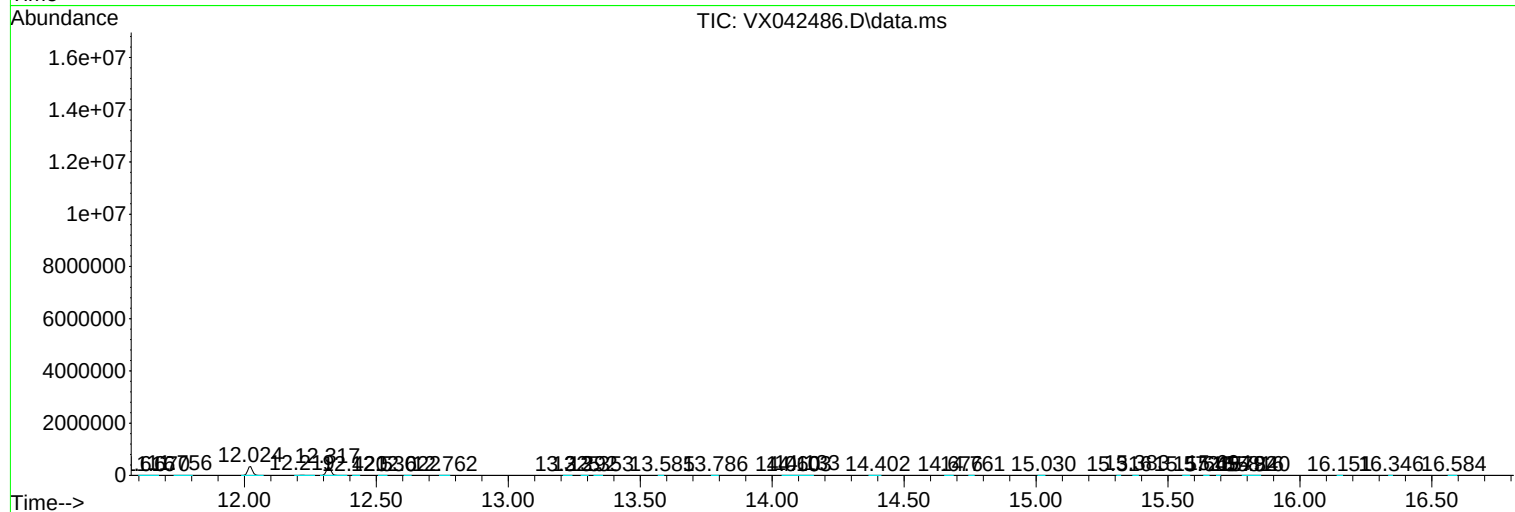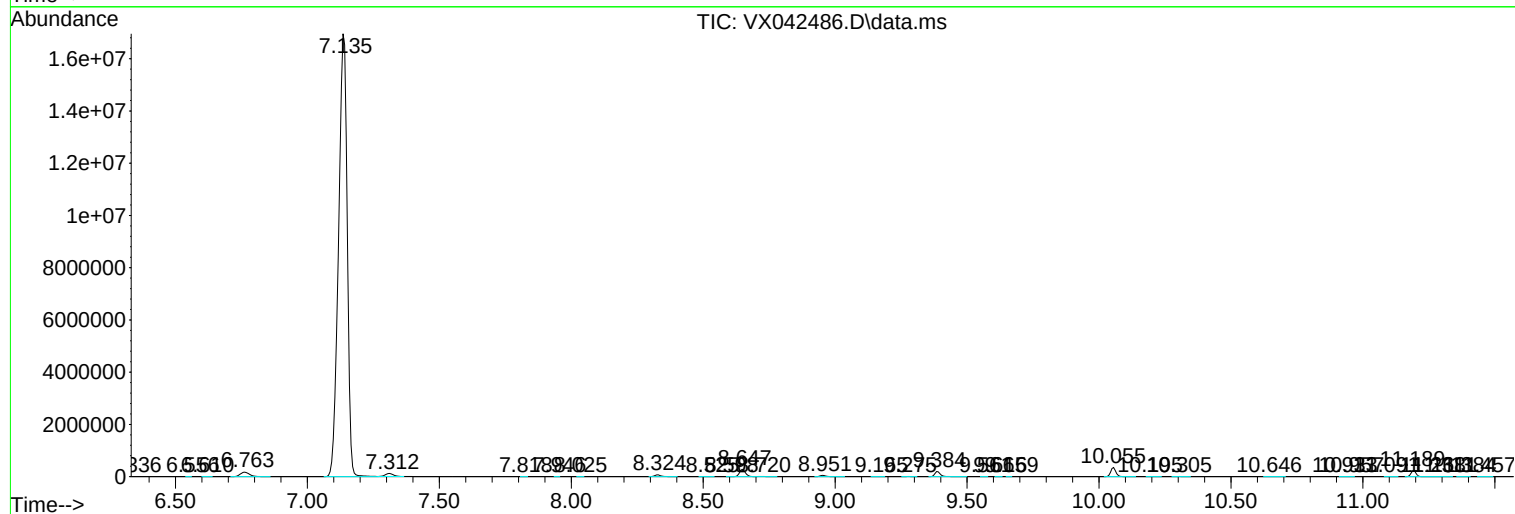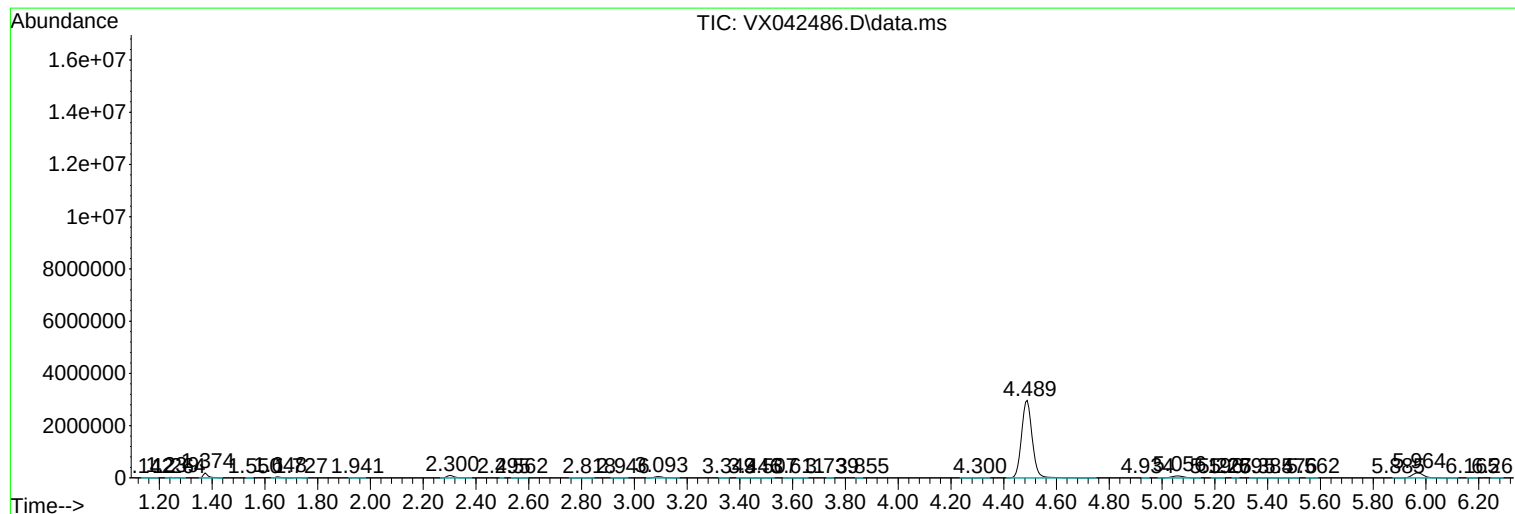

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072424\
Data File : VX042486.D
Acq On : 23 Jul 2024 20:46
Operator : JC/MD
Sample : P3327-17
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E1ZX2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072424\
Data File : VX042486.D
Acq On : 23 Jul 2024 20:46
Operator : JC/MD
Sample : P3327-17
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E1ZX2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------