

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072424\
 Data File : VX042494.D
 Acq On : 24 Jul 2024 00:13
 Operator : JC/MD
 Sample : P3327-23
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20F5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

Signal : TIC: VX042494.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	7	9	22	rVB	12960	18685	0.01%	0.010%
2	1.246	22	26	28	rBV	14982	19236	0.01%	0.010%
3	1.264	28	29	37	rVB2	10331	11093	0.01%	0.006%
4	1.374	43	47	64	rBV	751268	959397	0.62%	0.518%
5	1.648	89	92	101	rVB	53391	67611	0.04%	0.036%
6	1.721	101	104	112	rVB	9039	14142	0.01%	0.008%
7	1.941	136	140	145	rVB	5236	7571	0.00%	0.004%
8	2.099	163	166	168	rBV2	1266	1581	0.00%	0.001%
9	2.136	168	172	182	rVB	8411	14873	0.01%	0.008%
10	2.313	193	201	239	rBV3	257487	663215	0.43%	0.358%
11	2.654	255	257	262	rVB2	170	238	0.00%	0.000%
12	2.819	272	284	289	rBV4	2097	6861	0.00%	0.004%
13	2.941	299	304	305	rBV	1365	1725	0.00%	0.001%
14	3.093	321	329	366	rBV	129853	469102	0.30%	0.253%
15	3.447	380	387	394	rVB6	1750	4942	0.00%	0.003%
16	3.611	404	414	436	rBV	61965	166331	0.11%	0.090%
17	4.007	476	479	482	rVB2	219	262	0.00%	0.000%
18	4.306	520	528	535	rBV3	1168	3130	0.00%	0.002%
19	4.495	544	559	635	rBV	6767856	22581067	14.52%	12.181%
20	5.062	641	652	671	rVB	88010	276641	0.18%	0.149%
21	5.385	703	705	710	rVB4	517	589	0.00%	0.000%
22	5.471	715	719	724	rBV4	903	1804	0.00%	0.001%
23	5.562	729	734	741	rVB3	352	925	0.00%	0.000%
24	5.617	741	743	749	rBV3	167	241	0.00%	0.000%
25	5.733	759	762	763	rBV	186	223	0.00%	0.000%
26	5.818	774	776	778	rBV3	239	223	0.00%	0.000%
27	5.971	789	801	829	rBV2	233139	713972	0.46%	0.385%
28	6.379	865	868	874	rVV3	360	592	0.00%	0.000%
29	6.428	874	876	879	rVB2	201	200	0.00%	0.000%
30	6.605	903	905	910	rBV2	310	425	0.00%	0.000%
31	6.763	922	931	946	rBV	174392	444376	0.29%	0.240%
32	7.184	979	1000	1006	rBV	41098938	155534589	100.00%	83.900%
33	7.318	1016	1022	1043	rVB	155550	367704	0.24%	0.198%
34	8.324	1182	1187	1201	rBV	84365	146616	0.09%	0.079%
35	8.586	1227	1230	1232	rBV3	917	1077	0.00%	0.001%
36	8.647	1234	1240	1247	rBV	345866	545539	0.35%	0.294%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072424\
 Data File : VX042494.D
 Acq On : 24 Jul 2024 00:13
 Operator : JC/MD
 Sample : P3327-23
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20F5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

37	8.720	1247	1252	1262	rVB	63183	103407	0.07%	0.056%
38	8.952	1285	1290	1304	rBV	63003	94982	0.06%	0.051%
39	9.110	1314	1316	1320	rVB4	366	305	0.00%	0.000%
40	9.171	1324	1326	1327	rBV	326	244	0.00%	0.000%
41	9.208	1330	1332	1333	rVB2	365	223	0.00%	0.000%
42	9.275	1333	1343	1350	rBV2	9158	16914	0.01%	0.009%
43	9.385	1356	1361	1383	rBV	209938	318039	0.20%	0.172%
44	9.616	1396	1399	1401	rVV	297	246	0.00%	0.000%
45	9.647	1402	1404	1406	rVV2	429	351	0.00%	0.000%
46	9.665	1406	1407	1412	rVB3	485	561	0.00%	0.000%
47	9.744	1418	1420	1424	rBV3	413	422	0.00%	0.000%
48	9.854	1435	1438	1441	rVB3	292	346	0.00%	0.000%
49	10.055	1465	1471	1484	rBV	360050	503868	0.32%	0.272%
50	10.195	1491	1494	1501	rVB	3270	4684	0.00%	0.003%
51	10.305	1507	1512	1518	rBV	5339	8103	0.01%	0.004%
52	10.366	1521	1522	1526	rBV	284	220	0.00%	0.000%
53	10.433	1532	1533	1536	rVB2	249	196	0.00%	0.000%
54	10.647	1563	1568	1576	rVV2	2461	3998	0.00%	0.002%
55	10.738	1580	1583	1584	rBV2	243	242	0.00%	0.000%
56	10.884	1605	1607	1608	rBV	284	230	0.00%	0.000%
57	10.896	1608	1609	1614	rVV2	476	436	0.00%	0.000%
58	10.964	1617	1620	1625	rBV2	816	1053	0.00%	0.001%
59	11.061	1633	1636	1638	rBV2	163	209	0.00%	0.000%
60	11.104	1638	1643	1644	rBV	246	272	0.00%	0.000%
61	11.189	1652	1657	1670	rBV	265259	349215	0.22%	0.188%
62	11.281	1670	1672	1674	rBV3	252	266	0.00%	0.000%
63	11.311	1674	1677	1682	rVB	547	573	0.00%	0.000%
64	11.384	1685	1689	1692	rBV3	588	922	0.00%	0.000%
65	11.457	1697	1701	1707	rVB2	1004	1540	0.00%	0.001%
66	11.616	1723	1727	1730	rBV	414	577	0.00%	0.000%
67	11.756	1746	1750	1756	rVB	2495	3345	0.00%	0.002%
68	11.976	1782	1786	1788	rBV	1173	1335	0.00%	0.001%
69	12.018	1788	1793	1802	rVV	334297	437682	0.28%	0.236%
70	12.219	1821	1826	1834	rBV	7256	10744	0.01%	0.006%
71	12.317	1837	1842	1855	rVV	359135	455097	0.29%	0.245%
72	12.402	1855	1856	1860	rVB3	539	462	0.00%	0.000%
73	12.439	1860	1862	1865	rBV2	195	256	0.00%	0.000%
74	12.616	1888	1891	1892	rBV2	225	241	0.00%	0.000%
75	12.921	1939	1941	1945	rVV2	260	262	0.00%	0.000%
76	12.963	1945	1948	1954	rVV4	284	507	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072424\
 Data File : VX042494.D
 Acq On : 24 Jul 2024 00:13
 Operator : JC/MD
 Sample : P3327-23
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20F5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

77	13.122	1970	1974	1976	rVV3	772	827	0.00%	0.000%
78	13.280	1998	2000	2003	rBV2	332	448	0.00%	0.000%
79	13.591	2048	2051	2056	rVB4	716	1003	0.00%	0.001%
80	13.780	2079	2082	2086	rBV2	875	1101	0.00%	0.001%
81	13.963	2107	2112	2115	rBV3	653	914	0.00%	0.000%
82	14.018	2119	2121	2125	rVB3	202	224	0.00%	0.000%
83	14.134	2135	2140	2142	rBV2	507	748	0.00%	0.000%
84	14.170	2145	2146	2149	rBV2	203	200	0.00%	0.000%
85	14.445	2185	2191	2192	rBV4	225	359	0.00%	0.000%
86	14.585	2212	2214	2217	rBV2	197	195	0.00%	0.000%
87	14.774	2243	2245	2246	rBV	370	208	0.00%	0.000%
88	14.792	2246	2248	2249	rVV	332	228	0.00%	0.000%
89	14.987	2278	2280	2283	rVV3	239	232	0.00%	0.000%
90	15.012	2283	2284	2287	rVV2	257	229	0.00%	0.000%
91	15.390	2344	2346	2351	rVB2	733	953	0.00%	0.001%
92	15.451	2353	2356	2358	rVB2	378	293	0.00%	0.000%
93	15.542	2368	2371	2374	rBV4	266	466	0.00%	0.000%
94	15.572	2374	2376	2379	rVV2	225	262	0.00%	0.000%
95	15.670	2390	2392	2395	rBV3	266	214	0.00%	0.000%
96	15.841	2418	2420	2421	rBV2	302	225	0.00%	0.000%
97	16.377	2506	2508	2511	rBV4	384	432	0.00%	0.000%
98	16.493	2525	2527	2529	rBV3	268	197	0.00%	0.000%
99	16.609	2544	2546	2549	rBV2	373	382	0.00%	0.000%
100	16.719	2563	2564	2566	rBV2	314	255	0.00%	0.000%




Sum of corrected areas: 185379968

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072424\
Data File : VX042494.D
Acq On : 24 Jul 2024 00:13
Operator : JC/MD
Sample : P3327-23
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20F5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

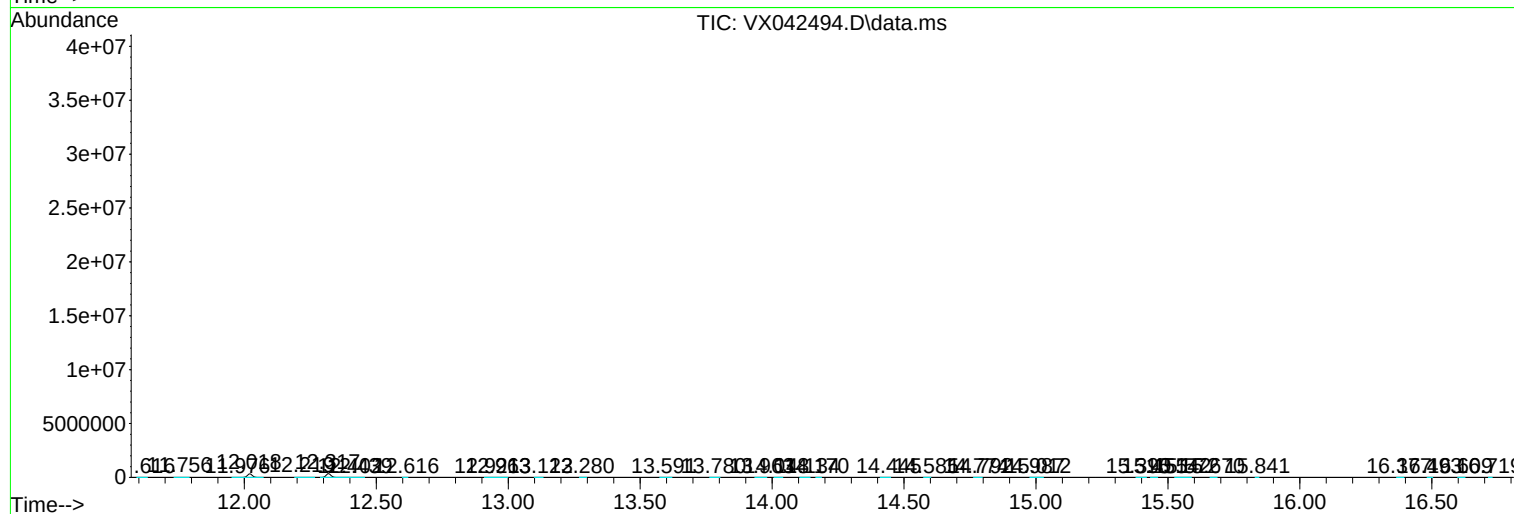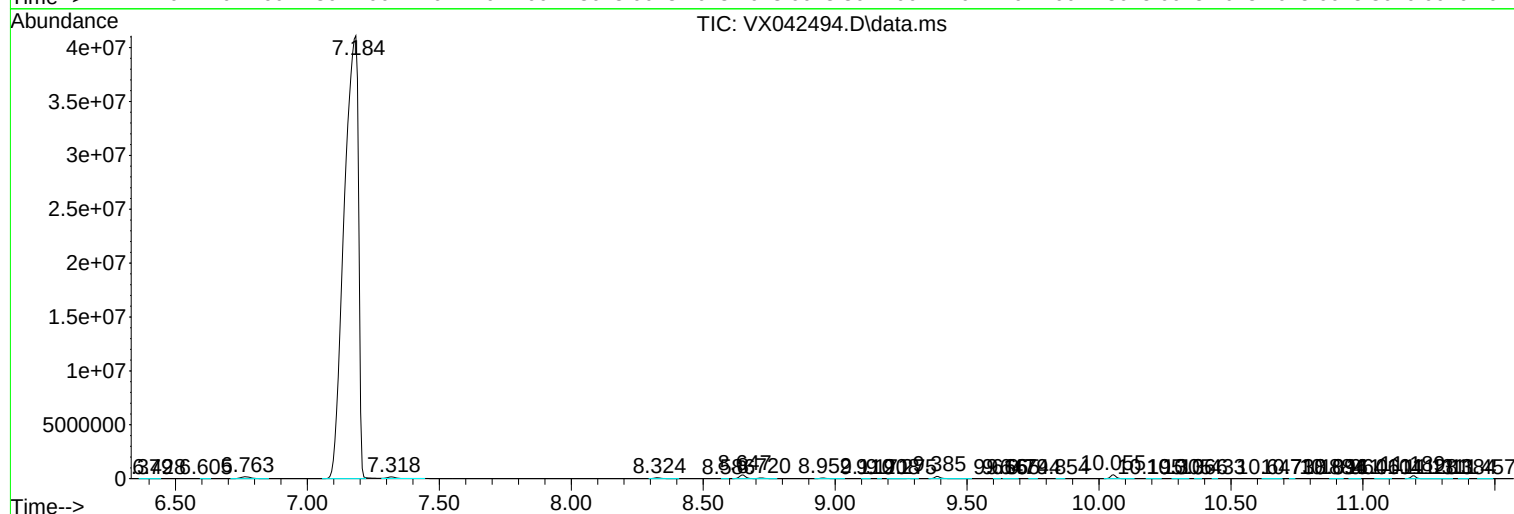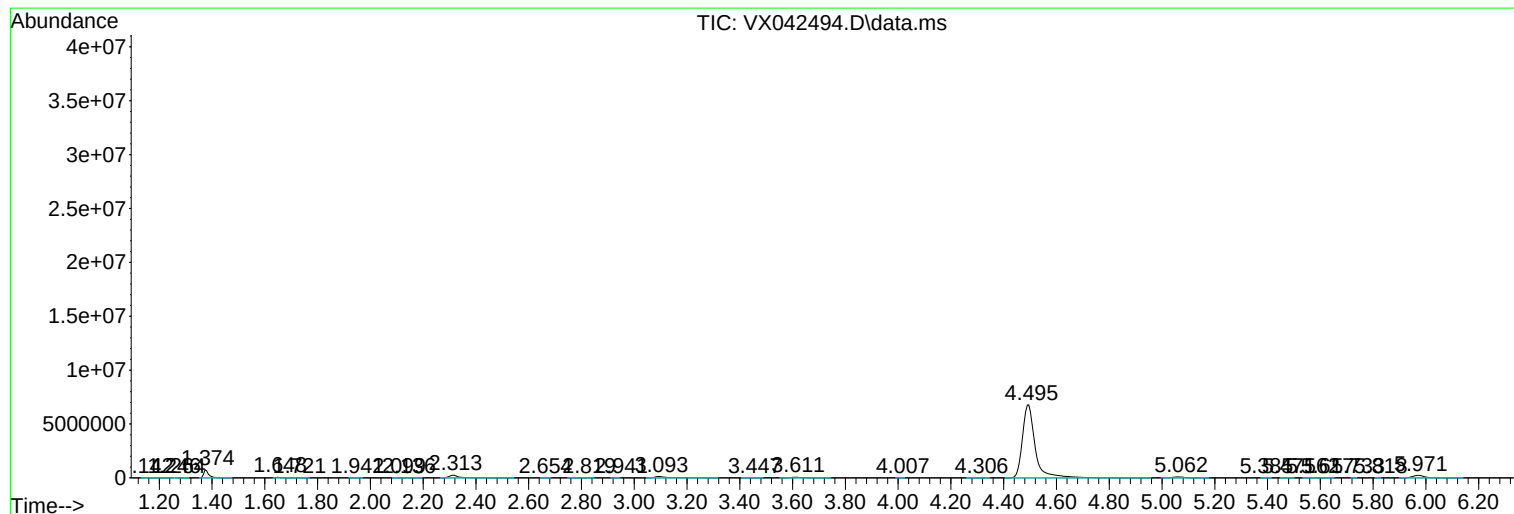

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072424\
Data File : VX042494.D
Acq On : 24 Jul 2024 00:13
Operator : JC/MD
Sample : P3327-23
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20F5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072424\
Data File : VX042494.D
Acq On : 24 Jul 2024 00:13
Operator : JC/MD
Sample : P3327-23
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20F5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc