

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072424\
 Data File : VX042495.D
 Acq On : 24 Jul 2024 00:36
 Operator : JC/MD
 Sample : P3327-24
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20F6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

Signal : TIC: VX042495.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	7	9	16	rVB2	4977	5988	0.01%	0.010%
2	1.240	22	25	28	rBV	15851	18206	0.04%	0.031%
3	1.374	43	47	58	rBV2	98760	132727	0.30%	0.223%
4	1.648	88	92	101	rVB	53031	73151	0.17%	0.123%
5	1.721	101	104	113	rVB4	5244	8714	0.02%	0.015%
6	1.941	136	140	146	rVB2	1959	3195	0.01%	0.005%
7	2.099	161	166	167	rBV2	2617	3509	0.01%	0.006%
8	2.136	168	172	181	rVB2	11949	21606	0.05%	0.036%
9	2.306	193	200	212	rBV2	147362	324761	0.74%	0.546%
10	2.562	238	242	247	rBV2	444	864	0.00%	0.001%
11	2.788	273	279	287	rBV4	1437	3785	0.01%	0.006%
12	2.947	297	305	310	rBV	1672	3888	0.01%	0.007%
13	3.087	321	328	341	rBV	37132	78845	0.18%	0.133%
14	3.379	373	376	379	rVB2	150	207	0.00%	0.000%
15	3.440	379	386	390	rBV4	597	1235	0.00%	0.002%
16	3.605	400	413	433	rBV	264942	638866	1.46%	1.074%
17	4.306	523	528	530	rVB2	487	544	0.00%	0.001%
18	4.373	535	539	542	rBV2	140	253	0.00%	0.000%
19	4.483	544	557	608	rBV	3518253	10002883	22.93%	16.818%
20	5.056	639	651	667	rBV	85149	266152	0.61%	0.447%
21	5.397	700	707	711	rBV5	401	767	0.00%	0.001%
22	5.745	763	764	769	rBV2	129	215	0.00%	0.000%
23	5.970	789	801	817	rBV2	225344	675844	1.55%	1.136%
24	6.294	849	854	856	rBV2	216	396	0.00%	0.001%
25	6.629	906	909	911	rVB2	232	254	0.00%	0.000%
26	6.763	921	931	948	rBV	177667	437980	1.00%	0.736%
27	6.970	963	965	971	rVB4	451	750	0.00%	0.001%
28	7.135	979	992	1013	rBV	18646236	43615222	100.00%	73.331%
29	7.312	1014	1021	1038	rVB	135182	315823	0.72%	0.531%
30	7.744	1090	1092	1095	rBV3	252	221	0.00%	0.000%
31	7.824	1103	1105	1110	rVB5	209	209	0.00%	0.000%
32	7.909	1117	1119	1123	rVB2	589	815	0.00%	0.001%
33	7.946	1123	1125	1126	rBV	315	285	0.00%	0.000%
34	8.122	1149	1154	1162	rVB4	326	583	0.00%	0.001%
35	8.196	1164	1166	1168	rBV2	275	305	0.00%	0.001%
36	8.232	1168	1172	1174	rVB3	256	253	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072424\
 Data File : VX042495.D
 Acq On : 24 Jul 2024 00:36
 Operator : JC/MD
 Sample : P3327-24
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20F6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

37	8.275	1177	1179	1181	rVV	237	269	0.00%	0.000%
38	8.324	1181	1187	1203	rVV	80228	134103	0.31%	0.225%
39	8.433	1203	1205	1209	rVB4	469	609	0.00%	0.001%
40	8.525	1218	1220	1224	rVB	338	251	0.00%	0.000%
41	8.592	1227	1231	1234	rBV4	449	685	0.00%	0.001%
42	8.647	1234	1240	1250	rVV	338610	536712	1.23%	0.902%
43	8.726	1250	1253	1262	rVB3	3510	7216	0.02%	0.012%
44	8.830	1269	1270	1275	rVB3	433	473	0.00%	0.001%
45	8.909	1281	1283	1285	rVB2	248	209	0.00%	0.000%
46	8.952	1285	1290	1308	rBV	57018	87851	0.20%	0.148%
47	9.275	1334	1343	1348	rBV5	3510	5925	0.01%	0.010%
48	9.384	1356	1361	1379	rVV	198622	300137	0.69%	0.505%
49	9.951	1452	1454	1458	rVB3	205	212	0.00%	0.000%
50	10.055	1465	1471	1491	rVV	361071	498411	1.14%	0.838%
51	10.201	1491	1495	1500	rVV2	1275	1985	0.00%	0.003%
52	10.244	1500	1502	1505	rVV4	418	522	0.00%	0.001%
53	10.311	1509	1513	1517	rBV	1586	2234	0.01%	0.004%
54	10.653	1565	1569	1577	rVB4	800	1456	0.00%	0.002%
55	10.823	1592	1597	1599	rVB3	175	287	0.00%	0.000%
56	10.841	1599	1600	1604	rBV2	154	197	0.00%	0.000%
57	10.963	1616	1620	1625	rVV2	381	483	0.00%	0.001%
58	11.189	1652	1657	1666	rBV	254979	332480	0.76%	0.559%
59	11.317	1674	1678	1682	rVB3	441	663	0.00%	0.001%
60	11.457	1698	1701	1705	rVV	409	497	0.00%	0.001%
61	11.713	1741	1743	1745	rBV2	184	213	0.00%	0.000%
62	11.756	1746	1750	1754	rVB2	790	1153	0.00%	0.002%
63	11.799	1754	1757	1760	rVB2	151	253	0.00%	0.000%
64	11.975	1783	1786	1788	rBV2	718	918	0.00%	0.002%
65	12.024	1788	1794	1804	rBV	330435	437773	1.00%	0.736%
66	12.219	1821	1826	1833	rBV	10173	14644	0.03%	0.025%
67	12.317	1837	1842	1856	rVV	355320	455994	1.05%	0.767%
68	12.573	1881	1884	1888	rBV2	149	223	0.00%	0.000%
69	12.670	1896	1900	1904	rVB2	328	520	0.00%	0.001%
70	12.914	1936	1940	1941	rVV2	216	243	0.00%	0.000%
71	12.933	1941	1943	1946	rVV2	262	247	0.00%	0.000%
72	12.963	1946	1948	1953	rVB2	157	231	0.00%	0.000%
73	13.115	1969	1973	1977	rVB3	369	572	0.00%	0.001%
74	13.225	1988	1991	1995	rVB3	220	300	0.00%	0.001%
75	13.286	1995	2001	2002	rBV2	161	264	0.00%	0.000%
76	13.597	2049	2052	2055	rVB3	612	634	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072424\
 Data File : VX042495.D
 Acq On : 24 Jul 2024 00:36
 Operator : JC/MD
 Sample : P3327-24
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20F6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

77	13.786	2078	2083	2093	rVB3	692	1455	0.00%	0.002%
78	13.963	2110	2112	2115	rVV2	538	536	0.00%	0.001%
79	14.048	2125	2126	2130	rVB	316	202	0.00%	0.000%
80	14.127	2135	2139	2144	rVV5	472	841	0.00%	0.001%
81	14.396	2181	2183	2186	rVB2	161	204	0.00%	0.000%
82	14.487	2196	2198	2200	rBV2	190	196	0.00%	0.000%
83	14.566	2209	2211	2216	rVB3	217	304	0.00%	0.001%
84	14.609	2216	2218	2221	rBV3	276	256	0.00%	0.000%
85	14.640	2221	2223	2227	rBV2	205	243	0.00%	0.000%
86	14.774	2242	2245	2247	rBV2	183	193	0.00%	0.000%
87	14.841	2255	2256	2258	rVV2	290	203	0.00%	0.000%
88	14.926	2268	2270	2274	rBV2	236	259	0.00%	0.000%
89	15.066	2291	2293	2294	rVV2	288	210	0.00%	0.000%
90	15.085	2294	2296	2298	rVB2	271	209	0.00%	0.000%
91	15.274	2326	2327	2330	rVB3	317	204	0.00%	0.000%
92	15.389	2342	2346	2353	rVB5	1040	1827	0.00%	0.003%
93	15.475	2359	2360	2365	rBV3	279	427	0.00%	0.001%
94	15.889	2426	2428	2430	rBV2	313	270	0.00%	0.000%
95	15.963	2438	2440	2443	rBV3	262	325	0.00%	0.001%
96	16.042	2449	2453	2454	rBV3	266	285	0.00%	0.000%
97	16.255	2486	2488	2489	rBV	254	256	0.00%	0.000%
98	16.438	2516	2518	2519	rBV2	275	204	0.00%	0.000%
99	16.511	2528	2530	2531	rBV2	289	214	0.00%	0.000%
100	16.725	2563	2565	2567	rBV3	386	228	0.00%	0.000%




Sum of corrected areas: 59476901

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072424\
Data File : VX042495.D
Acq On : 24 Jul 2024 00:36
Operator : JC/MD
Sample : P3327-24
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20F6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

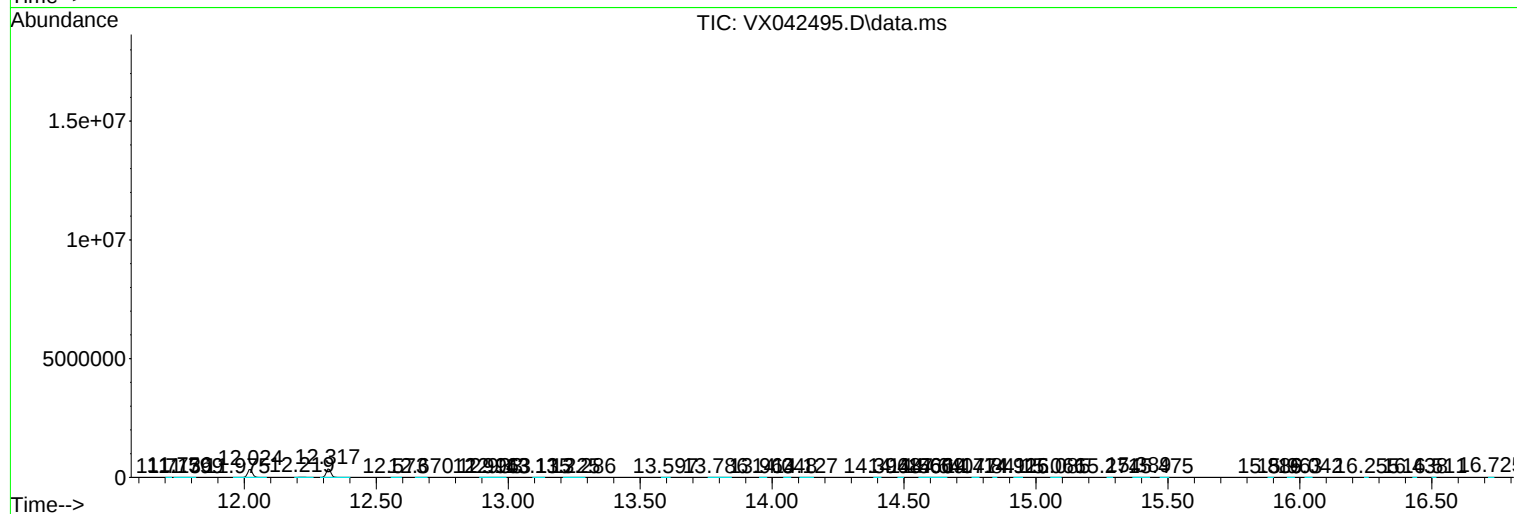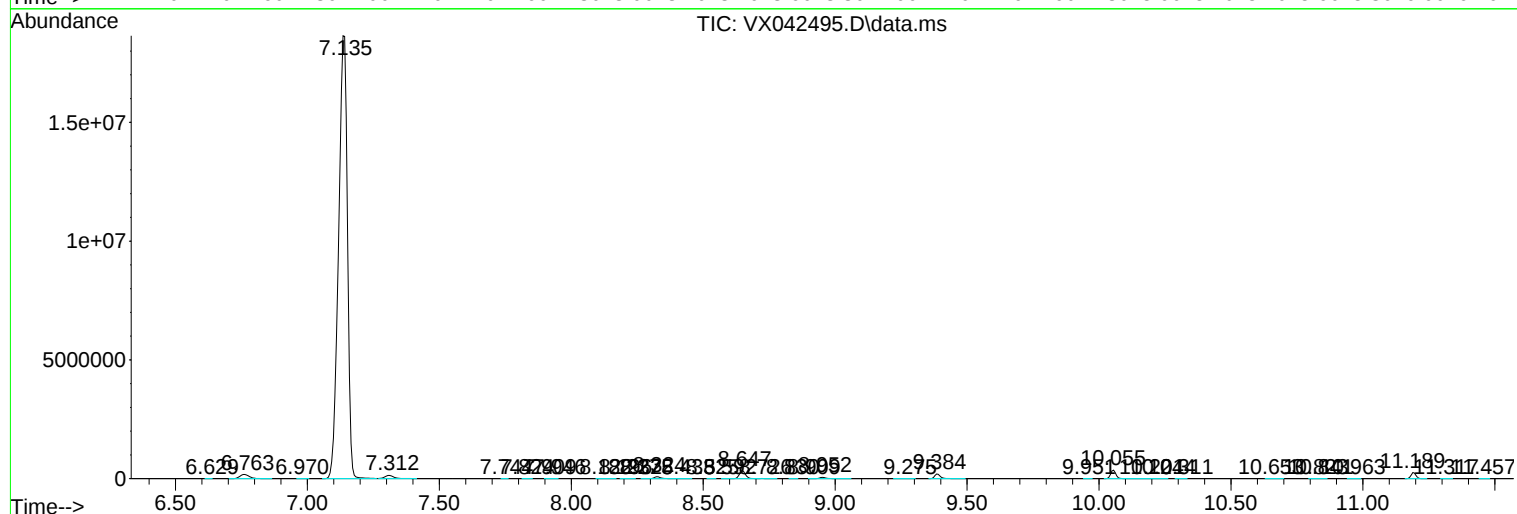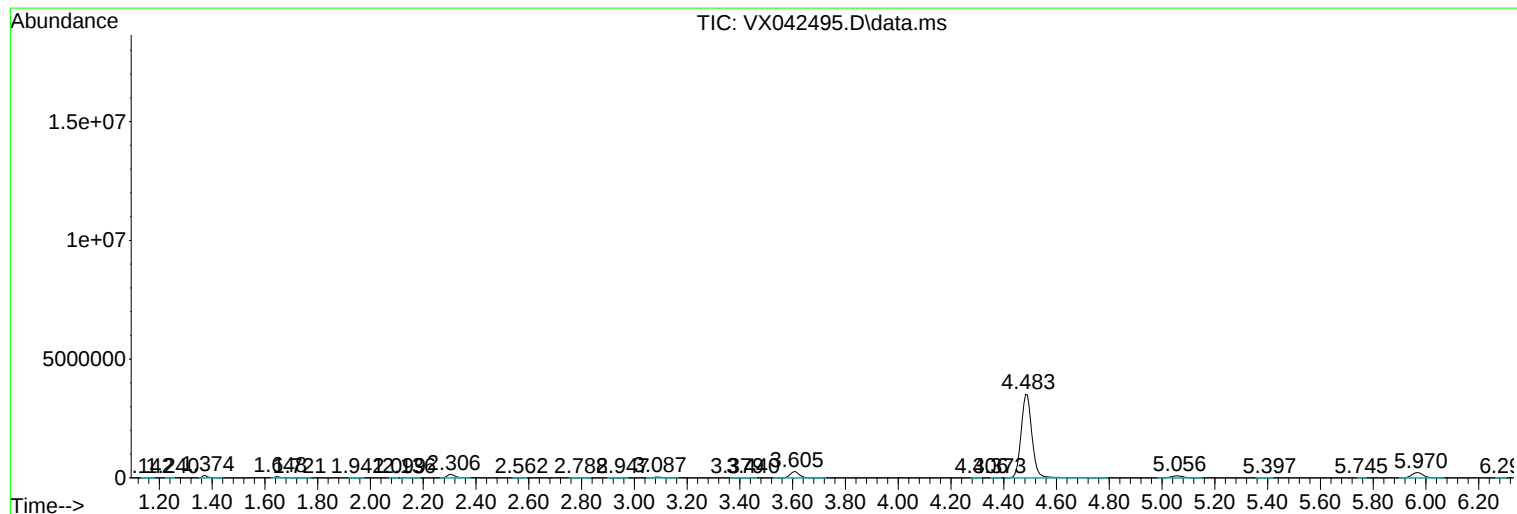

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072424\
Data File : VX042495.D
Acq On : 24 Jul 2024 00:36
Operator : JC/MD
Sample : P3327-24
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20F6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072424\
Data File : VX042495.D
Acq On : 24 Jul 2024 00:36
Operator : JC/MD
Sample : P3327-24
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20F6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------