

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072424\
 Data File : VX042497.D
 Acq On : 24 Jul 2024 01:22
 Operator : JC/MD
 Sample : P3327-29
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20F9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

Signal : TIC: VX042497.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	6	9	20	rVB	11075	15161	1.56%	0.264%
2	1.240	22	25	27	rBV	14175	14690	1.51%	0.256%
3	1.368	43	46	57	rVB	67715	85008	8.73%	1.481%
4	1.648	88	92	101	rVB	49624	61978	6.36%	1.079%
5	2.300	192	199	209	rBV	127716	204464	21.00%	3.561%
6	2.392	209	214	216	rBV2	2199	3423	0.35%	0.060%
7	2.788	273	279	280	rBV4	790	1179	0.12%	0.021%
8	2.947	297	305	312	rBV2	2009	4912	0.50%	0.086%
9	3.044	320	321	324	rVB	220	171	0.02%	0.003%
10	3.087	324	328	336	rBV6	1542	3279	0.34%	0.057%
11	3.233	351	352	356	rBV2	114	130	0.01%	0.002%
12	3.440	382	386	393	rVB3	697	1083	0.11%	0.019%
13	3.532	397	401	402	rBV	185	226	0.02%	0.004%
14	3.587	406	410	413	rBV4	191	293	0.03%	0.005%
15	3.739	433	435	439	rVB2	184	211	0.02%	0.004%
16	3.776	439	441	444	rBV3	149	136	0.01%	0.002%
17	3.837	448	451	453	rVB2	140	130	0.01%	0.002%
18	3.916	460	464	468	rBV	140	199	0.02%	0.003%
19	4.014	479	480	483	rVB	259	154	0.02%	0.003%
20	4.044	483	485	488	rBV2	216	237	0.02%	0.004%
21	4.087	488	492	494	rBV	156	143	0.01%	0.002%
22	4.166	502	505	506	rBV	159	199	0.02%	0.003%
23	4.239	515	517	522	rBV2	82	133	0.01%	0.002%
24	4.282	522	524	526	rBV2	462	494	0.05%	0.009%
25	4.471	545	555	577	rBV2	62684	222802	22.88%	3.880%
26	4.824	611	613	618	rVB3	162	204	0.02%	0.004%
27	4.867	618	620	623	rVB2	192	138	0.01%	0.002%
28	4.904	623	626	628	rBV3	197	213	0.02%	0.004%
29	5.056	638	651	669	rBV	82787	256114	26.30%	4.461%
30	5.312	690	693	697	rVB2	187	210	0.02%	0.004%
31	5.361	699	701	702	rBV	247	141	0.01%	0.002%
32	5.458	711	717	722	rBV3	996	2198	0.23%	0.038%
33	5.556	731	733	734	rBV	235	168	0.02%	0.003%
34	5.696	754	756	759	rBV	144	166	0.02%	0.003%
35	5.879	783	786	789	rBV2	128	181	0.02%	0.003%
36	5.964	789	800	822	rBV2	219987	653054	67.07%	11.374%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072424\
 Data File : VX042497.D
 Acq On : 24 Jul 2024 01:22
 Operator : JC/MD
 Sample : P3327-29
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20F9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

37	6.281	850	852	856	rBV2	240	287	0.03%	0.005%
38	6.361	862	865	866	rVV	270	291	0.03%	0.005%
39	6.598	902	904	909	rBV3	122	225	0.02%	0.004%
40	6.763	921	931	949	rBV	168098	409999	42.10%	7.141%
41	6.989	966	968	972	rVB	326	273	0.03%	0.005%
42	7.123	981	990	1012	rBV	445094	973756	100.00%	16.960%
43	7.306	1012	1020	1038	rVB	130753	295080	30.30%	5.139%
44	7.489	1048	1050	1053	rVB3	342	357	0.04%	0.006%
45	7.549	1056	1060	1061	rBV	145	130	0.01%	0.002%
46	7.659	1076	1078	1081	rBV2	120	144	0.01%	0.003%
47	7.952	1122	1126	1129	rBV2	343	473	0.05%	0.008%
48	8.232	1168	1172	1174	rBV2	137	158	0.02%	0.003%
49	8.324	1181	1187	1199	rBV	71420	121822	12.51%	2.122%
50	8.507	1215	1217	1218	rBV	233	168	0.02%	0.003%
51	8.592	1226	1231	1234	rBV3	385	458	0.05%	0.008%
52	8.647	1234	1240	1249	rBV	309041	492101	50.54%	8.571%
53	8.952	1285	1290	1299	rBV	49552	77042	7.91%	1.342%
54	9.220	1331	1334	1337	rBV	189	229	0.02%	0.004%
55	9.275	1337	1343	1349	rBV4	2849	4597	0.47%	0.080%
56	9.385	1356	1361	1382	rBV	193829	299993	30.81%	5.225%
57	9.683	1408	1410	1412	rVB2	257	192	0.02%	0.003%
58	9.762	1421	1423	1425	rBV2	157	153	0.02%	0.003%
59	9.854	1433	1438	1440	rBV2	147	233	0.02%	0.004%
60	9.878	1440	1442	1446	rBV2	156	202	0.02%	0.004%
61	9.988	1458	1460	1462	rBV2	128	147	0.02%	0.003%
62	10.055	1465	1471	1486	rBV	314706	440620	45.25%	7.674%
63	10.201	1491	1495	1501	rVB	1465	1924	0.20%	0.034%
64	10.311	1507	1513	1519	rBV3	2311	4213	0.43%	0.073%
65	10.415	1528	1530	1531	rBV	168	134	0.01%	0.002%
66	10.494	1539	1543	1547	rBV2	219	290	0.03%	0.005%
67	10.646	1564	1568	1572	rBV3	872	1408	0.14%	0.025%
68	10.903	1608	1610	1612	rBV	157	156	0.02%	0.003%
69	10.970	1616	1621	1624	rVB2	354	475	0.05%	0.008%
70	11.189	1652	1657	1669	rBV	246720	322061	33.07%	5.609%
71	11.305	1674	1676	1678	rBV2	281	214	0.02%	0.004%
72	11.384	1687	1689	1691	rBV2	275	301	0.03%	0.005%
73	11.457	1696	1701	1704	rVV2	578	949	0.10%	0.017%
74	11.549	1715	1716	1720	rVV2	198	165	0.02%	0.003%
75	11.756	1747	1750	1757	rVB	1416	1671	0.17%	0.029%
76	11.878	1768	1770	1773	rBV	235	175	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072424\
 Data File : VX042497.D
 Acq On : 24 Jul 2024 01:22
 Operator : JC/MD
 Sample : P3327-29
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20F9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

77	11.933	1778	1779	1784	rBV2	87	134	0.01%	0.002%
78	11.969	1784	1785	1789	rBV2	298	322	0.03%	0.006%
79	12.024	1789	1794	1808	rBV	273110	352268	36.18%	6.135%
80	12.219	1821	1826	1831	rBV	9897	13337	1.37%	0.232%
81	12.317	1837	1842	1854	rBV	302386	384415	39.48%	6.695%
82	12.597	1886	1888	1892	rBV2	176	252	0.03%	0.004%
83	12.963	1944	1948	1954	rBV2	294	429	0.04%	0.007%
84	13.012	1954	1956	1958	rBV	211	193	0.02%	0.003%
85	13.042	1958	1961	1963	rVB2	127	165	0.02%	0.003%
86	13.122	1972	1974	1976	rVB2	219	192	0.02%	0.003%
87	13.292	1998	2002	2004	rBV2	224	200	0.02%	0.003%
88	13.390	2017	2018	2022	rBV2	122	151	0.02%	0.003%
89	13.475	2030	2032	2036	rVB2	124	140	0.01%	0.002%
90	13.597	2050	2052	2054	rVB2	271	236	0.02%	0.004%
91	13.646	2059	2060	2064	rBV	123	181	0.02%	0.003%
92	13.701	2068	2069	2071	rBV	154	149	0.02%	0.003%
93	13.865	2092	2096	2098	rVB2	136	163	0.02%	0.003%
94	13.969	2110	2113	2115	rVB2	251	246	0.03%	0.004%
95	14.060	2125	2128	2130	rBV	132	145	0.01%	0.003%
96	14.121	2136	2138	2143	rVB2	389	546	0.06%	0.010%
97	14.189	2147	2149	2152	rBV2	147	188	0.02%	0.003%
98	14.268	2161	2162	2166	rVV4	193	150	0.02%	0.003%
99	14.695	2230	2232	2233	rBV	225	198	0.02%	0.003%
100	16.639	2549	2551	2552	rBV2	433	313	0.03%	0.005%




Sum of corrected areas: 5741601

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072424\
Data File : VX042497.D
Acq On : 24 Jul 2024 01:22
Operator : JC/MD
Sample : P3327-29
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20F9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

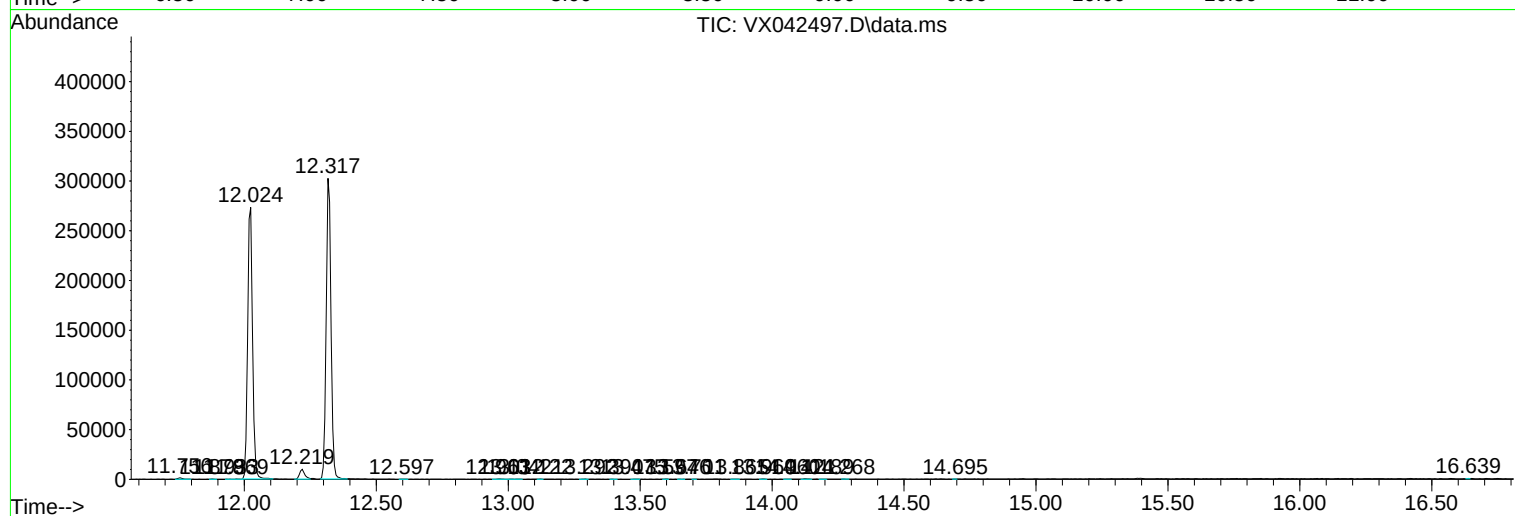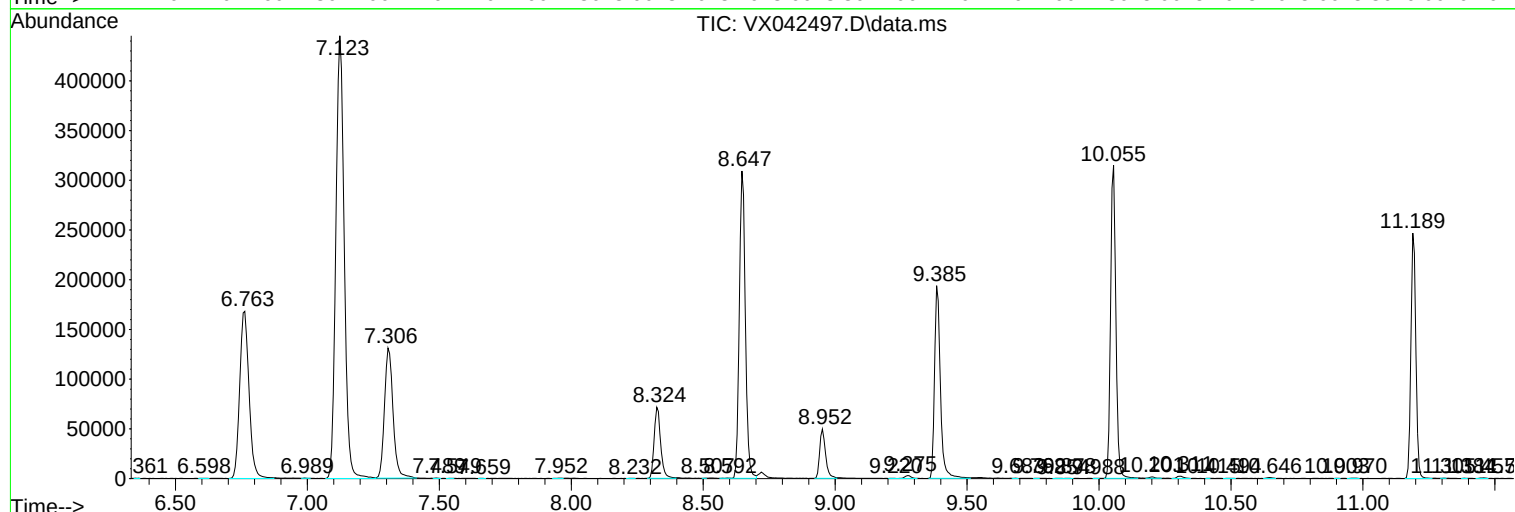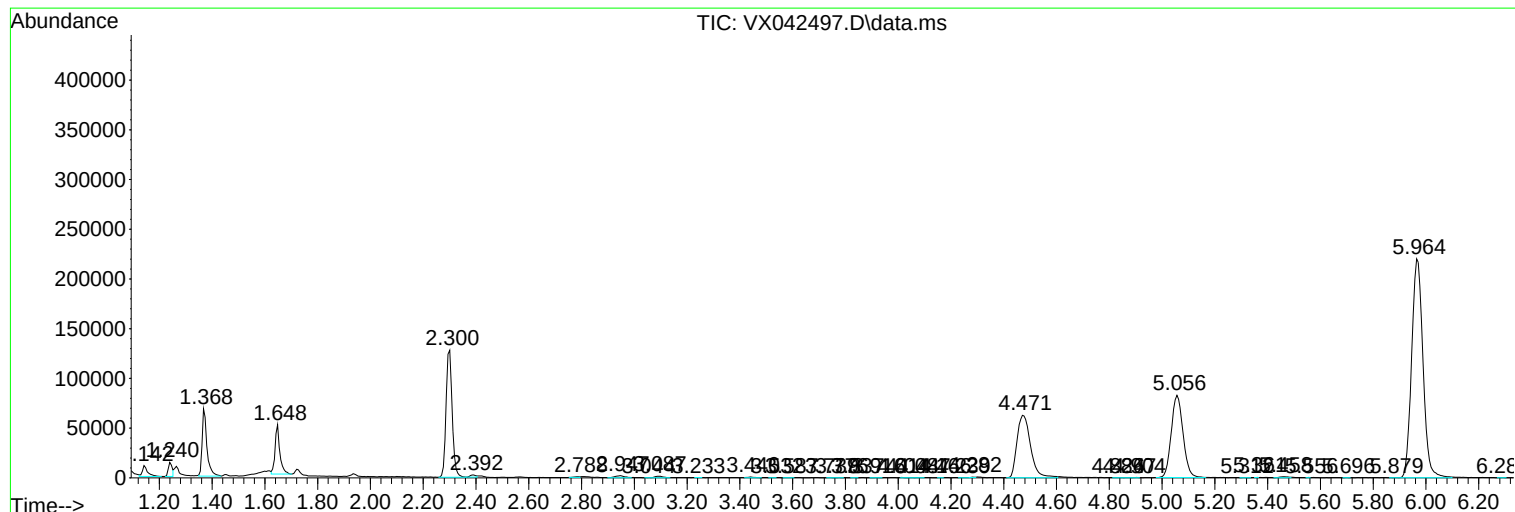

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072424\
Data File : VX042497.D
Acq On : 24 Jul 2024 01:22
Operator : JC/MD
Sample : P3327-29
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20F9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072424\
Data File : VX042497.D
Acq On : 24 Jul 2024 01:22
Operator : JC/MD
Sample : P3327-29
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20F9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc