
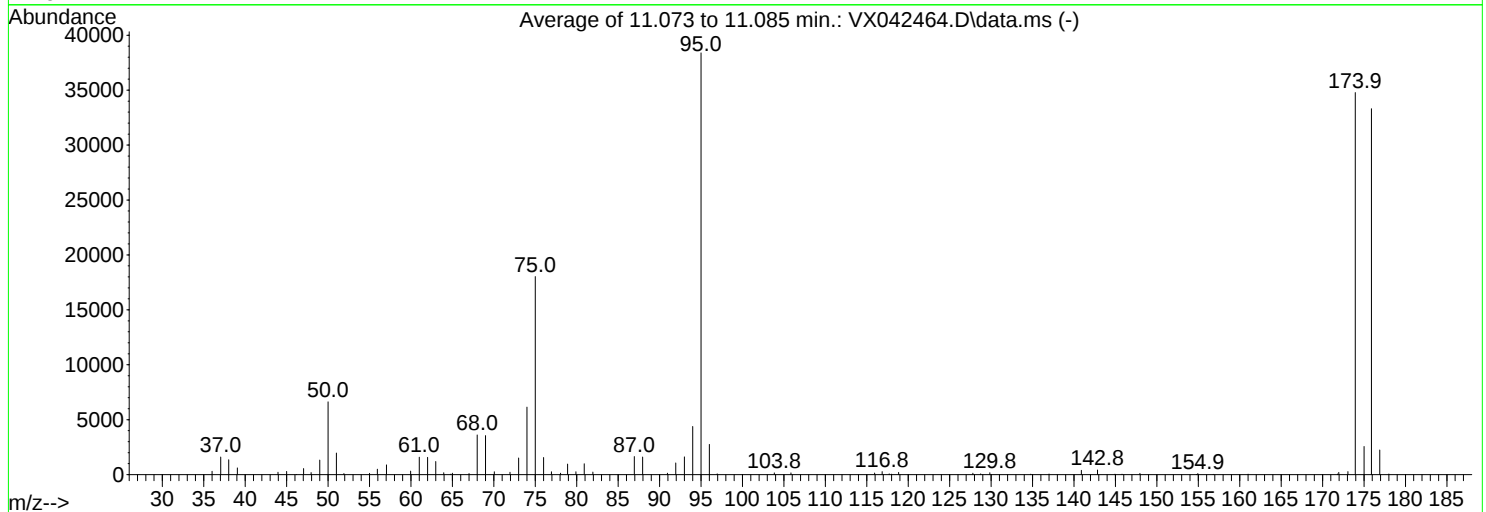


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072424\
Data File : VX042464.D
Acq On : 23 Jul 2024 11:58
Operator : JC/MD
Sample : BFB683
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB683

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM070324WMA.M
Title : VOC Analysis
Last Update : Wed Jul 24 03:44:32 2024

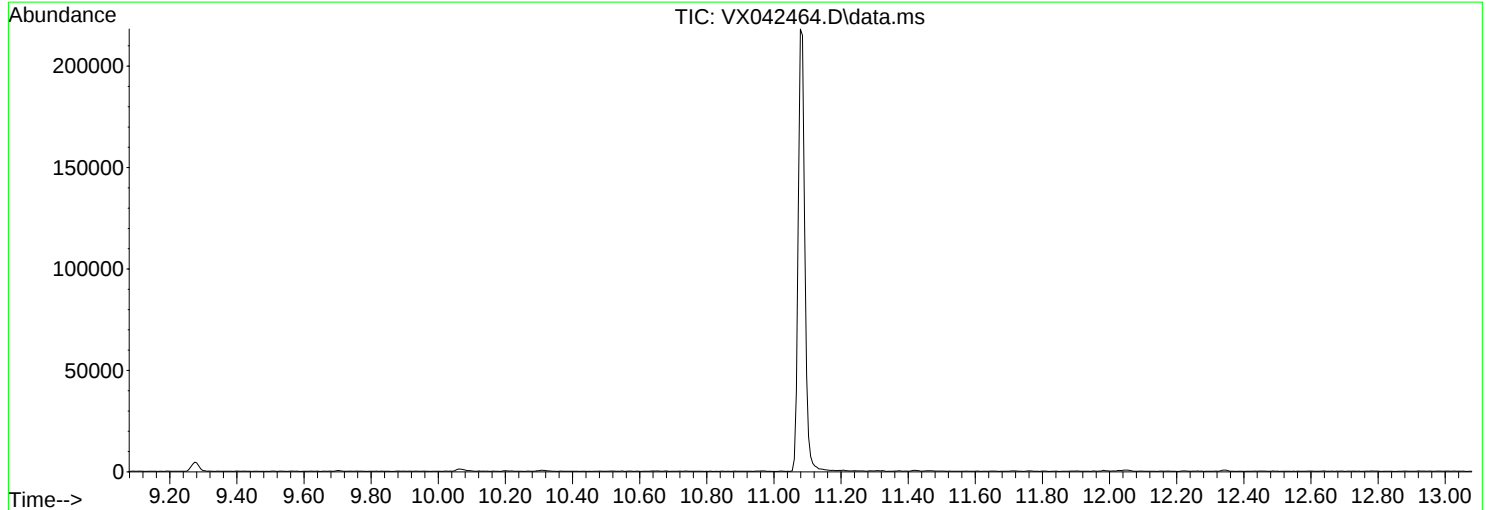

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	6621	PASS
75	95	30	80	47.0	18030	PASS
95	95	100	100	100.0	38395	PASS
96	95	5	9	7.2	2750	PASS
173	174	0.00	2	0.8	277	PASS
174	95	50	120	90.6	34784	PASS
175	174	5	9	7.4	2560	PASS
176	174	95	101	95.8	33307	PASS
177	176	5	9	6.7	2247	PASS

m/z	Abundance
40.00	188.0
43.90	136.0

Instrument :
MSVOA_X
ClientSampleId :
BFB683

m/z	Abundance
36.00	197.0
37.10	1407.0
38.00	1040.0
39.00	451.0
40.00	152.0
44.00	270.0
44.90	219.0
47.10	448.0
47.90	144.0
49.00	962.0
50.00	5187.0
51.00	1533.0
51.90	96.0
54.90	87.0
56.00	416.0
57.10	727.0
59.90	263.0
61.00	1411.0
62.00	1165.0
63.00	956.0
64.00	173.0
64.80	131.0
67.00	63.0
68.00	2780.0
69.00	2749.0
70.10	232.0
72.10	173.0
73.00	1230.0
74.00	4802.0
75.00	13257.0
76.00	1344.0
76.90	242.0
78.90	707.0
79.90	150.0
80.90	747.0
82.00	181.0
86.90	1325.0
88.00	1183.0
91.00	90.0
91.90	634.0
93.00	1144.0
94.00	2965.0
95.00	28040.0
96.00	2128.0
96.90	74.0
103.90	103.0
105.80	153.0
116.00	126.0
116.80	171.0
117.70	75.0
118.90	134.0
127.80	91.0
128.70	57.0
129.80	168.0
140.90	272.0
142.80	263.0
145.80	54.0
148.00	59.0
154.80	69.0
171.80	177.0
173.10	301.0
173.90	20896.0
175.00	1722.0
175.90	19992.0
176.90	1453.0

Instrument :
MSVOA_X
ClientSampleId :
BFB683

m/z	Abundance
36.10	341.0
37.10	1865.0
38.00	1741.0
39.10	839.0
40.00	173.0
44.00	427.0
45.00	381.0
47.00	666.0
48.00	267.0
49.00	1681.0
50.00	7834.0
51.00	2327.0
51.90	92.0
55.00	158.0
55.90	632.0
57.00	1092.0
60.00	378.0
61.00	1872.0
62.00	1891.0
63.00	1404.0
64.00	198.0
65.00	155.0
67.10	110.0
68.00	4241.0
69.00	4187.0
70.00	270.0
71.90	209.0
73.00	1768.0
74.00	7243.0
75.00	21664.0
76.00	1786.0
77.00	294.0
78.00	222.0
78.90	1173.0
79.90	326.0
80.90	1115.0
82.00	261.0
87.00	1957.0
87.90	1938.0
90.90	186.0
92.00	1231.0
93.00	2008.0
94.00	5053.0
95.00	44896.0
96.00	3225.0
97.00	91.0
103.90	177.0
105.90	171.0
115.90	208.0
116.80	313.0
117.70	165.0
118.80	171.0
127.80	145.0
128.70	79.0
129.80	185.0
134.80	67.0
137.00	109.0
140.90	495.0
142.90	470.0
145.00	82.0
145.80	80.0
148.00	159.0
155.00	166.0
156.80	71.0
161.00	56.0
172.00	232.0
173.90	39928.0
175.00	2953.0
175.90	37368.0
176.90	2480.0
178.00	103.0

Instrument :
MSVOA_X
ClientSampleId :
BFB683

m/z	Abundance
35.90	380.0
37.00	1550.0
38.00	1295.0
39.00	555.0
40.00	213.0
44.00	365.0
45.10	292.0
46.20	64.0
47.10	552.0
48.00	168.0
49.00	1340.0
50.00	6842.0
51.00	2026.0
51.90	126.0
55.10	85.0
56.00	435.0
57.00	860.0
60.00	345.0
61.00	1474.0
62.00	1677.0
63.00	1222.0
63.90	145.0
65.00	222.0
66.90	137.0
68.00	3799.0
69.00	3739.0
70.10	272.0
71.90	268.0
73.00	1554.0
74.00	6396.0
75.00	19168.0
76.00	1535.0
76.90	253.0
78.10	184.0
78.90	1010.0
79.90	317.0
80.90	1122.0
81.80	249.0
86.90	1666.0
87.90	1675.0
91.00	130.0
92.00	1329.0
93.00	1709.0
94.00	5131.0
95.00	42248.0
96.00	2897.0
96.90	79.0
103.80	219.0
105.90	156.0
115.90	118.0
116.90	334.0
118.00	154.0
118.90	291.0
127.80	156.0
128.80	69.0
129.90	163.0
134.80	56.0
137.00	62.0
140.90	421.0
142.90	535.0
144.90	68.0
147.90	142.0
154.90	155.0
161.00	74.0
171.90	373.0
173.00	530.0
174.00	43528.0
175.00	3004.0
175.90	42560.0
176.90	2807.0
178.00	73.0

Instrument :
MSVOA_X
ClientSampleId :
BFB683