

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072425\
 Data File : VX047124.D
 Acq On : 24 Jul 2025 16:37
 Operator : JC/MD
 Sample : IBLK
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 IBLK

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072125W.M

Title : SW846 8260

Signal : TIC: VX047124.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.173	10	14	21	rVB	58323	65686	1.41%	0.379%
2	2.745	252	272	326	rBV3	612756	4672415	100.00%	26.985%
3	5.397	695	707	724	rBV2	237662	734723	15.72%	4.243%
4	5.562	724	734	755	rVB	362867	1100023	23.54%	6.353%
5	5.964	790	800	822	rBV	256363	745170	15.95%	4.304%
6	6.769	921	932	952	rBV	624242	1591978	34.07%	9.194%
7	8.653	1234	1241	1258	rBV	1353643	2206000	47.21%	12.741%
8	9.214	1327	1333	1339	rBV2	38278	60372	1.29%	0.349%
9	9.427	1361	1368	1377	rBV2	141320	219475	4.70%	1.268%
10	10.055	1465	1471	1487	rBV	1519347	2061420	44.12%	11.906%
11	11.079	1633	1639	1655	rBV	1360335	1683740	36.04%	9.724%
12	12.018	1788	1793	1804	rBV	1795825	2173608	46.52%	12.554%




Sum of corrected areas: 17314610

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072425\
Data File : VX047124.D
Acq On : 24 Jul 2025 16:37
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072125W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

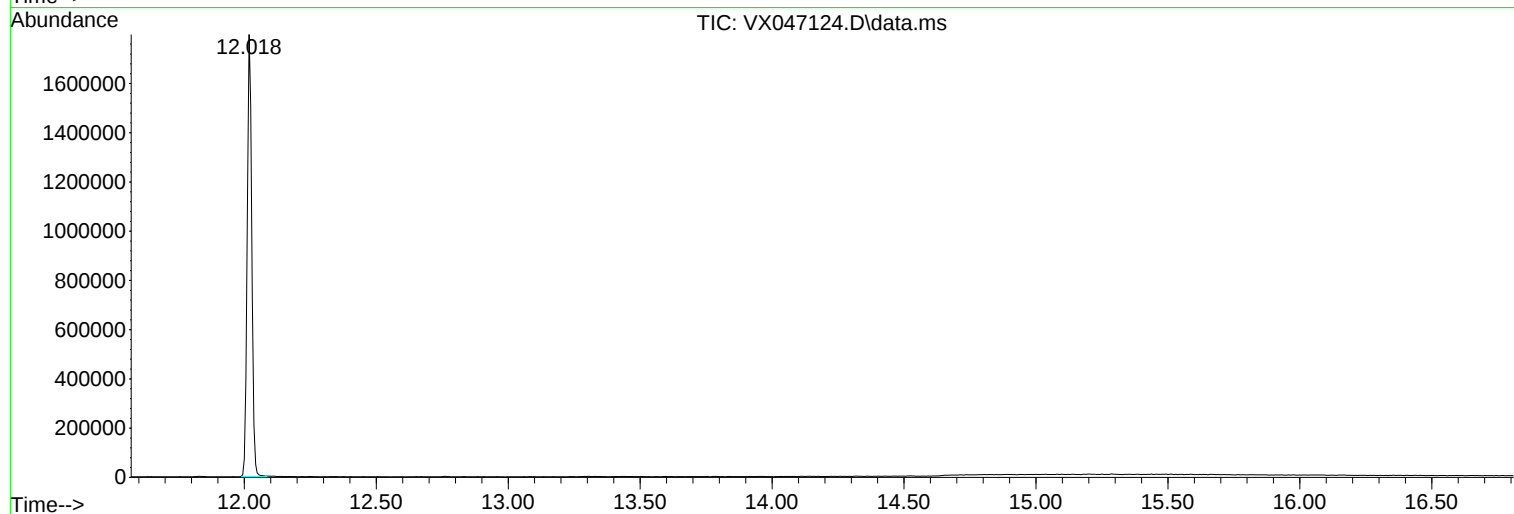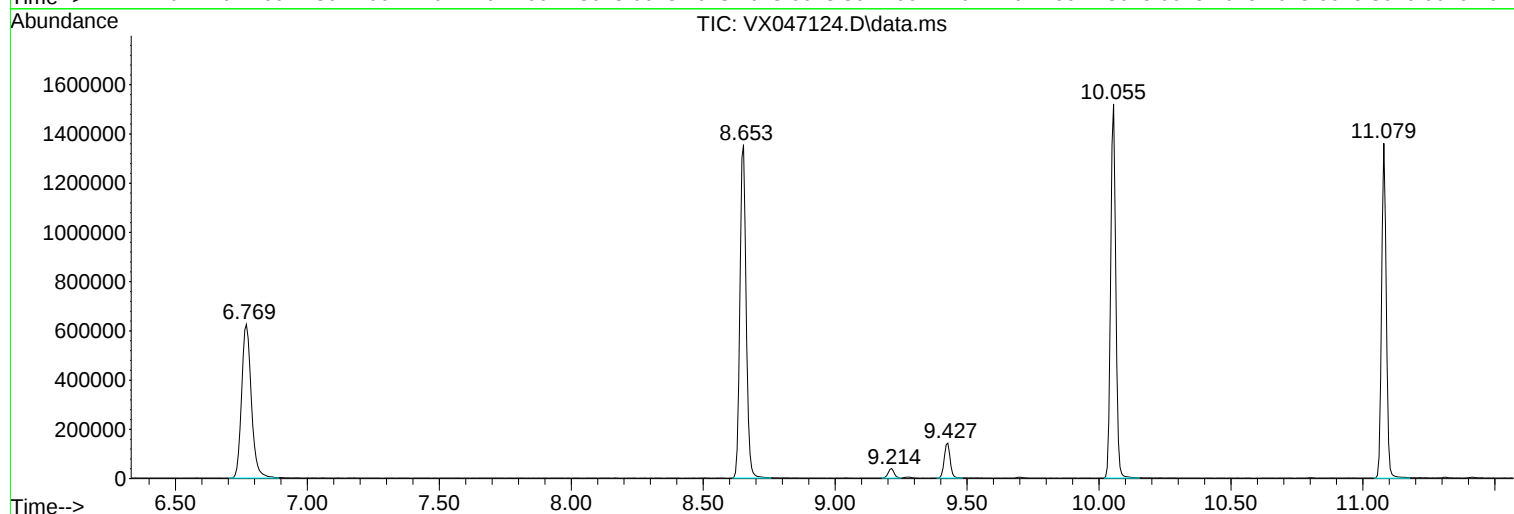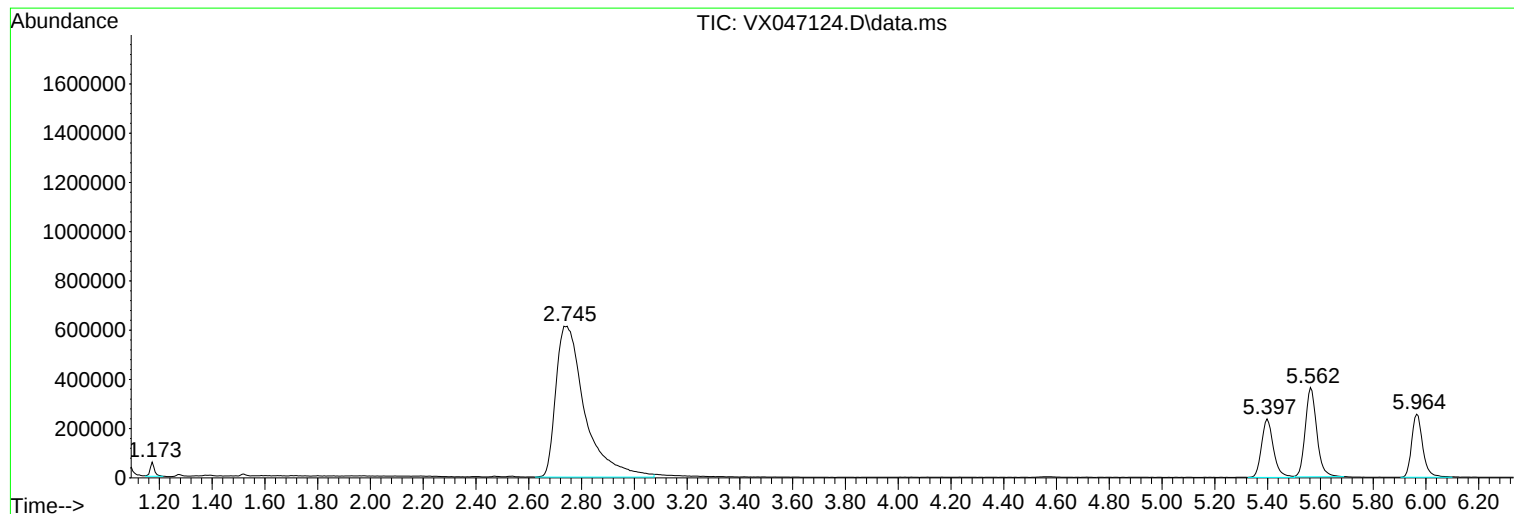

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072425\
Data File : VX047124.D
Acq On : 24 Jul 2025 16:37
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072125W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Methyl isocyanide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.745	212.38 ug/l	4672420	Pentafluorobenzene	5.562

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Methyl isocyanide	41	C2H3N	000593-75-9	56
2			Acetonitrile	41	C2H3N	000075-05-8	56
3			Propyne	40	C3H4	000074-99-7	4
4			Allene	40	C3H4	000463-49-0	1
5			Borane, trimethyl-	56	C3H9B	000593-90-8	1

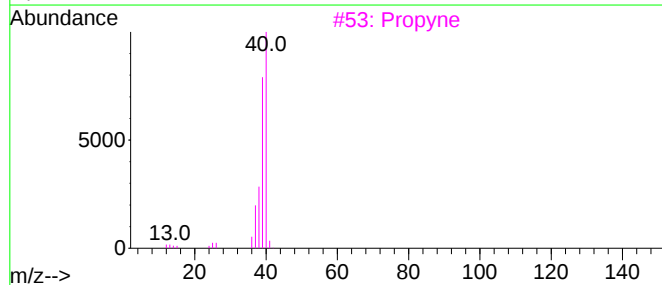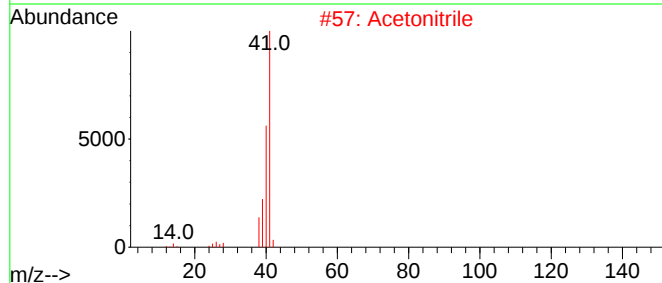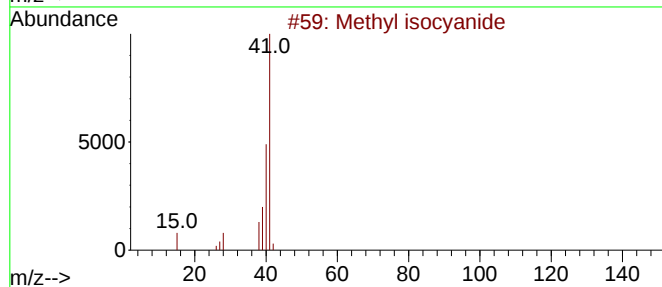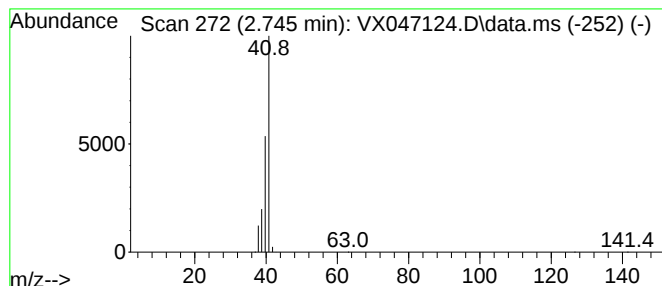

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072425\
Data File : VX047124.D
Acq On : 24 Jul 2025 16:37
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072125W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Methyl isocyanide	2.745	212.4	ug/l	4672420	1	5.562	1100020	50.0