

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX072518\
 Data File : VX003667.D
 Acq On : 25 Jul 2018 19:30
 Operator : JC/SP
 Sample : J4073-13
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE109D1-071618

Quant Time: Jul 27 15:03:27 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X072418W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jul 25 04:33:52 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	82416	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.87	114	129446	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	123179	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	78824	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.07	65	67221	55.06	ug/l	0.00
Spiked Amount	50.000		Recovery	=	110.12%	
35) Dibromofluoromethane	5.51	113	53444	50.50	ug/l	0.00
Spiked Amount	50.000		Recovery	=	101.00%	
50) Toluene-d8	8.72	98	235287	58.26	ug/l	0.00
Spiked Amount	50.000		Recovery	=	116.52%	
62) 4-Bromofluorobenzene	11.14	95	87196	59.20	ug/l	0.00
Spiked Amount	50.000		Recovery	=	118.40%	
Target Compounds						
44) Trichloroethene	7.22	130	25567	21.30	ug/l	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX072518\
 Data File : VX003667.D
 Acq On : 25 Jul 2018 19:30
 Operator : JC/SP
 Sample : J4073-13
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleID :
 RE109D1-071618

Quant Time: Jul 27 15:03:27 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X072418W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jul 25 04:33:52 2018
 Response via : Initial Calibration




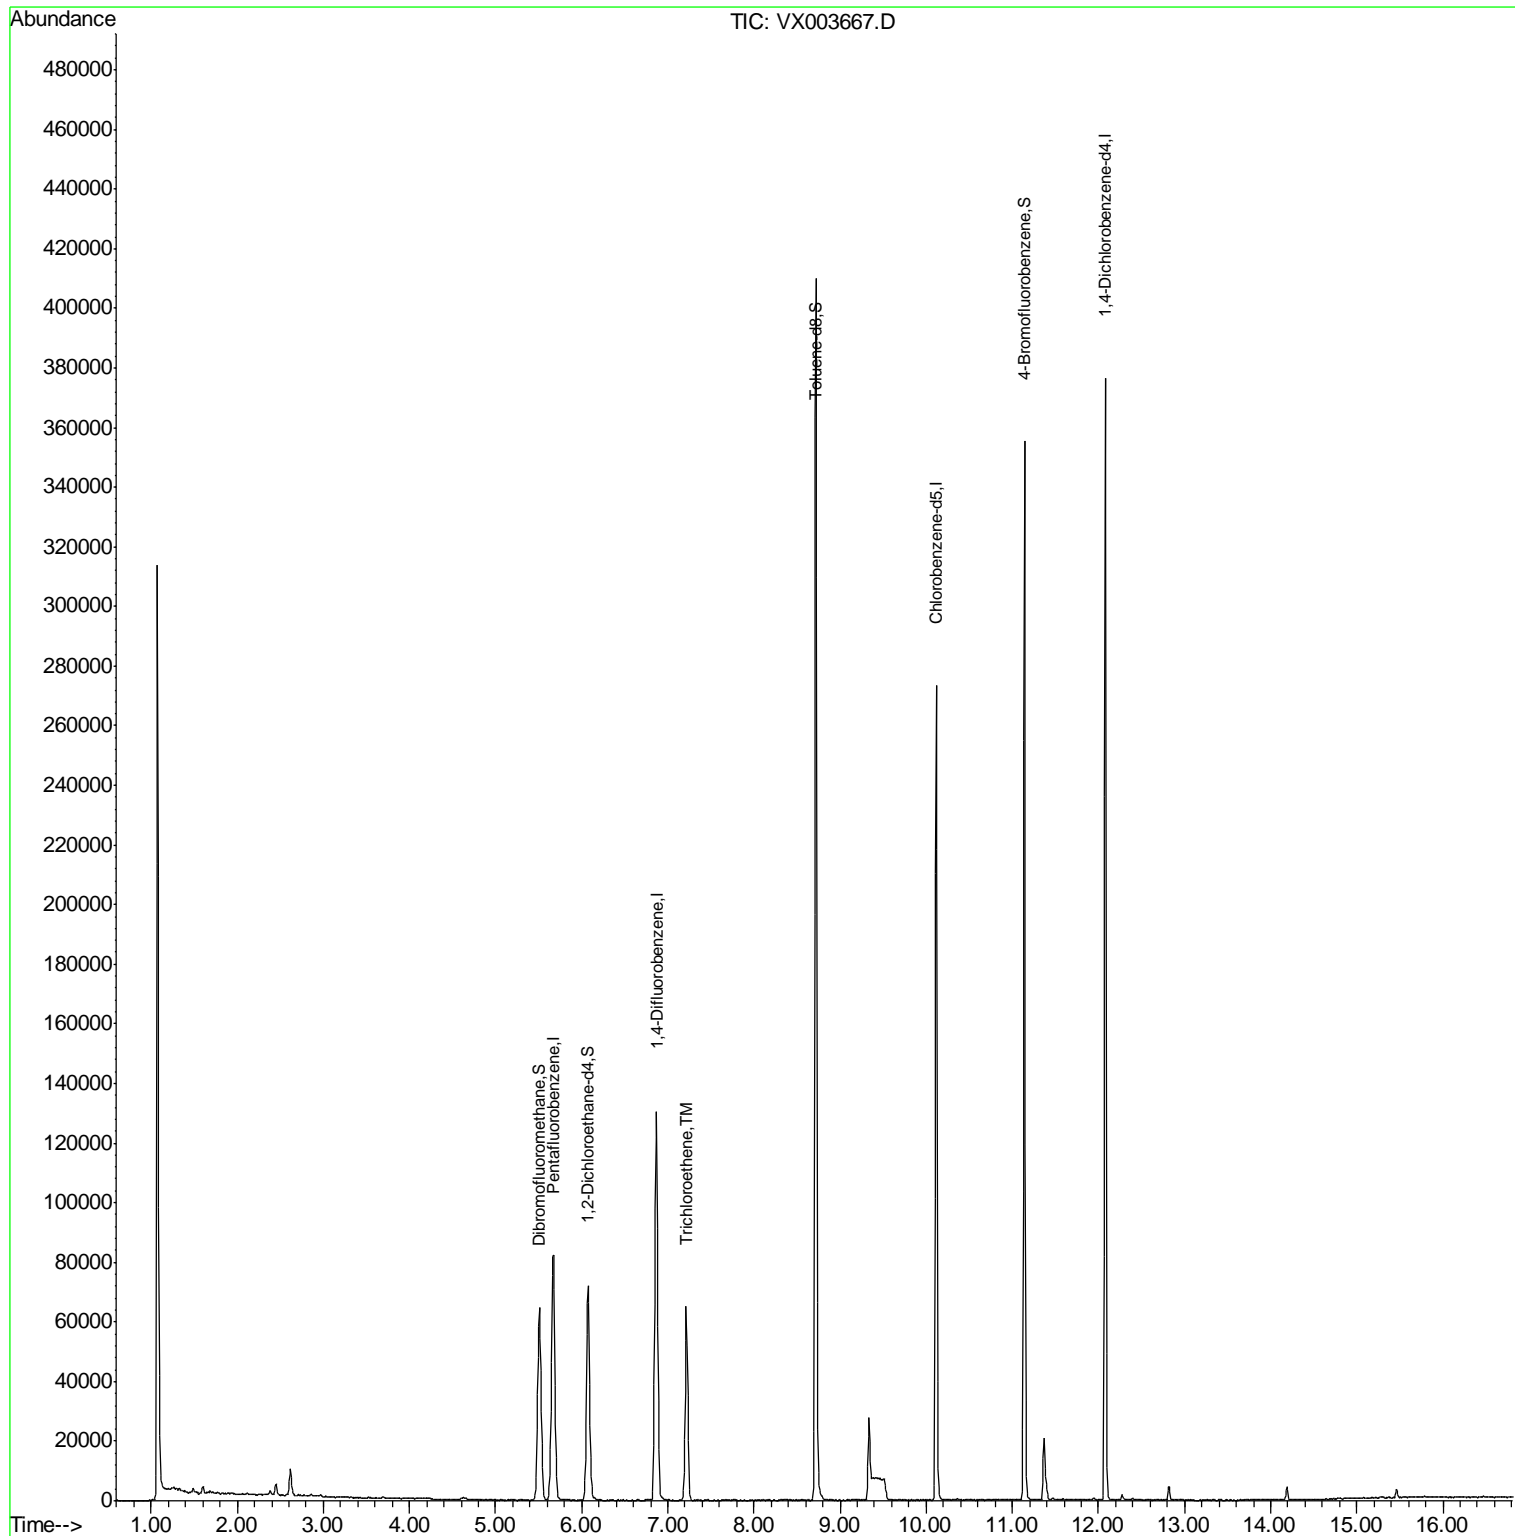


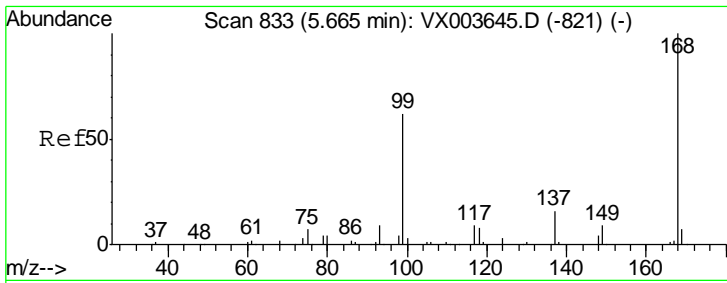

#1
 Pentafluorobenzene
 Concen: 50.00 ug/l
 RT: 5.67 min Scan# 834
 Delta R.T. 0.01 min
 Lab File: VX003667.D
 Acq: 25 Jul 2018 19:30




Instrument : MSVOA_X
 ClientSampleID : RE109D1-071618


Tgt Ion	Resp	Lower	Upper
168	100		
99	49.5	49.5	74.3#

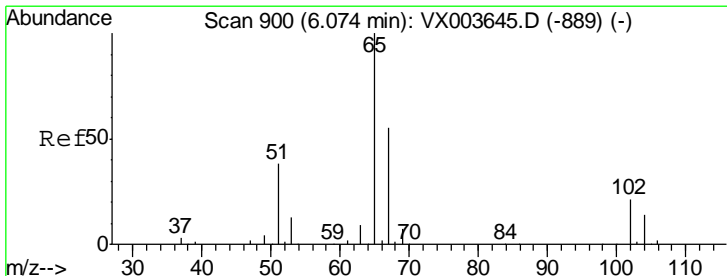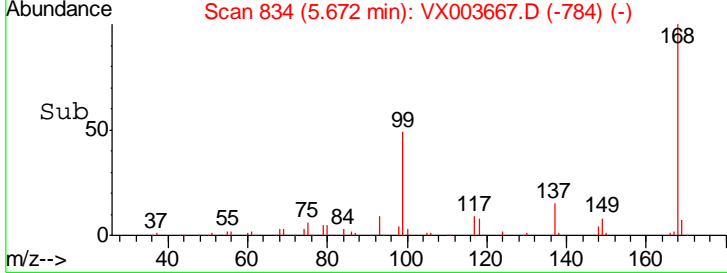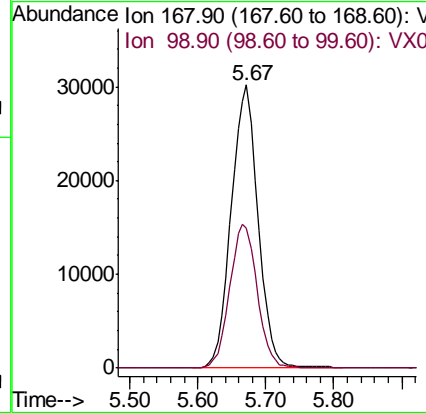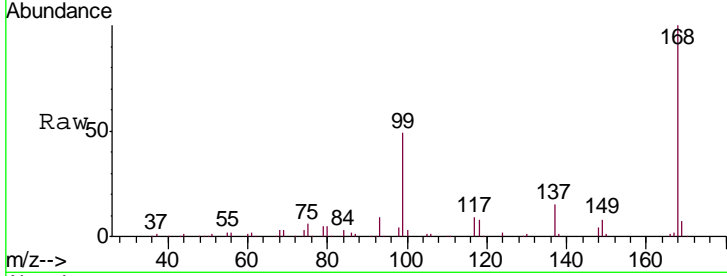

#33
 1,2-Dichloroethane-d4
 Concen: 55.06 ug/l
 RT: 6.07 min Scan# 900
 Delta R.T. 0.00 min
 Lab File: VX003667.D
 Acq: 25 Jul 2018 19:30

Tgt Ion	Resp	Lower	Upper
65	100		
67	53.1	0.0	107.8

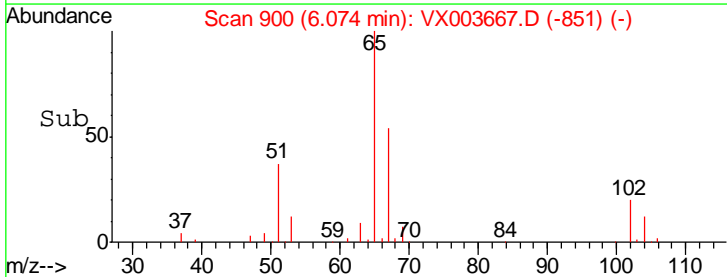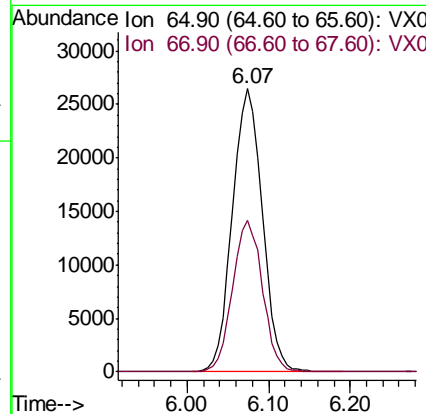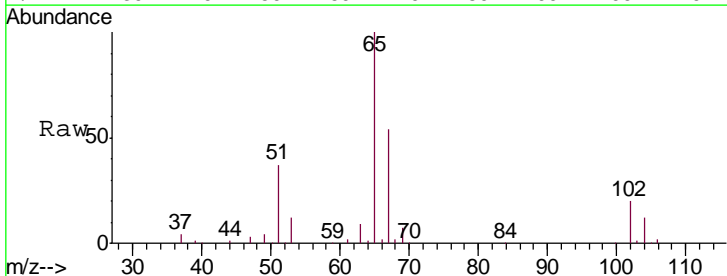


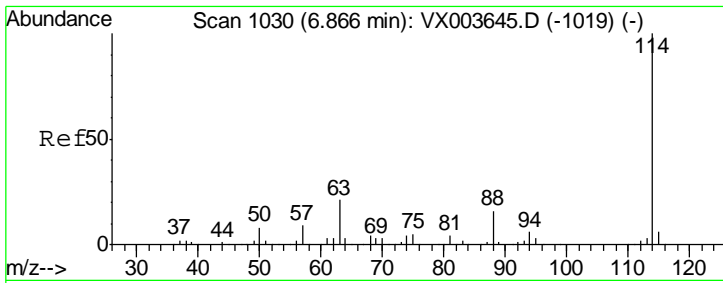




#34
 1,4-Difluorobenzene
 Concen: 50.00 ug/l
 RT: 6.87 min Scan# 1030
 Delta R.T. 0.00 min
 Lab File: VX003667.D
 Acq: 25 Jul 2018 19:30

Instrument : MSVOA_X
 ClientSampled : RE109D1-071618

Tgt Ion	Resp	Lower	Upper
114	129446		
63	20.8	0.0	41.0
88	15.5	0.0	31.8

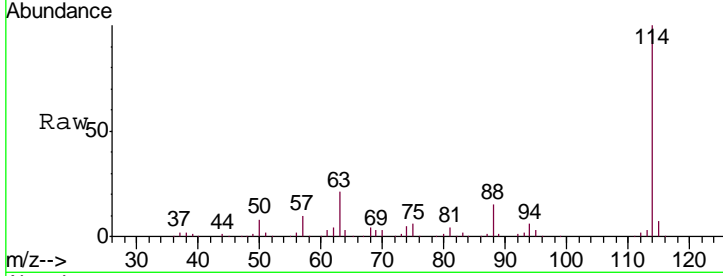


Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): VX0
 Ion 87.90 (87.60 to 88.60): VX0

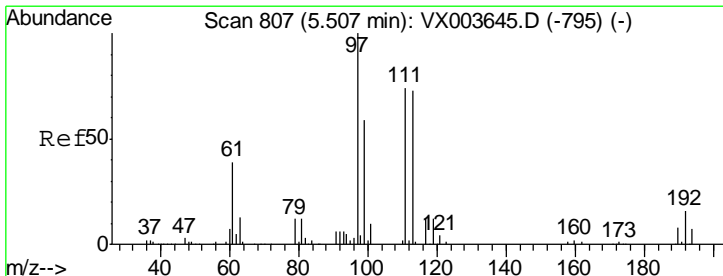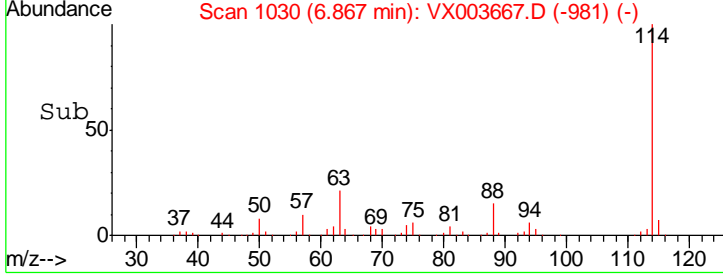
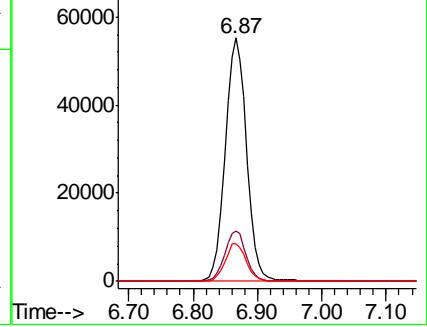



#35
 Dibromofluoromethane
 Concen: 50.50 ug/l
 RT: 5.51 min Scan# 807
 Delta R.T. 0.00 min
 Lab File: VX003667.D
 Acq: 25 Jul 2018 19:30

Tgt Ion	Resp	Lower	Upper
113	53444		
111	102.6	81.2	121.8
192	22.5	18.2	27.4

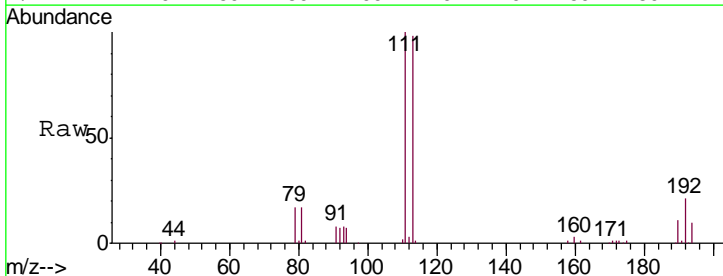

Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V



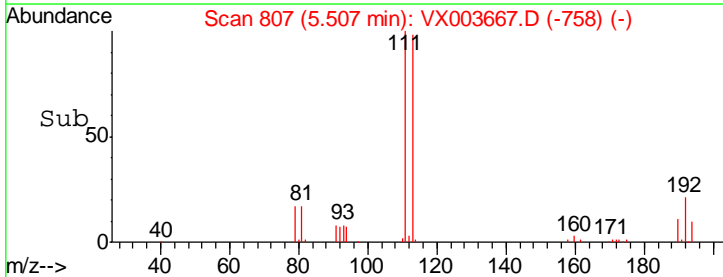
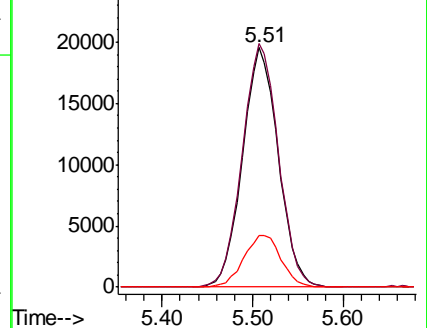


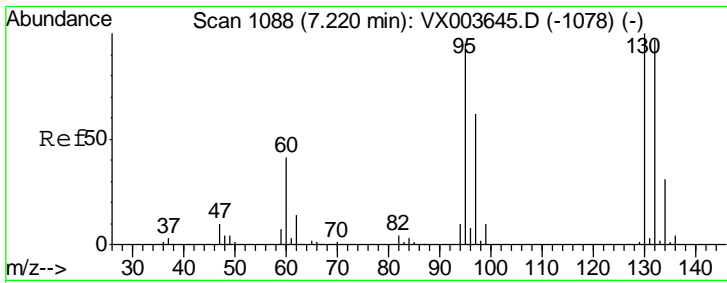

#44
 Trichloroethene
 Concen: 21.30 ug/l
 RT: 7.22 min Scan# 1088
 Delta R.T. 0.00 min
 Lab File: VX003667.D
 Acq: 25 Jul 2018 19:30




Instrument : MSVOA_X
 ClientSampled : RE109D1-071618


Tgt Ion	Resp	Lower	Upper
130	100		
95	86.1	0.0	190.0

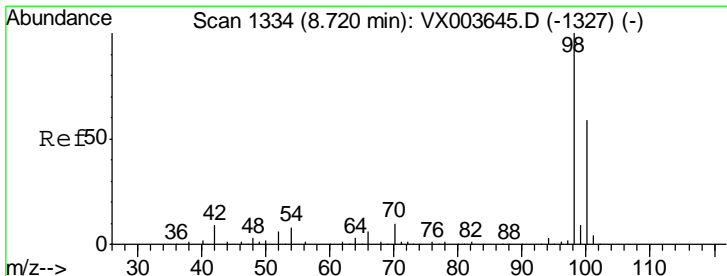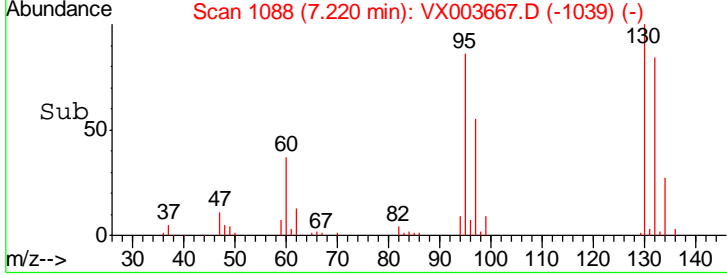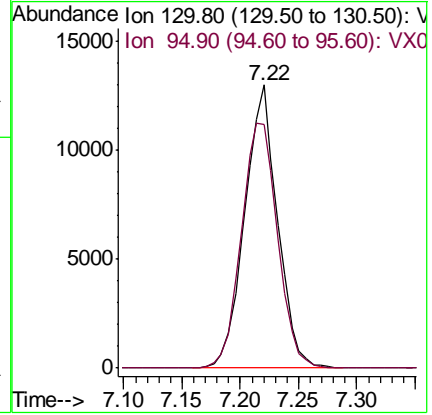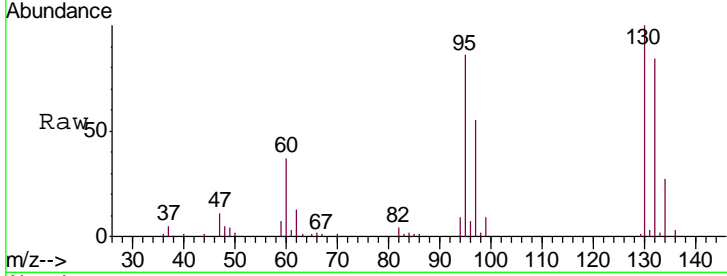

#50
 Toluene-d8
 Concen: 58.26 ug/l
 RT: 8.72 min Scan# 1334
 Delta R.T. 0.00 min
 Lab File: VX003667.D
 Acq: 25 Jul 2018 19:30

Tgt Ion	Resp	Lower	Upper
98	100		
100	63.6	50.9	76.3


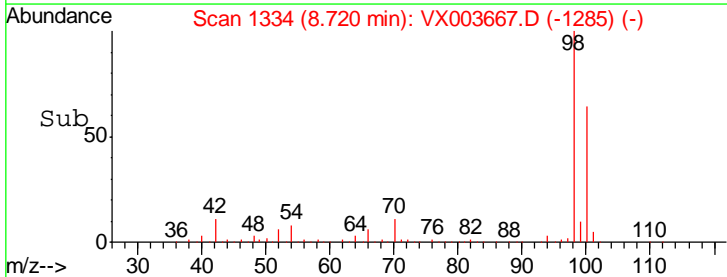
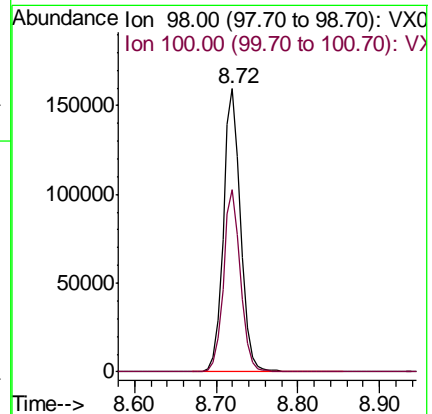
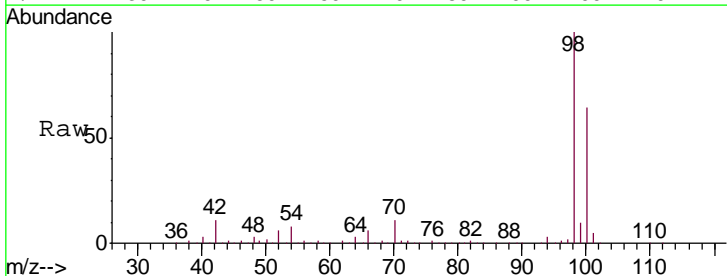


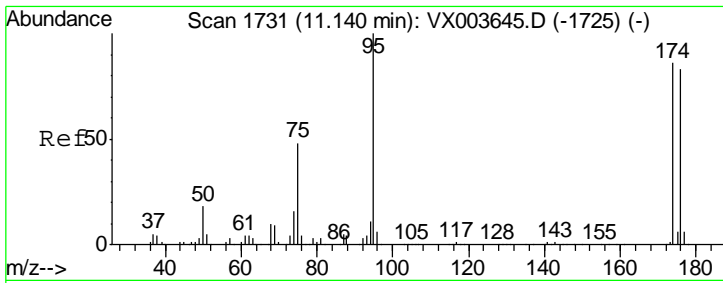

#62
 4-Bromofluorobenzene
 Concen: 59.20 ug/l
 RT: 11.14 min Scan# 1731
 Delta R.T. 0.00 min
 Lab File: VX003667.D
 Acq: 25 Jul 2018 19:30




Instrument : MSVOA_X
 ClientSampled : RE109D1-071618


Tgt Ion	Resp	Lower	Upper
95	87196		
174	89.6	0.0	179.0
176	86.9	0.0	173.0

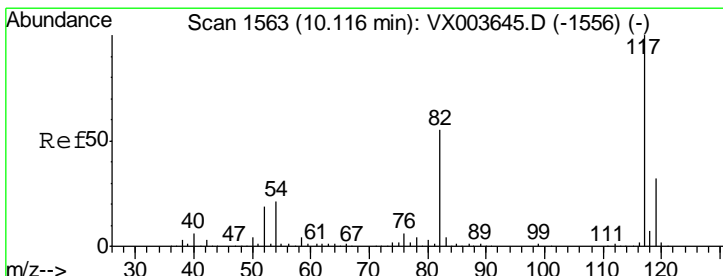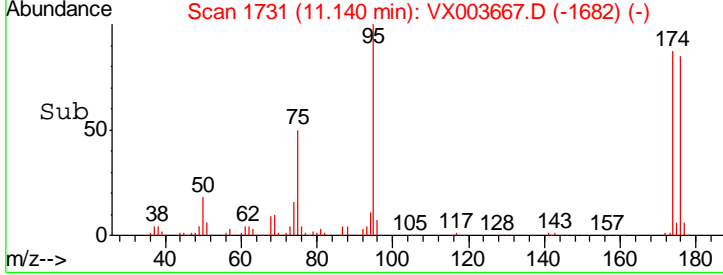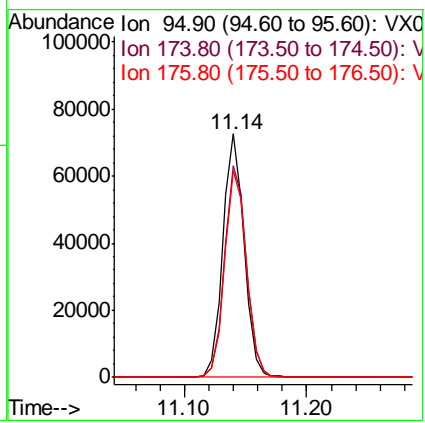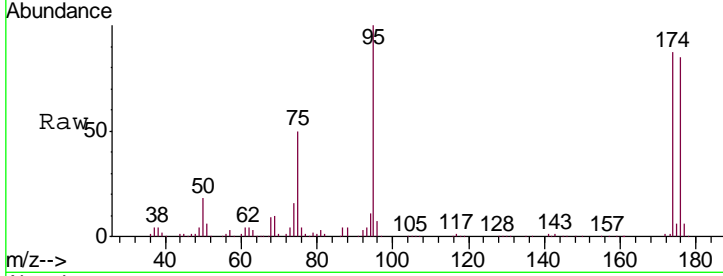

#63
 Chlorobenzene-d5
 Concen: 50.00 ug/l
 RT: 10.12 min Scan# 1563
 Delta R.T. 0.00 min
 Lab File: VX003667.D
 Acq: 25 Jul 2018 19:30

Tgt Ion	Resp	Lower	Upper
117	123179		
82	54.1	44.3	66.5
119	32.6	25.6	38.4

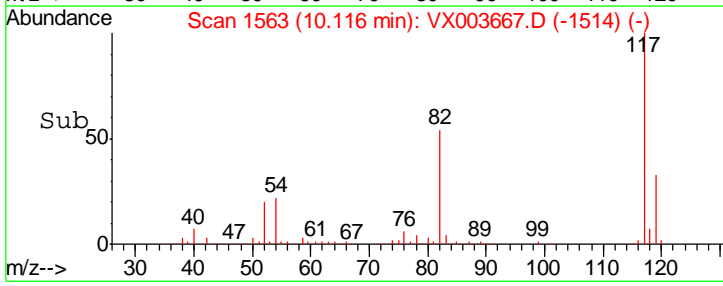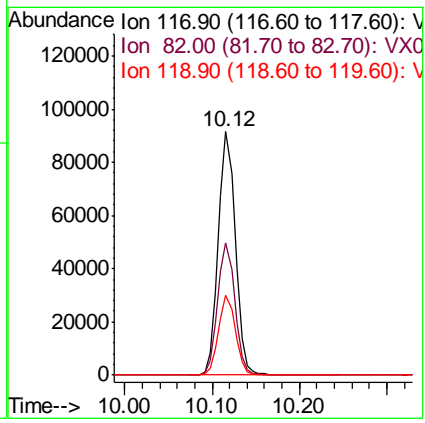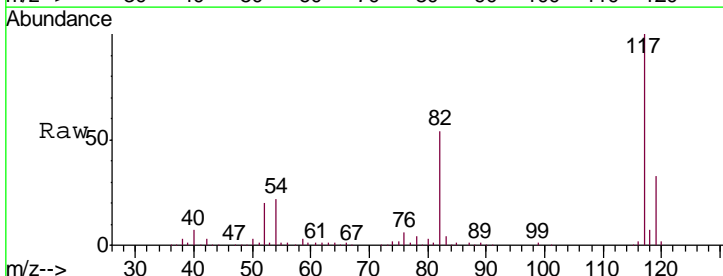

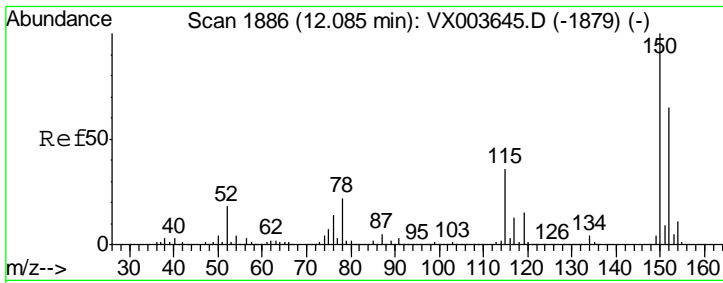

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.00 ug/l
 RT: 12.08 min Scan# 1885
 Delta R.T. -0.01 min
 Lab File: VX003667.D
 Acq: 25 Jul 2018 19:30

Instrument : MSVOA_X
 ClientSampleID : RE109D1-071618

Tot Ion	Resp	Lower	Upper
152	100		
115	55.8	40.0	119.9
150	156.9	0.0	348.4

