


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX072519\  
Data File : VX011063.D  
Acq On : 25 Jul 2019 08:22  
Operator : JC/SP  
Sample : BFB  
Misc : 5.0mL/MSVOA X/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampled :  
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X071619W.M  
Title : SW846 8260  
Last Update : Wed Jul 24 05:39:23 2019

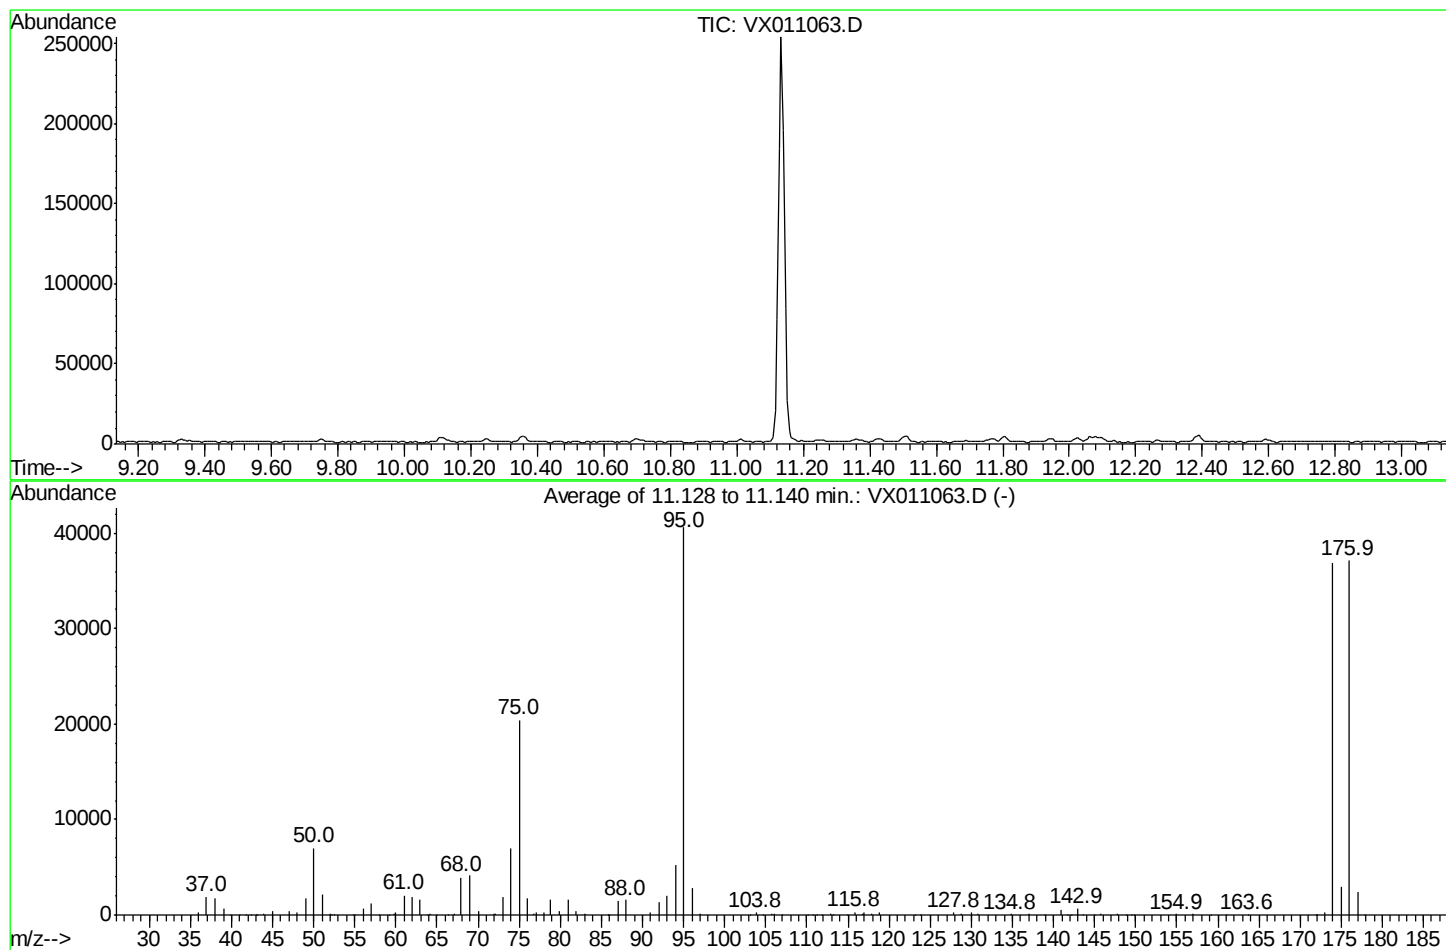

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1629

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 17.2      | 6982    | PASS             |
| 75          | 95           | 30           | 60           | 50.3      | 20442   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 40626   | PASS             |
| 96          | 95           | 5            | 9            | 7.0       | 2827    | PASS             |
| 173         | 174          | 0.00         | 2            | 0.9       | 336     | PASS             |
| 174         | 95           | 50           | 100          | 90.7      | 36850   | PASS             |
| 175         | 174          | 5            | 9            | 8.0       | 2958    | PASS             |
| 176         | 174          | 95           | 101          | 100.7     | 37112   | PASS             |
| 177         | 176          | 5            | 9            | 6.5       | 2426    | PASS             |