



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072523\
Data File : VX036641.D
Acq On : 25 Jul 2023 09:53
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072123W.M
Title : SW846 8260
Last Update : Fri Jul 21 12:14:12 2023

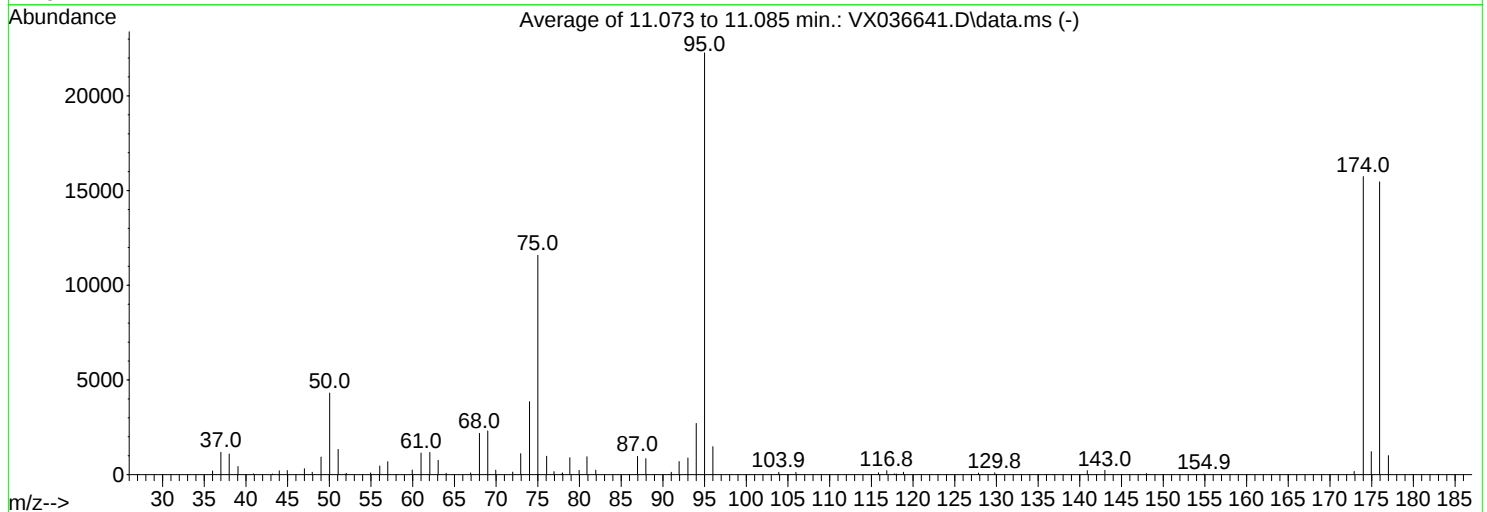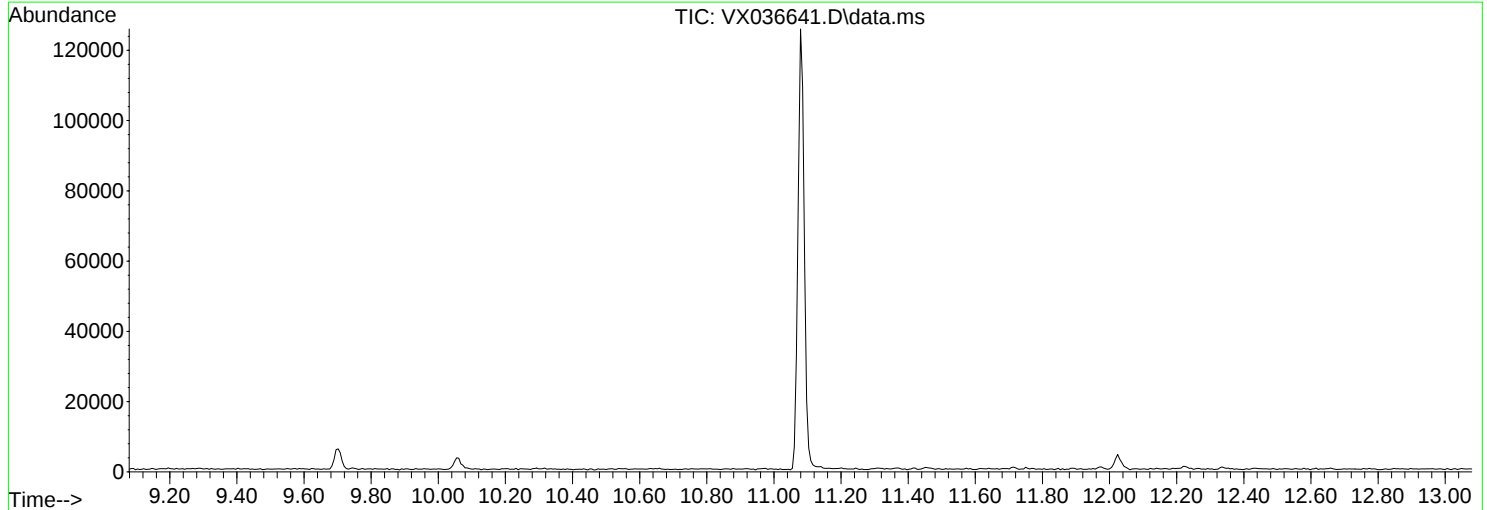

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	4308	PASS
75	95	30	60	52.0	11582	PASS
95	95	100	100	100.0	22272	PASS
96	95	5	9	6.6	1475	PASS
173	174	0.00	2	1.1	169	PASS
174	95	50	100	70.7	15742	PASS
175	174	5	9	7.7	1213	PASS
176	174	95	101	98.2	15459	PASS
177	176	5	9	6.5	1006	PASS