

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042529.D
 Acq On : 24 Jul 2024 20:05
 Operator : JC/MD
 Sample : VX0725MBL02
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jul 25 04:45:25 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jul 25 04:44:43 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	185708	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	166744	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	76856	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	37177	34.393	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	68.780%
7) Chloroethane-d5	1.648	69	26080	38.320	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	76.640%
11) 1,1-Dichloroethene-d2	2.300	65	20476	43.282	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	86.560%
21) 2-Butanone-d5	4.471	46	77235	99.151	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	99.150%
24) Chloroform-d	5.062	84	99680	45.864	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.720%
26) 1,2-Dichloroethane-d4	5.958	65	65209	50.832	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	101.660%
32) Benzene-d6	5.977	84	202840	47.063	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.120%
36) 1,2-Dichloropropane-d6	7.312	67	62298	48.031	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	96.060%
41) Toluene-d8	8.647	98	181589	45.212	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	90.420%
43) trans-1,3-Dichloroprop...	8.952	79	24201	43.172	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	86.340%
47) 2-Hexanone-d5	9.385	63	55379	94.062	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	94.060%
56) 1,1,2,2-Tetrachloroeth...	11.189	84	89019	46.423	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	92.840%
66) 1,2-Dichlorobenzene-d4	12.317	152	75410	50.516	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	101.040%
Target Compounds						
					Qvalue	
37) 1,2-Dichloropropane	7.306	63	6629	5.541	ug/L #	84
61) 1,2,3-Trichloropropane	12.024	75	7075	5.184	ug/L #	63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042529.D
Acq On : 24 Jul 2024 20:05
Operator : JC/MD
Sample : VX0725MBL02
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Jul 25 04:45:25 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jul 25 04:44:43 2024
Response via : Initial Calibration

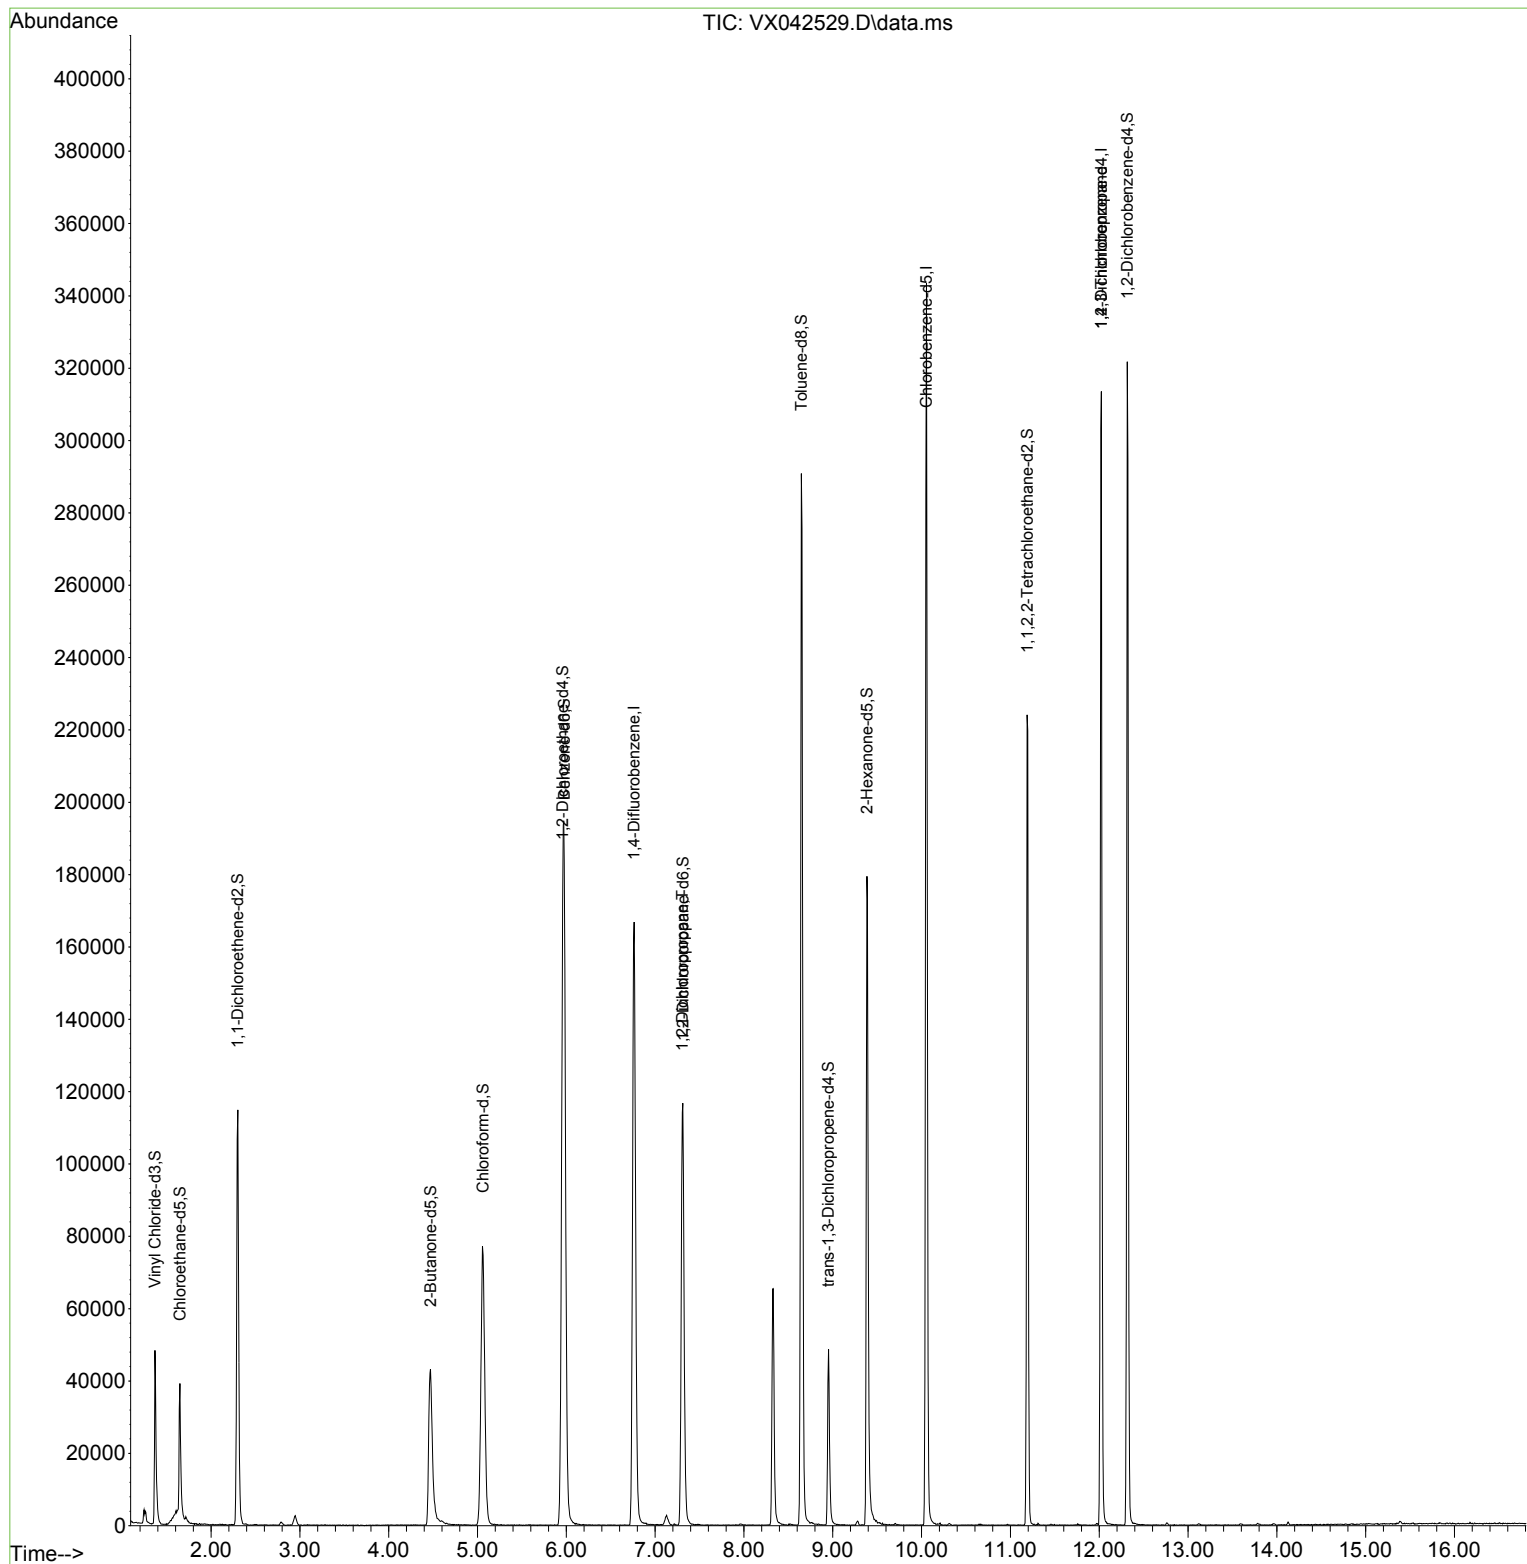

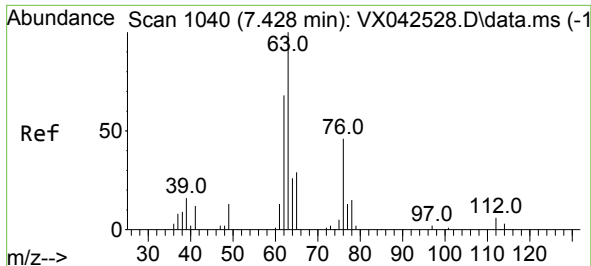

#37

1,2-Dichloropropane

Concen: 5.541 ug/L

RT: 7.306 min Scan# 1

Delta R.T. -0.122 min

Lab File: VX042529.D

Acq: 24 Jul 2024 20:05

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 63 Resp: 6629

Ion Ratio Lower Upper

63 100

112 0.0 4.3 6.5#

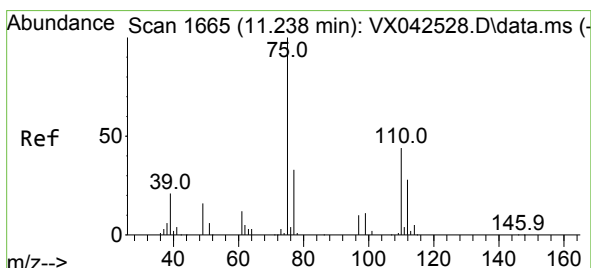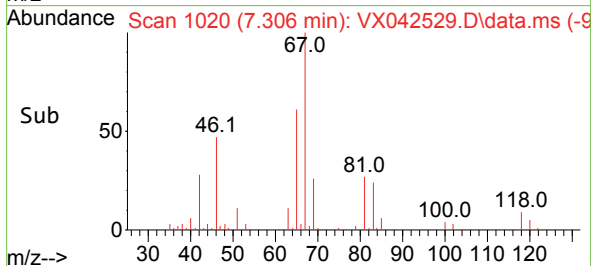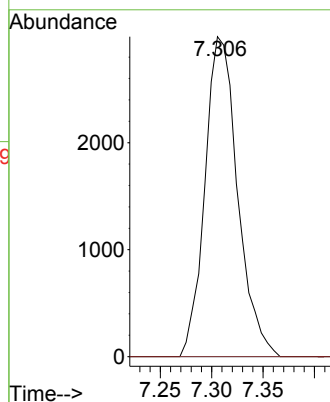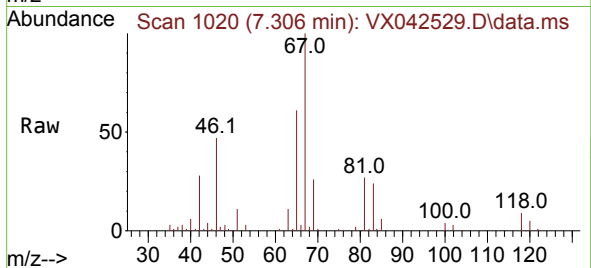

#61

1,2,3-Trichloropropane

Concen: 5.184 ug/L

RT: 12.024 min Scan# 1794

Delta R.T. 0.786 min

Lab File: VX042529.D

Acq: 24 Jul 2024 20:05

Tgt Ion: 75 Resp: 7075

Ion Ratio Lower Upper

75 100

77 32.7 25.8 38.8

110 2.8 35.4 53.0#

