

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042533.D
 Acq On : 24 Jul 2024 21:38
 Operator : JC/MD
 Sample : P3334-17 200X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jul 25 04:57:48 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jul 25 04:44:43 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	197642	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	176920	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	82791	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	26321	22.880	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	45.760%#
7) Chloroethane-d5	1.648	69	19045	26.293	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	52.580%#
11) 1,1-Dichloroethene-d2	2.294	65	14533	28.865	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	57.740%#
21) 2-Butanone-d5	4.465	46	67307	81.188	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	81.190%
24) Chloroform-d	5.056	84	80922	34.985	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	69.960%#
26) 1,2-Dichloroethane-d4	5.958	65	52308	38.313	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	76.620%
32) Benzene-d6	5.971	84	156876	34.305	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	68.600%#
36) 1,2-Dichloropropane-d6	7.306	67	51096	37.128	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	74.260%
41) Toluene-d8	8.647	98	135035	31.687	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	63.380%#
43) trans-1,3-Dichloroprop...	8.952	79	19164	32.220	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	64.440%
47) 2-Hexanone-d5	9.385	63	48937	78.339	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	78.340%
56) 1,1,2,2-Tetrachloroeth...	11.189	84	77740	38.210	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	76.420%
66) 1,2-Dichlorobenzene-d4	12.317	152	60825	37.825	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	75.640%#
Target Compounds						
					Qvalue	
37) 1,2-Dichloropropane	7.306	63	5704	4.493	ug/L #	84
61) 1,2,3-Trichloropropane	12.018	75	7614	5.179	ug/L #	63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042533.D
Acq On : 24 Jul 2024 21:38
Operator : JC/MD
Sample : P3334-17 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Jul 25 04:57:48 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jul 25 04:44:43 2024
Response via : Initial Calibration




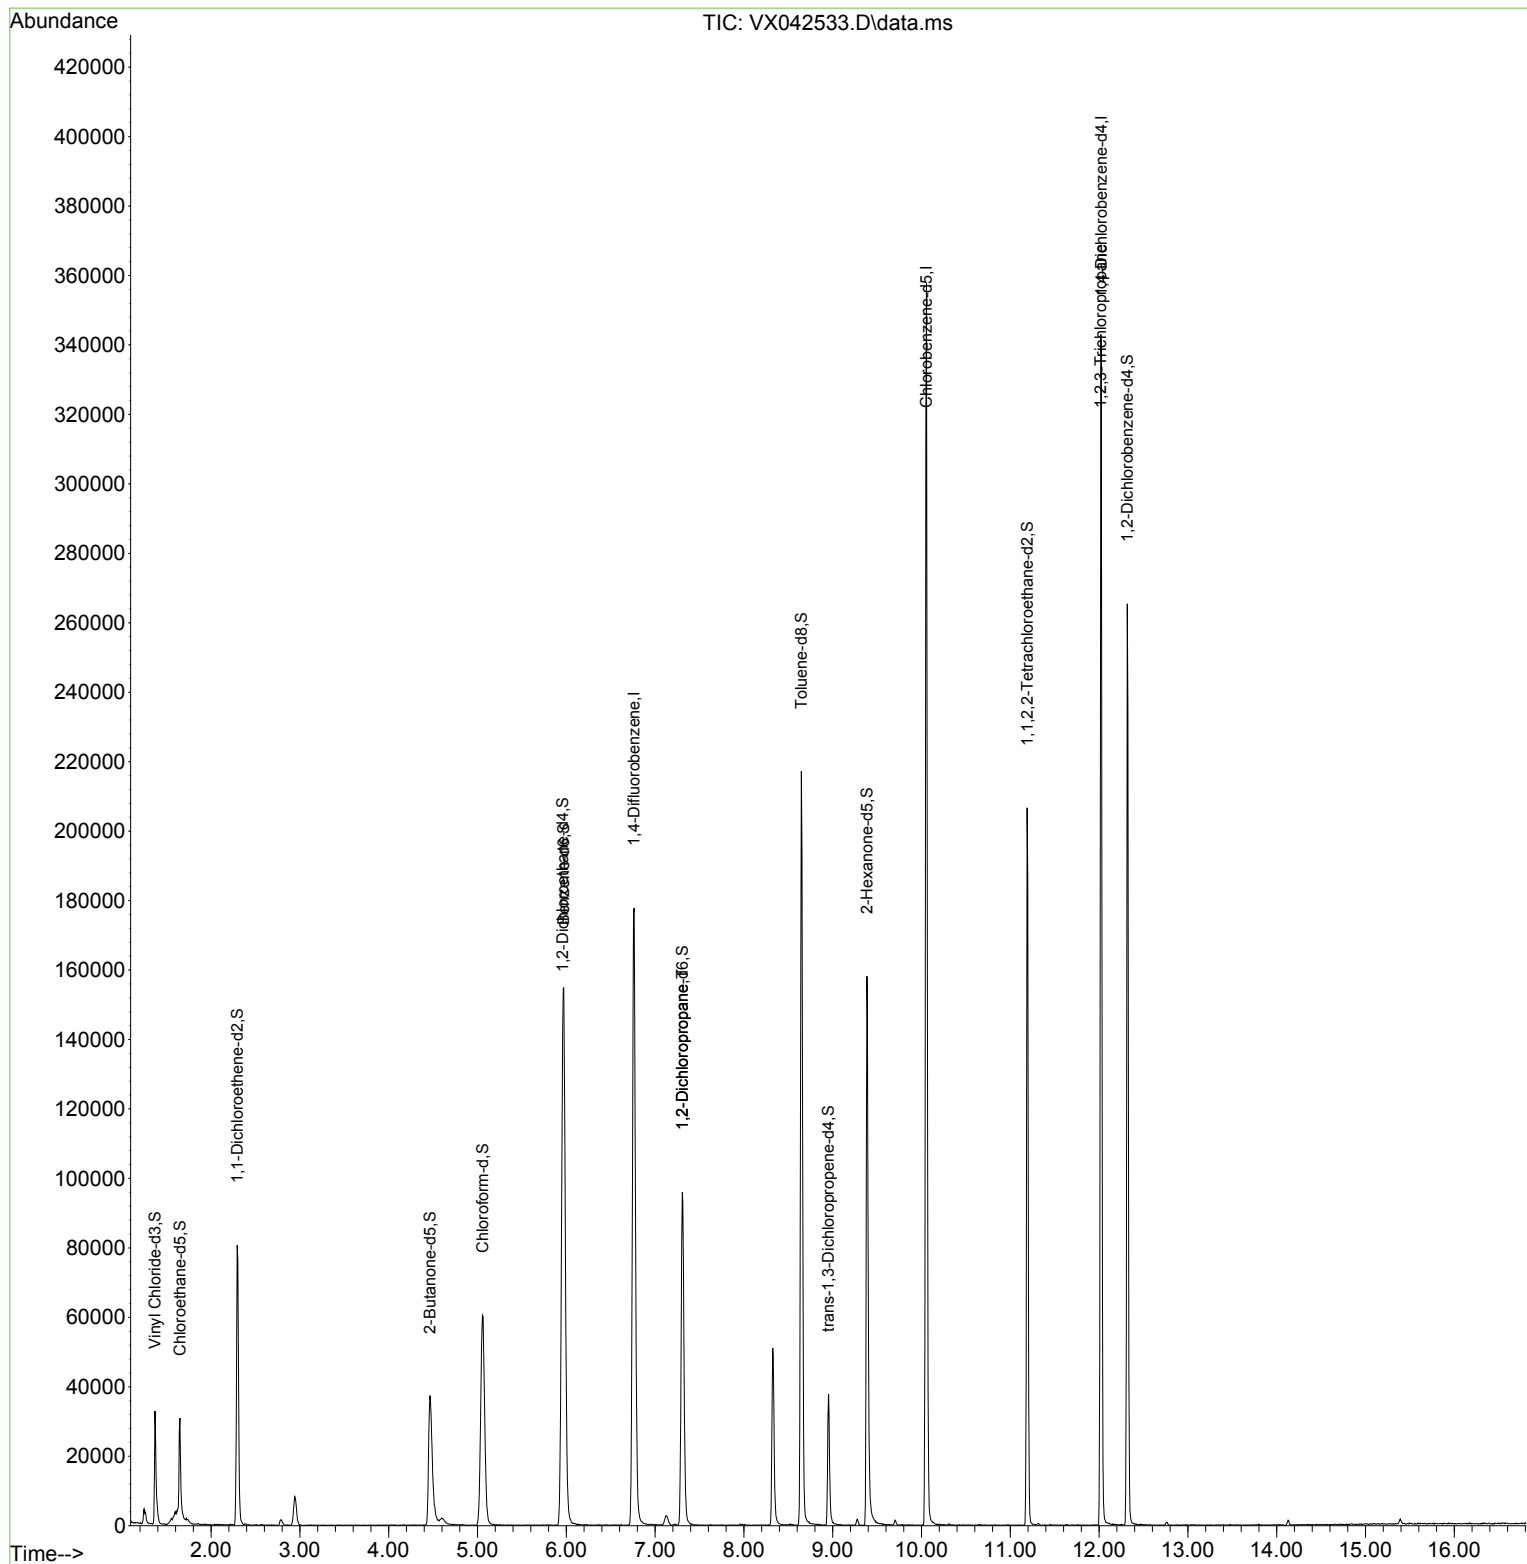


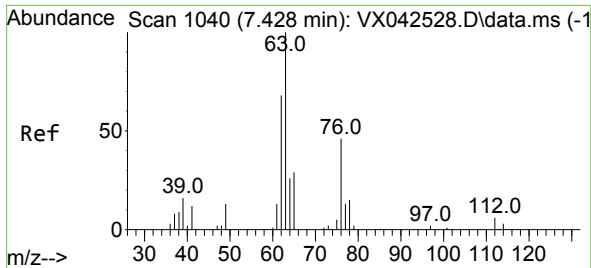

#37
1,2-Dichloropropane
Concen: 4.493 ug/L
RT: 7.306 min Scan# 11
Delta R.T. -0.122 min
Lab File: VX042533.D
Acq: 24 Jul 2024 21:38

Instrument :
MSVOA_X
ClientSampleId :

Tgt Ion: 63 Resp: 5704
Ion Ratio Lower Upper
63 100
112 0.0 4.3 6.5#

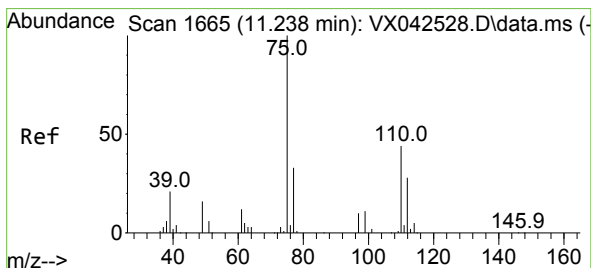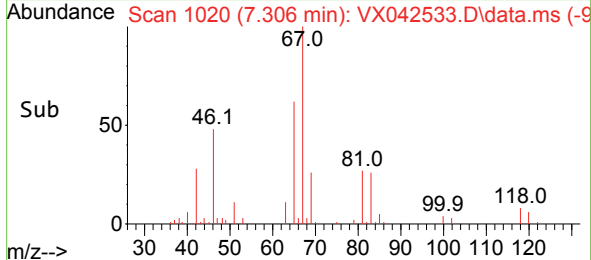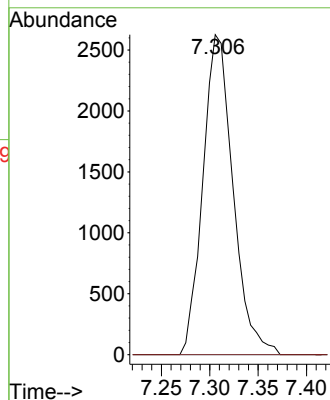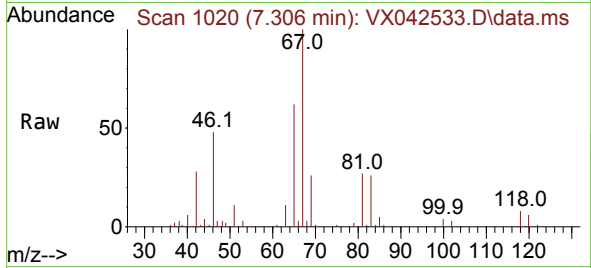

#61
1,2,3-Trichloropropane
Concen: 5.179 ug/L
RT: 12.018 min Scan# 1793
Delta R.T. 0.780 min
Lab File: VX042533.D
Acq: 24 Jul 2024 21:38

Tgt Ion: 75 Resp: 7614
Ion Ratio Lower Upper
75 100
77 33.0 25.8 38.8
110 2.7 35.4 53.0#

