

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042542.D
 Acq On : 25 Jul 2024 01:06
 Operator : JC/MD
 Sample : P3344-09 100X
 Misc : 5.03g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jul 25 04:59:56 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jul 25 04:44:43 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	193392	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	176333	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	82227	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	25242	22.424	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	44.840%#
7) Chloroethane-d5	1.648	69	19542	27.572	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	55.140%#
11) 1,1-Dichloroethene-d2	2.300	65	14149	28.720	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	57.440%#
21) 2-Butanone-d5	4.465	46	69824	86.075	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	86.080%
24) Chloroform-d	5.062	84	80898	35.743	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	71.480%
26) 1,2-Dichloroethane-d4	5.952	65	53252	39.862	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	79.720%
32) Benzene-d6	5.970	84	156326	34.298	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	68.600%#
36) 1,2-Dichloropropane-d6	7.306	67	51274	37.382	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	74.760%
41) Toluene-d8	8.647	98	137100	32.279	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	64.560%#
43) trans-1,3-Dichloroprop...	8.952	79	18496	31.201	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	62.400%
47) 2-Hexanone-d5	9.384	63	49300	79.183	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	79.180%
56) 1,1,2,2-Tetrachloroeth...	11.189	84	79723	39.315	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	78.620%
66) 1,2-Dichlorobenzene-d4	12.317	152	61436	38.467	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	76.940%#
Target Compounds						
61) 1,2,3-Trichloropropane	12.018	75	7510	5.143	ug/L	Qvalue # 62


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042542.D
Acq On : 25 Jul 2024 01:06
Operator : JC/MD
Sample : P3344-09 100X
Misc : 5.03g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :


Quant Time: Jul 25 04:59:56 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jul 25 04:44:43 2024
Response via : Initial Calibration

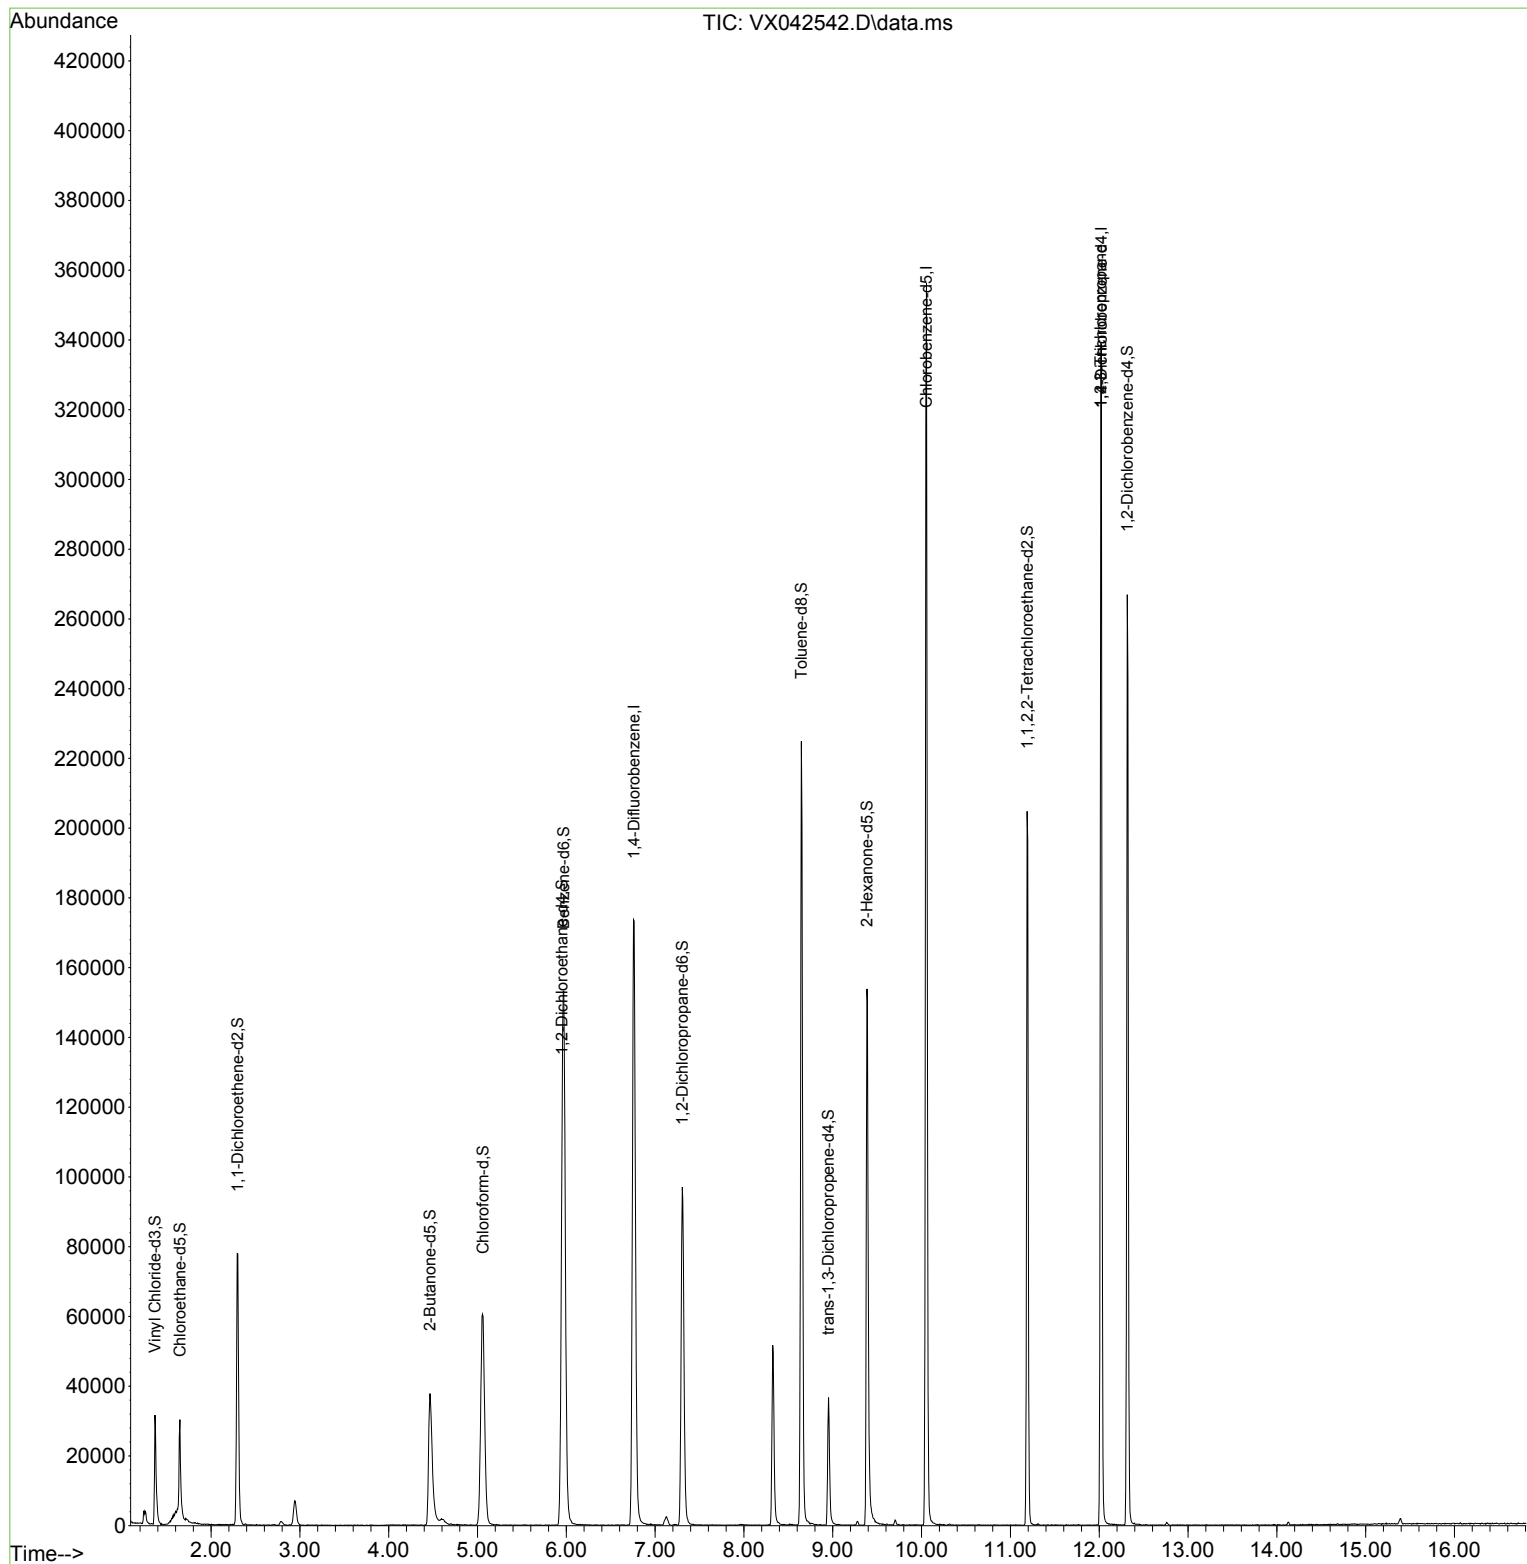

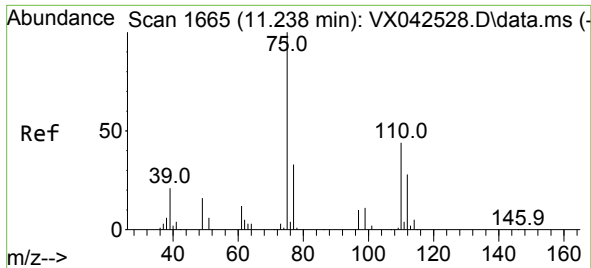

#61
 1,2,3-Trichloropropane
 Concen: 5.143 ug/L
 RT: 12.018 min Scan# 11
 Delta R.T. 0.780 min
 Lab File: VX042542.D
 Acq: 25 Jul 2024 01:06

Instrument :
 MSVOA_X
 ClientSampleId :

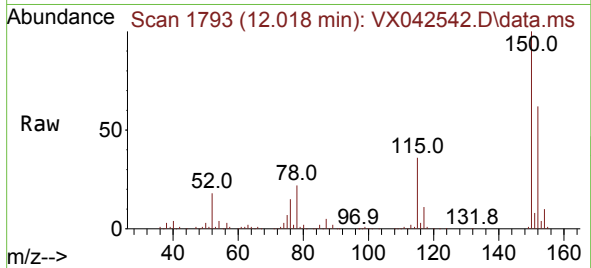

Tgt Ion:	75	Resp:	7510
Ion	Ratio	Lower	Upper
75	100		
77	34.4	25.8	38.8
110	3.6	35.4	53.0#

