

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042506.D
 Acq On : 24 Jul 2024 10:50
 Operator : JC/MD
 Sample : P3298-06MEDL 1000X
 Misc : 5.52g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BHB26MEDL

Quant Time: Jul 25 01:40:54 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jul 25 01:37:54 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	166748	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	149276	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	71204	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	24236	24.971	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	49.940%#		
7) Chloroethane-d5	1.648	69	19043	31.162	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	62.320%#		
11) 1,1-Dichloroethene-d2	2.300	65	15411	36.280	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	72.560%		
21) 2-Butanone-d5	4.465	46	67335	96.270	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	96.270%		
24) Chloroform-d	5.056	84	83964	43.025	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	86.060%		
26) 1,2-Dichloroethane-d4	5.952	65	54053	46.927	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	93.860%		
32) Benzene-d6	5.970	84	166677	43.198	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	86.400%		
36) 1,2-Dichloropropane-d6	7.312	67	51988	44.772	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	89.540%		
41) Toluene-d8	8.647	98	148603	41.329	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	82.660%		
43) trans-1,3-Dichloroprop...	8.952	79	20976	41.798	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	83.600%		
47) 2-Hexanone-d5	9.384	63	49051	93.063	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	93.060%		
56) 1,1,2,2-Tetrachloroeth...	11.189	84	78953	45.992	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	91.980%		
66) 1,2-Dichlorobenzene-d4	12.317	152	66336	47.965	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	95.920%		
Target Compounds						Qvalue
46) Tetrachloroethene	9.275	164	75423	73.691	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042506.D
Acq On : 24 Jul 2024 10:50
Operator : JC/MD
Sample : P3298-06MEDL 1000X
Misc : 5.52g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BHB26MEDL


Quant Time: Jul 25 01:40:54 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jul 25 01:37:54 2024
Response via : Initial Calibration

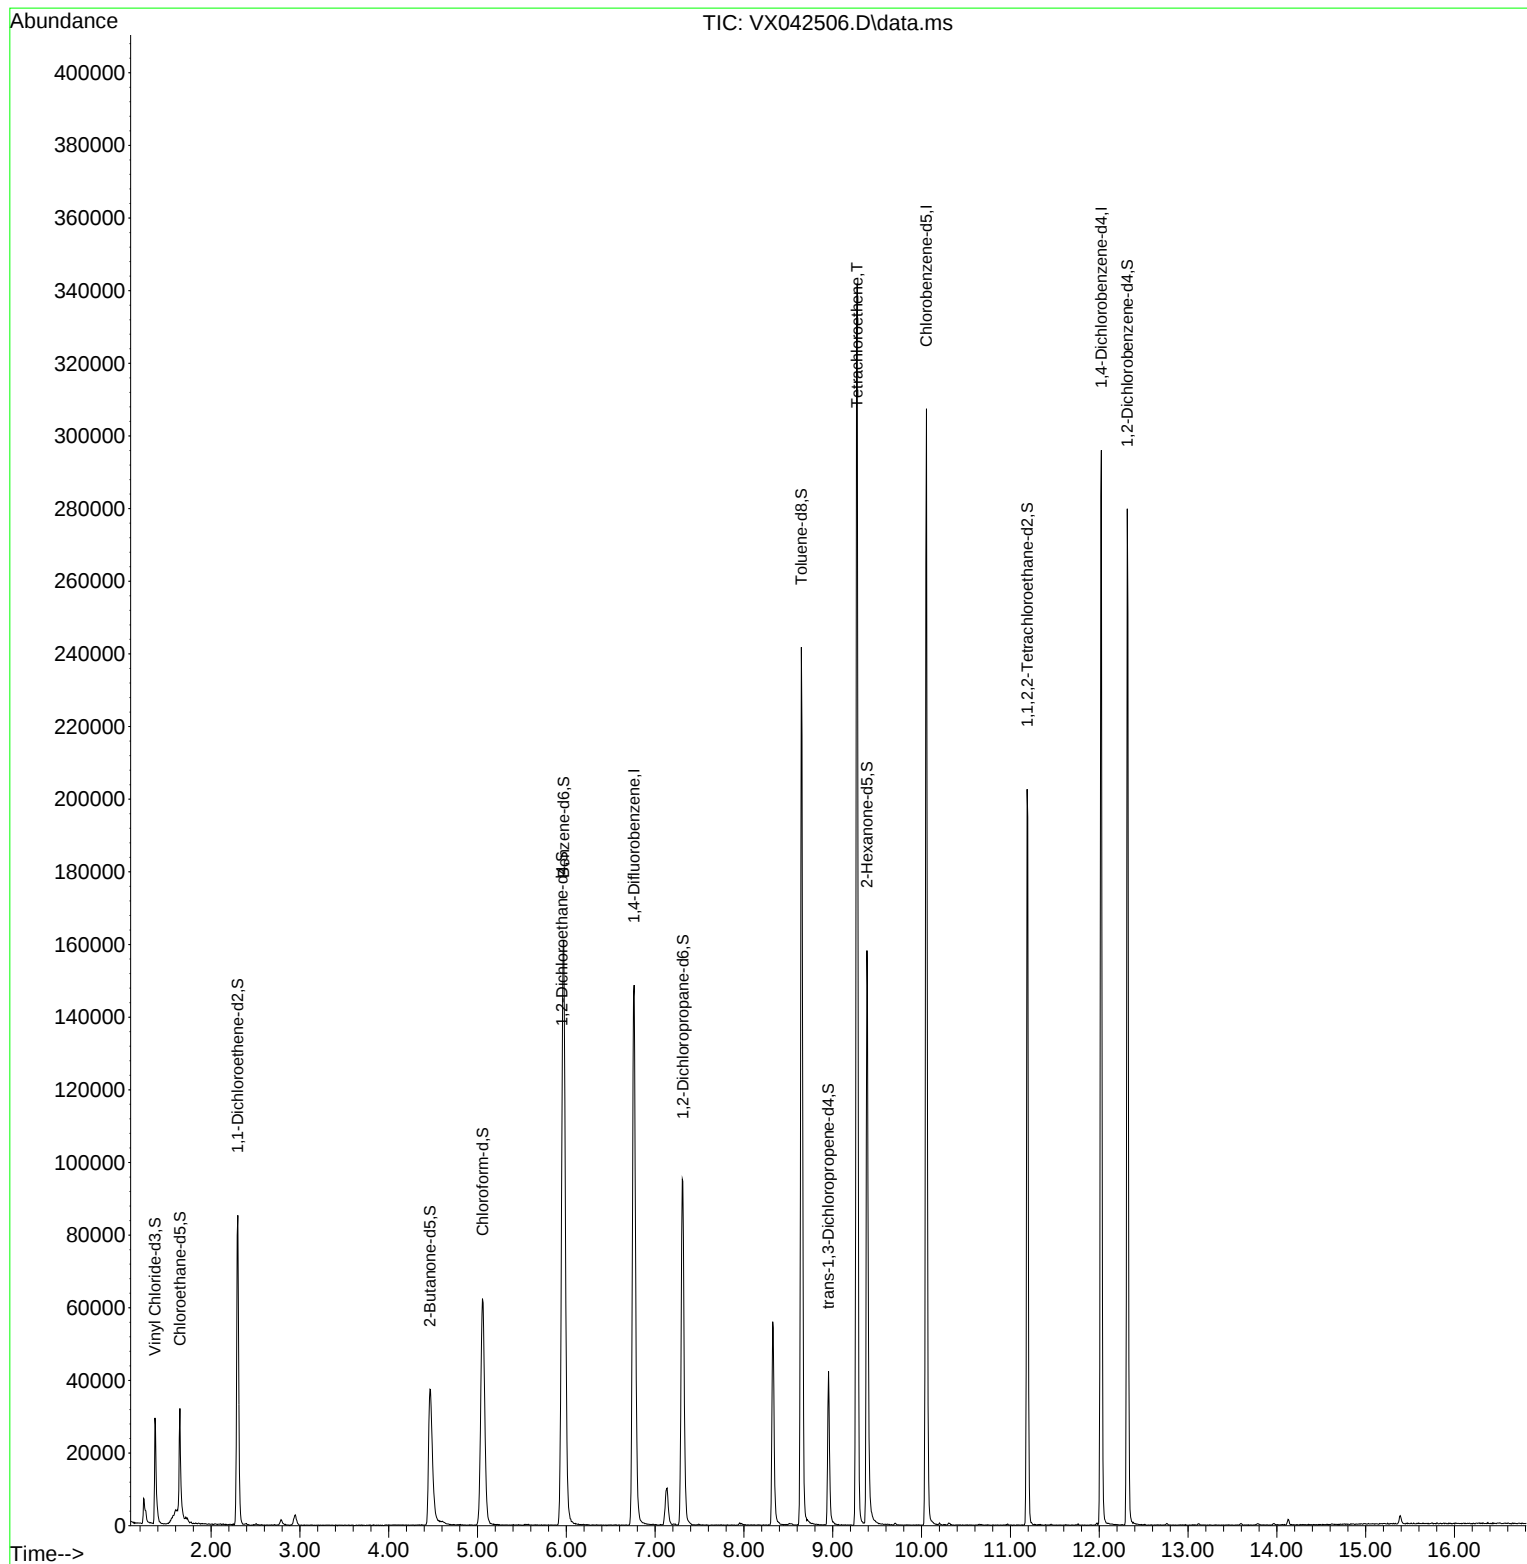

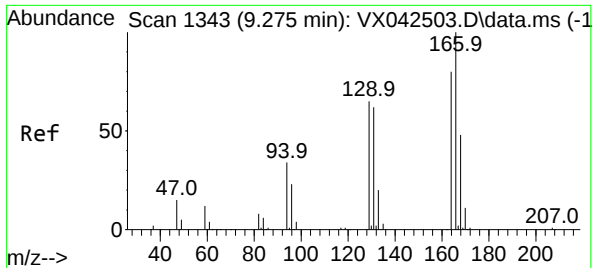

#46
Tetrachloroethene
Concen: 73.691 ug/L
RT: 9.275 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX042506.D
Acq: 24 Jul 2024 10:50

Instrument :
MSVOA_X
ClientSampleId :
BHB26MEDL

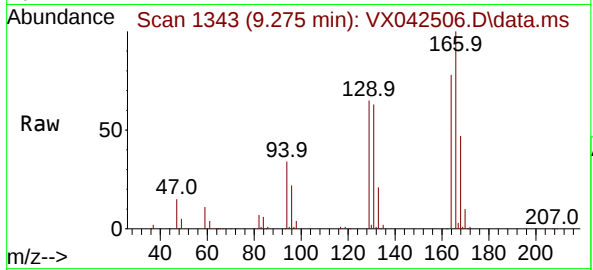

Tgt Ion:164	Resp:	75423
Ion	Ratio	Lower Upper
164	100	
129	82.8	58.6 108.8
131	81.4	57.9 107.5
166	128.2	91.8 170.4

