

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042504.D
 Acq On : 24 Jul 2024 10:04
 Operator : JC/MD
 Sample : VX0725MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK693

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M

Title : VOC Analysis

Signal : TIC: VX042504.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	22	26	33	rBV	6556	9671	1.45%	0.189%
2	1.368	42	46	57	rVB	58322	64588	9.66%	1.264%
3	1.666	90	95	111	rVB	38745	60525	9.05%	1.185%
4	2.203	181	183	185	rBV	237	229	0.03%	0.004%
5	2.306	193	200	209	rBV	133742	210998	31.57%	4.130%
6	2.441	220	222	225	rVB2	185	194	0.03%	0.004%
7	2.508	229	233	239	rBV	655	1222	0.18%	0.024%
8	2.617	250	251	252	rBV	143	67	0.01%	0.001%
9	2.703	262	265	268	rVB2	249	324	0.05%	0.006%
10	2.733	268	270	274	rBV	184	263	0.04%	0.005%
11	2.782	274	278	286	rVB3	906	1881	0.28%	0.037%
12	2.843	286	288	290	rBV3	179	190	0.03%	0.004%
13	2.867	290	292	293	rBV3	185	94	0.01%	0.002%
14	2.934	300	303	305	rBV3	417	637	0.10%	0.012%
15	3.087	327	328	332	rVB3	320	351	0.05%	0.007%
16	3.123	332	334	340	rVB2	225	289	0.04%	0.006%
17	3.184	342	344	345	rVB	107	70	0.01%	0.001%
18	3.203	345	347	348	rBV2	120	97	0.01%	0.002%
19	3.233	351	352	353	rBV	127	52	0.01%	0.001%
20	3.367	372	374	376	rBV2	130	125	0.02%	0.002%
21	3.440	384	386	387	rBV	105	60	0.01%	0.001%
22	3.459	387	389	394	rVV2	147	168	0.03%	0.003%
23	3.562	405	406	407	rBV2	129	70	0.01%	0.001%
24	3.581	407	409	413	rVV	186	193	0.03%	0.004%
25	3.629	416	417	419	rVB	79	35	0.01%	0.001%
26	3.666	421	423	424	rBV	162	146	0.02%	0.003%
27	3.757	434	438	441	rBV2	179	340	0.05%	0.007%
28	3.824	447	449	452	rVB2	116	125	0.02%	0.002%
29	3.849	452	453	454	rBV2	162	68	0.01%	0.001%
30	3.952	468	470	471	rBV	83	53	0.01%	0.001%
31	4.038	481	484	485	rBV2	167	188	0.03%	0.004%
32	4.373	537	539	542	rBV2	107	111	0.02%	0.002%
33	4.452	544	552	568	rBV	50464	148112	22.16%	2.899%
34	5.056	638	651	669	rBV	88643	269009	40.25%	5.266%
35	5.397	700	707	710	rBV2	420	924	0.14%	0.018%
36	5.623	743	744	745	rBV	138	58	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042504.D
 Acq On : 24 Jul 2024 10:04
 Operator : JC/MD
 Sample : VX0725MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK693

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

37	5.708	755	758	760	rVB	129	173	0.03%	0.003%
38	5.733	760	762	764	rBV	152	132	0.02%	0.003%
39	5.787	769	771	772	rBV	115	89	0.01%	0.002%
40	5.885	785	787	788	rBV	153	90	0.01%	0.002%
41	5.964	788	800	815	rBV2	224662	668426	100.00%	13.084%
42	6.275	848	851	852	rBV	103	104	0.02%	0.002%
43	6.379	866	868	871	rVB	135	169	0.03%	0.003%
44	6.428	875	876	878	rBV	150	122	0.02%	0.002%
45	6.543	894	895	897	rBV	139	123	0.02%	0.002%
46	6.757	921	930	946	rBV	182519	432178	64.66%	8.459%
47	6.897	952	953	955	rVB	380	150	0.02%	0.003%
48	7.129	983	991	1001	rBV4	7466	17612	2.63%	0.345%
49	7.305	1012	1020	1036	rBV	134467	297433	44.50%	5.822%
50	7.616	1070	1071	1073	rBV	134	101	0.02%	0.002%
51	7.671	1078	1080	1083	rVB	198	174	0.03%	0.003%
52	7.708	1083	1086	1087	rBV	160	135	0.02%	0.003%
53	7.744	1091	1092	1093	rBV	112	49	0.01%	0.001%
54	7.952	1123	1126	1127	rBV2	460	519	0.08%	0.010%
55	8.141	1156	1157	1160	rVB	148	105	0.02%	0.002%
56	8.324	1181	1187	1202	rBV	86317	145002	21.69%	2.838%
57	8.519	1215	1219	1225	rBV4	404	760	0.11%	0.015%
58	8.647	1234	1240	1259	rBV	359280	552550	82.66%	10.816%
59	8.952	1285	1290	1309	rBV	61154	94699	14.17%	1.854%
60	9.214	1332	1333	1334	rBV	242	123	0.02%	0.002%
61	9.275	1339	1343	1349	rVB2	1710	2559	0.38%	0.050%
62	9.384	1356	1361	1381	rBV	222443	324168	48.50%	6.345%
63	9.744	1418	1420	1421	rBV	158	76	0.01%	0.001%
64	9.872	1440	1441	1442	rBV	159	76	0.01%	0.001%
65	9.994	1459	1461	1463	rBV	146	178	0.03%	0.003%
66	10.055	1465	1471	1488	rBV	357630	501950	75.09%	9.825%
67	10.195	1493	1494	1502	rVB2	635	883	0.13%	0.017%
68	10.311	1509	1513	1520	rVB2	889	1352	0.20%	0.026%
69	10.512	1544	1546	1548	rBV	132	117	0.02%	0.002%
70	10.659	1564	1570	1575	rBV2	583	1247	0.19%	0.024%
71	10.762	1584	1587	1588	rBV	149	173	0.03%	0.003%
72	10.963	1616	1620	1625	rVB2	664	1019	0.15%	0.020%
73	11.006	1625	1627	1628	rBV	158	113	0.02%	0.002%
74	11.189	1652	1657	1666	rBV	269461	342424	51.23%	6.703%
75	11.317	1676	1678	1682	rVB2	564	544	0.08%	0.011%
76	11.451	1698	1700	1704	rVB2	561	701	0.10%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042504.D
 Acq On : 24 Jul 2024 10:04
 Operator : JC/MD
 Sample : VX0725MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK693

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

77	11.543	1713	1715	1716	rBV	135	127	0.02%	0.002%
78	11.610	1724	1726	1727	rBV	121	71	0.01%	0.001%
79	11.713	1742	1743	1744	rBV	151	80	0.01%	0.002%
80	11.762	1746	1751	1755	rVB	549	881	0.13%	0.017%
81	11.872	1767	1769	1772	rVB	148	111	0.02%	0.002%
82	11.969	1782	1785	1788	rBV2	1180	1567	0.23%	0.031%
83	12.018	1788	1793	1802	rVV	351436	452994	67.77%	8.867%
84	12.317	1837	1842	1855	rBV	368046	475268	71.10%	9.303%
85	12.701	1903	1905	1907	rBV2	136	133	0.02%	0.003%
86	12.762	1911	1915	1921	rVB2	690	1083	0.16%	0.021%
87	12.957	1945	1947	1948	rBV	137	107	0.02%	0.002%
88	13.115	1969	1973	1978	rVB2	1414	1837	0.27%	0.036%
89	13.408	2019	2021	2022	rBV	116	83	0.01%	0.002%
90	13.591	2047	2051	2058	rVB2	2447	3299	0.49%	0.065%
91	13.780	2077	2082	2092	rVB	3785	5629	0.84%	0.110%
92	13.963	2108	2112	2116	rBV2	2567	3320	0.50%	0.065%
93	14.024	2121	2122	2124	rBV	237	187	0.03%	0.004%
94	14.127	2135	2139	2144	rBV2	1102	1518	0.23%	0.030%
95	14.213	2149	2153	2155	rBV3	259	410	0.06%	0.008%



Sum of corrected areas: 5108830

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042504.D
Acq On : 24 Jul 2024 10:04
Operator : JC/MD
Sample : VX0725MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK693

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

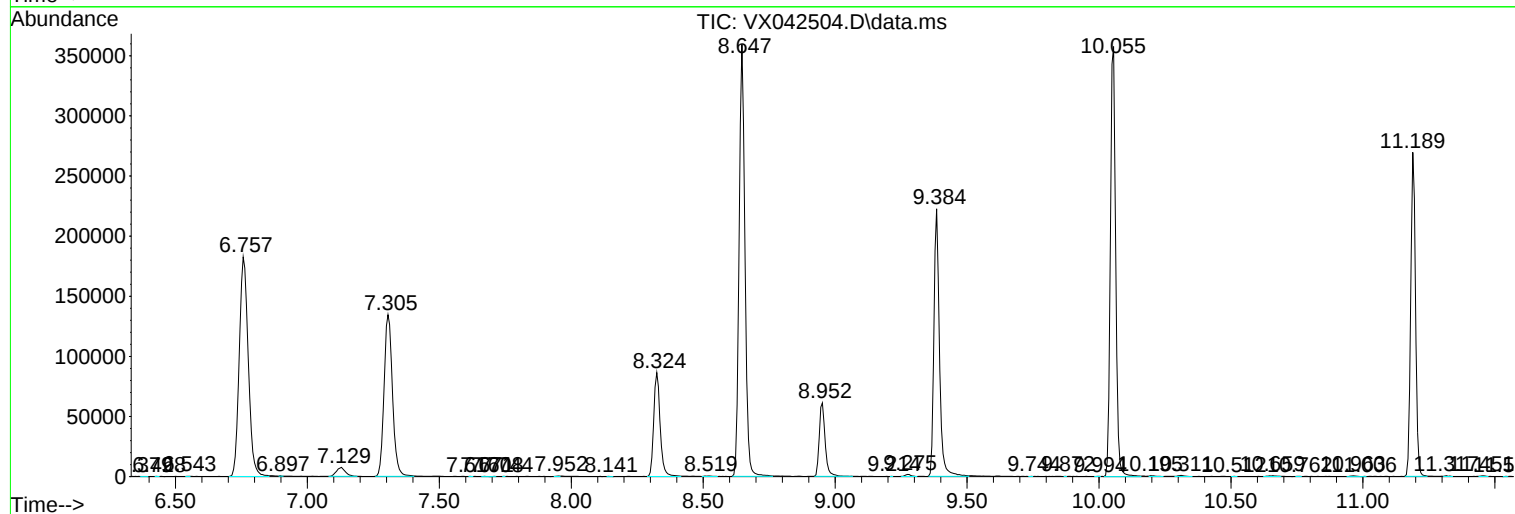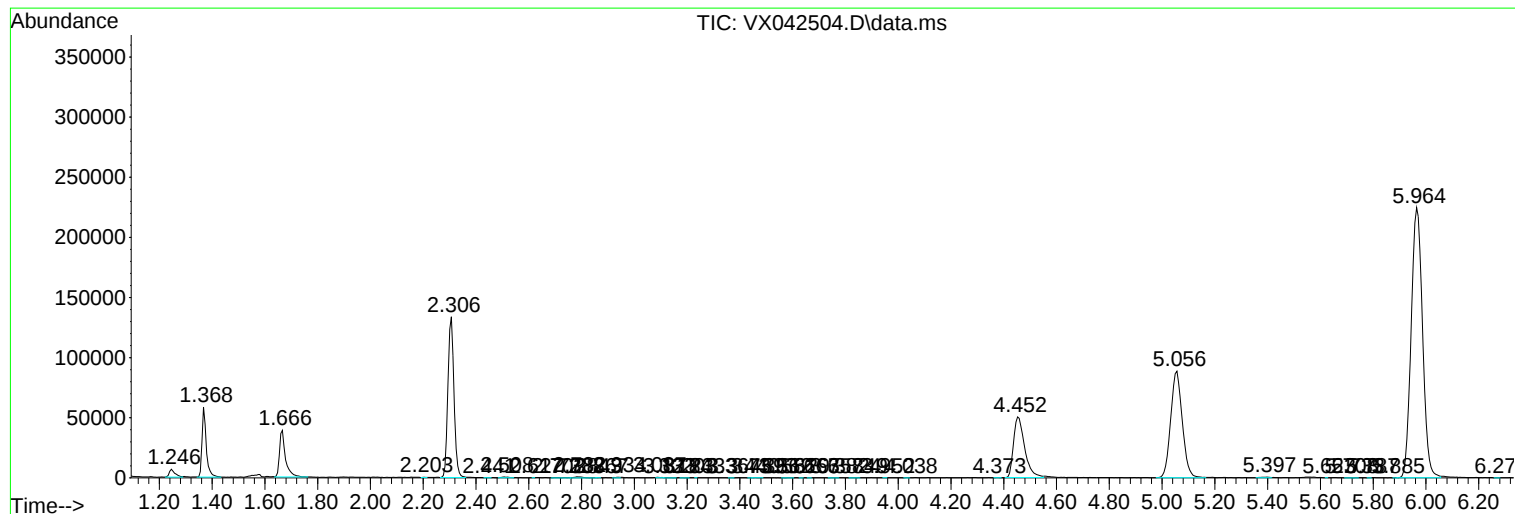

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042504.D
Acq On : 24 Jul 2024 10:04
Operator : JC/MD
Sample : VX0725MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK693

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042504.D
Acq On : 24 Jul 2024 10:04
Operator : JC/MD
Sample : VX0725MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK693

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc