

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042505.D
 Acq On : 24 Jul 2024 10:27
 Operator : JC/MD
 Sample : VX0725WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK694

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

Signal : TIC: VX042505.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	36	rVB2	6408	10736	1.75%	0.230%
2	1.368	43	46	59	rBV	45690	60255	9.81%	1.293%
3	1.551	69	76	77	rBV2	1743	2231	0.36%	0.048%
4	1.581	79	81	83	rVV2	2231	2884	0.47%	0.062%
5	1.612	83	86	87	rVV3	3581	4428	0.72%	0.095%
6	1.648	88	92	101	rVB	38213	51342	8.36%	1.102%
7	2.038	154	156	159	rBV2	262	306	0.05%	0.007%
8	2.087	162	164	165	rBV2	253	174	0.03%	0.004%
9	2.300	193	199	211	rVV	119415	188661	30.71%	4.048%
10	2.435	219	221	226	rVB	230	299	0.05%	0.006%
11	2.508	228	233	238	rBV2	553	1058	0.17%	0.023%
12	2.794	273	280	284	rBV3	722	1498	0.24%	0.032%
13	2.941	299	304	305	rBV2	598	772	0.13%	0.017%
14	3.002	312	314	317	rBV2	111	154	0.03%	0.003%
15	3.093	327	329	331	rVV	207	179	0.03%	0.004%
16	3.910	461	463	466	rBV2	109	150	0.02%	0.003%
17	4.270	520	522	524	rBV2	179	178	0.03%	0.004%
18	4.465	545	554	574	rBV	46488	137460	22.38%	2.950%
19	4.873	618	621	624	rBV2	98	154	0.03%	0.003%
20	5.056	639	651	670	rBV	79214	243867	39.70%	5.233%
21	5.379	702	704	705	rBV2	243	254	0.04%	0.005%
22	5.495	720	723	724	rBV2	136	152	0.02%	0.003%
23	5.544	727	731	732	rVV2	371	396	0.06%	0.008%
24	5.562	732	734	739	rVV2	463	705	0.11%	0.015%
25	5.696	755	756	760	rBV2	196	263	0.04%	0.006%
26	5.794	769	772	776	rVB2	233	297	0.05%	0.006%
27	5.971	788	801	821	rBV2	206644	614318	100.00%	13.183%
28	6.196	836	838	843	rVB2	223	400	0.07%	0.009%
29	6.233	843	844	846	rBV	210	179	0.03%	0.004%
30	6.269	849	850	854	rVV2	200	218	0.04%	0.005%
31	6.391	867	870	873	rBV2	179	298	0.05%	0.006%
32	6.556	894	897	901	rVB2	205	216	0.04%	0.005%
33	6.672	914	916	918	rBV	153	157	0.03%	0.003%
34	6.757	921	930	949	rVV	160266	388621	63.26%	8.339%
35	7.129	983	991	1001	rVB4	8682	22083	3.59%	0.474%
36	7.208	1001	1004	1011	rVB4	248	454	0.07%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042505.D
 Acq On : 24 Jul 2024 10:27
 Operator : JC/MD
 Sample : VX0725WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK694

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

37	7.306	1011	1020	1037	rBV	123291	274230	44.64%	5.885%
38	7.434	1039	1041	1045	rVB2	241	318	0.05%	0.007%
39	7.470	1045	1047	1048	rBV2	220	203	0.03%	0.004%
40	7.860	1107	1111	1112	rBV	175	238	0.04%	0.005%
41	7.958	1121	1127	1129	rBV2	480	571	0.09%	0.012%
42	8.019	1136	1137	1141	rBV2	226	349	0.06%	0.007%
43	8.324	1181	1187	1202	rVV	74936	129669	21.11%	2.783%
44	8.427	1202	1204	1205	rVV	324	278	0.05%	0.006%
45	8.446	1205	1207	1213	rVB3	273	356	0.06%	0.008%
46	8.647	1234	1240	1258	rBV	313360	491891	80.07%	10.555%
47	8.854	1272	1274	1277	rVB2	225	209	0.03%	0.004%
48	8.885	1277	1279	1282	rVB2	176	150	0.02%	0.003%
49	8.952	1284	1290	1302	rBV	56295	84195	13.71%	1.807%
50	9.238	1334	1337	1338	rBV2	129	180	0.03%	0.004%
51	9.275	1338	1343	1350	rVB2	2295	3611	0.59%	0.077%
52	9.330	1350	1352	1354	rBV2	127	169	0.03%	0.004%
53	9.385	1356	1361	1383	rBV	206415	303594	49.42%	6.515%
54	9.616	1397	1399	1402	rVB2	287	185	0.03%	0.004%
55	9.659	1404	1406	1411	rVB3	194	214	0.03%	0.005%
56	9.708	1411	1414	1416	rBV	295	296	0.05%	0.006%
57	10.055	1465	1471	1490	rBV	320390	444578	72.37%	9.540%
58	10.305	1509	1512	1519	rVB3	537	1075	0.17%	0.023%
59	10.360	1519	1521	1522	rBV	204	158	0.03%	0.003%
60	10.586	1556	1558	1560	rBV2	150	189	0.03%	0.004%
61	10.640	1565	1567	1569	rVV2	286	286	0.05%	0.006%
62	10.677	1571	1573	1575	rBV	307	308	0.05%	0.007%
63	10.970	1617	1621	1623	rBV2	320	308	0.05%	0.007%
64	11.073	1635	1638	1641	rBV	187	235	0.04%	0.005%
65	11.189	1652	1657	1668	rBV	249159	324069	52.75%	6.954%
66	11.317	1674	1678	1681	rVB	642	727	0.12%	0.016%
67	11.457	1699	1701	1704	rVB2	318	303	0.05%	0.007%
68	11.543	1712	1715	1717	rBV	146	173	0.03%	0.004%
69	11.762	1746	1751	1754	rBV3	430	681	0.11%	0.015%
70	11.933	1776	1779	1780	rBV2	185	222	0.04%	0.005%
71	11.976	1783	1786	1788	rBV	764	918	0.15%	0.020%
72	12.018	1788	1793	1806	rVV	303116	404449	65.84%	8.679%
73	12.317	1837	1842	1856	rVV	351843	442327	72.00%	9.492%
74	12.762	1911	1915	1919	rBV2	908	1049	0.17%	0.023%
75	12.878	1931	1934	1937	rBV2	91	150	0.02%	0.003%
76	13.122	1969	1974	1978	rVB3	596	805	0.13%	0.017%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042505.D
 Acq On : 24 Jul 2024 10:27
 Operator : JC/MD
 Sample : VX0725WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK694

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

77	13.445	2025	2027	2033	rVB2	128	165	0.03%	0.004%
78	13.555	2041	2045	2047	rBV2	114	168	0.03%	0.004%
79	13.597	2048	2052	2056	rVB2	745	1017	0.17%	0.022%
80	13.780	2079	2082	2088	rVV	800	1226	0.20%	0.026%
81	13.865	2093	2096	2099	rBV2	139	225	0.04%	0.005%
82	13.963	2108	2112	2117	rBV	825	947	0.15%	0.020%
83	14.128	2135	2139	2145	rBV2	1114	1680	0.27%	0.036%
84	14.499	2197	2200	2201	rBV2	208	232	0.04%	0.005%
85	14.640	2220	2223	2224	rBV	183	170	0.03%	0.004%
86	14.707	2232	2234	2236	rBV2	173	183	0.03%	0.004%
87	14.853	2257	2258	2261	rBV2	178	150	0.02%	0.003%
88	14.884	2261	2263	2264	rVV2	253	214	0.03%	0.005%
89	14.926	2267	2270	2272	rVB3	207	265	0.04%	0.006%
90	14.945	2272	2273	2276	rBV2	213	210	0.03%	0.005%
91	15.158	2307	2308	2310	rBV2	202	167	0.03%	0.004%
92	15.243	2320	2322	2325	rBV2	320	277	0.05%	0.006%
93	15.390	2342	2346	2349	rBV	1058	1402	0.23%	0.030%
94	15.707	2397	2398	2400	rBV	305	268	0.04%	0.006%
95	15.847	2419	2421	2423	rBV3	252	241	0.04%	0.005%
96	15.865	2423	2424	2426	rVV2	319	158	0.03%	0.003%
97	15.896	2426	2429	2432	rVV2	301	385	0.06%	0.008%
98	15.969	2439	2441	2443	rVB2	329	223	0.04%	0.005%
99	16.237	2483	2485	2487	rVB3	264	193	0.03%	0.004%
100	16.627	2547	2549	2550	rBV2	216	178	0.03%	0.004%




Sum of corrected areas: 4660057

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042505.D
Acq On : 24 Jul 2024 10:27
Operator : JC/MD
Sample : VX0725WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK694

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

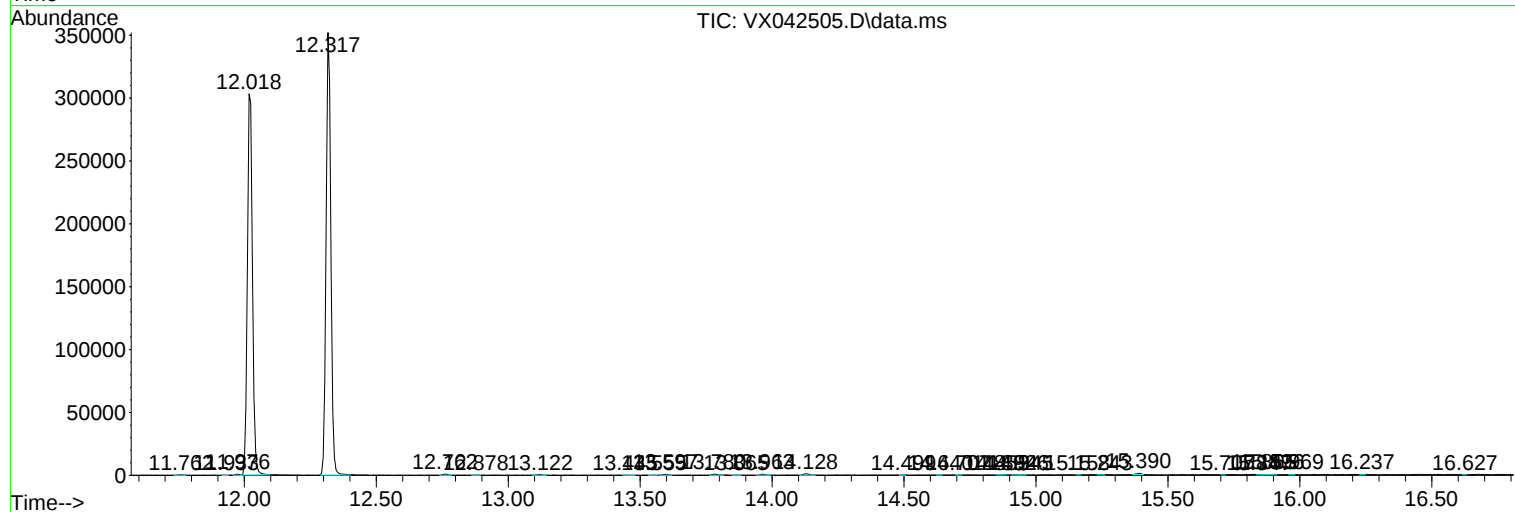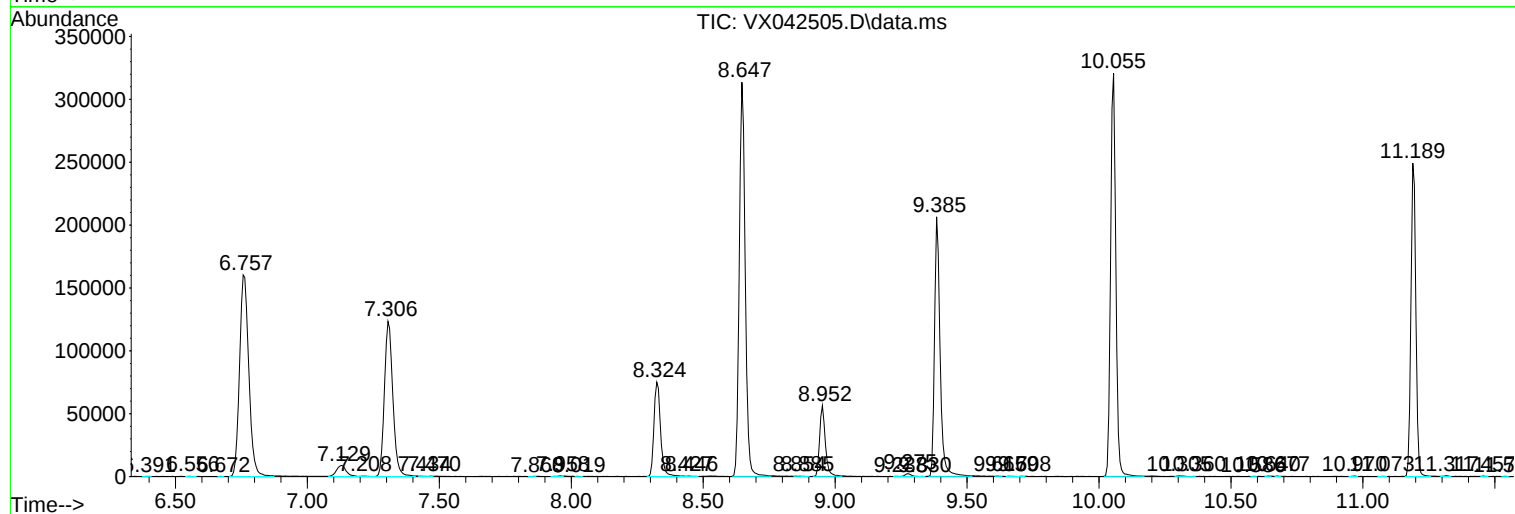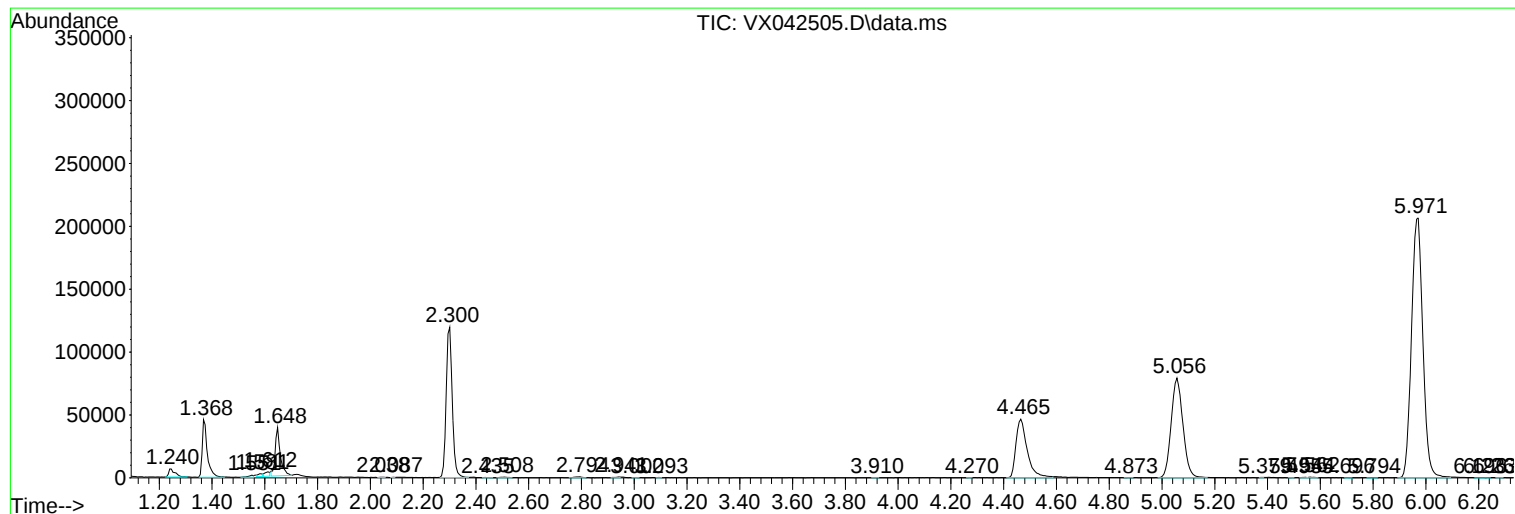

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042505.D
Acq On : 24 Jul 2024 10:27
Operator : JC/MD
Sample : VX0725WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK694

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042505.D
Acq On : 24 Jul 2024 10:27
Operator : JC/MD
Sample : VX0725WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK694

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------