

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042508.D
 Acq On : 24 Jul 2024 11:36
 Operator : JC/MD
 Sample : P3327-14DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E1ZW9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

Signal : TIC: VX042508.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	22	26	28	rBV	6697	8281	1.30%	0.143%
2	1.374	43	47	62	rVB2	130055	180297	28.24%	3.120%
3	1.569	69	79	81	rBV5	2108	4878	0.76%	0.084%
4	1.648	89	92	101	rVB	39178	48015	7.52%	0.831%
5	1.715	101	103	112	rVB4	2326	4877	0.76%	0.084%
6	1.874	127	129	130	rVB2	253	147	0.02%	0.003%
7	1.898	130	133	135	rBV2	209	298	0.05%	0.005%
8	2.002	148	150	153	rBV2	151	185	0.03%	0.003%
9	2.069	158	161	164	rBV	222	301	0.05%	0.005%
10	2.105	164	167	169	rBV2	244	263	0.04%	0.005%
11	2.227	185	187	189	rVV2	175	193	0.03%	0.003%
12	2.300	193	199	211	rVV	126944	201776	31.61%	3.492%
13	2.386	211	213	219	rVV3	667	1036	0.16%	0.018%
14	2.459	222	225	227	rBV	122	159	0.02%	0.003%
15	2.489	227	230	231	rVV	143	156	0.02%	0.003%
16	2.502	231	232	236	rVB	335	236	0.04%	0.004%
17	2.575	242	244	248	rVB2	250	283	0.04%	0.005%
18	2.666	257	259	262	rVB2	174	177	0.03%	0.003%
19	2.709	262	266	269	rBV2	215	377	0.06%	0.007%
20	2.788	273	279	286	rBV2	1840	3768	0.59%	0.065%
21	2.947	296	305	314	rBV	9824	22832	3.58%	0.395%
22	3.008	314	315	318	rVV2	173	151	0.02%	0.003%
23	3.093	322	329	337	rVB2	2256	4531	0.71%	0.078%
24	3.245	350	354	359	rBV2	171	325	0.05%	0.006%
25	3.416	379	382	383	rVB	183	170	0.03%	0.003%
26	3.611	409	414	416	rBV2	336	556	0.09%	0.010%
27	3.751	431	437	438	rBV	97	176	0.03%	0.003%
28	3.806	444	446	448	rVB2	159	159	0.02%	0.003%
29	3.831	448	450	453	rBV2	176	278	0.04%	0.005%
30	3.855	453	454	459	rVB2	218	334	0.05%	0.006%
31	3.910	461	463	469	rVB2	133	165	0.03%	0.003%
32	4.056	483	487	491	rBV2	154	348	0.05%	0.006%
33	4.483	546	557	571	rBV2	181066	555657	87.05%	9.616%
34	4.891	622	624	627	rVB	152	172	0.03%	0.003%
35	5.056	639	651	668	rBV2	81735	253978	39.79%	4.395%
36	5.416	702	710	712	rVB3	246	419	0.07%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042508.D
 Acq On : 24 Jul 2024 11:36
 Operator : JC/MD
 Sample : P3327-14DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E1ZW9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

37	5.452	715	716	719	rBV2	148	176	0.03%	0.003%
38	5.562	728	734	735	rBV3	315	537	0.08%	0.009%
39	5.623	742	744	747	rVB	169	186	0.03%	0.003%
40	5.659	747	750	752	rBV2	155	203	0.03%	0.004%
41	5.702	752	757	760	rBV	127	198	0.03%	0.003%
42	5.970	790	801	821	rVV2	215182	638349	100.00%	11.047%
43	6.196	837	838	840	rBV2	170	166	0.03%	0.003%
44	6.324	857	859	862	rBV2	126	160	0.03%	0.003%
45	6.452	878	880	883	rBV2	156	186	0.03%	0.003%
46	6.562	894	898	900	rBV2	237	306	0.05%	0.005%
47	6.763	921	931	946	rBV	187476	448195	70.21%	7.756%
48	6.958	961	963	969	rBV3	267	404	0.06%	0.007%
49	7.123	982	990	1002	rBV	126578	281968	44.17%	4.880%
50	7.306	1011	1020	1038	rBV	127143	285018	44.65%	4.932%
51	7.482	1046	1049	1050	rBV2	260	243	0.04%	0.004%
52	7.659	1075	1078	1082	rVB2	151	283	0.04%	0.005%
53	7.799	1100	1101	1105	rBV2	156	182	0.03%	0.003%
54	7.946	1123	1125	1126	rBV2	270	188	0.03%	0.003%
55	8.324	1181	1187	1200	rBV	79832	131844	20.65%	2.282%
56	8.647	1234	1240	1254	rBV	330196	518588	81.24%	8.974%
57	8.763	1257	1259	1264	rVB3	555	661	0.10%	0.011%
58	8.952	1285	1290	1302	rBV	56882	85024	13.32%	1.471%
59	9.134	1318	1320	1323	rVB2	164	161	0.03%	0.003%
60	9.195	1327	1330	1334	rVB2	130	182	0.03%	0.003%
61	9.275	1339	1343	1350	rVB4	1911	3032	0.47%	0.052%
62	9.384	1356	1361	1379	rBV	194988	297991	46.68%	5.157%
63	9.653	1402	1405	1409	rVB2	208	295	0.05%	0.005%
64	10.055	1465	1471	1480	rBV	367454	509274	79.78%	8.813%
65	10.305	1508	1512	1518	rVB5	621	942	0.15%	0.016%
66	10.646	1566	1568	1571	rBV2	198	233	0.04%	0.004%
67	10.963	1618	1620	1622	rBV2	235	215	0.03%	0.004%
68	11.189	1652	1657	1670	rVV	251471	332048	52.02%	5.746%
69	11.311	1675	1677	1681	rVB2	287	321	0.05%	0.006%
70	11.378	1687	1688	1691	rBV	136	176	0.03%	0.003%
71	11.433	1693	1697	1698	rBV2	111	164	0.03%	0.003%
72	11.451	1698	1700	1702	rBV2	179	176	0.03%	0.003%
73	11.762	1748	1751	1754	rVB3	170	240	0.04%	0.004%
74	11.975	1783	1786	1788	rVB	281	252	0.04%	0.004%
75	12.024	1788	1794	1809	rBV	365686	472218	73.97%	8.172%
76	12.317	1837	1842	1854	rBV	348591	460221	72.10%	7.964%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042508.D
 Acq On : 24 Jul 2024 11:36
 Operator : JC/MD
 Sample : P3327-14DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E1ZW9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

77	12.536	1876	1878	1881	rVB	288	283	0.04%	0.005%
78	12.561	1881	1882	1886	rBV2	172	260	0.04%	0.004%
79	12.762	1912	1915	1920	rBV3	864	1048	0.16%	0.018%
80	12.829	1924	1926	1929	rBV	168	160	0.03%	0.003%
81	13.000	1952	1954	1957	rBV2	140	210	0.03%	0.004%
82	13.122	1972	1974	1976	rBV	310	283	0.04%	0.005%
83	13.591	2049	2051	2055	rBV3	272	335	0.05%	0.006%
84	13.786	2080	2083	2086	rBV2	382	525	0.08%	0.009%
85	13.969	2111	2113	2115	rBV2	319	223	0.03%	0.004%
86	14.127	2135	2139	2144	rVV	1620	2189	0.34%	0.038%
87	14.195	2147	2150	2153	rBV3	151	198	0.03%	0.003%
88	14.219	2153	2154	2157	rBV2	188	148	0.02%	0.003%
89	14.274	2162	2163	2165	rBV	196	160	0.03%	0.003%
90	14.316	2168	2170	2173	rBV2	171	172	0.03%	0.003%
91	14.633	2220	2222	2224	rVB	193	151	0.02%	0.003%
92	14.664	2224	2227	2231	rBV3	187	300	0.05%	0.005%
93	14.804	2249	2250	2252	rBV2	219	171	0.03%	0.003%
94	14.963	2274	2276	2277	rBV	269	156	0.02%	0.003%
95	15.280	2326	2328	2329	rBV	214	199	0.03%	0.003%
96	15.389	2341	2346	2353	rBV3	1918	3462	0.54%	0.060%
97	15.554	2371	2373	2376	rBV2	236	219	0.03%	0.004%
98	15.932	2433	2435	2436	rBV2	218	154	0.02%	0.003%
99	16.097	2460	2462	2463	rBV	255	169	0.03%	0.003%
100	16.542	2534	2535	2536	rBV	282	161	0.03%	0.003%

Sum of corrected areas: 5778496




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042508.D
Acq On : 24 Jul 2024 11:36
Operator : JC/MD
Sample : P3327-14DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E1ZW9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

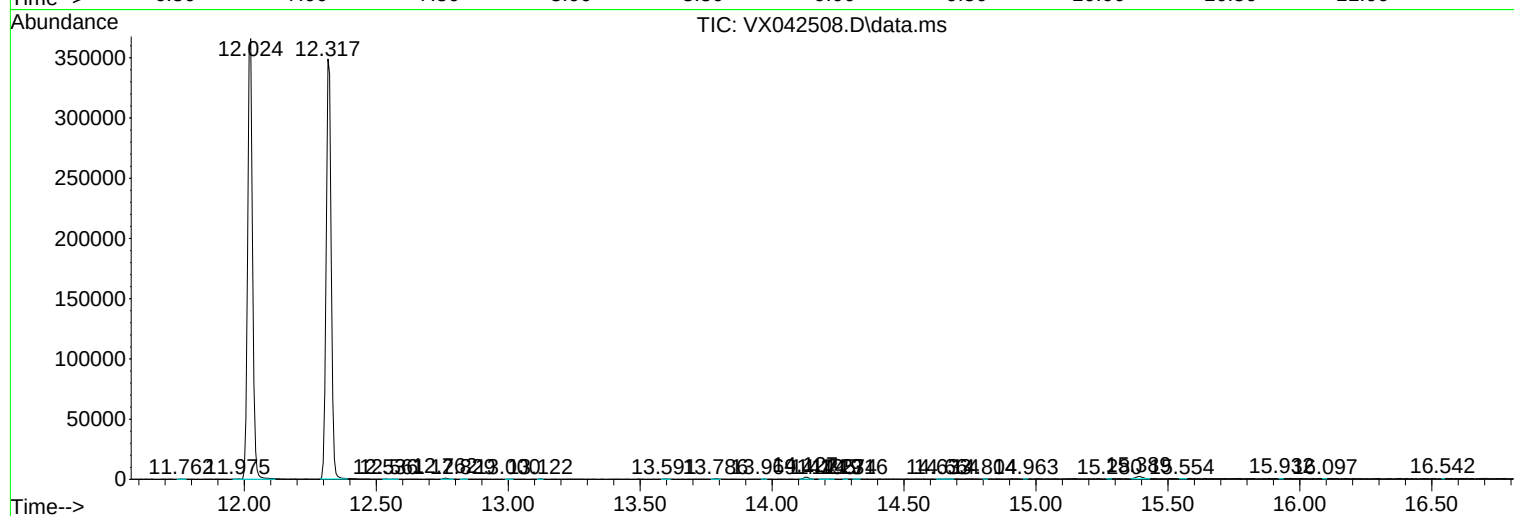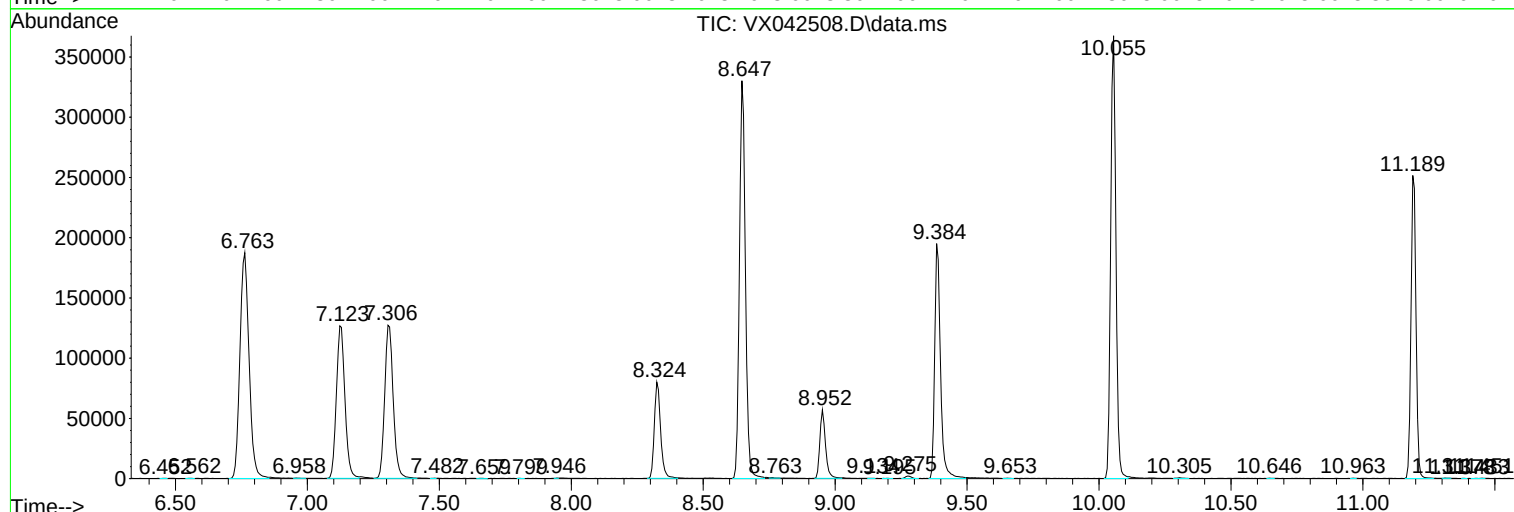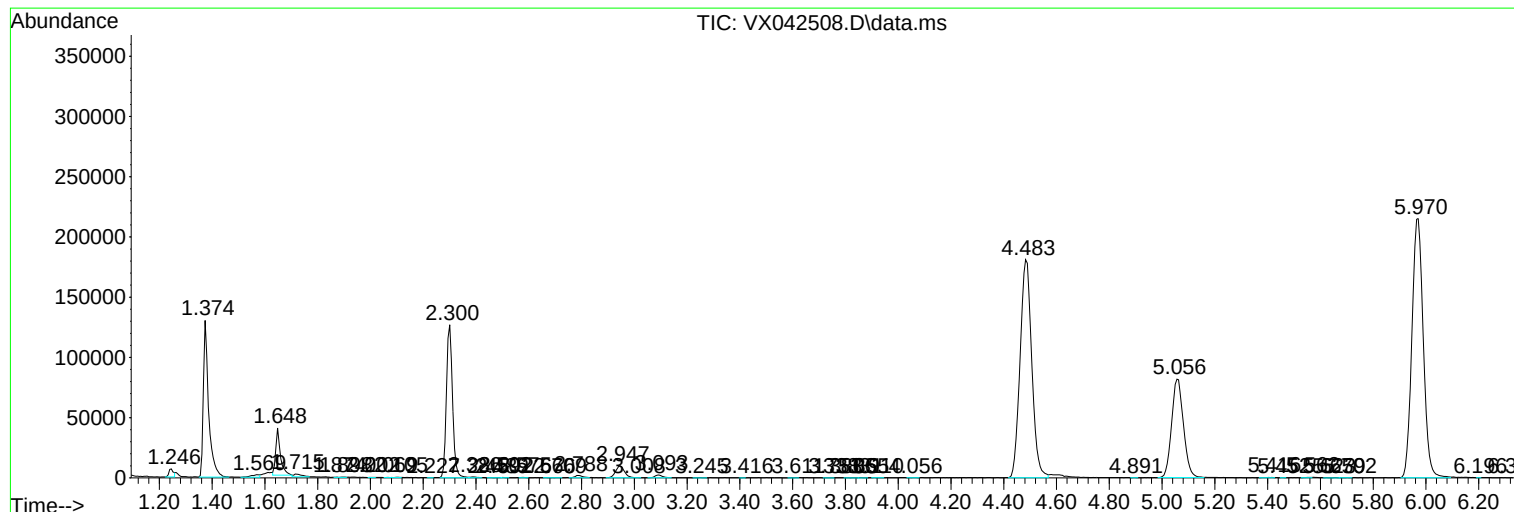

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042508.D
Acq On : 24 Jul 2024 11:36
Operator : JC/MD
Sample : P3327-14DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E1ZW9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042508.D
Acq On : 24 Jul 2024 11:36
Operator : JC/MD
Sample : P3327-14DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E1ZW9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc