

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042511.D
 Acq On : 24 Jul 2024 12:45
 Operator : JC/MD
 Sample : P3327-17DL 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E1ZX2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

Signal : TIC: VX042511.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	33	rBV2	5631	10119	1.29%	0.188%
2	1.368	43	46	58	rVB	44353	59696	7.62%	1.108%
3	1.557	71	77	78	rBV3	1651	2243	0.29%	0.042%
4	1.648	88	92	101	rVB	36454	47171	6.02%	0.876%
5	2.136	171	172	176	rBV3	165	237	0.03%	0.004%
6	2.246	189	190	192	rBV	205	73	0.01%	0.001%
7	2.300	192	199	211	rBV	104689	169033	21.57%	3.138%
8	2.453	221	224	225	rBV2	200	186	0.02%	0.003%
9	2.563	240	242	243	rBV	105	76	0.01%	0.001%
10	2.666	257	259	260	rBV	105	69	0.01%	0.001%
11	2.746	270	272	274	rBV	90	77	0.01%	0.001%
12	2.782	274	278	287	rVV2	1658	3275	0.42%	0.061%
13	2.947	295	305	315	rBV	8668	20869	2.66%	0.387%
14	3.014	315	316	319	rBV2	121	131	0.02%	0.002%
15	3.038	319	320	322	rVB	117	64	0.01%	0.001%
16	3.087	324	328	334	rVB2	945	1503	0.19%	0.028%
17	3.136	334	336	340	rBV2	81	132	0.02%	0.002%
18	3.343	366	370	372	rBV2	101	140	0.02%	0.003%
19	3.373	373	375	379	rVB2	209	230	0.03%	0.004%
20	3.410	379	381	383	rVB	177	140	0.02%	0.003%
21	3.428	383	384	386	rBV	99	81	0.01%	0.002%
22	3.477	389	392	395	rBV	110	164	0.02%	0.003%
23	3.575	406	408	410	rBV	107	132	0.02%	0.002%
24	3.709	428	430	431	rBV2	107	93	0.01%	0.002%
25	3.764	438	439	443	rBV	134	172	0.02%	0.003%
26	3.812	445	447	448	rBV	144	104	0.01%	0.002%
27	3.928	464	466	468	rBV	123	123	0.02%	0.002%
28	3.971	470	473	475	rBV2	175	187	0.02%	0.003%
29	4.026	480	482	484	rBV	143	98	0.01%	0.002%
30	4.184	507	508	509	rBV	129	79	0.01%	0.001%
31	4.373	537	539	540	rVB	133	64	0.01%	0.001%
32	4.477	546	556	572	rBV2	80434	270825	34.56%	5.028%
33	5.056	639	651	667	rBV2	71129	222466	28.39%	4.130%
34	5.221	677	678	682	rVB2	275	188	0.02%	0.003%
35	5.257	682	684	685	rVB2	174	117	0.01%	0.002%
36	5.276	685	687	688	rBV2	126	100	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042511.D
 Acq On : 24 Jul 2024 12:45
 Operator : JC/MD
 Sample : P3327-17DL 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E1ZX2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

37	5.391	703	706	707	rBV	175	191	0.02%	0.004%
38	5.452	713	716	717	rBV2	87	72	0.01%	0.001%
39	5.654	743	749	751	rBV2	148	261	0.03%	0.005%
40	5.721	755	760	761	rBV2	140	174	0.02%	0.003%
41	5.964	789	800	818	rBV2	187556	556259	70.98%	10.327%
42	6.245	844	846	847	rBV	123	99	0.01%	0.002%
43	6.409	871	873	875	rBV	80	73	0.01%	0.001%
44	6.659	912	914	916	rBV	130	145	0.02%	0.003%
45	6.763	921	931	949	rBV	172393	417701	53.30%	7.755%
46	7.123	981	990	1008	rBV	359064	783733	100.00%	14.551%
47	7.306	1012	1020	1032	rBV	111236	245879	31.37%	4.565%
48	7.482	1046	1049	1050	rBV2	159	162	0.02%	0.003%
49	7.745	1091	1092	1096	rBV	109	97	0.01%	0.002%
50	7.799	1099	1101	1103	rBV2	95	93	0.01%	0.002%
51	7.860	1109	1111	1113	rBV2	95	109	0.01%	0.002%
52	7.976	1123	1130	1131	rBV4	319	626	0.08%	0.012%
53	8.080	1145	1147	1148	rVB	131	65	0.01%	0.001%
54	8.190	1164	1165	1168	rBV2	116	120	0.02%	0.002%
55	8.324	1181	1187	1204	rBV	65988	116466	14.86%	2.162%
56	8.513	1216	1218	1223	rBV4	286	440	0.06%	0.008%
57	8.647	1234	1240	1251	rBV	285980	447387	57.08%	8.306%
58	8.952	1285	1290	1300	rBV	49384	73537	9.38%	1.365%
59	9.153	1321	1323	1324	rVB	147	75	0.01%	0.001%
60	9.275	1338	1343	1349	rVB4	1846	2821	0.36%	0.052%
61	9.348	1353	1355	1356	rBV	156	152	0.02%	0.003%
62	9.385	1356	1361	1383	rBV	180888	279698	35.69%	5.193%
63	9.702	1408	1413	1417	rVB	1391	1980	0.25%	0.037%
64	9.738	1417	1419	1422	rVB2	131	121	0.02%	0.002%
65	9.775	1422	1425	1426	rBV	127	147	0.02%	0.003%
66	10.055	1465	1471	1487	rBV	355661	480447	61.30%	8.920%
67	10.281	1506	1508	1509	rBV	107	71	0.01%	0.001%
68	10.305	1509	1512	1515	rVV2	383	424	0.05%	0.008%
69	10.427	1530	1532	1534	rBV2	162	117	0.01%	0.002%
70	10.555	1552	1553	1555	rBV	144	104	0.01%	0.002%
71	10.616	1561	1563	1566	rBV2	109	158	0.02%	0.003%
72	10.811	1592	1595	1596	rBV2	159	166	0.02%	0.003%
73	10.970	1619	1621	1623	rVB	213	142	0.02%	0.003%
74	11.006	1626	1627	1630	rBV2	104	101	0.01%	0.002%
75	11.134	1647	1648	1652	rBV2	119	172	0.02%	0.003%
76	11.189	1652	1657	1671	rVV	229919	305326	38.96%	5.669%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042511.D
 Acq On : 24 Jul 2024 12:45
 Operator : JC/MD
 Sample : P3327-17DL 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E1ZX2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

77	11.317	1675	1678	1682	rVB	508	721	0.09%	0.013%
78	11.354	1682	1684	1685	rBV	103	72	0.01%	0.001%
79	11.634	1728	1730	1733	rBV	155	150	0.02%	0.003%
80	11.689	1737	1739	1740	rBV	144	144	0.02%	0.003%
81	11.732	1744	1746	1747	rBV2	106	108	0.01%	0.002%
82	11.756	1748	1750	1754	rVB2	218	282	0.04%	0.005%
83	11.793	1754	1756	1758	rBV	104	65	0.01%	0.001%
84	12.024	1788	1794	1806	rBV	335846	441320	56.31%	8.193%
85	12.213	1824	1825	1828	rBV	176	189	0.02%	0.004%
86	12.317	1837	1842	1855	rBV	319235	412199	52.59%	7.653%
87	12.518	1874	1875	1876	rBV	118	82	0.01%	0.002%
88	12.768	1911	1916	1919	rBV2	703	1059	0.14%	0.020%
89	12.829	1925	1926	1927	rBV	147	71	0.01%	0.001%
90	13.122	1972	1974	1978	rBV3	302	466	0.06%	0.009%
91	13.256	1994	1996	2000	rBV2	152	182	0.02%	0.003%
92	13.536	2041	2042	2046	rVB	149	137	0.02%	0.003%
93	13.634	2056	2058	2059	rVB2	155	87	0.01%	0.002%
94	13.652	2059	2061	2063	rBV2	134	150	0.02%	0.003%
95	13.786	2081	2083	2088	rVB3	179	275	0.04%	0.005%
96	13.884	2098	2099	2102	rBV	186	225	0.03%	0.004%
97	14.134	2135	2140	2145	rBV	995	1544	0.20%	0.029%
98	14.219	2153	2154	2156	rBV2	179	151	0.02%	0.003%
99	14.292	2165	2166	2167	rBV	141	90	0.01%	0.002%
100	14.439	2189	2190	2191	rBV	239	155	0.02%	0.003%

Sum of corrected areas: 5386292




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042511.D
Acq On : 24 Jul 2024 12:45
Operator : JC/MD
Sample : P3327-17DL 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E1ZX2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

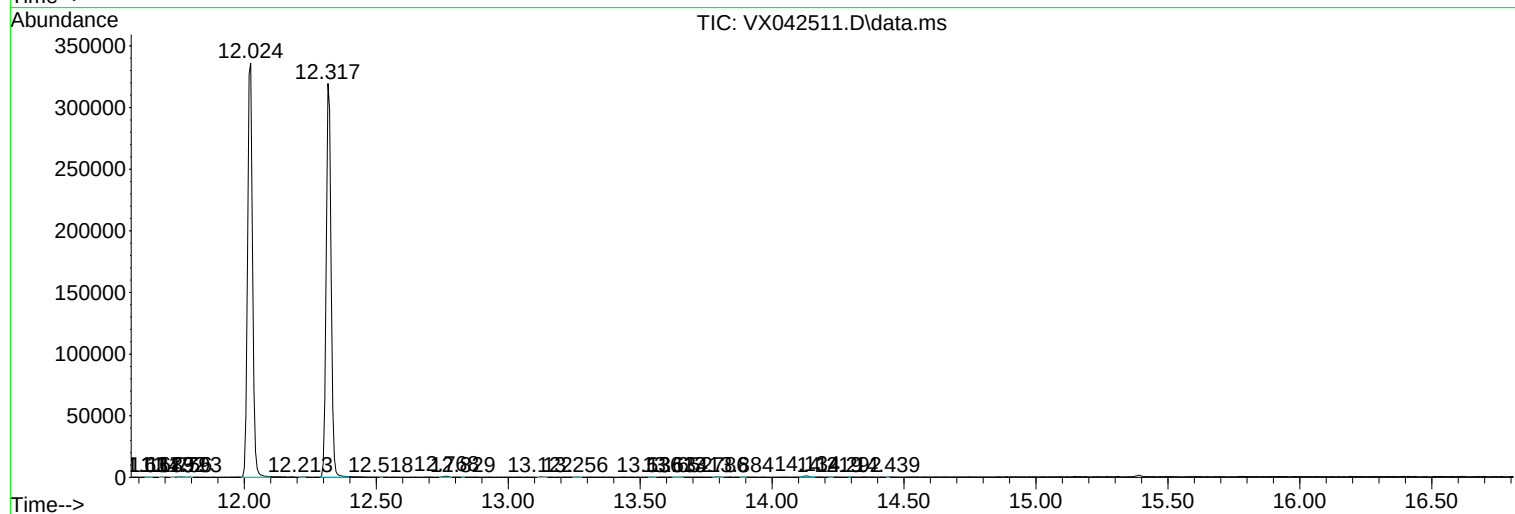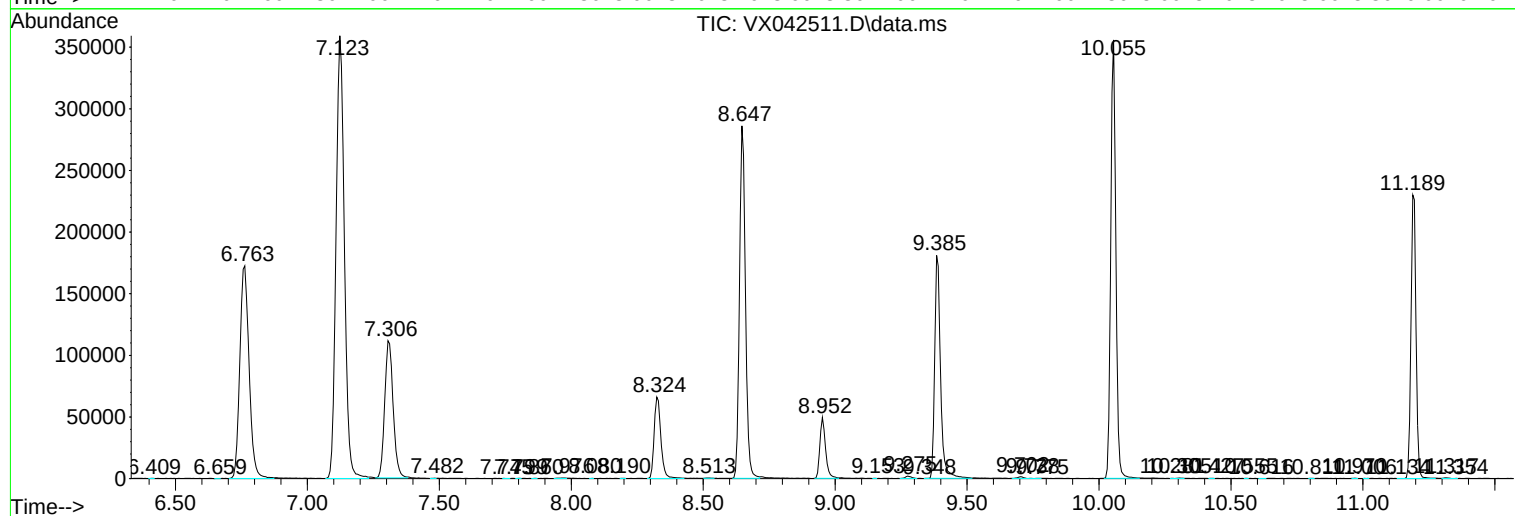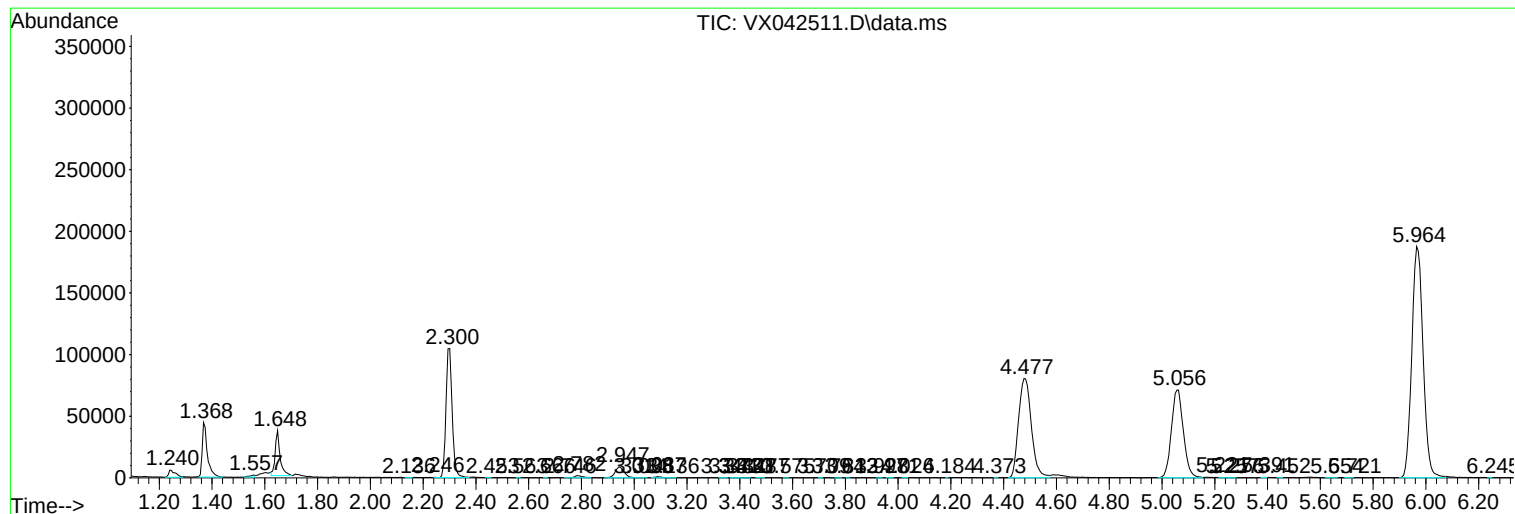

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042511.D
Acq On : 24 Jul 2024 12:45
Operator : JC/MD
Sample : P3327-17DL 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E1ZX2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042511.D
Acq On : 24 Jul 2024 12:45
Operator : JC/MD
Sample : P3327-17DL 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E1ZX2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------