

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042513.D
 Acq On : 24 Jul 2024 13:31
 Operator : JC/MD
 Sample : P3264-24
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

Signal : TIC: VX042513.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.245	22	26	27	rBV	5515	5946	1.10%	0.141%
2	1.367	43	46	62	rVB	38641	52460	9.67%	1.240%
3	1.648	88	92	101	rVB	32065	42446	7.83%	1.003%
4	1.879	128	130	131	rVB	315	137	0.03%	0.003%
5	2.123	164	170	171	rBV2	202	352	0.06%	0.008%
6	2.190	179	181	182	rBV	153	74	0.01%	0.002%
7	2.294	192	198	210	rBV	98977	160140	29.53%	3.784%
8	2.562	240	242	248	rBV2	205	271	0.05%	0.006%
9	2.690	261	263	265	rVB	209	153	0.03%	0.004%
10	2.709	265	266	271	rBV2	212	334	0.06%	0.008%
11	2.788	274	279	289	rVB2	1866	4252	0.78%	0.100%
12	2.898	293	297	298	rBV	190	226	0.04%	0.005%
13	2.952	299	306	311	rVB4	574	1368	0.25%	0.032%
14	3.062	321	324	326	rVB2	184	190	0.04%	0.004%
15	3.111	331	332	335	rBV2	130	142	0.03%	0.003%
16	3.282	358	360	361	rBV	135	121	0.02%	0.003%
17	3.361	371	373	375	rBV	112	141	0.03%	0.003%
18	3.452	386	388	390	rVB	143	132	0.02%	0.003%
19	3.501	394	396	398	rVB	120	85	0.02%	0.002%
20	3.532	400	401	402	rBV	134	84	0.02%	0.002%
21	3.678	424	425	428	rVB	141	112	0.02%	0.003%
22	3.836	449	451	455	rBV2	96	132	0.02%	0.003%
23	3.989	473	476	478	rBV	218	264	0.05%	0.006%
24	4.111	494	496	498	rBV	127	116	0.02%	0.003%
25	4.300	526	527	529	rVB	153	70	0.01%	0.002%
26	4.464	546	554	576	rBV	41151	125789	23.19%	2.973%
27	4.867	618	620	624	rBV2	117	136	0.03%	0.003%
28	5.056	640	651	675	rBV	70190	214620	39.57%	5.072%
29	5.348	697	699	701	rBV2	239	238	0.04%	0.006%
30	5.385	703	705	706	rBV	194	122	0.02%	0.003%
31	5.452	714	716	717	rVB	123	79	0.01%	0.002%
32	5.470	717	719	720	rBV	220	128	0.02%	0.003%
33	5.623	743	744	746	rVB	117	79	0.01%	0.002%
34	5.647	746	748	750	rBV	184	131	0.02%	0.003%
35	5.732	760	762	766	rBV2	103	141	0.03%	0.003%
36	5.763	766	767	769	rVB2	168	98	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042513.D
 Acq On : 24 Jul 2024 13:31
 Operator : JC/MD
 Sample : P3264-24
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

37	5.787	769	771	772	rBV	84	80	0.01%	0.002%
38	5.964	787	800	820	rBV2	181439	542316	100.00%	12.816%
39	6.244	844	846	847	rBV	109	67	0.01%	0.002%
40	6.305	855	856	860	rVB2	201	206	0.04%	0.005%
41	6.336	860	861	864	rBV	160	168	0.03%	0.004%
42	6.568	893	899	901	rBV2	153	273	0.05%	0.006%
43	6.610	905	906	908	rVV	116	78	0.01%	0.002%
44	6.629	908	909	912	rVB	104	64	0.01%	0.002%
45	6.763	921	931	947	rBV	157250	378791	69.85%	8.951%
46	7.037	975	976	977	rBV	150	64	0.01%	0.002%
47	7.128	983	991	1001	rVB5	5825	14933	2.75%	0.353%
48	7.202	1001	1003	1004	rBV2	172	168	0.03%	0.004%
49	7.311	1012	1021	1039	rBV	109844	244321	45.05%	5.774%
50	7.470	1045	1047	1049	rBV	195	193	0.04%	0.005%
51	7.488	1049	1050	1056	rVV2	271	255	0.05%	0.006%
52	7.531	1056	1057	1060	rVV	140	91	0.02%	0.002%
53	7.762	1093	1095	1098	rVB	149	102	0.02%	0.002%
54	7.793	1098	1100	1103	rBV	131	102	0.02%	0.002%
55	7.951	1123	1126	1129	rBV2	349	504	0.09%	0.012%
56	8.012	1135	1136	1137	rBV	125	75	0.01%	0.002%
57	8.080	1145	1147	1149	rBV2	124	110	0.02%	0.003%
58	8.214	1168	1169	1175	rBV2	101	146	0.03%	0.003%
59	8.323	1181	1187	1201	rBV	62728	110116	20.30%	2.602%
60	8.525	1216	1220	1227	rVB3	336	793	0.15%	0.019%
61	8.646	1234	1240	1257	rBV	268409	432129	79.68%	10.212%
62	8.805	1264	1266	1268	rBV2	200	107	0.02%	0.003%
63	8.915	1282	1284	1285	rBV	151	108	0.02%	0.003%
64	8.951	1285	1290	1306	rVB	47640	72516	13.37%	1.714%
65	9.281	1339	1344	1348	rVB3	1496	2297	0.42%	0.054%
66	9.384	1356	1361	1381	rBV	175855	277200	51.11%	6.551%
67	9.835	1431	1435	1438	rBV2	142	229	0.04%	0.005%
68	9.860	1438	1439	1441	rBV	155	98	0.02%	0.002%
69	9.878	1441	1442	1443	rBV	99	60	0.01%	0.001%
70	9.963	1453	1456	1457	rBV	190	171	0.03%	0.004%
71	9.994	1457	1461	1465	rVV	116	166	0.03%	0.004%
72	10.055	1465	1471	1486	rBV	327614	443170	81.72%	10.473%
73	10.299	1510	1511	1520	rVB3	366	557	0.10%	0.013%
74	10.396	1525	1527	1529	rBV2	178	214	0.04%	0.005%
75	10.628	1563	1565	1567	rBV	108	67	0.01%	0.002%
76	10.689	1571	1575	1576	rVB	118	129	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042513.D
 Acq On : 24 Jul 2024 13:31
 Operator : JC/MD
 Sample : P3264-24
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

77	10.707	1576	1578	1579	rBV	115	83	0.02%	0.002%
78	10.841	1599	1600	1602	rBV2	117	80	0.01%	0.002%
79	11.055	1631	1635	1638	rBV2	103	170	0.03%	0.004%
80	11.195	1652	1658	1671	rBV	223545	297564	54.87%	7.032%
81	11.311	1675	1677	1681	rVB2	555	569	0.10%	0.013%
82	11.536	1713	1714	1716	rBV	111	82	0.02%	0.002%
83	11.670	1735	1736	1738	rBV2	132	90	0.02%	0.002%
84	11.756	1749	1750	1753	rVB2	177	114	0.02%	0.003%
85	11.969	1784	1785	1788	rVB	216	231	0.04%	0.005%
86	12.024	1788	1794	1804	rBV	303095	397448	73.29%	9.392%
87	12.237	1827	1829	1830	rVB2	222	111	0.02%	0.003%
88	12.317	1837	1842	1854	rBV	296828	395513	72.93%	9.347%
89	12.682	1900	1902	1904	rBV	140	111	0.02%	0.003%
90	12.762	1911	1915	1919	rVB2	1009	1367	0.25%	0.032%
91	12.798	1919	1921	1923	rBV2	71	85	0.02%	0.002%
92	12.829	1925	1926	1928	rBV2	135	123	0.02%	0.003%
93	12.884	1933	1935	1937	rBV	132	151	0.03%	0.004%
94	13.341	2009	2010	2013	rBV2	135	129	0.02%	0.003%
95	13.877	2096	2098	2099	rBV2	101	67	0.01%	0.002%
96	14.133	2136	2140	2144	rVB	1293	1716	0.32%	0.041%
97	14.188	2144	2149	2153	rBV2	198	478	0.09%	0.011%
98	14.298	2165	2167	2168	rVB	192	103	0.02%	0.002%
99	14.676	2227	2229	2230	rBV	275	203	0.04%	0.005%
100	14.993	2278	2281	2284	rBV3	376	465	0.09%	0.011%




Sum of corrected areas: 4231596

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042513.D
Acq On : 24 Jul 2024 13:31
Operator : JC/MD
Sample : P3264-24
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

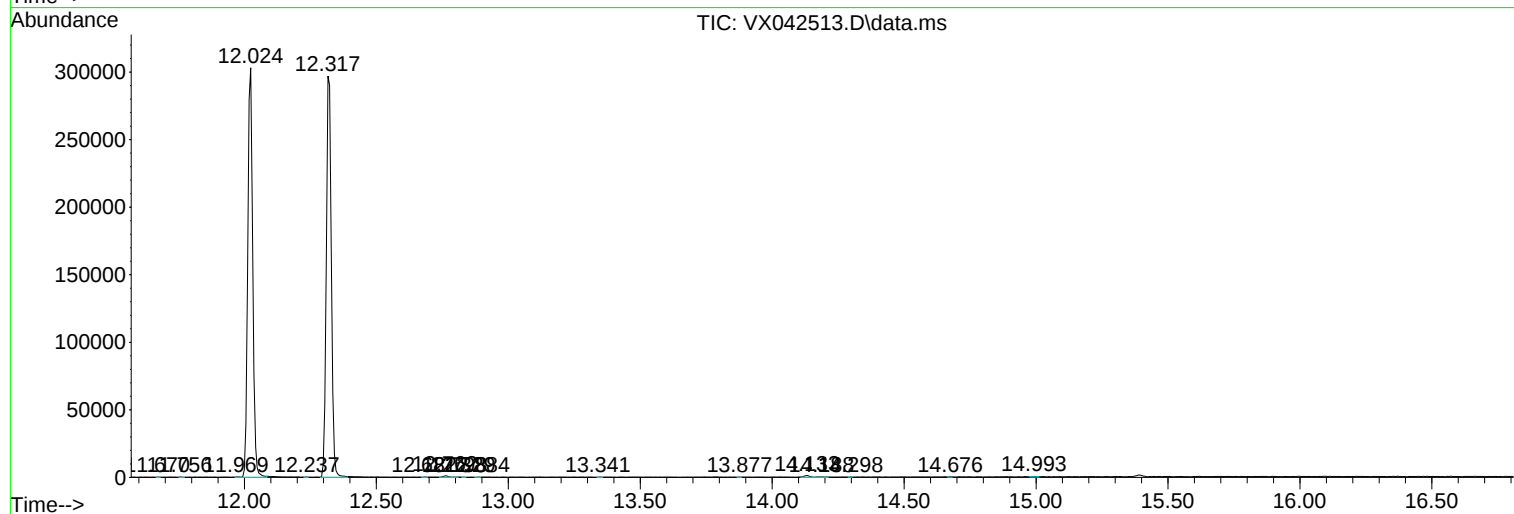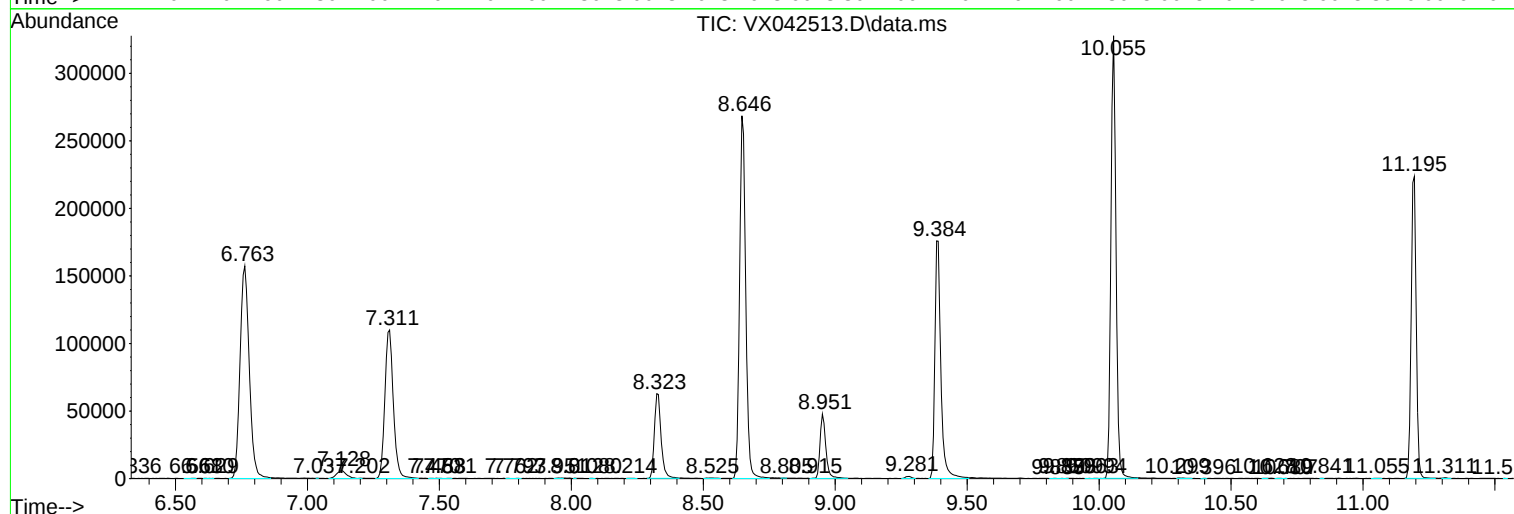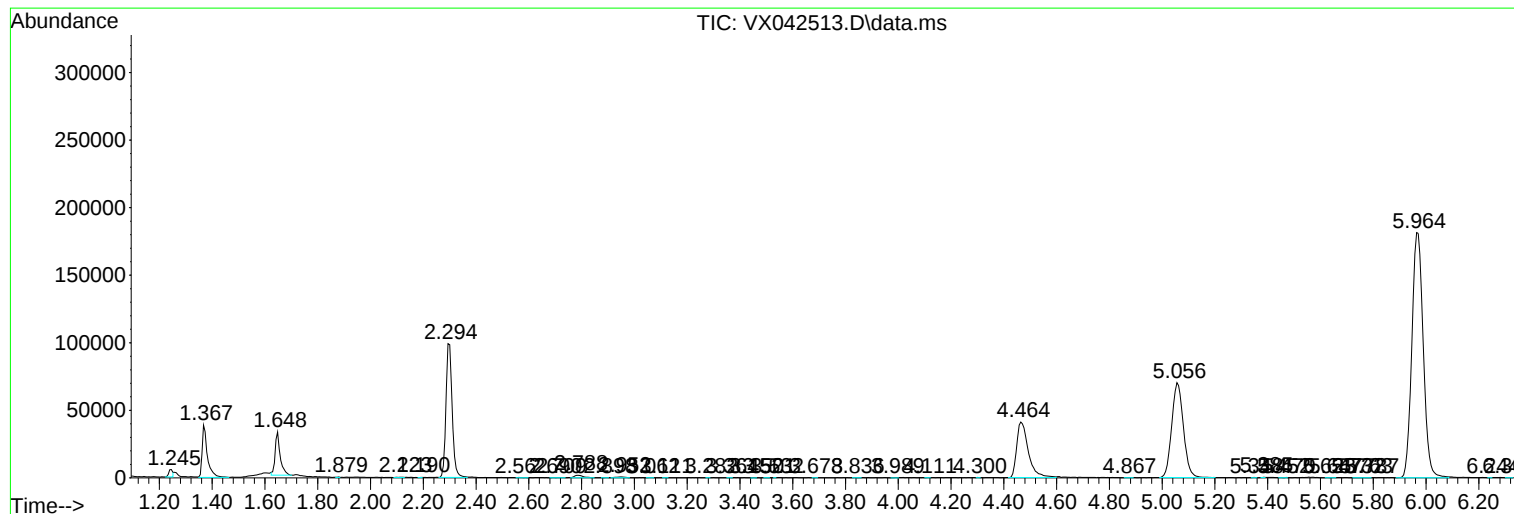

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042513.D
Acq On : 24 Jul 2024 13:31
Operator : JC/MD
Sample : P3264-24
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042513.D
Acq On : 24 Jul 2024 13:31
Operator : JC/MD
Sample : P3264-24
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------