

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042515.D
 Acq On : 24 Jul 2024 14:18
 Operator : JC/MD
 Sample : P3327-23 400X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20F5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

Signal : TIC: VX042515.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	27	rBV	5525	6037	1.09%	0.123%
2	1.368	42	46	60	rVB	40969	54905	9.91%	1.121%
3	1.563	71	78	79	rBV3	1507	2775	0.50%	0.057%
4	1.648	88	92	101	rVB	33770	44868	8.10%	0.916%
5	1.715	101	103	107	rVB	1402	1534	0.28%	0.031%
6	2.057	157	159	160	rVB2	241	161	0.03%	0.003%
7	2.111	165	168	174	rVV3	236	411	0.07%	0.008%
8	2.166	174	177	182	rVB3	190	325	0.06%	0.007%
9	2.203	182	183	187	rBV2	192	192	0.03%	0.004%
10	2.252	189	191	192	rBV	211	191	0.03%	0.004%
11	2.294	192	198	211	rVV	105039	166344	30.02%	3.397%
12	2.380	211	212	219	rVB2	465	768	0.14%	0.016%
13	2.508	228	233	235	rBV	234	251	0.05%	0.005%
14	2.569	240	243	245	rBV	291	335	0.06%	0.007%
15	2.624	248	252	255	rBV2	130	222	0.04%	0.005%
16	2.703	264	265	269	rBV3	164	167	0.03%	0.003%
17	2.788	274	279	285	rBV2	1976	4226	0.76%	0.086%
18	2.947	296	305	317	rVB	11998	28223	5.09%	0.576%
19	3.093	324	329	331	rBV	227	349	0.06%	0.007%
20	3.288	357	361	363	rBV2	174	251	0.05%	0.005%
21	3.398	377	379	380	rBV	177	147	0.03%	0.003%
22	3.502	393	396	397	rBV	137	142	0.03%	0.003%
23	3.697	422	428	432	rVB2	124	288	0.05%	0.006%
24	3.745	432	436	437	rBV2	152	184	0.03%	0.004%
25	3.855	450	454	457	rVB2	104	174	0.03%	0.004%
26	3.898	457	461	462	rVB	160	142	0.03%	0.003%
27	4.160	502	504	507	rVB2	151	164	0.03%	0.003%
28	4.251	517	519	525	rVB2	110	154	0.03%	0.003%
29	4.471	546	555	570	rBV2	50886	164254	29.65%	3.354%
30	5.056	639	651	670	rVV	71499	222113	40.09%	4.536%
31	5.196	672	674	675	rVB2	245	169	0.03%	0.003%
32	5.215	675	677	679	rBV3	214	180	0.03%	0.004%
33	5.330	692	696	698	rBV2	144	199	0.04%	0.004%
34	5.391	702	706	708	rBV	263	279	0.05%	0.006%
35	5.550	729	732	734	rBV2	272	310	0.06%	0.006%
36	5.745	761	764	771	rVB2	163	374	0.07%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042515.D
 Acq On : 24 Jul 2024 14:18
 Operator : JC/MD
 Sample : P3327-23 400X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20F5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

37	5.964	789	800	824	rBV2	189004	554053	100.00%	11.314%
38	6.538	890	894	896	rBV2	133	214	0.04%	0.004%
39	6.763	921	931	951	rBV	181963	442180	79.81%	9.029%
40	6.940	958	960	964	rVB3	246	269	0.05%	0.005%
41	7.123	982	990	1004	rBV	166754	376089	67.88%	7.680%
42	7.306	1012	1020	1037	rBV	111027	249953	45.11%	5.104%
43	7.440	1041	1042	1044	rBV2	174	168	0.03%	0.003%
44	7.489	1048	1050	1054	rBV2	275	274	0.05%	0.006%
45	7.690	1081	1083	1086	rBV	125	151	0.03%	0.003%
46	7.842	1105	1108	1111	rBV2	117	183	0.03%	0.004%
47	7.885	1113	1115	1117	rVB2	158	150	0.03%	0.003%
48	7.964	1124	1128	1129	rBV2	371	525	0.09%	0.011%
49	7.982	1129	1131	1133	rVB2	313	213	0.04%	0.004%
50	8.056	1141	1143	1145	rBV	171	155	0.03%	0.003%
51	8.153	1157	1159	1162	rBV2	125	162	0.03%	0.003%
52	8.220	1168	1170	1173	rBV2	161	219	0.04%	0.004%
53	8.324	1181	1187	1197	rBV	66349	111605	20.14%	2.279%
54	8.647	1234	1240	1250	rBV	273874	433639	78.27%	8.855%
55	8.836	1269	1271	1272	rBV2	200	176	0.03%	0.004%
56	8.903	1279	1282	1285	rBV	128	171	0.03%	0.003%
57	8.952	1285	1290	1307	rBV	48747	73010	13.18%	1.491%
58	9.165	1322	1325	1328	rBV	111	153	0.03%	0.003%
59	9.275	1340	1343	1348	rVB2	1424	2120	0.38%	0.043%
60	9.385	1356	1361	1384	rBV	170731	272732	49.22%	5.569%
61	9.702	1409	1413	1419	rVB	1810	2426	0.44%	0.050%
62	9.744	1419	1420	1423	rVB	200	177	0.03%	0.004%
63	9.988	1458	1460	1462	rVB2	184	165	0.03%	0.003%
64	10.055	1465	1471	1483	rBV	367401	502346	90.67%	10.258%
65	10.305	1510	1512	1518	rVB2	322	418	0.08%	0.009%
66	10.647	1567	1568	1572	rVB2	256	271	0.05%	0.006%
67	10.799	1590	1593	1594	rBV2	143	169	0.03%	0.003%
68	10.970	1617	1621	1622	rBV	233	314	0.06%	0.006%
69	11.189	1652	1657	1667	rBV	220013	294847	53.22%	6.021%
70	11.274	1670	1671	1675	rVV2	217	270	0.05%	0.006%
71	11.311	1675	1677	1681	rVV2	575	558	0.10%	0.011%
72	11.500	1704	1708	1711	rVB	150	149	0.03%	0.003%
73	11.579	1719	1721	1723	rVB	213	158	0.03%	0.003%
74	11.762	1749	1751	1755	rVB2	160	179	0.03%	0.004%
75	11.805	1755	1758	1762	rBV2	141	238	0.04%	0.005%
76	11.933	1775	1779	1781	rBV2	122	199	0.04%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042515.D
 Acq On : 24 Jul 2024 14:18
 Operator : JC/MD
 Sample : P3327-23 400X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20F5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

77	12.024	1788	1794	1806	rBV	347435	460439	83.10%	9.402%
78	12.317	1837	1842	1861	rBV	313785	403659	72.86%	8.243%
79	12.768	1910	1916	1920	rBV2	945	1233	0.22%	0.025%
80	12.847	1927	1929	1931	rBV	180	206	0.04%	0.004%
81	13.664	2061	2063	2069	rVV2	149	256	0.05%	0.005%
82	13.786	2081	2083	2087	rVB3	154	190	0.03%	0.004%
83	14.054	2124	2127	2129	rBV2	129	158	0.03%	0.003%
84	14.128	2134	2139	2145	rBV2	1331	1854	0.33%	0.038%
85	14.292	2161	2166	2167	rBV3	140	193	0.03%	0.004%
86	14.365	2176	2178	2180	rBV2	139	141	0.03%	0.003%
87	14.481	2194	2197	2199	rBV	255	219	0.04%	0.004%
88	14.548	2205	2208	2209	rVV2	171	161	0.03%	0.003%
89	14.591	2213	2215	2219	rBV2	180	252	0.05%	0.005%
90	14.853	2256	2258	2259	rBV	234	214	0.04%	0.004%
91	14.938	2269	2272	2274	rBV3	142	151	0.03%	0.003%
92	15.006	2281	2283	2285	rBV3	169	150	0.03%	0.003%
93	15.390	2340	2346	2352	rVB4	1502	2324	0.42%	0.047%
94	15.530	2365	2369	2371	rBV2	399	437	0.08%	0.009%
95	15.822	2414	2417	2422	rVB3	350	439	0.08%	0.009%
96	15.987	2442	2444	2446	rVB2	359	280	0.05%	0.006%
97	16.018	2446	2449	2450	rVV2	241	287	0.05%	0.006%
98	16.048	2452	2454	2457	rVV	318	294	0.05%	0.006%
99	16.237	2484	2485	2488	rBV2	280	203	0.04%	0.004%
100	16.268	2488	2490	2491	rVB2	319	211	0.04%	0.004%

Sum of corrected areas: 4897207




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042515.D
Acq On : 24 Jul 2024 14:18
Operator : JC/MD
Sample : P3327-23 400X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20F5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

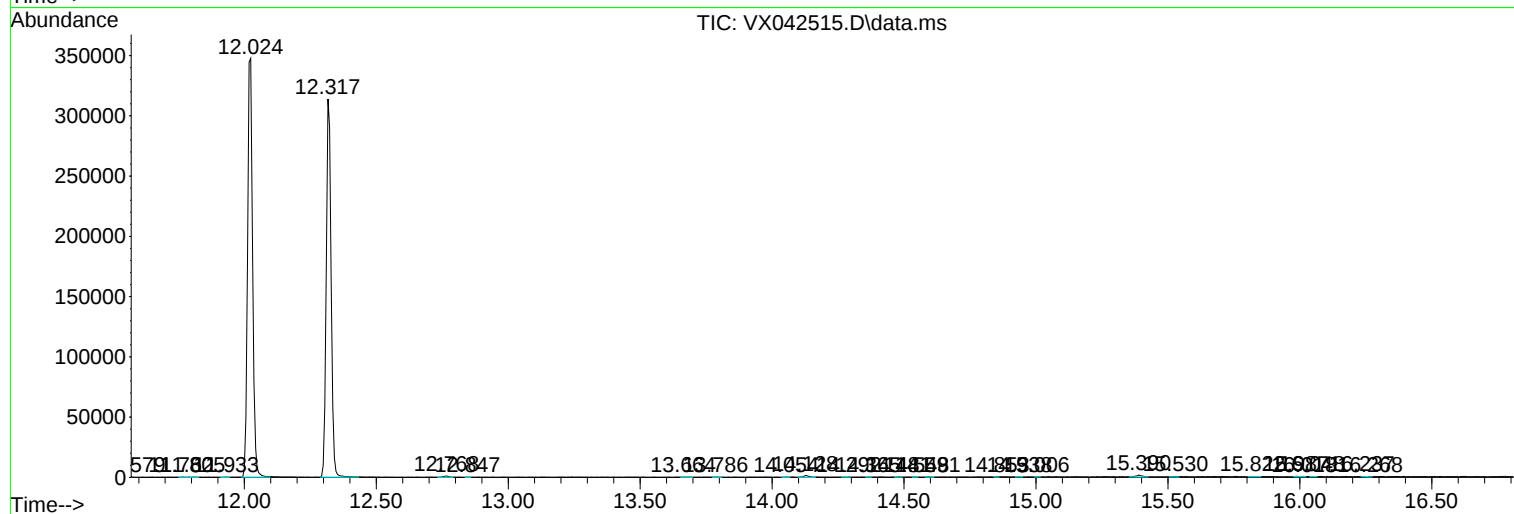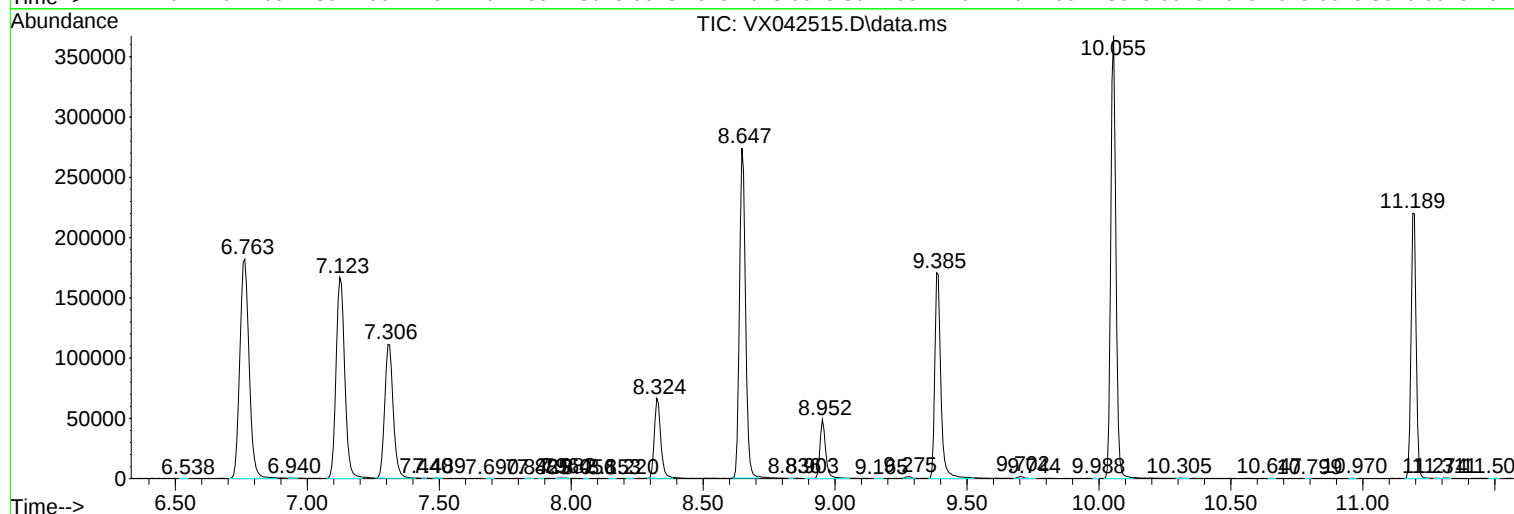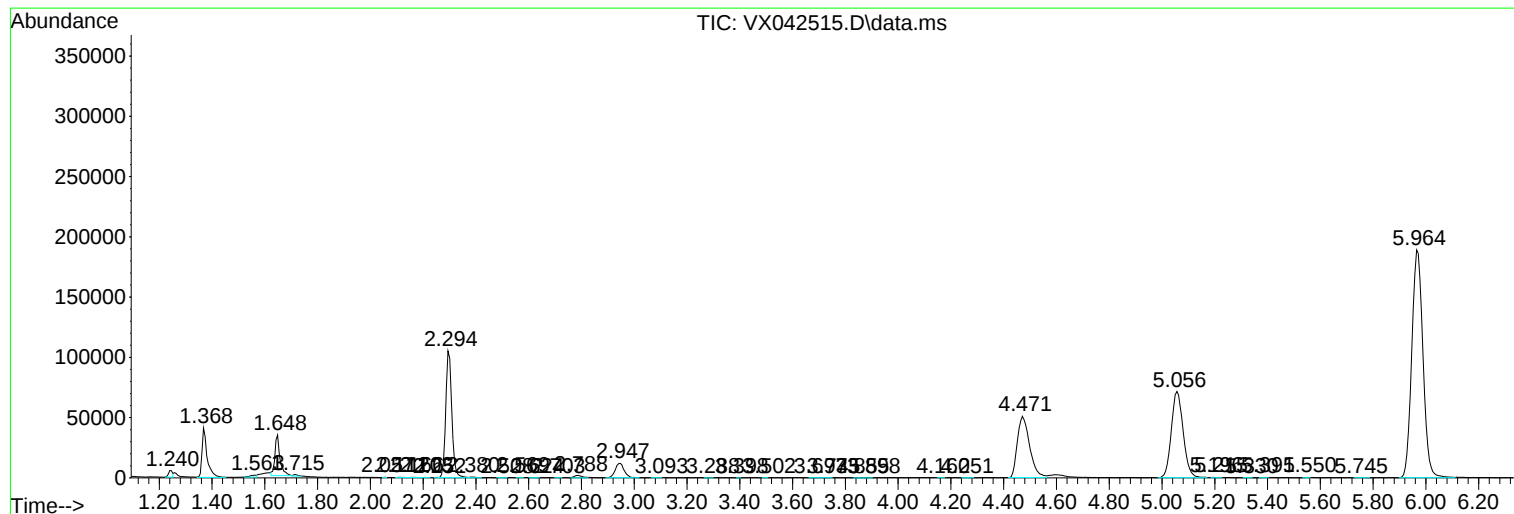

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042515.D
Acq On : 24 Jul 2024 14:18
Operator : JC/MD
Sample : P3327-23 400X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20F5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042515.D
Acq On : 24 Jul 2024 14:18
Operator : JC/MD
Sample : P3327-23 400X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20F5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc